
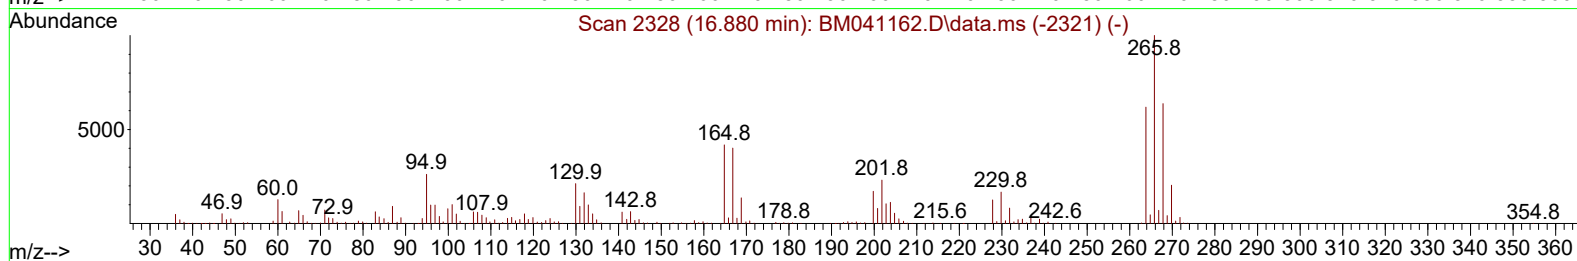
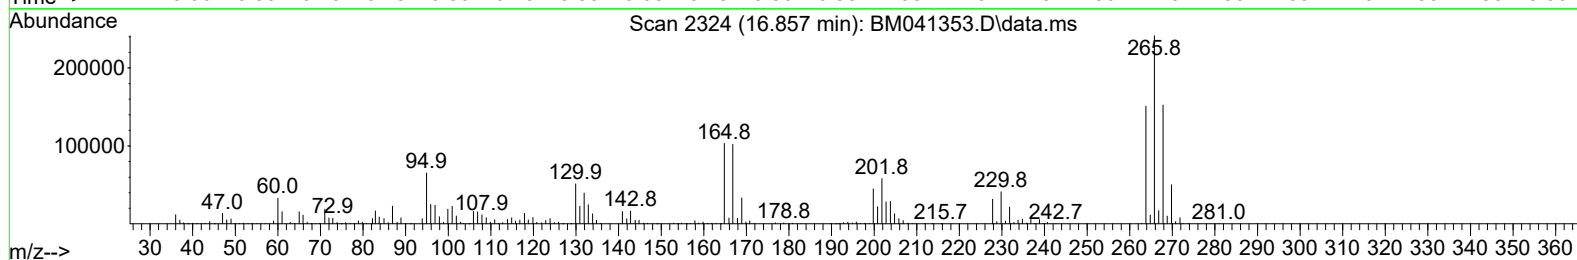


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041353.D
Acq On : 10 Aug 2023 07:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 08:21:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 12:20:12 2023
Response via : Initial Calibration

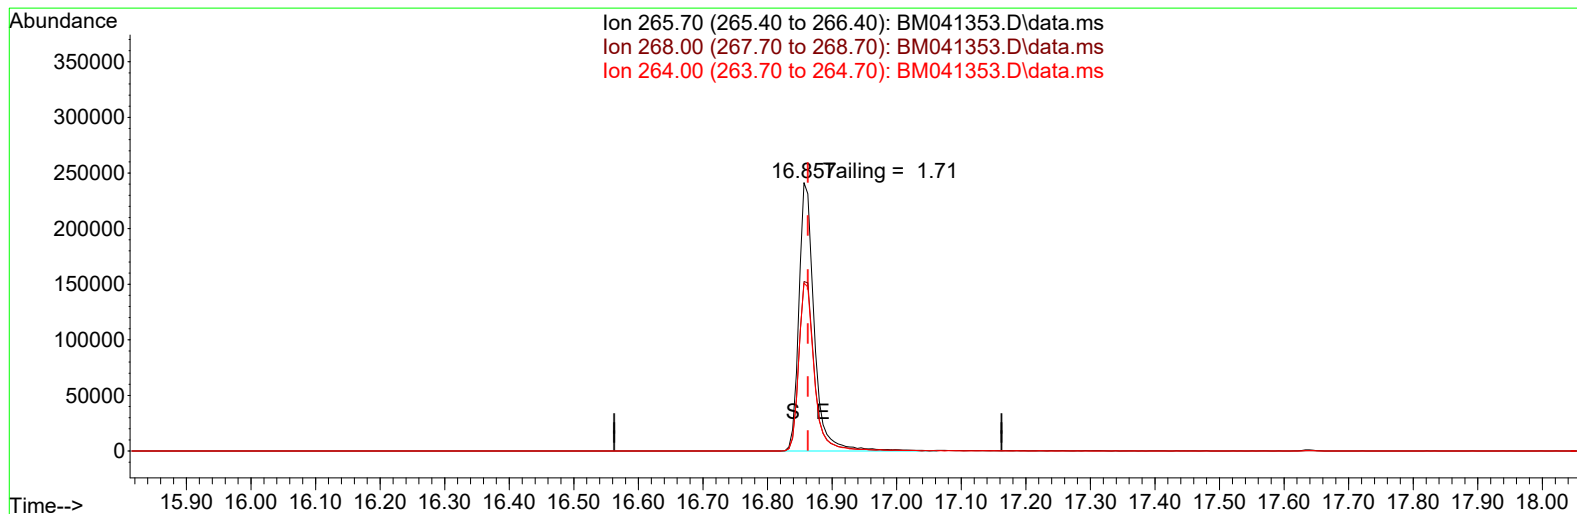

TIC: BM041353.D\data.ms

(70) Pentachlorophenol (C)




16.857min (-0.006) 0.00 ng

response 400774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.17
264.00	61.80	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041353.D
Acq On : 10 Aug 2023 07:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 08:21:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 12:20:12 2023
Response via : Initial Calibration

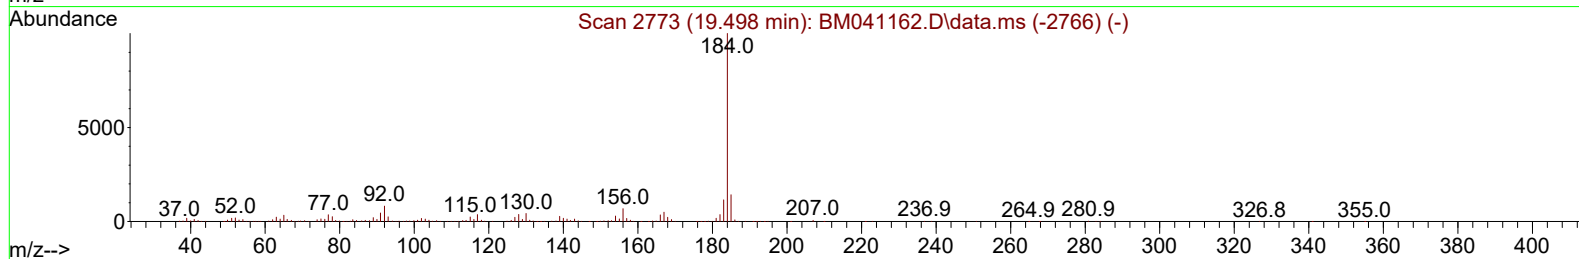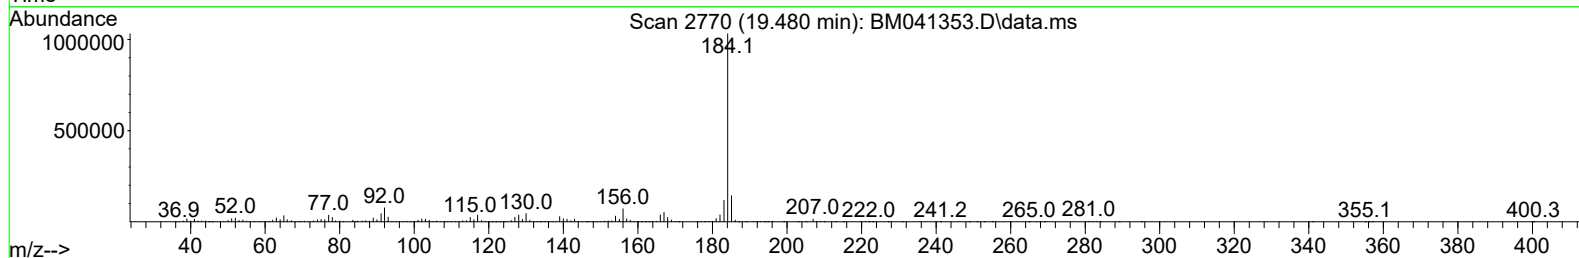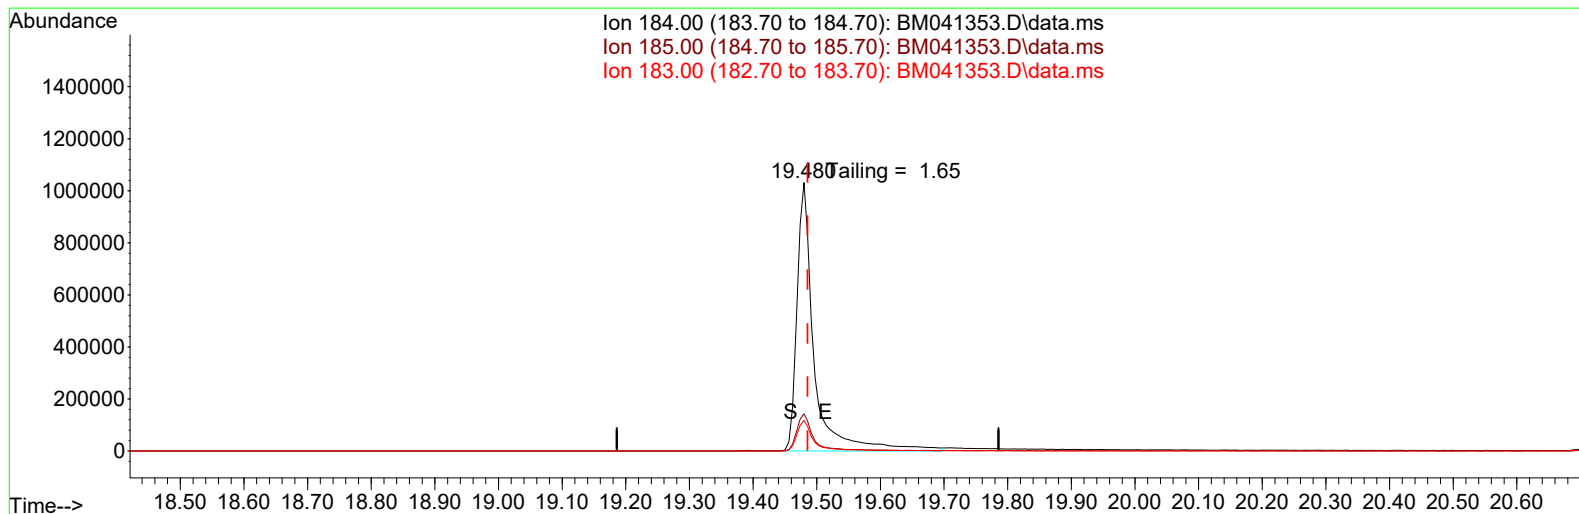

TIC: BM041353.D\data.ms

(77) Benzidine**19.480min (-0.006) 367924.72 ng****response 1940718**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.85
183.00	11.50	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_M	<u>BM041353.D</u>
Compound Name	Response	Retention Time
DDT	1296620	20.697
DDD	23028	20.262
DDE	1723	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24751	1321371	1.87