

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
 Data File : BM041357.D
 Acq On : 10 Aug 2023 11:10
 Operator : MA/JU
 Sample : PB154720BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB154720BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	285	290	308	rVB	1481800	2078555	13.99%	3.980%
2	5.357	363	369	383	rBV	2329814	3415149	22.99%	6.539%
3	6.963	635	642	664	rBV	1997412	3365741	22.66%	6.444%
4	7.781	774	781	791	rBV	610215	991905	6.68%	1.899%
5	8.957	971	981	1001	rBV	1909929	3246639	21.85%	6.216%
6	10.586	1250	1258	1270	rBV	734239	1316793	8.86%	2.521%
7	13.063	1672	1679	1702	rBV	5535685	8122333	54.68%	15.551%
8	14.445	1907	1914	1930	rBV	1199356	1907222	12.84%	3.652%
9	15.951	2163	2170	2199	rBV	2805623	4765368	32.08%	9.124%
10	17.210	2377	2384	2399	rBV	1540183	2482567	16.71%	4.753%
11	19.851	2827	2833	2846	rBV	11553206	14855503	100.00%	28.443%
12	21.415	3094	3099	3110	rBV	1976764	2920767	19.66%	5.592%
13	23.786	3496	3502	3518	rVB	1270044	2760921	18.59%	5.286%




Sum of corrected areas: 52229463

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041357.D
Acq On : 10 Aug 2023 11:10
Operator : MA/JU
Sample : PB154720BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154720BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

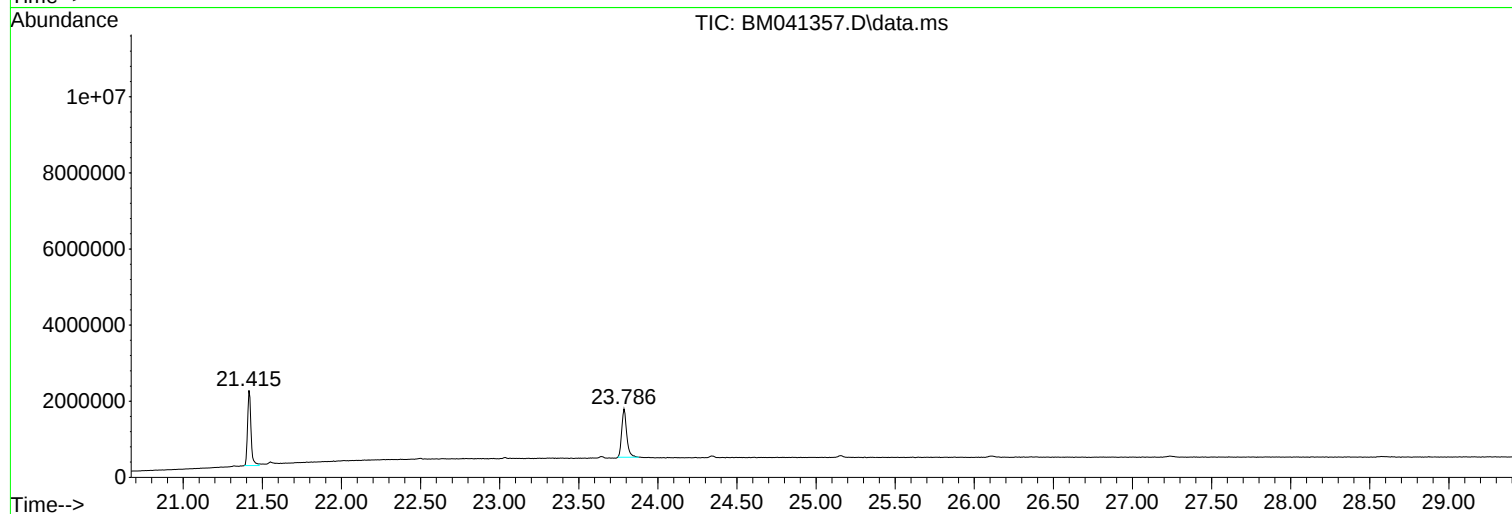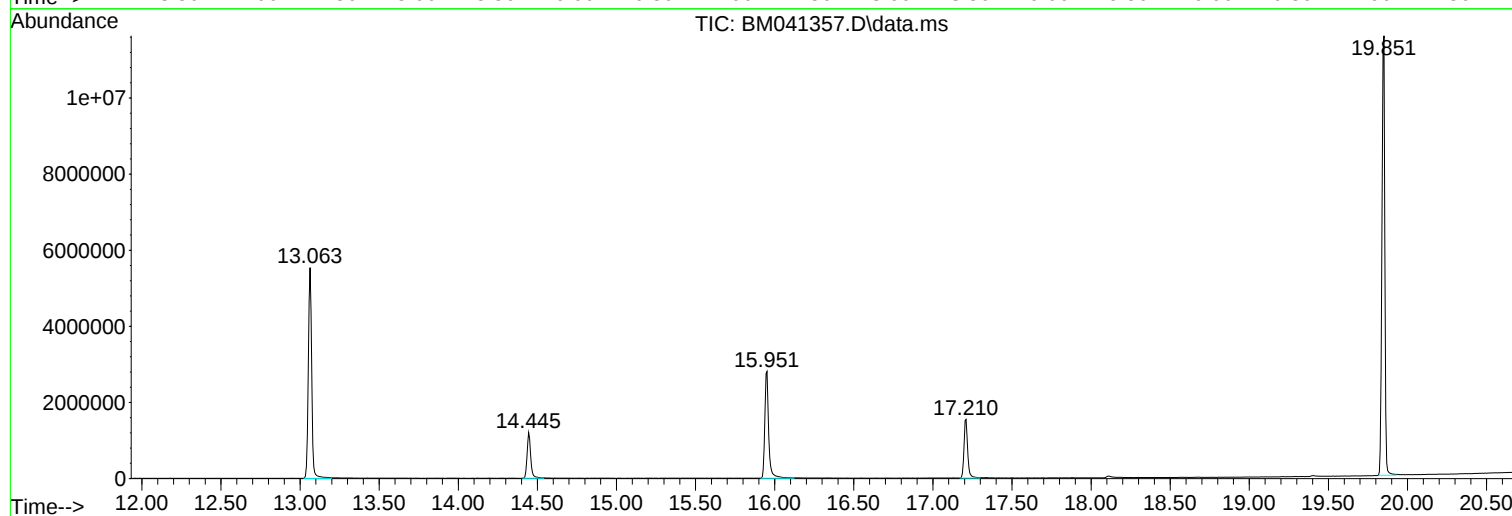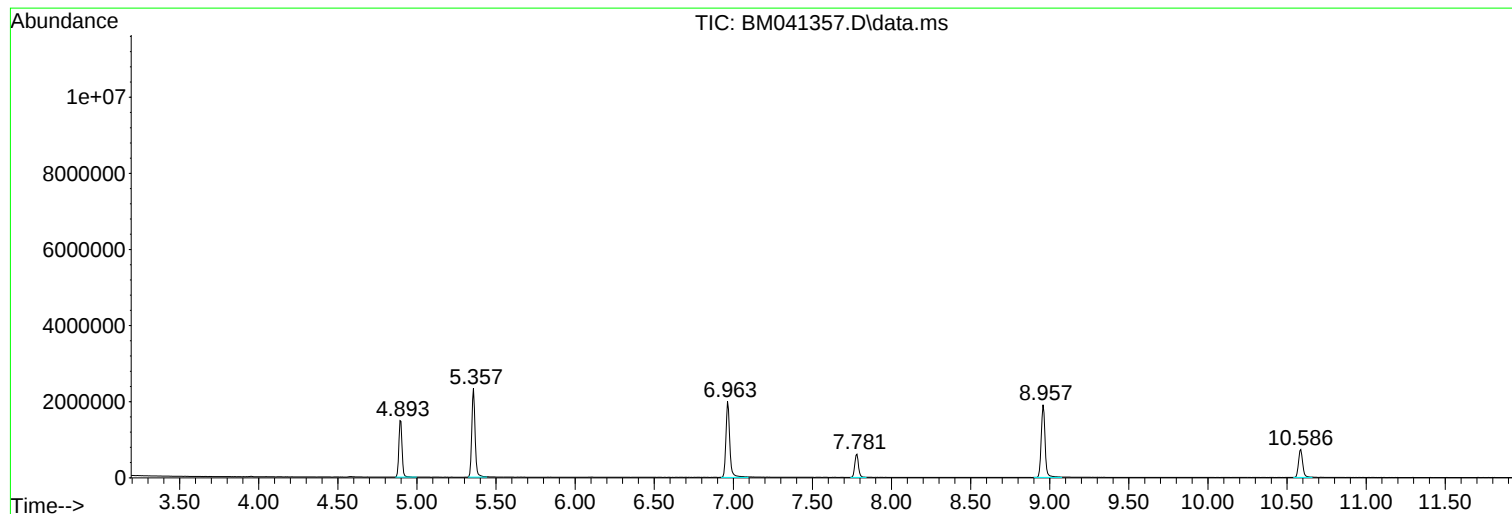

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041357.D
Acq On : 10 Aug 2023 11:10
Operator : MA/JU
Sample : PB154720BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154720BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.893	41.91 ng	2078560	1,4-Dichlorobenzene-d4	7.781

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

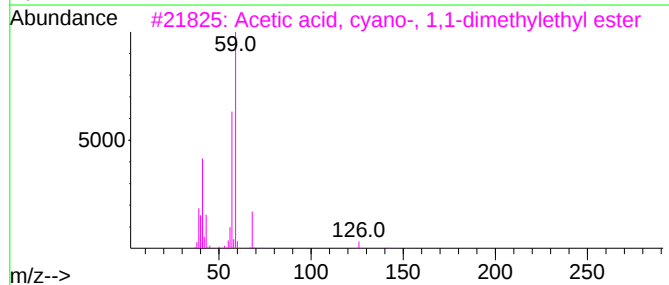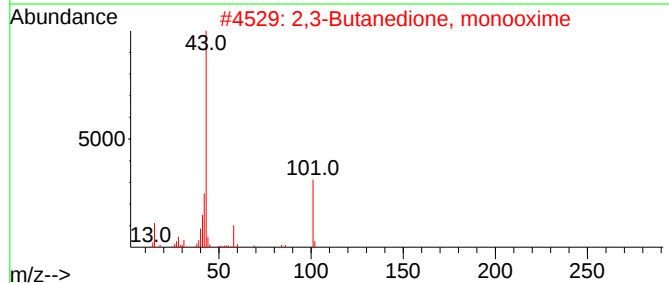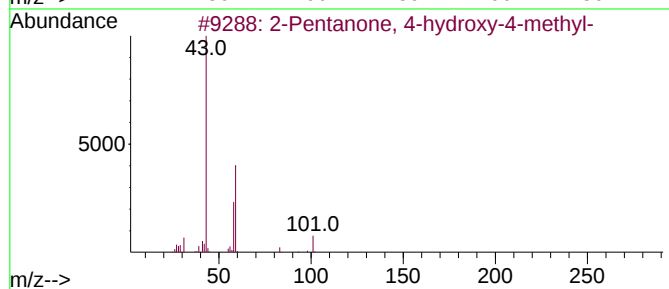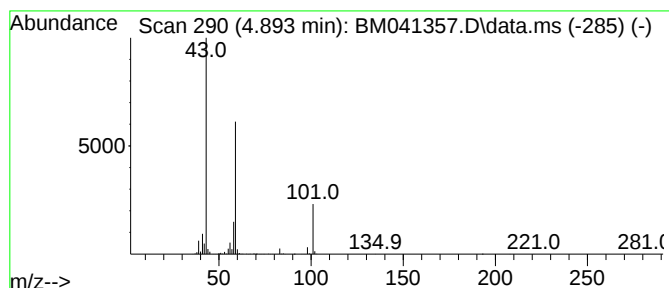

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041357.D
Acq On : 10 Aug 2023 11:10
Operator : MA/JU
Sample : PB154720BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154720BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.893	41.9	ng	2078560	1	7.781	991905	20.0