

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
 Data File : BM041363.D
 Acq On : 10 Aug 2023 15:17
 Operator : MA/JU
 Sample : 03954-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	283	290	297	rBV	43501	64293	1.61%	0.231%
2	5.352	362	368	386	rBV	1870563	2727085	68.24%	9.793%
3	6.957	633	641	660	rBV	1563122	2641536	66.10%	9.485%
4	7.775	773	780	789	rBV	542004	854180	21.37%	3.067%
5	8.951	971	980	997	rBV	959998	1649796	41.28%	5.924%
6	10.581	1249	1257	1270	rBV	624191	1108051	27.73%	3.979%
7	13.057	1671	1678	1699	rBV	2326559	3552759	88.90%	12.757%
8	13.333	1720	1725	1735	rVB2	32302	58516	1.46%	0.210%
9	14.445	1907	1914	1932	rBV	816846	1365895	34.18%	4.905%
10	14.886	1984	1989	1998	rBV3	25080	69221	1.73%	0.249%
11	15.945	2162	2169	2194	rBV	1710097	2780624	69.58%	9.985%
12	17.204	2377	2383	2395	rBV	928868	1433714	35.88%	5.148%
13	18.110	2531	2537	2567	rBV	731804	1488021	37.23%	5.343%
14	19.392	2750	2755	2773	rBV	389755	824457	20.63%	2.961%
15	19.839	2826	2831	2848	rBV	3204443	3996304	100.00%	14.350%
16	21.109	3044	3047	3054	rBV3	141089	187419	4.69%	0.673%
17	21.409	3094	3098	3109	rBV	993280	1445483	36.17%	5.191%
18	23.780	3495	3501	3516	rVB	697390	1601052	40.06%	5.749%




Sum of corrected areas: 27848406

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041363.D
Acq On : 10 Aug 2023 15:17
Operator : MA/JU
Sample : 03954-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

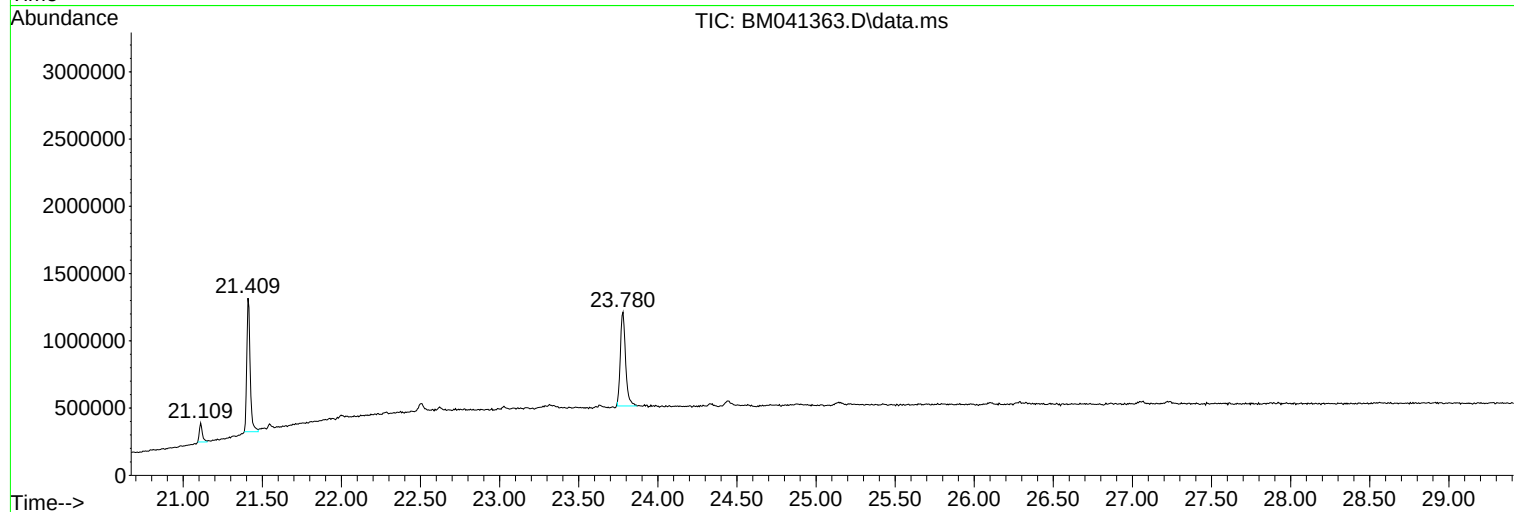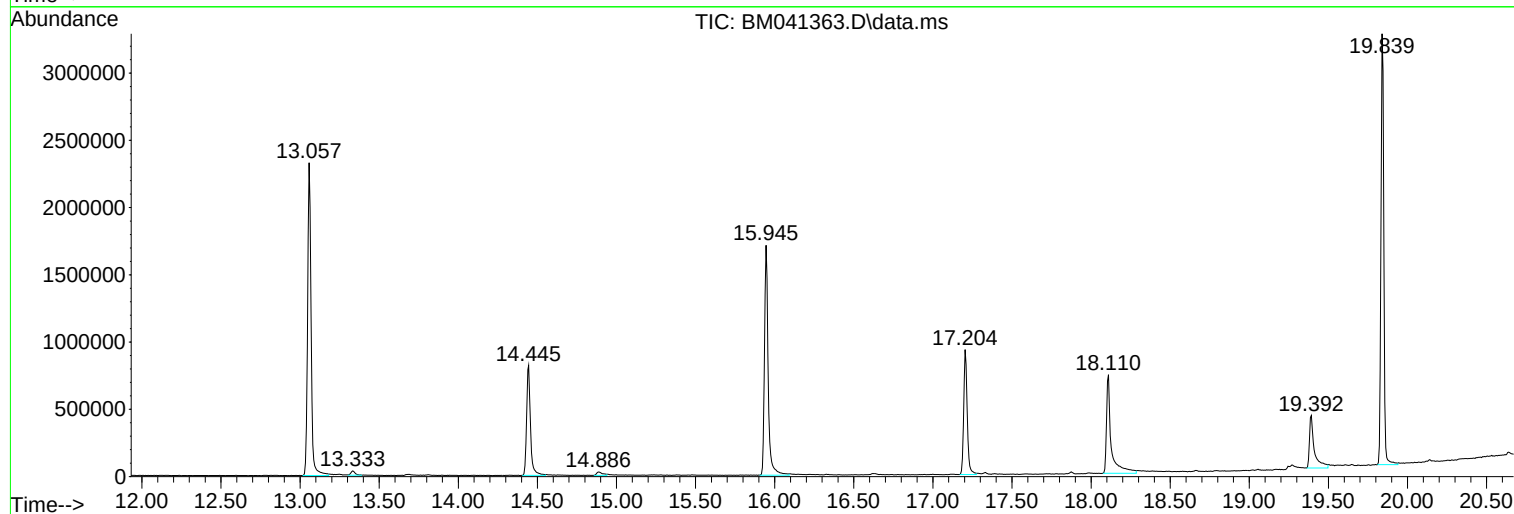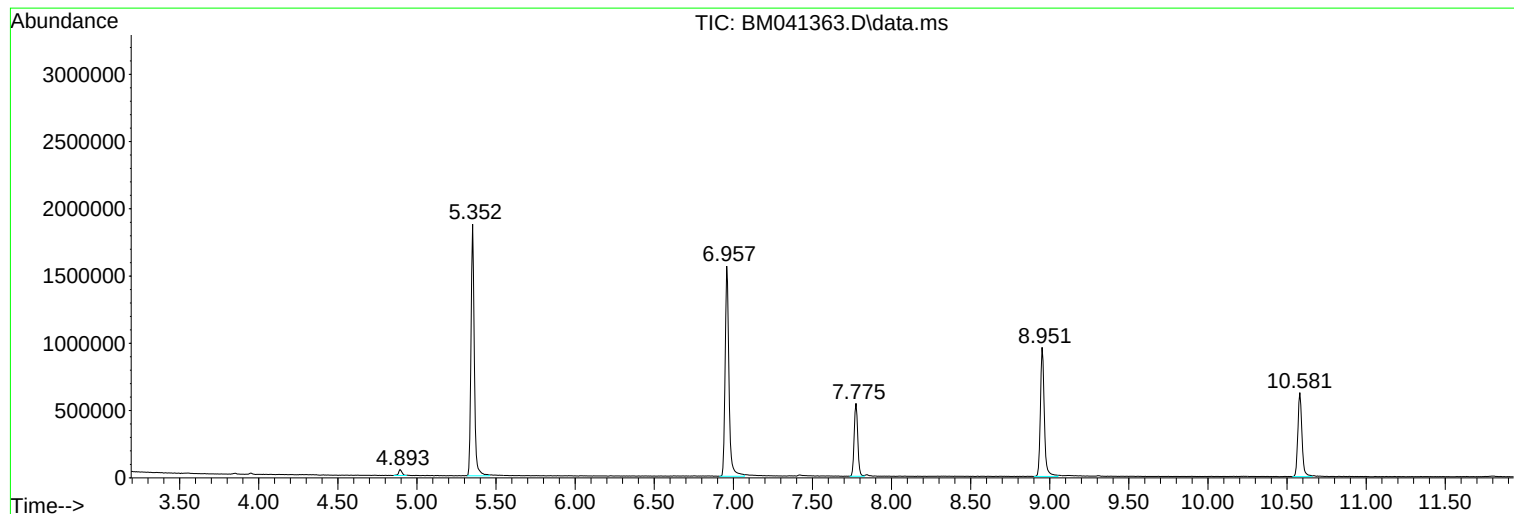

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041363.D
Acq On : 10 Aug 2023 15:17
Operator : MA/JU
Sample : 03954-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041363.D
Acq On : 10 Aug 2023 15:17
Operator : MA/JU
Sample : 03954-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------