

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
 Data File : BM041371.D
 Acq On : 10 Aug 2023 20:16
 Operator : MA/JU
 Sample : 03954-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	9	12	23	rVB	263532	292802	3.81%	0.751%
2	3.681	79	84	93	rVB	104475	130300	1.69%	0.334%
3	4.287	182	187	198	rBV	195399	261510	3.40%	0.671%
4	4.381	198	203	204	rBV	86283	113960	1.48%	0.292%
5	4.846	278	282	286	rBV	86476	118182	1.54%	0.303%
6	4.893	286	290	297	rVB	177722	251748	3.27%	0.646%
7	5.351	361	368	385	rBV	2924185	4104310	53.36%	10.532%
8	6.869	621	626	631	rBV	56948	77624	1.01%	0.199%
9	6.957	634	641	663	rBV	2207223	3570293	46.42%	9.161%
10	7.775	773	780	789	rBV	577695	911854	11.86%	2.340%
11	8.757	941	947	953	rBV	103736	152631	1.98%	0.392%
12	8.951	967	980	999	rBV	1727628	2913185	37.87%	7.475%
13	10.580	1250	1257	1276	rVB	675041	1181740	15.36%	3.032%
14	13.057	1671	1678	1703	rBV	4479732	6529496	84.89%	16.754%
15	13.921	1819	1825	1838	rBV	47720	113966	1.48%	0.292%
16	14.439	1905	1913	1929	rBV2	863671	1401958	18.23%	3.597%
17	15.945	2162	2169	2192	rBV	2843286	4708472	61.22%	12.082%
18	17.204	2377	2383	2405	rBV	946085	1536455	19.98%	3.942%
19	18.103	2531	2536	2549	rBV	107175	263234	3.42%	0.675%
20	19.392	2751	2755	2766	rBV3	65994	160460	2.09%	0.412%
21	19.839	2826	2831	2844	rBV	6099799	7691578	100.00%	19.736%
22	21.415	3094	3099	3110	rBV	920321	1482249	19.27%	3.803%
23	23.785	3497	3502	3520	rVB2	384505	1003634	13.05%	2.575%




Sum of corrected areas: 38971641

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041371.D
Acq On : 10 Aug 2023 20:16
Operator : MA/JU
Sample : 03954-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

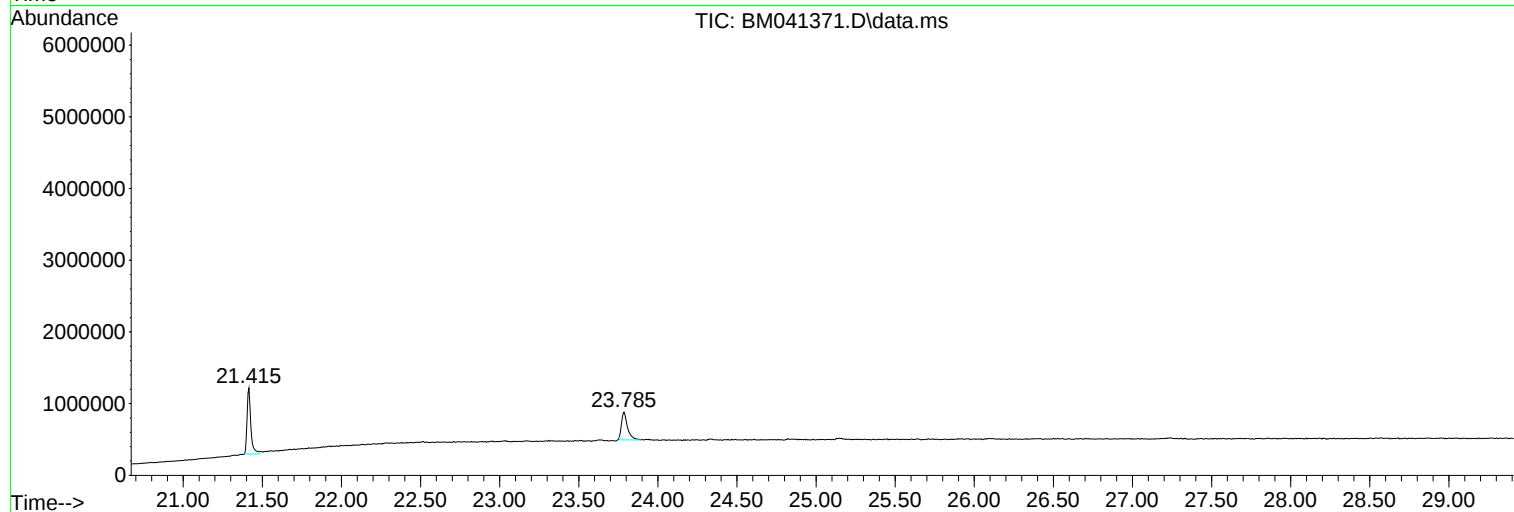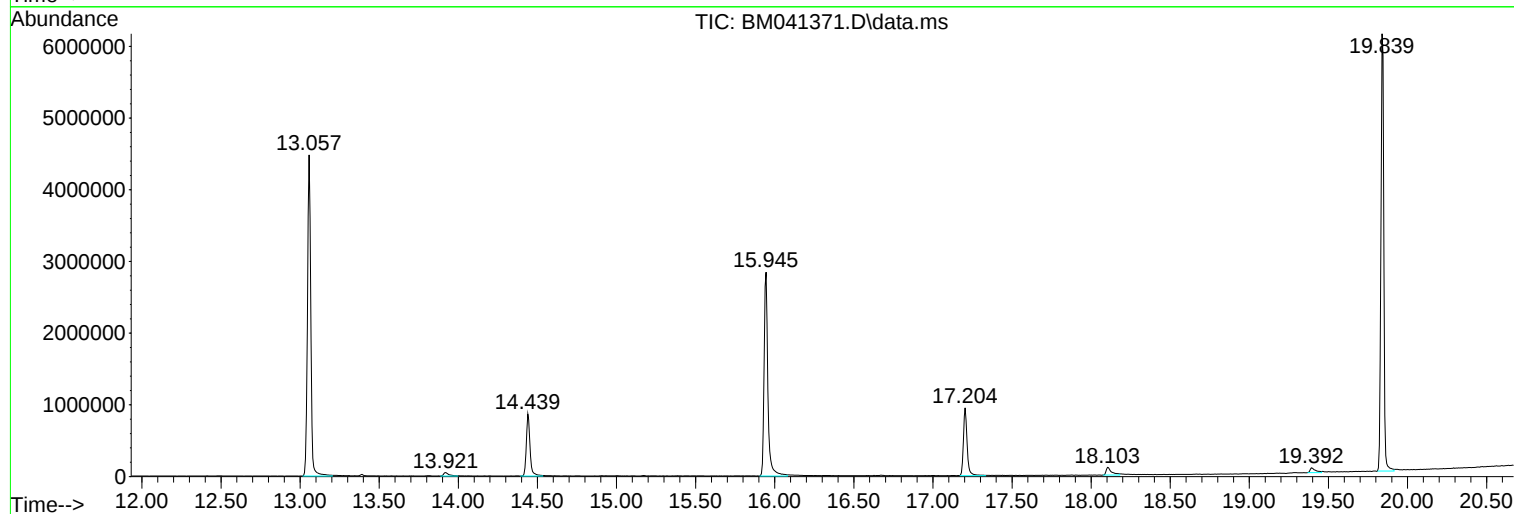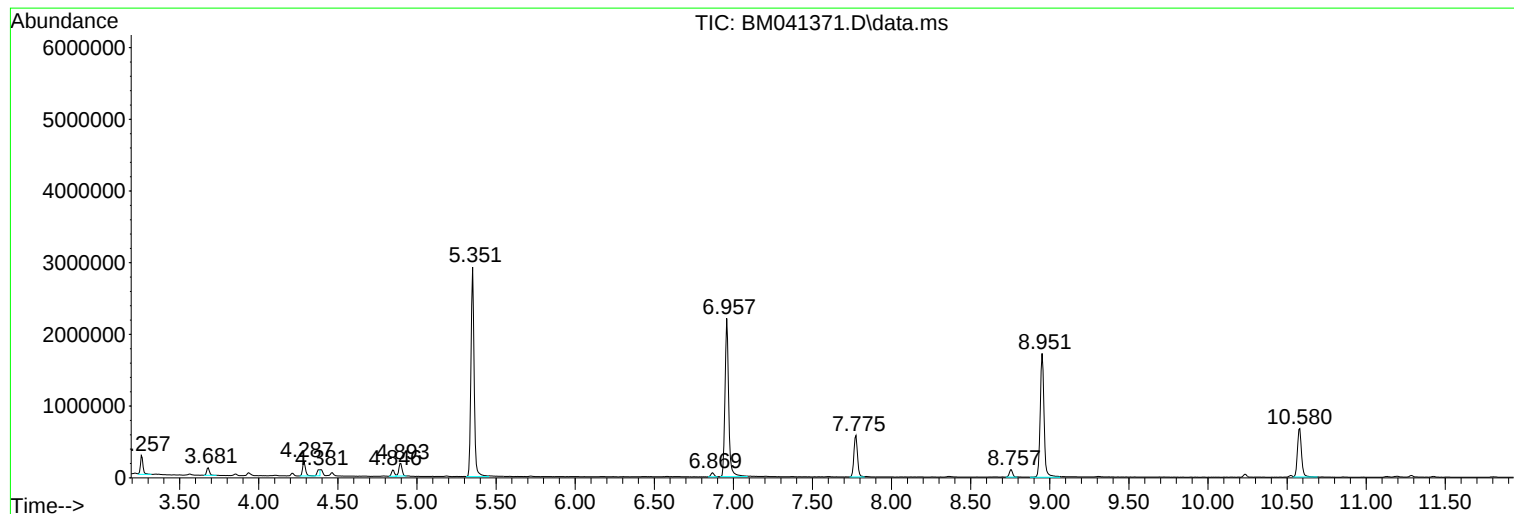

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041371.D
Acq On : 10 Aug 2023 20:16
Operator : MA/JU
Sample : 03954-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041371.D
Acq On : 10 Aug 2023 20:16
Operator : MA/JU
Sample : 03954-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------