


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041353.D
Acq On : 10 Aug 2023 07:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 09 12:20:12 2023

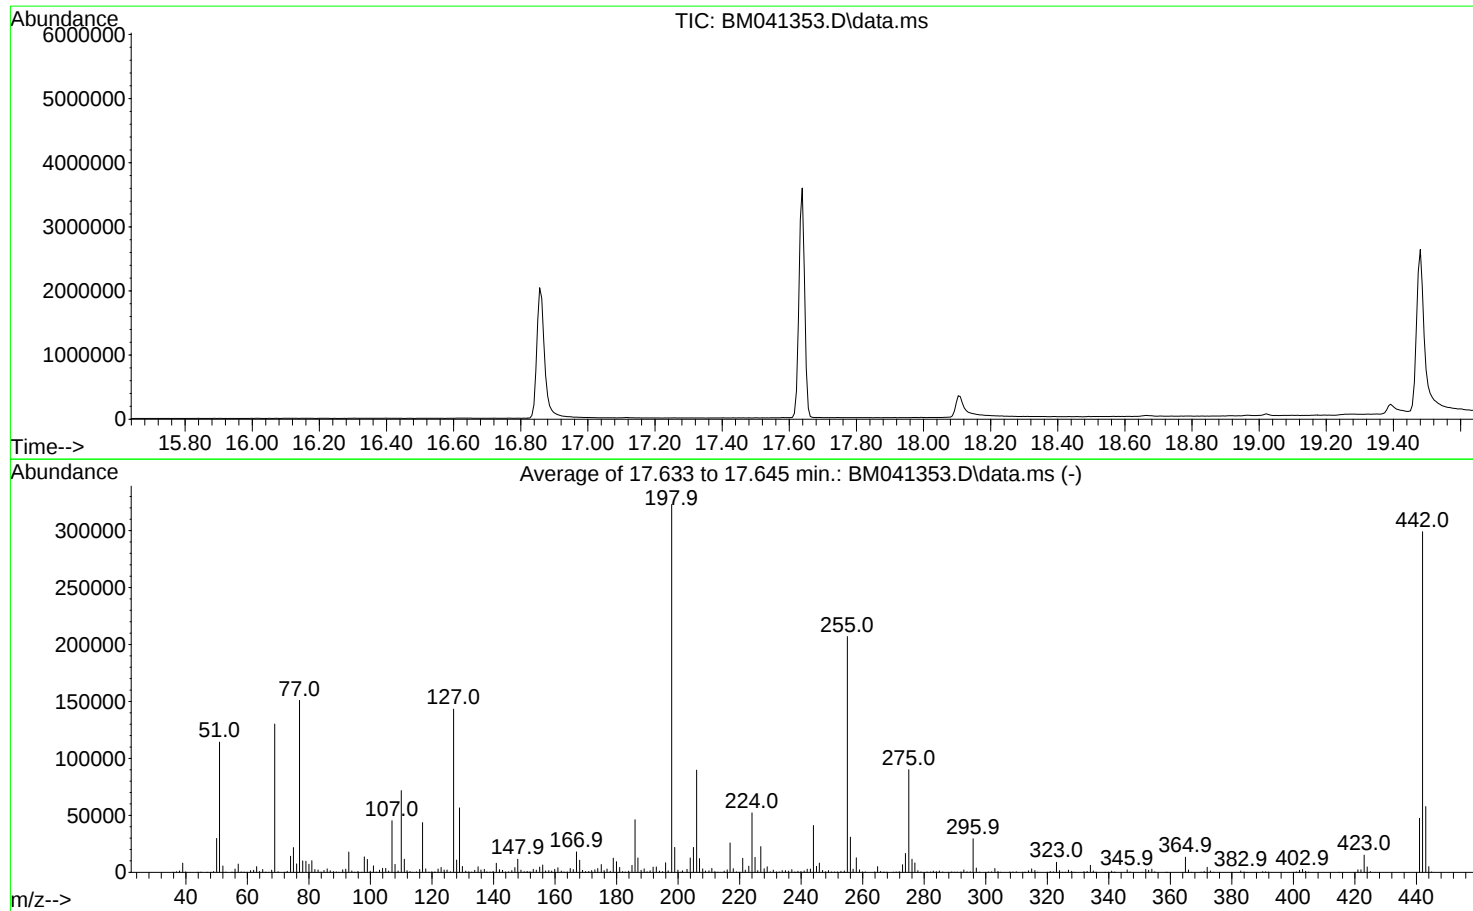




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	114290	PASS
68	69	0.00	2	1.4	1866	PASS
69	198	0.00	100	40.3	130193	PASS
70	69	0.00	2	0.4	511	PASS
127	198	10	80	44.3	143184	PASS
197	198	0.00	2	0.4	1306	PASS
198	198	100	100	100.0	322987	PASS
199	198	5	9	6.8	21804	PASS
275	198	10	60	27.9	90080	PASS
365	198	1	100	4.1	13244	PASS
441	198	0.01	100	14.7	47387	PASS
442	442	50	100	100.0	299029	PASS
443	442	15	24	19.3	57709	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041353.D
Acq On : 10 Aug 2023 07:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 10 08:21:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 12:20:12 2023
Response via : Initial Calibration

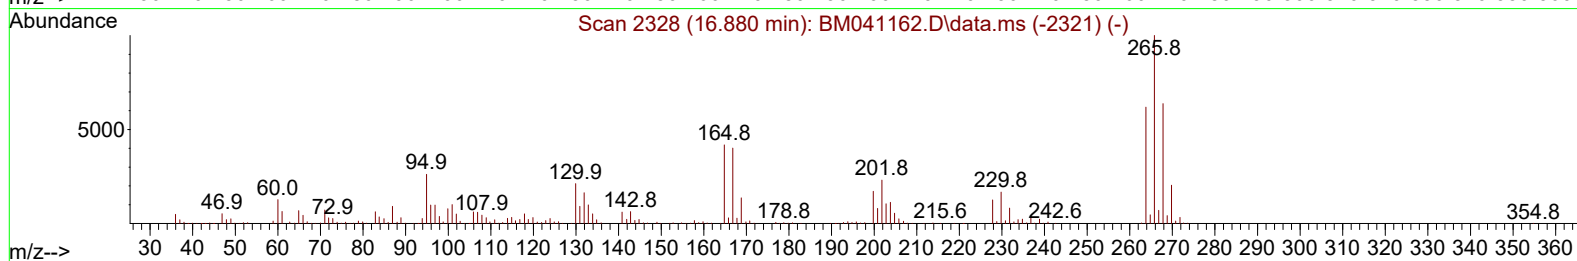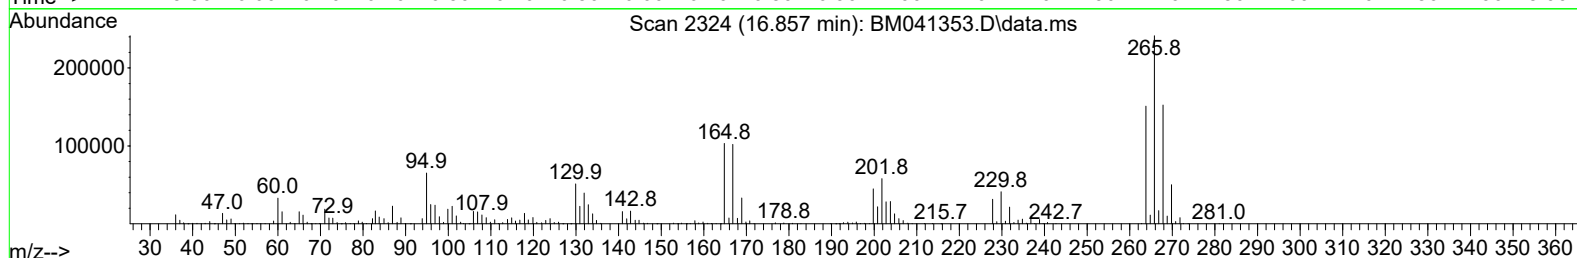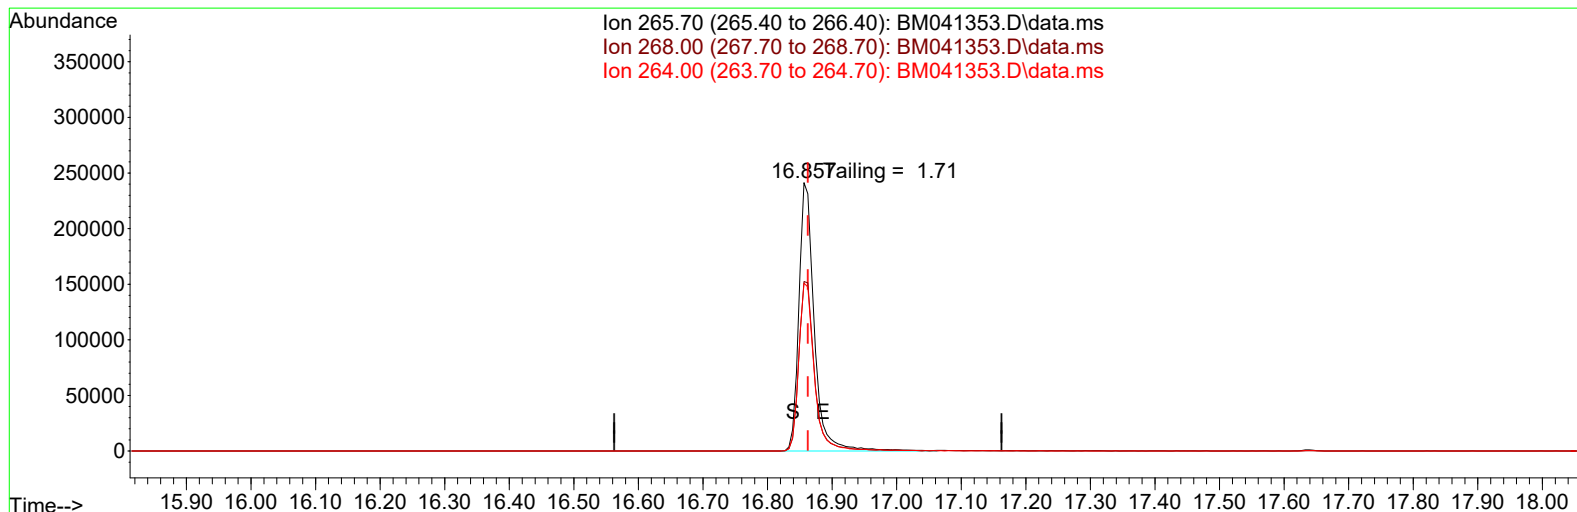

TIC: BM041353.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.006) 0.00 ng




response 400774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.17
264.00	61.80	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081023\
Data File : BM041353.D
Acq On : 10 Aug 2023 07:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 10 08:21:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 12:20:12 2023
Response via : Initial Calibration

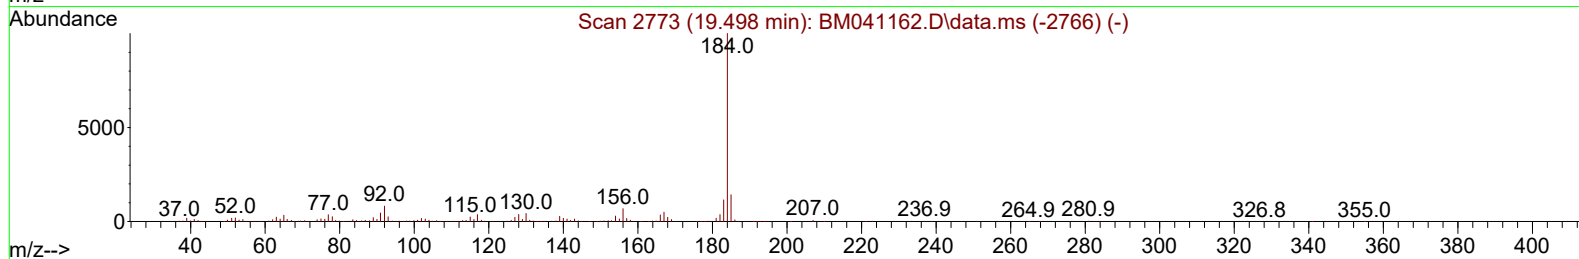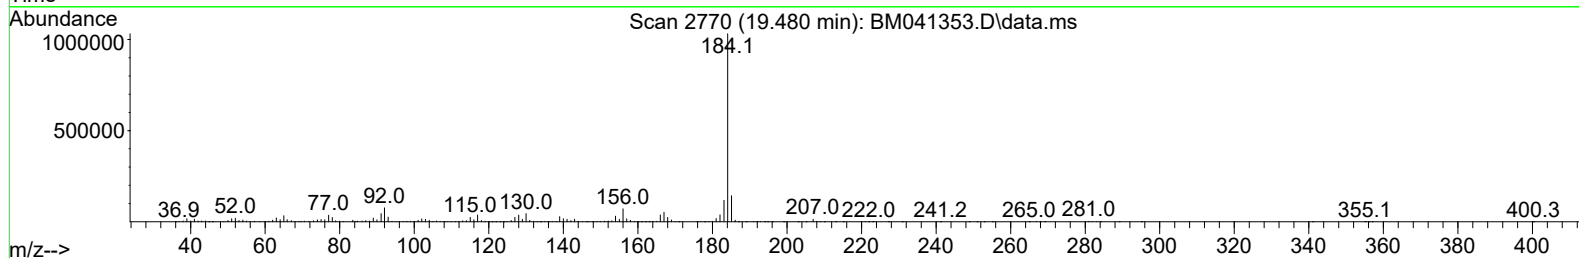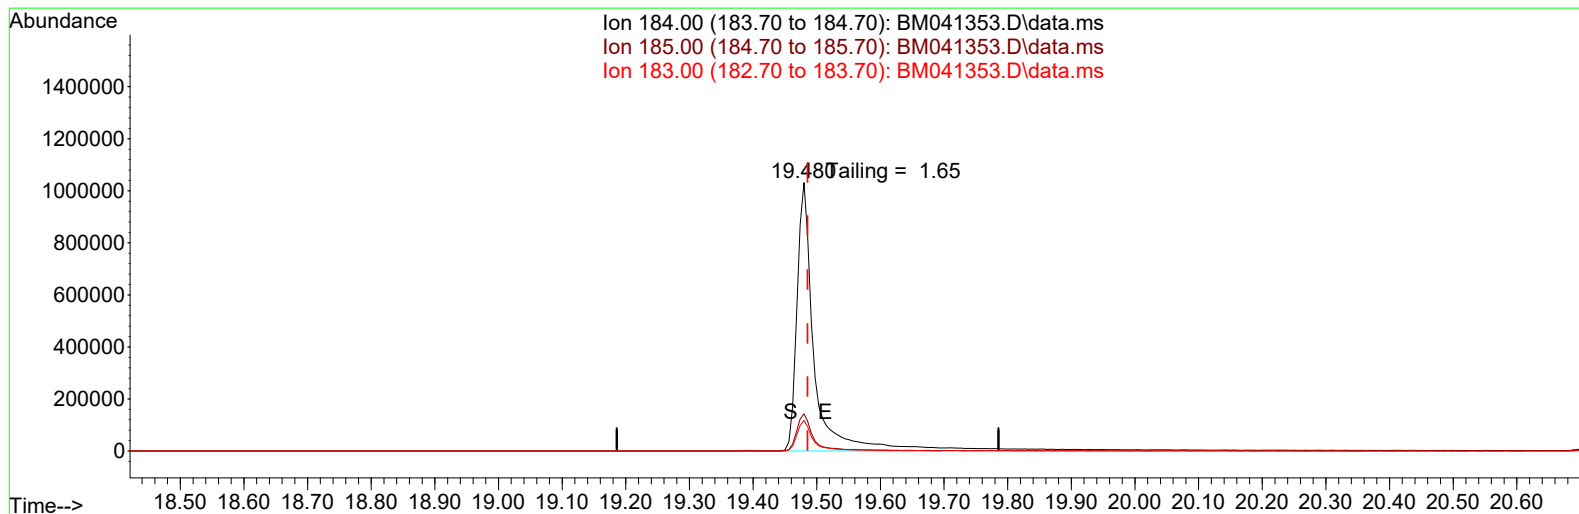

TIC: BM041353.D\data.ms

(77) Benzidine

19.480min (-0.006) 367924.72 ng

response 1940718

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.85
183.00	11.50	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_M	<u>BM041353.D</u>
Compound Name	Response	Retention Time
DDT	1296620	20.697
DDD	23028	20.262
DDE	1723	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24751	1321371	1.87

Instrument :
BNA_M
ClientSampleId :
DFTPP