


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081023\  
 Data File : BM041359.D  
 Acq On : 10 Aug 2023 12:43  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Aug 09 12:20:12 2023

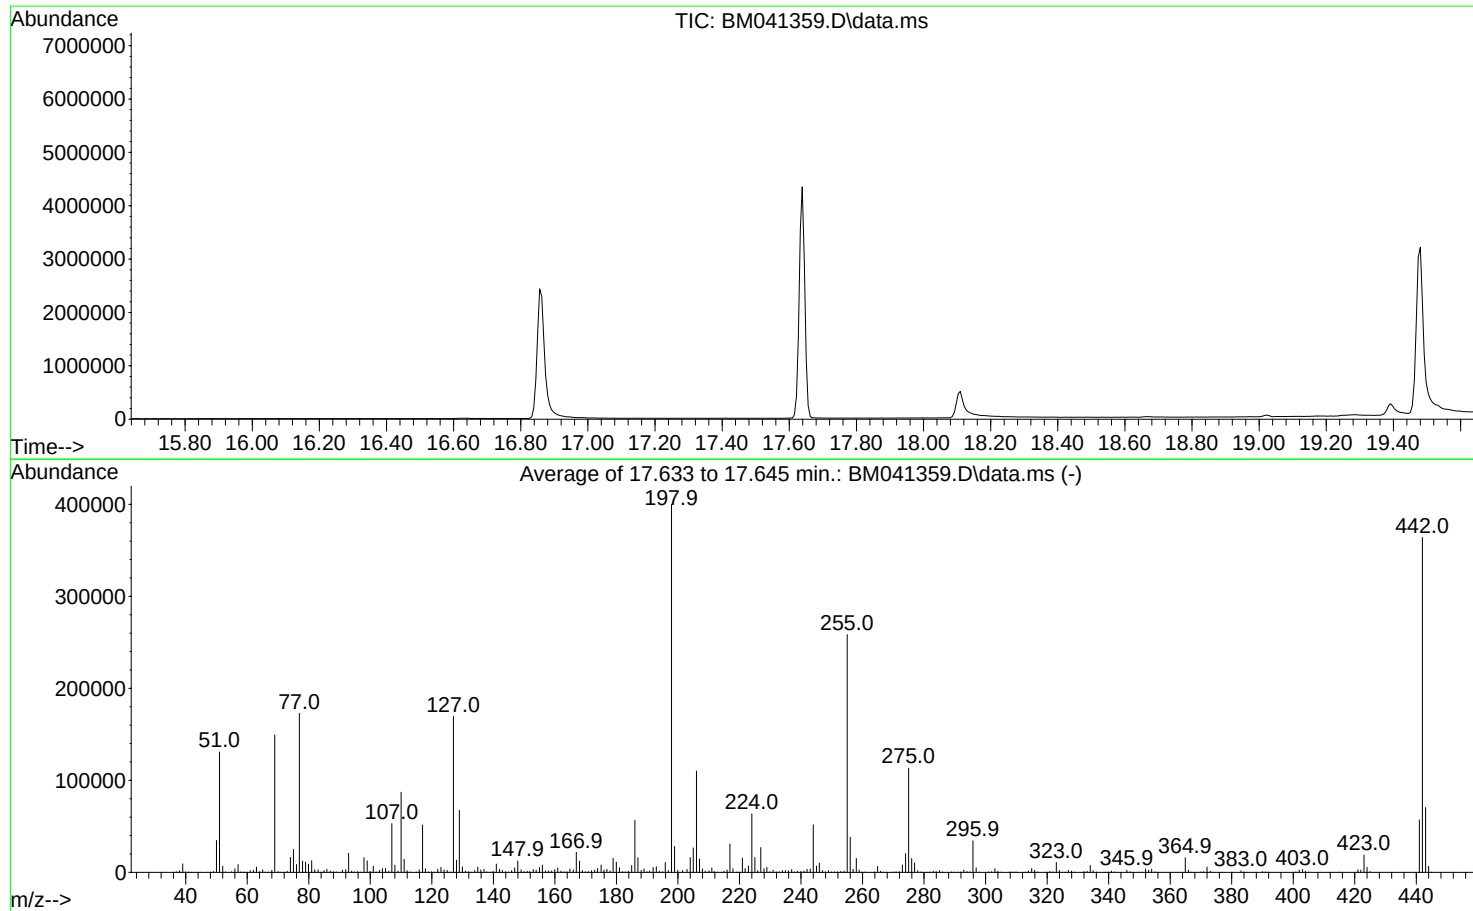




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.7         | 130812     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 2189       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.3         | 149335     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 706        | PASS                |
| 127            | 198             | 10              | 80              | 42.4         | 169432     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1915       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 399957     | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 28019      | PASS                |
| 275            | 198             | 10              | 60              | 28.3         | 113251     | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 15963      | PASS                |
| 441            | 198             | 0.01            | 100             | 14.3         | 57024      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 364011     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 70325      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081023\  
Data File : BM041359.D  
Acq On : 10 Aug 2023 12:43  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Aug 11 05:52:54 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 09 12:20:12 2023  
Response via : Initial Calibration

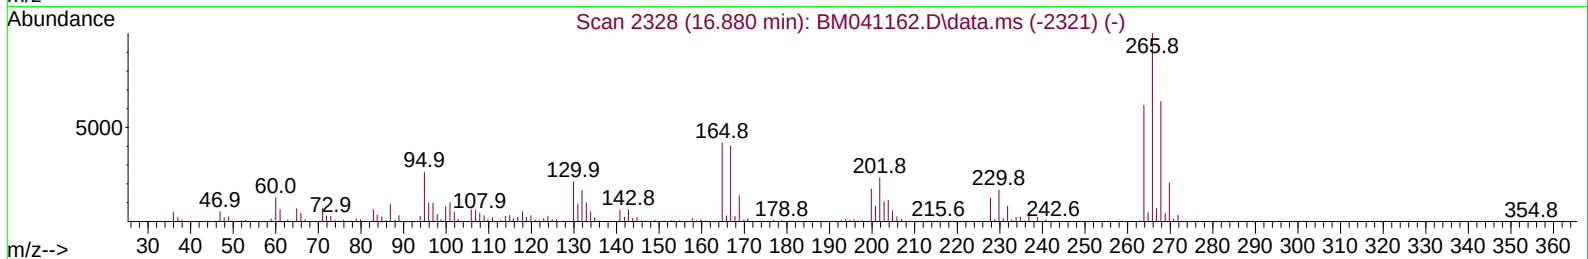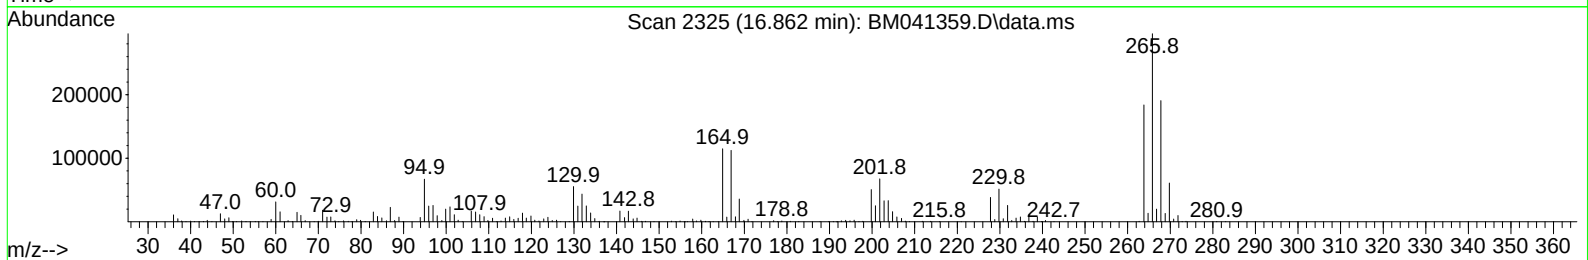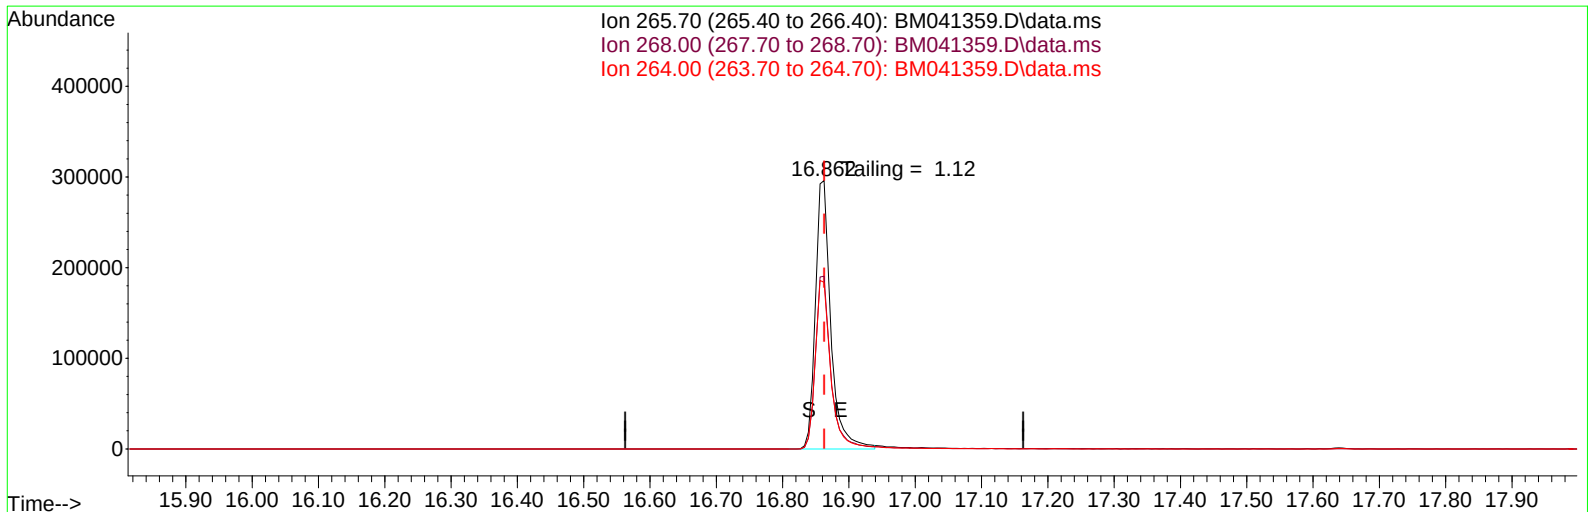

TIC: BM041359.D\data.ms

**(70) Pentachlorophenol (C)**

16.862min (-0.000) 0.00 ng




response 487486

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 64.38  |
| 264.00 | 61.80  | 62.13  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081023\  
Data File : BM041359.D  
Acq On : 10 Aug 2023 12:43  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Aug 11 05:52:54 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 09 12:20:12 2023  
Response via : Initial Calibration

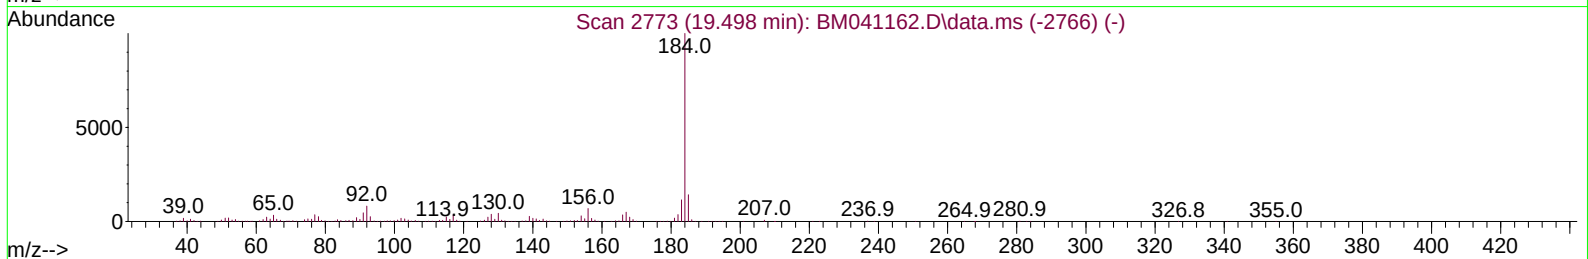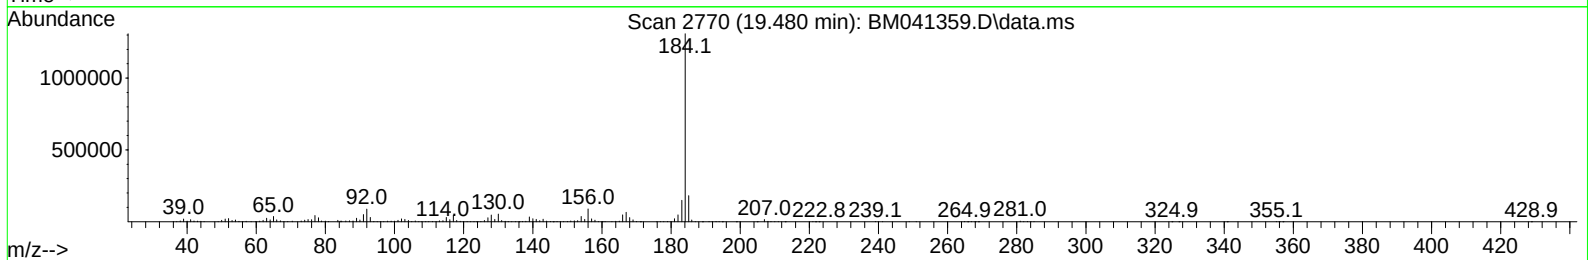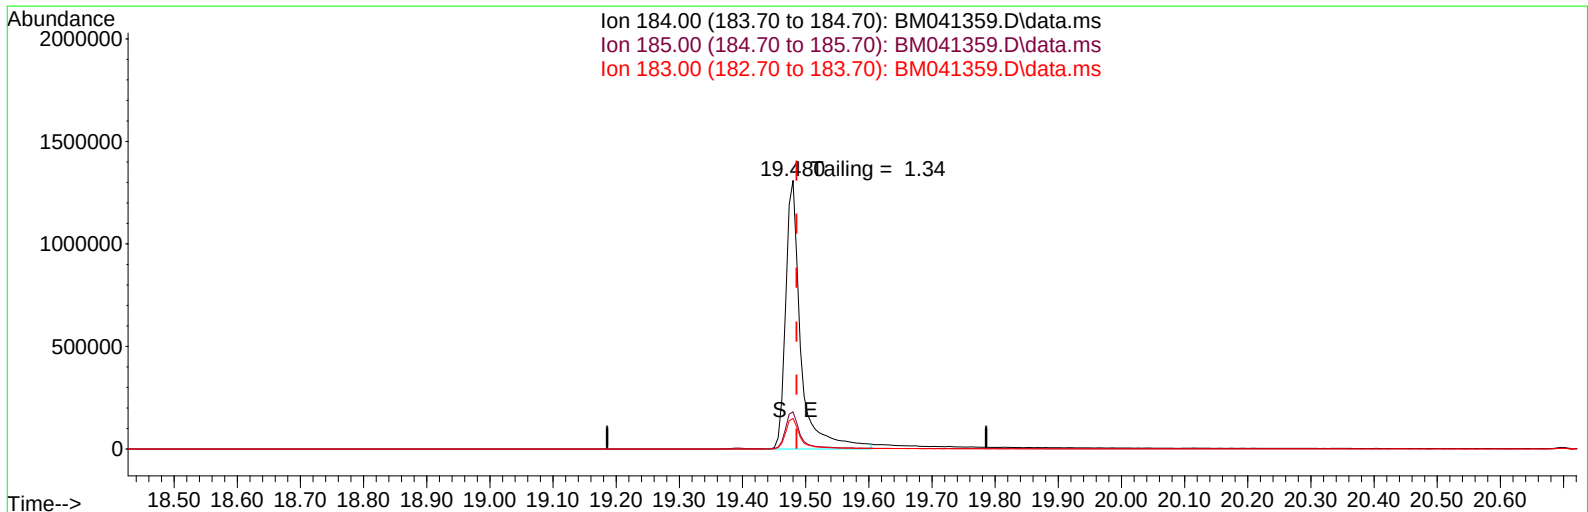

TIC: BM041359.D\data.ms

(77) Benzidine

19.480min (-0.006) 173925.46 ng

response 2294727

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 13.84  |
| 183.00 | 11.50  | 11.37  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/10/2023     | BNA_M            | <u>BM041359.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1504837          | 20.697             |
| DDD           | 23914            | 20.303             |
| DDE           | 2815             | 19.745             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 26729         | 1531566          | 1.75               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP