
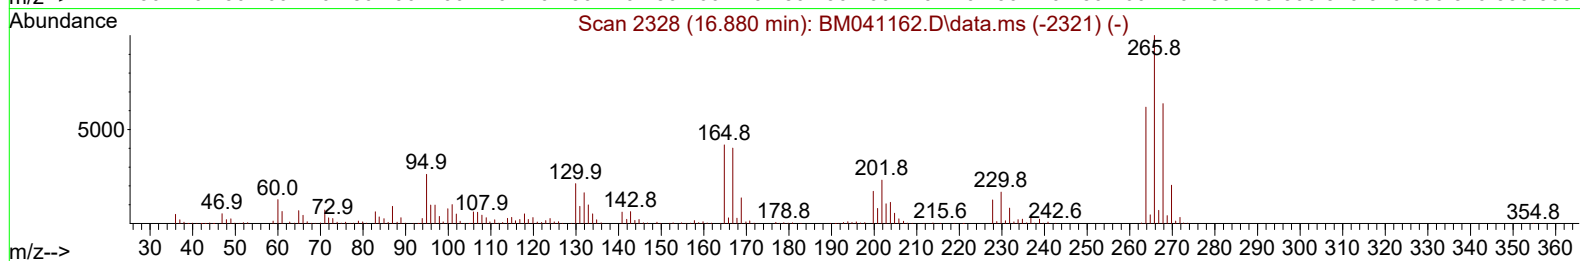
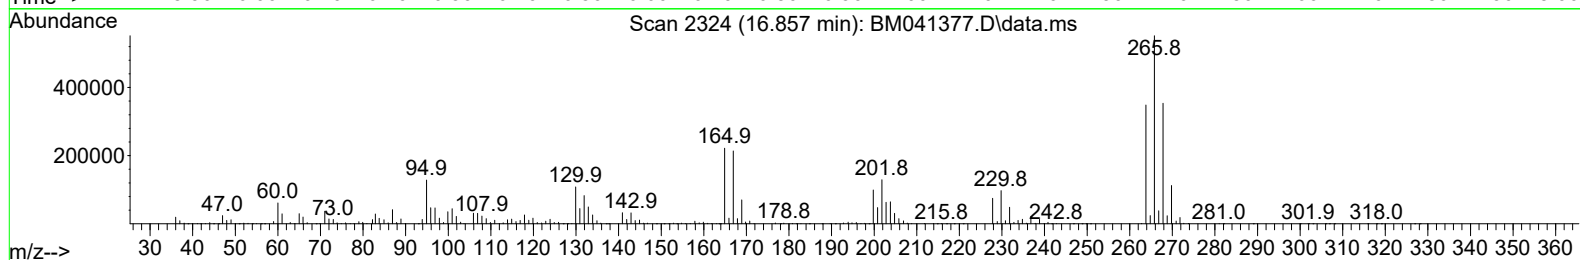


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
 Data File : BM041377.D
 Acq On : 11 Aug 2023 08:13
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 11:00:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 12:20:12 2023
 Response via : Initial Calibration

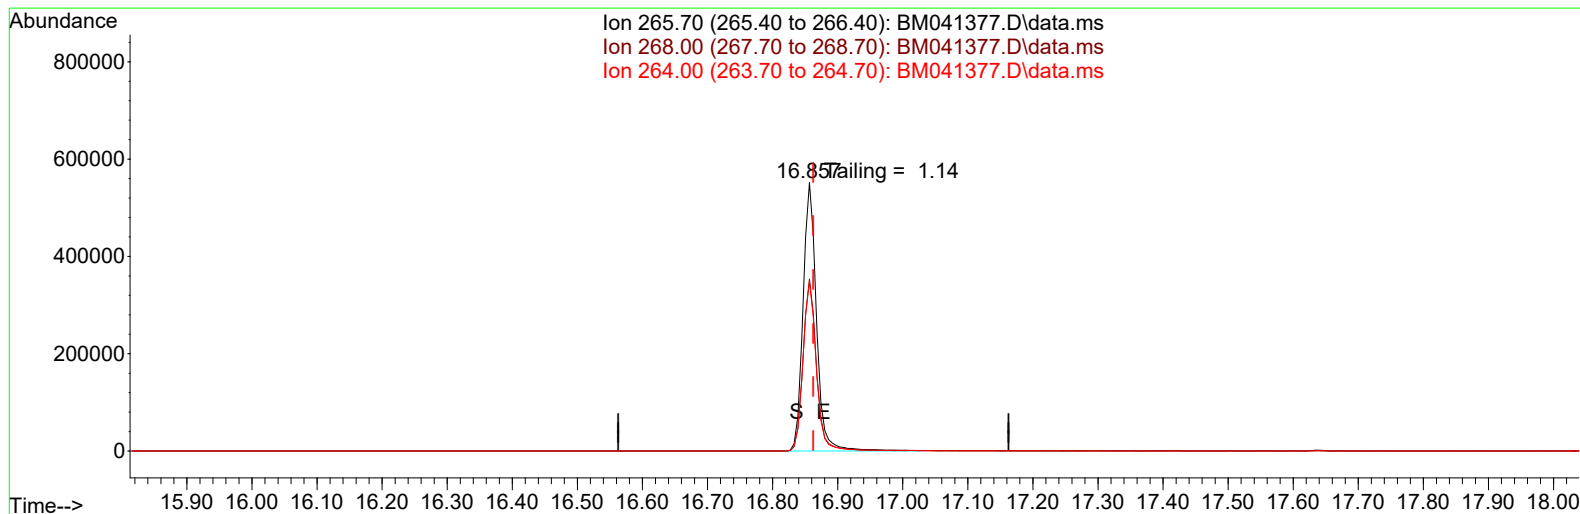

TIC: BM041377.D\data.ms

(70) Pentachlorophenol (C)




16.857min (-0.006) 397758.31 ng

response 795841

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.08
264.00	61.80	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041377.D
Acq On : 11 Aug 2023 08:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 11:00:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 12:20:12 2023
Response via : Initial Calibration

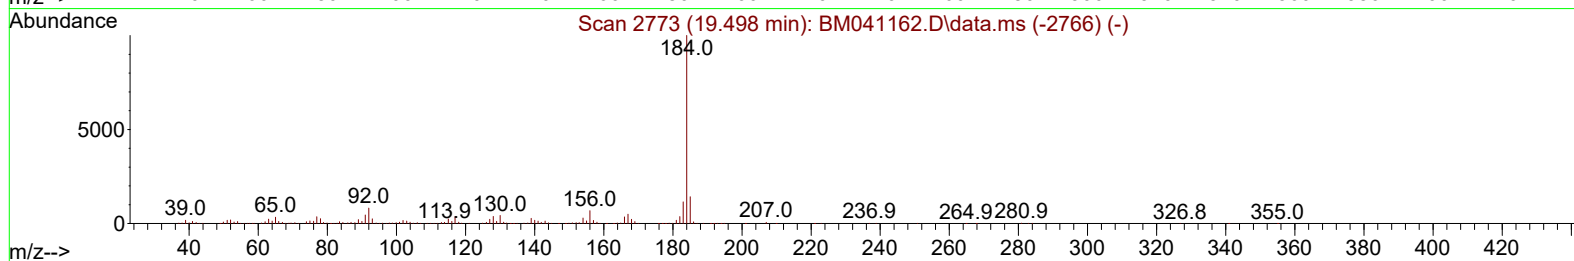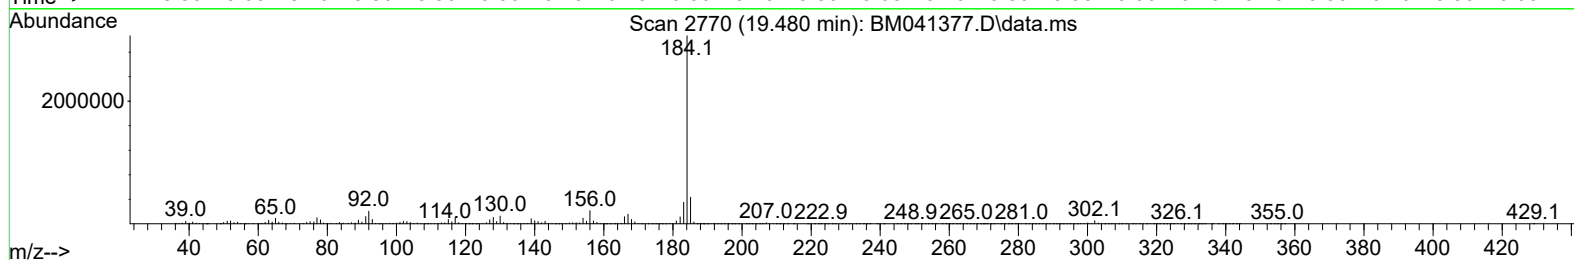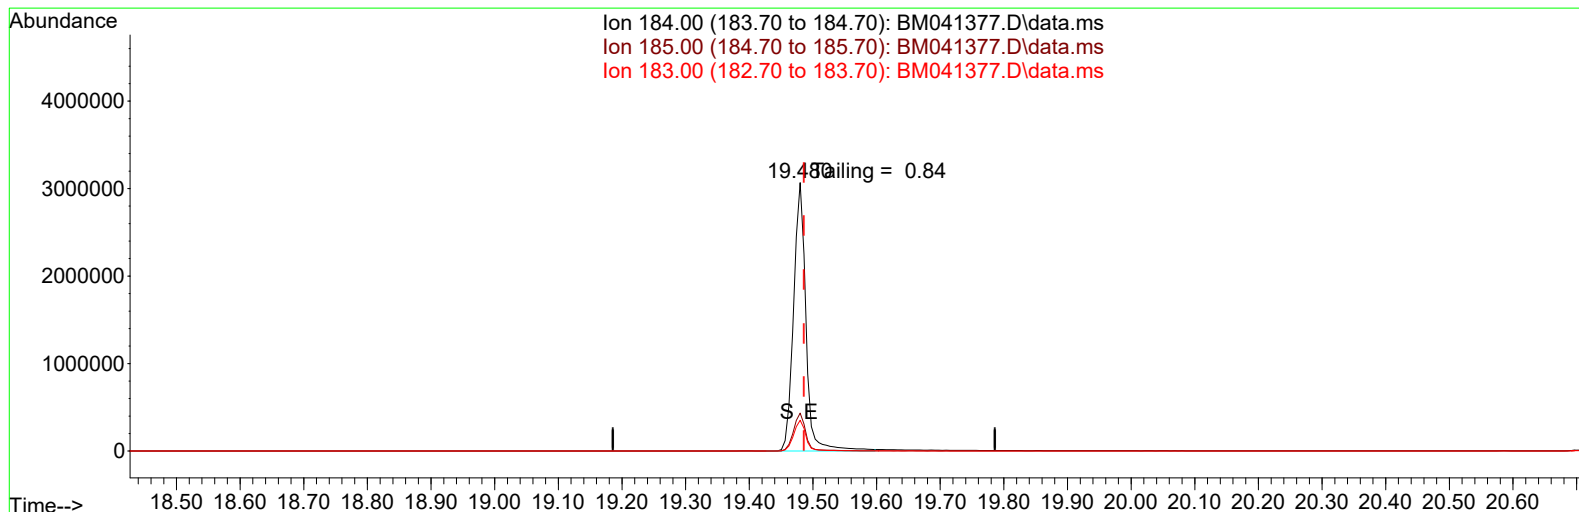

TIC: BM041377.D\data.ms

(77) Benzidine**19.480min (-0.006) 212708.86 ng****response 4218335**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.13
183.00	11.50	11.46
0.00	0.00	0.00