

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
 Data File : BM041383.D
 Acq On : 11 Aug 2023 12:30
 Operator : MA/JU
 Sample : 03954-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-20

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	8	12	21	rVB	215487	262811	2.05%	0.534%
2	3.675	79	83	92	rVB	212735	263472	2.05%	0.535%
3	4.281	181	186	196	rBV	569778	757547	5.90%	1.538%
4	4.375	197	202	212	rBV	712376	1107916	8.62%	2.249%
5	4.893	286	290	297	rVB	110422	156412	1.22%	0.318%
6	5.351	362	368	386	rBV	2550119	3717208	28.93%	7.546%
7	6.869	619	626	635	rBV	815892	1260857	9.81%	2.560%
8	6.963	635	642	661	rVB	1974177	3420216	26.62%	6.943%
9	7.775	773	780	790	rBV	539409	845241	6.58%	1.716%
10	8.951	969	980	1000	rBV	1566916	2686843	20.91%	5.454%
11	9.310	1035	1041	1053	rBV	154274	259207	2.02%	0.526%
12	10.580	1251	1257	1273	rVB	678266	1146653	8.92%	2.328%
13	11.810	1460	1466	1473	rBV2	92703	147489	1.15%	0.299%
14	13.057	1671	1678	1695	rBV	4502488	6524000	50.77%	13.244%
15	13.916	1819	1824	1837	rBV	66690	137223	1.07%	0.279%
16	14.439	1907	1913	1937	rBV2	956139	1583224	12.32%	3.214%
17	15.945	2162	2169	2202	rBV	3956127	6009888	46.77%	12.200%
18	17.204	2376	2383	2397	rBV	1512048	2243101	17.46%	4.553%
19	18.104	2531	2536	2546	rBV2	105447	227881	1.77%	0.463%
20	19.392	2751	2755	2764	rBV3	61489	133289	1.04%	0.271%
21	19.845	2826	2832	2848	rBV	10805434	12848917	100.00%	26.083%
22	21.415	3094	3099	3110	rBV	1800818	2653216	20.65%	5.386%
23	23.786	3498	3502	3516	rVB4	330737	868930	6.76%	1.764%




Sum of corrected areas: 49261541

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041383.D
Acq On : 11 Aug 2023 12:30
Operator : MA/JU
Sample : 03954-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

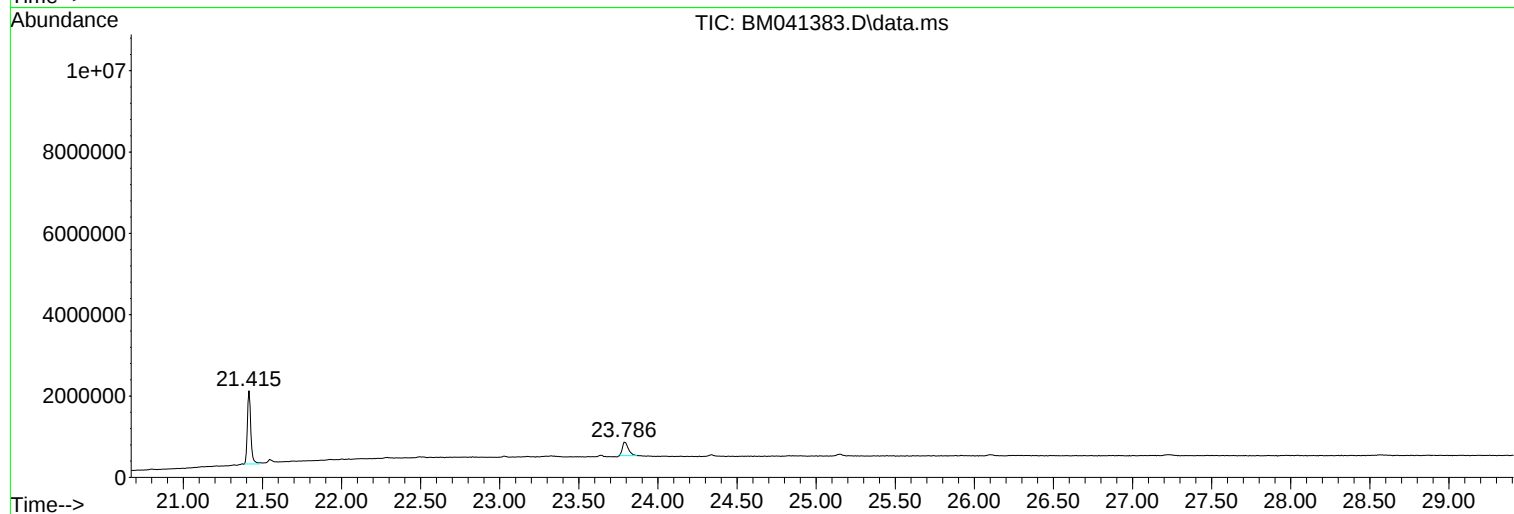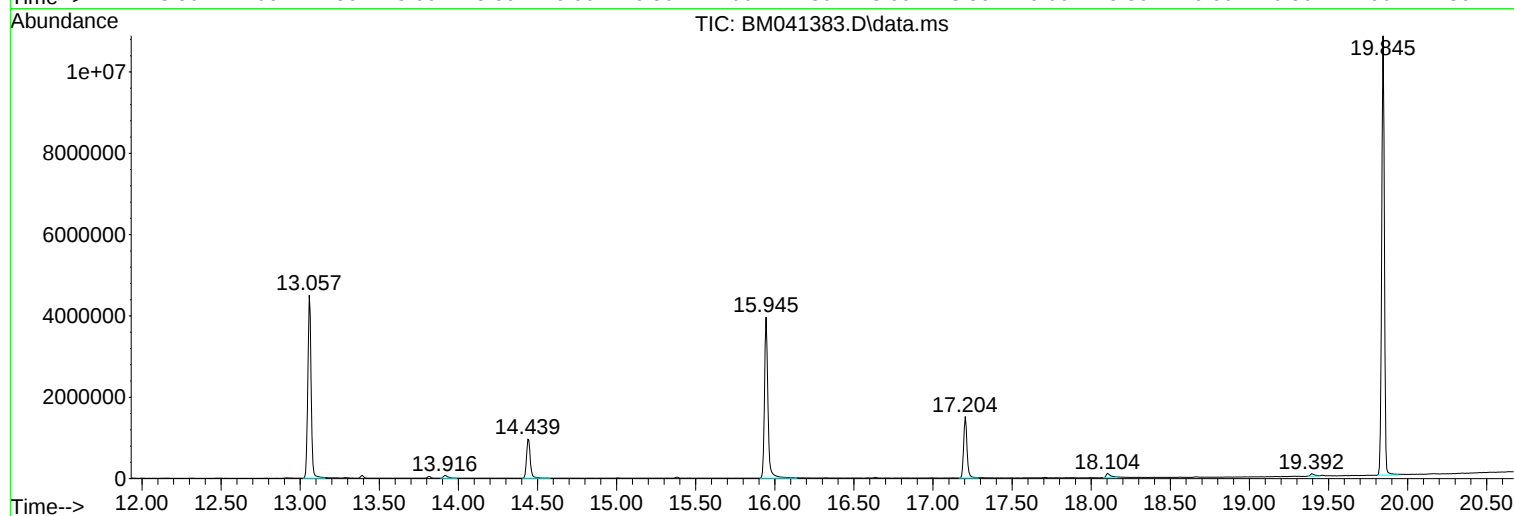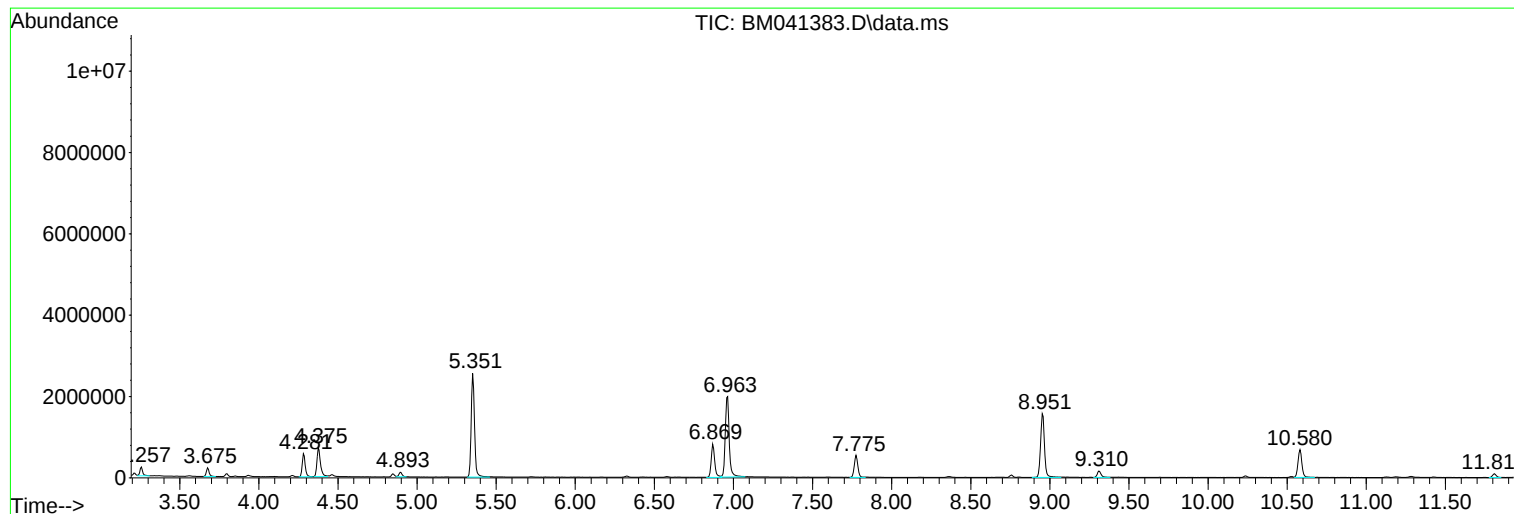

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041383.D
Acq On : 11 Aug 2023 12:30
Operator : MA/JU
Sample : 03954-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041383.D
Acq On : 11 Aug 2023 12:30
Operator : MA/JU
Sample : 03954-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------