

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
 Data File : BM041392.D
 Acq On : 11 Aug 2023 18:07
 Operator : MA/JU
 Sample : 03955-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	283	290	305	rVB	249923	379056	3.92%	0.809%
2	5.351	362	368	382	rBV	2353698	3440563	35.55%	7.345%
3	6.957	634	641	669	rBV	2103685	3626843	37.47%	7.742%
4	7.775	773	780	789	rBV	669950	1051974	10.87%	2.246%
5	8.951	973	980	1001	rBV	1248894	2193997	22.67%	4.683%
6	10.581	1249	1257	1270	rBV	852535	1516864	15.67%	3.238%
7	13.057	1672	1678	1695	rBV	3691088	5403339	55.82%	11.534%
8	14.439	1906	1913	1938	rBV	1325971	2142355	22.13%	4.573%
9	15.945	2162	2169	2189	rBV	3167751	4842795	50.03%	10.338%
10	17.204	2376	2383	2389	rBV	1874119	2722390	28.13%	5.811%
11	18.104	2530	2536	2555	rBV	470103	856043	8.84%	1.827%
12	19.274	2731	2735	2745	rVB	105777	155700	1.61%	0.332%
13	19.386	2750	2754	2767	rBV	238541	421154	4.35%	0.899%
14	19.645	2794	2798	2803	rVB2	90638	124657	1.29%	0.266%
15	19.845	2826	2832	2847	rBV	8041065	9679426	100.00%	20.663%
16	21.109	3043	3047	3056	rBV	429966	615157	6.36%	1.313%
17	21.409	3093	3098	3111	rBV	2679427	3582709	37.01%	7.648%
18	21.545	3117	3121	3129	rVB3	144551	239006	2.47%	0.510%
19	22.497	3279	3283	3290	rVB5	196537	335161	3.46%	0.715%
20	23.774	3493	3500	3518	rVB	1740136	3516097	36.33%	7.506%




Sum of corrected areas: 46845286

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041392.D
Acq On : 11 Aug 2023 18:07
Operator : MA/JU
Sample : 03955-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

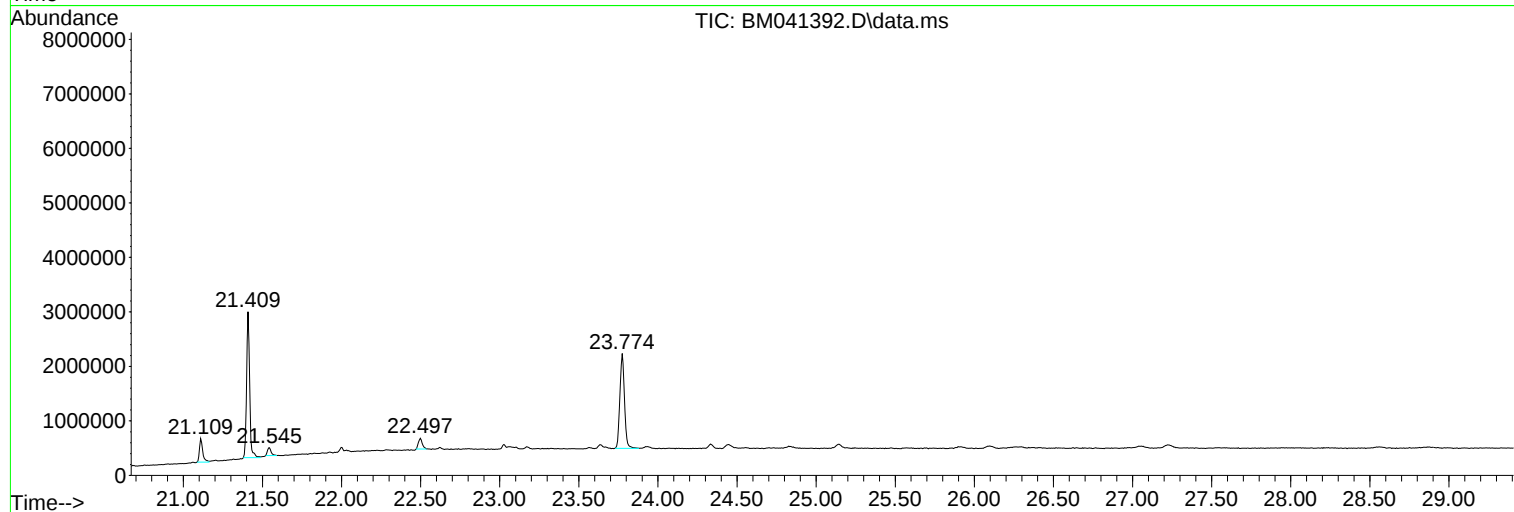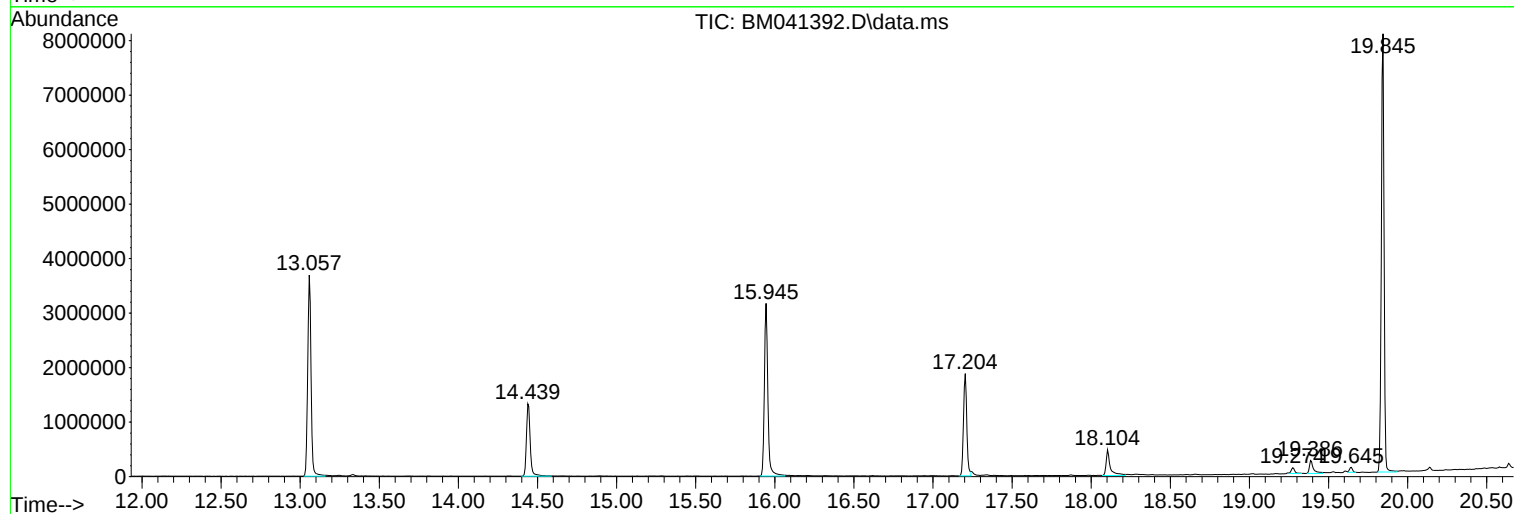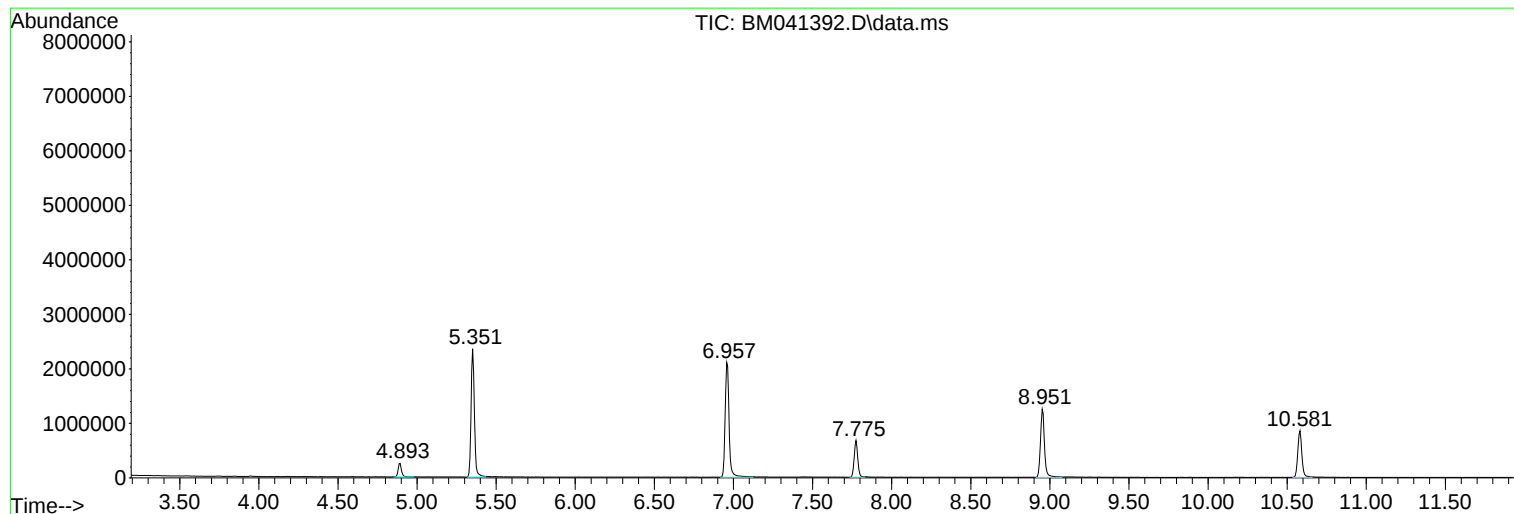

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041392.D
Acq On : 11 Aug 2023 18:07
Operator : MA/JU
Sample : 03955-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041392.D
Acq On : 11 Aug 2023 18:07
Operator : MA/JU
Sample : 03955-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc