


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
 Data File : BM041377.D
 Acq On : 11 Aug 2023 08:13
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 11 17:51:06 2023

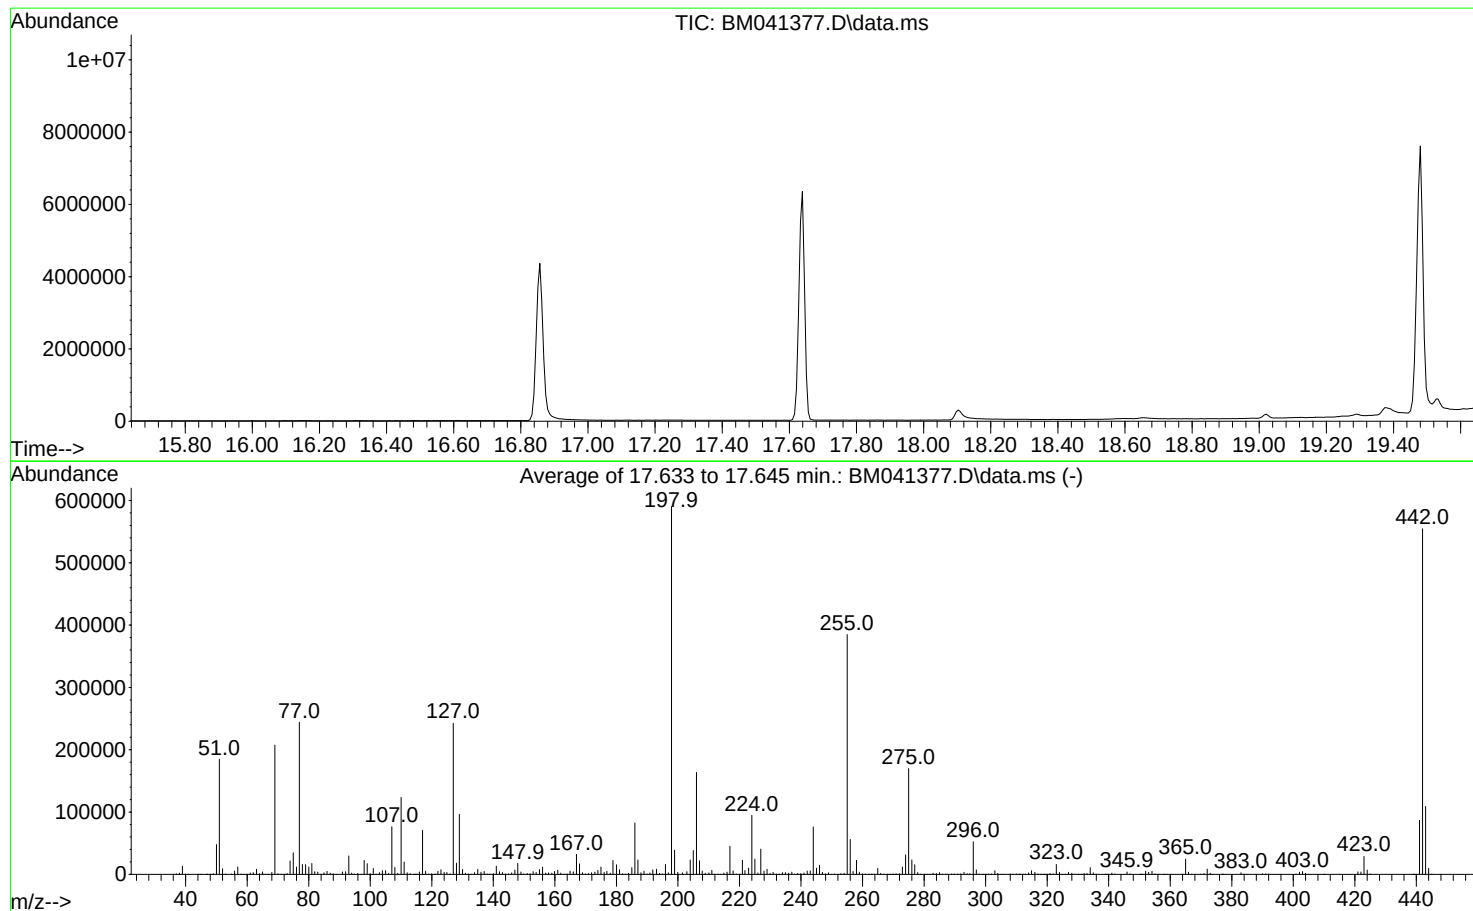




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	184604	PASS
68	69	0.00	2	1.5	3193	PASS
69	198	0.00	100	35.1	207500	PASS
70	69	0.00	2	0.5	1066	PASS
127	198	10	80	41.1	242475	PASS
197	198	0.00	2	0.4	2612	PASS
198	198	100	100	100.0	590357	PASS
199	198	5	9	6.6	38744	PASS
275	198	10	60	28.8	169877	PASS
365	198	1	100	4.1	24405	PASS
441	198	0.01	100	14.7	86717	PASS
442	442	50	100	100.0	554795	PASS
443	442	15	24	19.6	108936	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
 Data File : BM041377.D
 Acq On : 11 Aug 2023 08:13
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 11 11:00:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 12:20:12 2023
 Response via : Initial Calibration

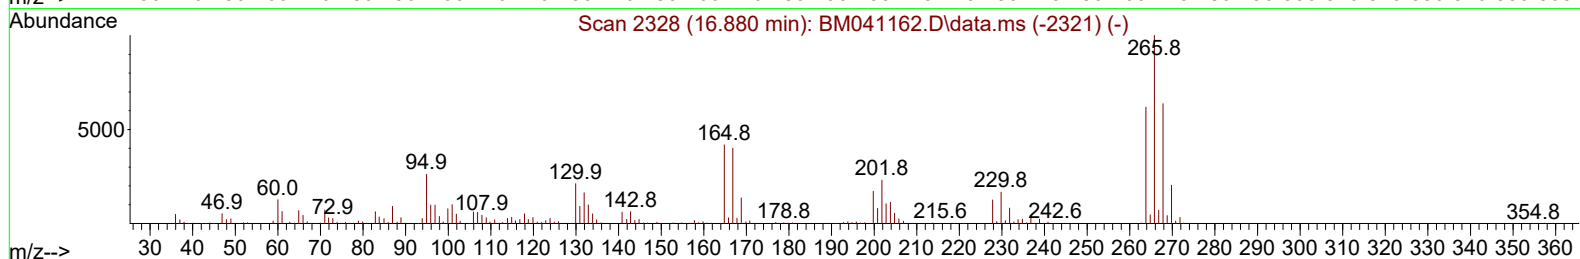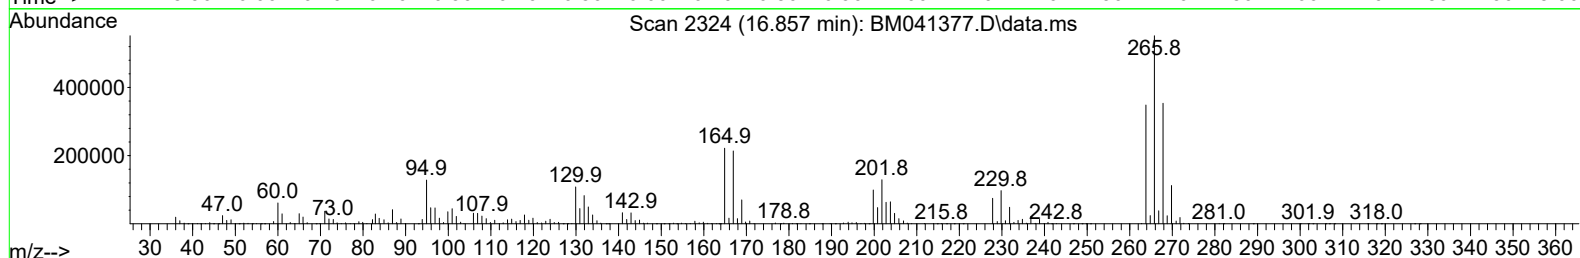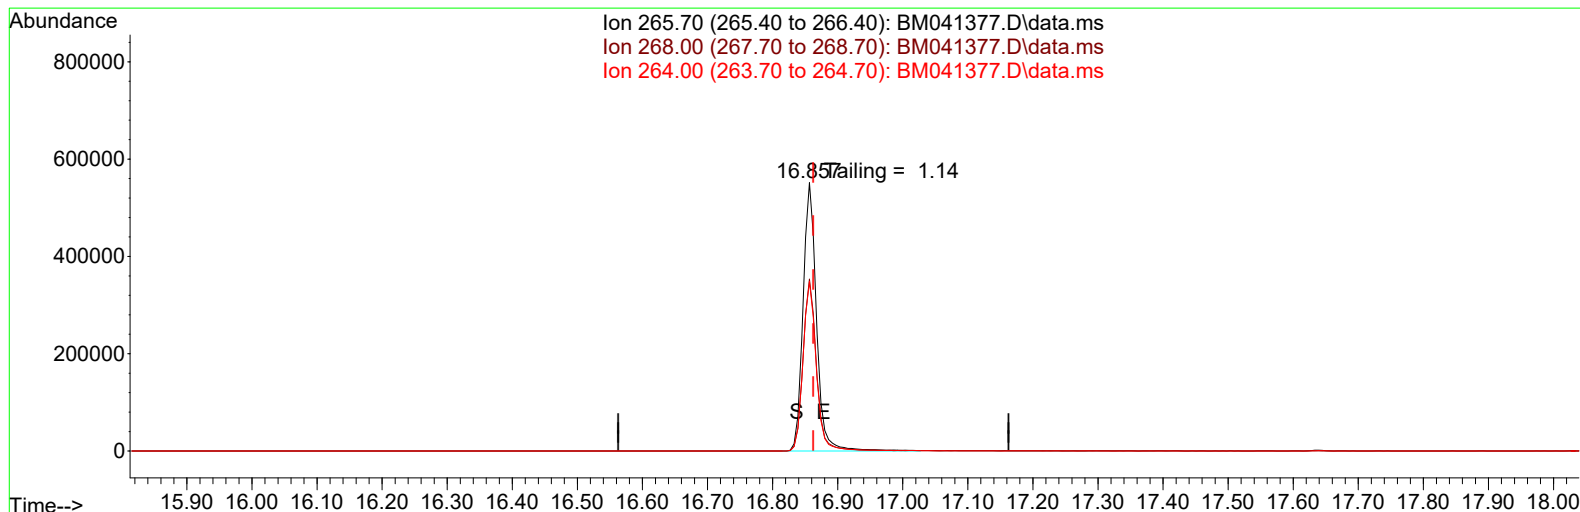

TIC: BM041377.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.006) 397758.31 ng




response 795841

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.08
264.00	61.80	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081123\
Data File : BM041377.D
Acq On : 11 Aug 2023 08:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 11 11:00:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 12:20:12 2023
Response via : Initial Calibration

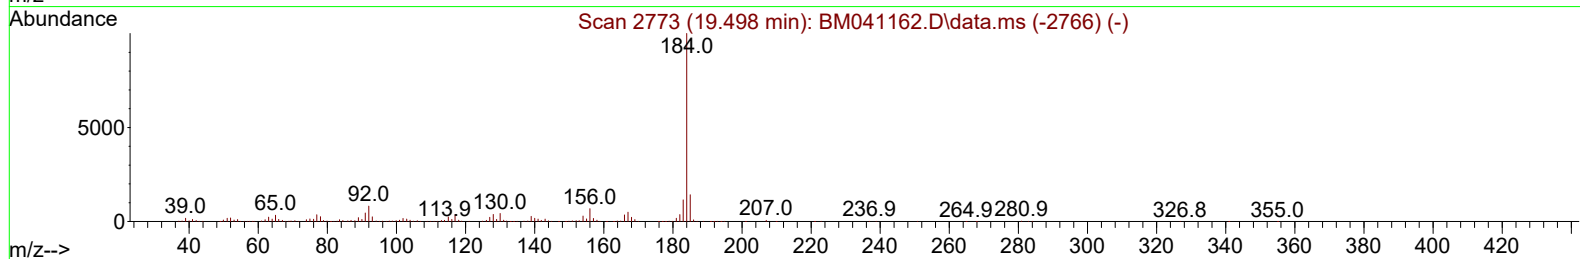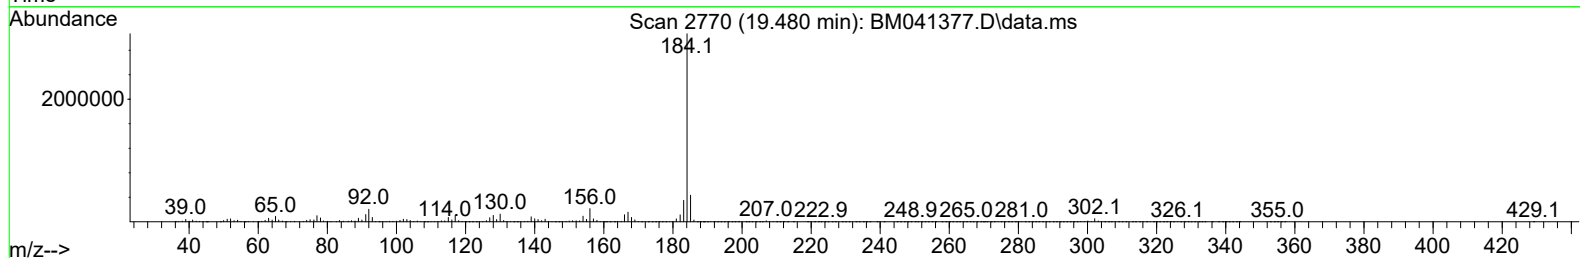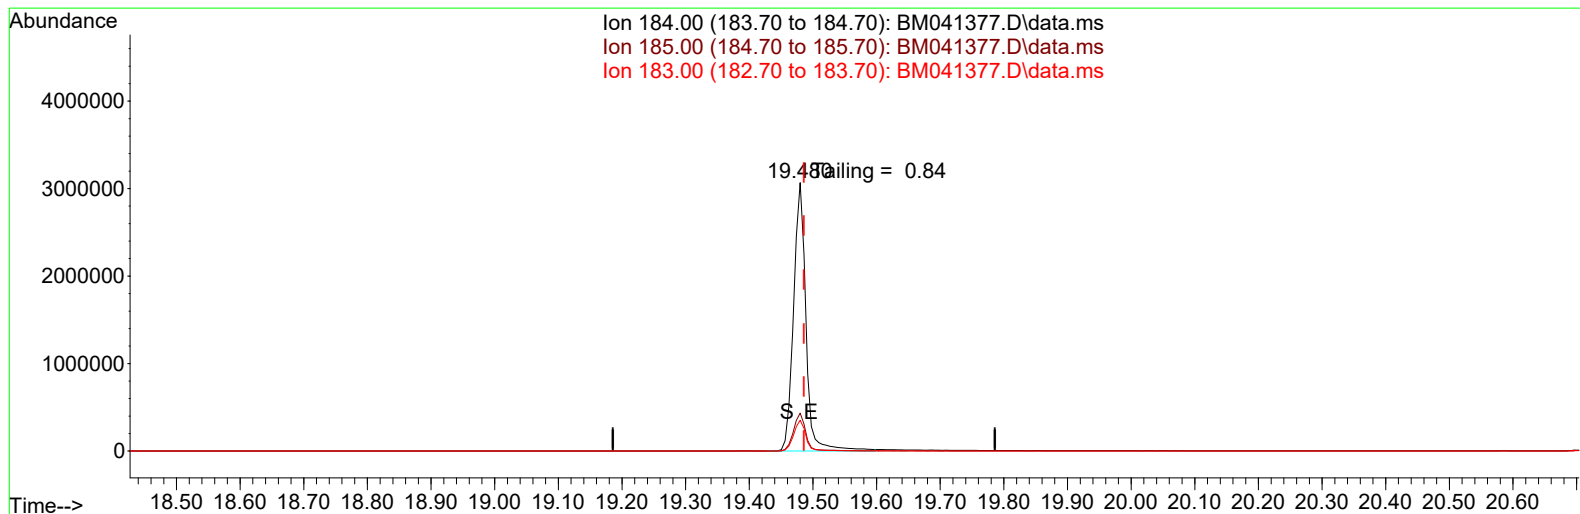

TIC: BM041377.D\data.ms

(77) Benzidine

19.480min (-0.006) 212708.86 ng

response 4218335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.13
183.00	11.50	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2023	BNA_M	<u>BM041377.D</u>
Compound Name	Response	Retention Time
DDT	2423802	20.703
DDD	43219	20.303
DDE	2729	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45948	2469750	1.86

Instrument :
BNA_M
ClientSampleId :
DFTPP