

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
 Data File : BM016324.D
 Acq On : 13 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4272-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JC-03-080918-I

Quant Time: Aug 14 03:51:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 10 18:44:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	24921	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	81090	20.00	ng	-0.01
38) Acenaphthene-d10	14.76	164	37470	20.00	ng	-0.01
63) Phenanthrene-d10	17.49	188	75093	20.00	ng	-0.02
75) Chrysene-d12	21.62	240	88344	20.00	ng	-0.02
86) Perylene-d12	23.96	264	102944	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	224769	149.82	ng	0.00
7) Phenol-d6	7.30	99	224574	114.62	ng	0.00
23) Nitrobenzene-d5	9.31	82	220490	126.47	ng	-0.01
41) 2,4,6-Tribromophenol	16.25	330	71552	150.56	ng	-0.01
44) 2-Fluorobiphenyl	13.38	172	390580	126.83	ng	-0.01
78) Terphenyl-d14	20.07	244	580658	137.59	ng	-0.01
Target Compounds						
15) Benzyl Alcohol	8.45	79	5433	3.483	ng	Qvalue # 31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
Data File : BM016324.D
Acq On : 13 Aug 2018 13:59
Operator : SJ/JU
Sample : J4272-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JC-03-080918-I

Quant Time: Aug 14 03:51:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 10 18:44:22 2018
Response via : Initial Calibration

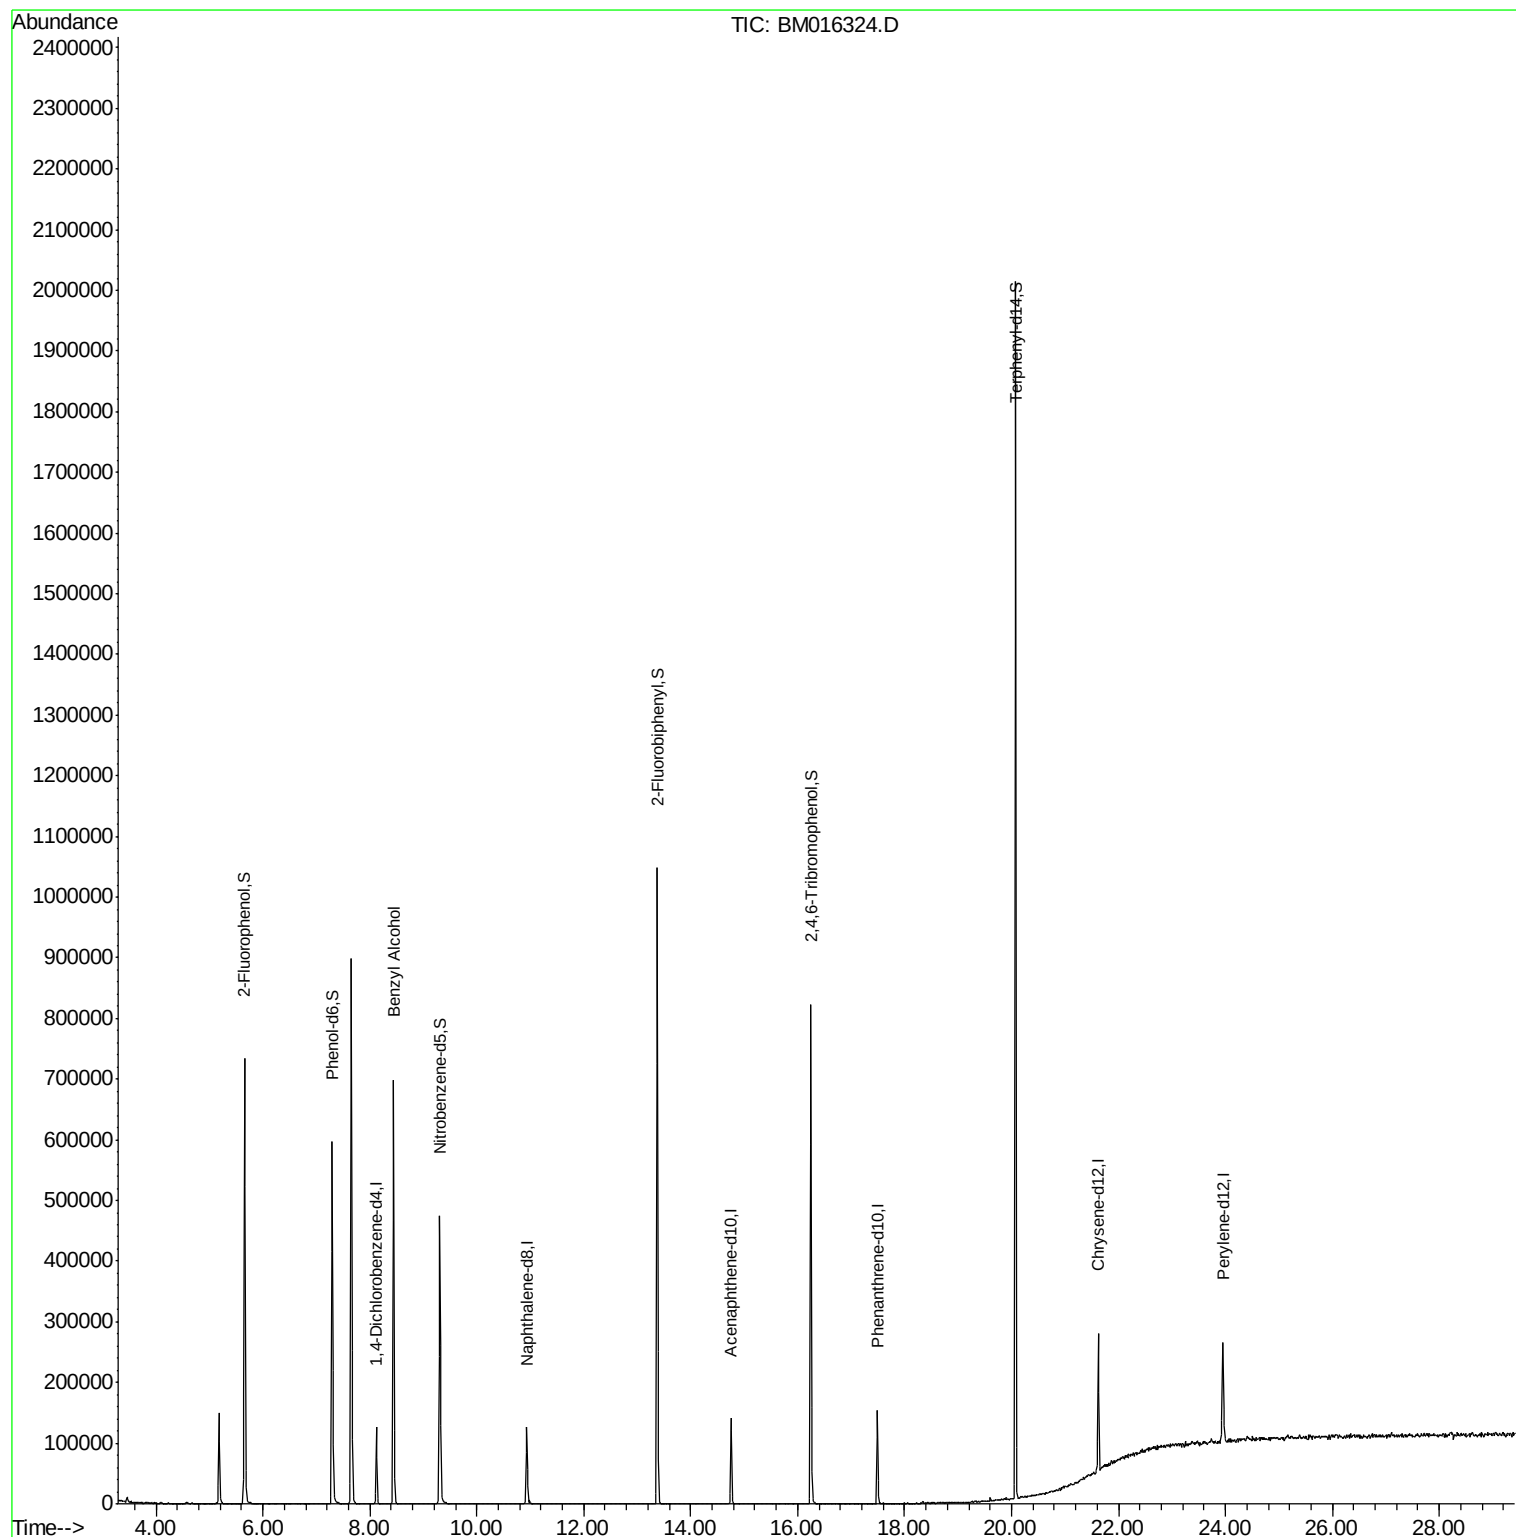

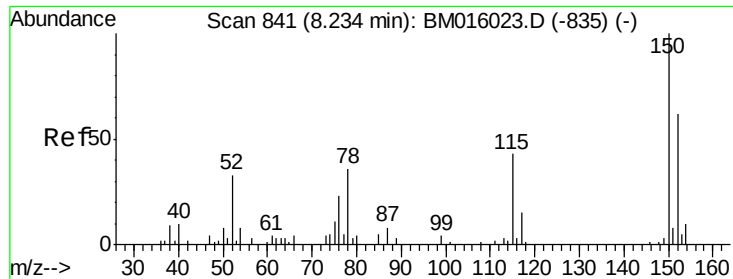


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.13 min Scan# 823
Delta R.T. -0.01 min
Lab File: BM016324.D
Acq: 13 Aug 2018 13:59

Instrument :
BNA_M
ClientSampleId :
JC-03-080918-I

Tgt Ion:152 Resp: 24921
Ion Ratio Lower Upper
152 100
150 136.0 119.5 179.3
115 66.5 43.0 64.4#

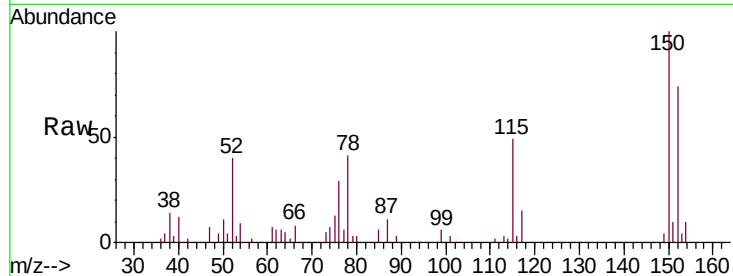


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

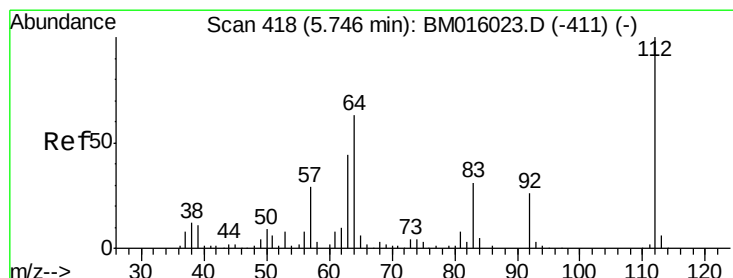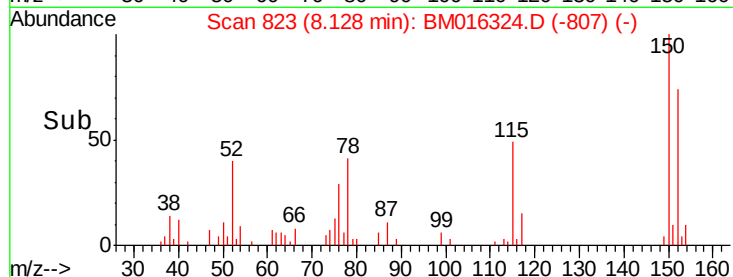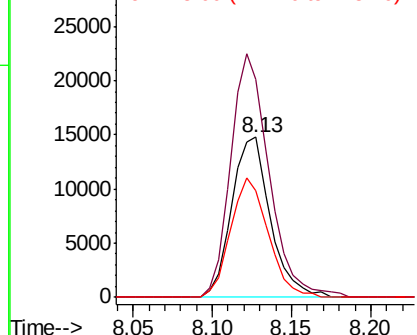



#5


2-Fluorophenol
Concen: N.D. ng
RT: 5.66 min Scan# 403
Delta R.T. -0.01 min
Lab File: BM016324.D
Acq: 13 Aug 2018 13:59

Tgt Ion:112 Resp: 224769
Ion Ratio Lower Upper
112 100
64 62.7 38.6 57.8#
63 49.1 19.3 28.9#

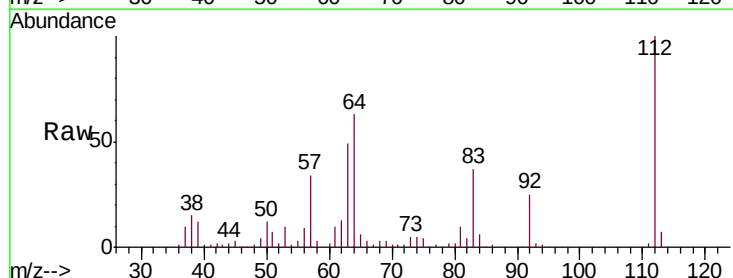

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

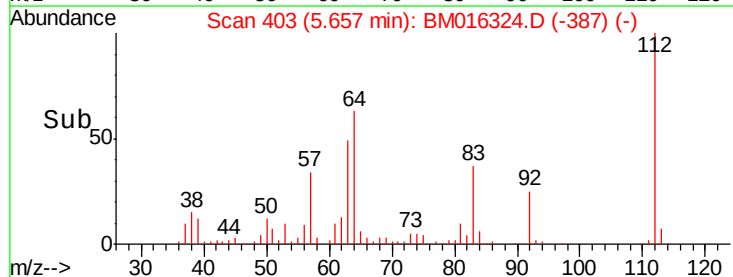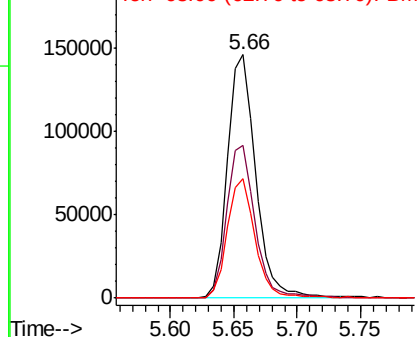

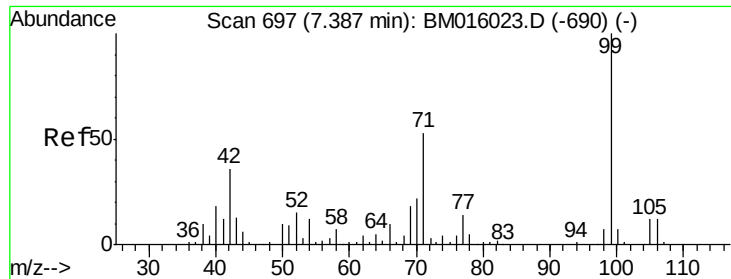

#7

Phenol-d6

Concen: N.D. ng

RT: 7.30 min Scan# 682

Delta R.T. -0.01 min

Lab File: BM016324.D

Acq: 13 Aug 2018 13:59

Instrument :

BNA_M

ClientSampleId :

JC-03-080918-I


Tgt Ion: 99 Resp: 224574

Ion Ratio Lower Upper

99 100

42 40.4 11.0 16.4#




71 60.5 23.4 35.2#

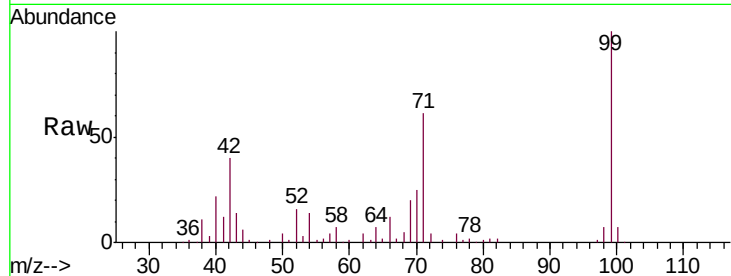

Abundance Ion 99.00 (98.70 to 99.70): BM016324.D (-690) (-)

Ion 42.00 (41.70 to 42.70): BM016324.D (-690) (-)

Ion 71.00 (70.70 to 71.70): BM016324.D (-690) (-)

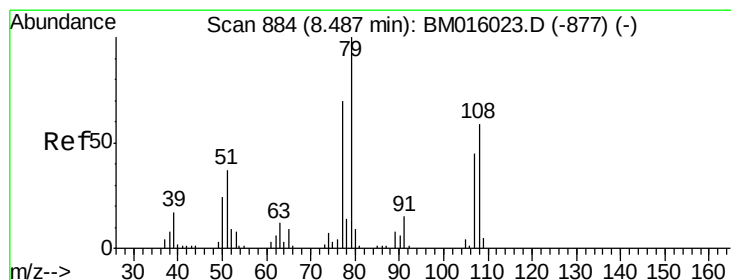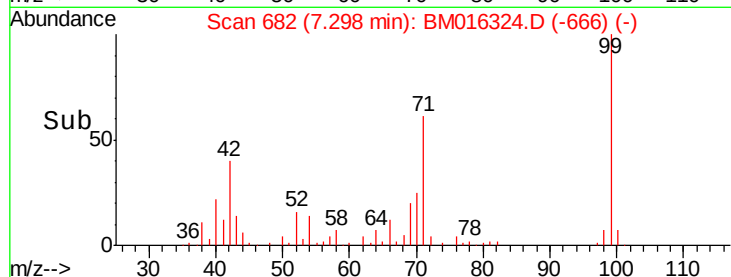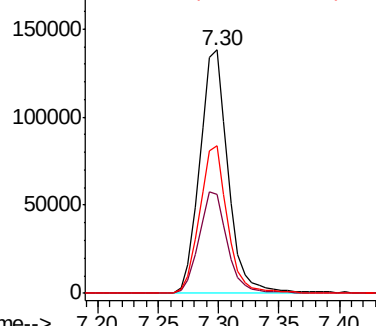

#15

Benzyl Alcohol

Concen: 3.483 ng

RT: 8.45 min Scan# 877

Delta R.T. 0.05 min

Lab File: BM016324.D

Acq: 13 Aug 2018 13:59


Tgt Ion: 79 Resp: 5433

Ion Ratio Lower Upper

79 100

108 78.1 65.0 97.4



77 185.0 53.0 79.6#

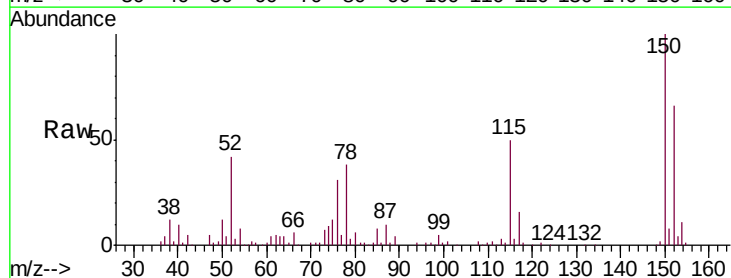


Abundance Ion 79.00 (78.70 to 79.70): BM016324.D (-877) (-)

Ion 108.00 (107.70 to 108.70): BM016324.D (-877) (-)

Ion 77.00 (76.70 to 77.70): BM016324.D (-877) (-)

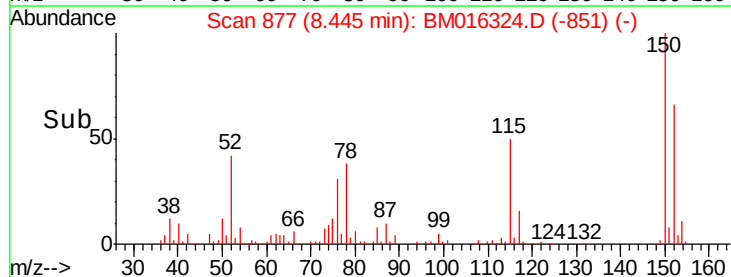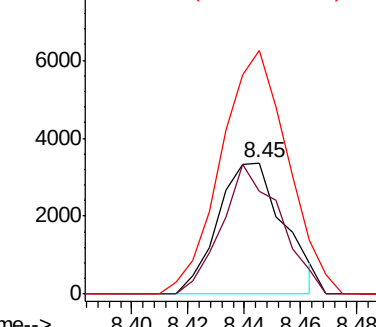


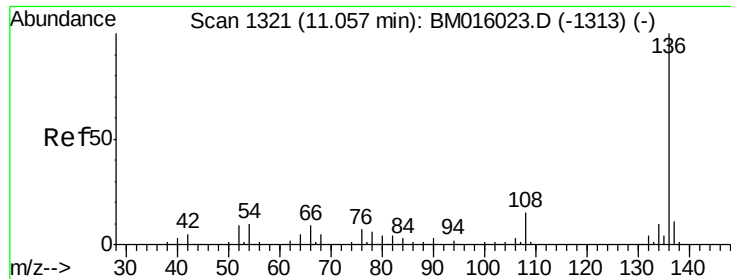




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.94 min Scan# 1301
Delta R.T. -0.01 min
Lab File: BM016324.D
Acq: 13 Aug 2018 13:59

Instrument :
BNA_M
ClientSampleId :
JC-03-080918-I

Tgt Ion:	136	Resp:	81090
Ion	Ratio	Lower	Upper
136	100		
137	9.5	8.7	13.1
54	10.2	4.6	6.8#
68	4.1	3.7	5.5

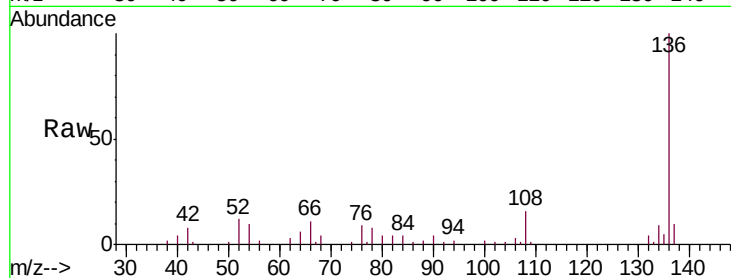


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

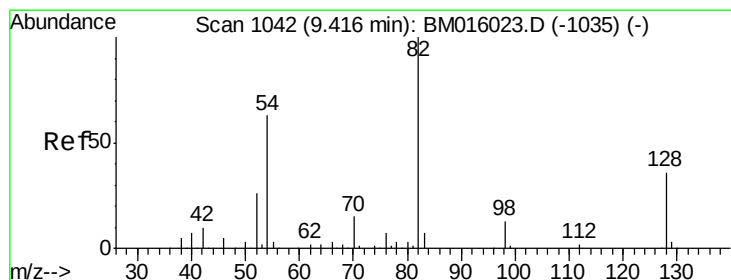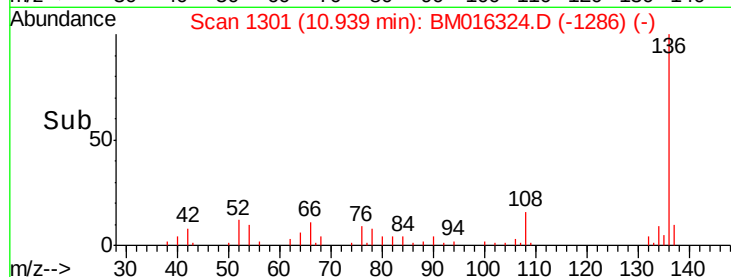
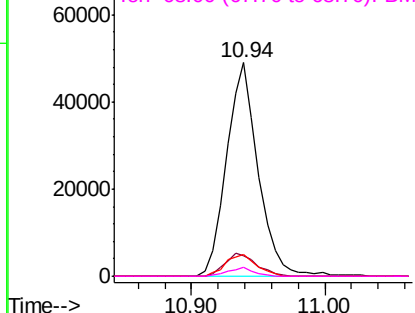



#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.31 min Scan# 1024
Delta R.T. -0.01 min
Lab File: BM016324.D
Acq: 13 Aug 2018 13:59

Tgt Ion:	82	Resp:	220490
Ion	Ratio	Lower	Upper
82	100		
128	35.2	32.8	49.2
54	67.1	40.6	60.8#

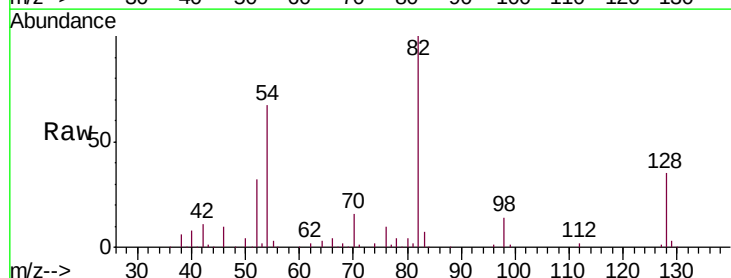

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

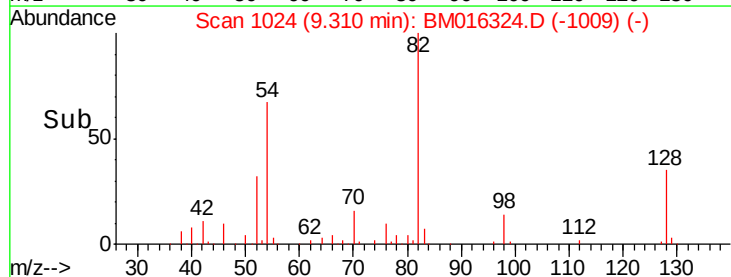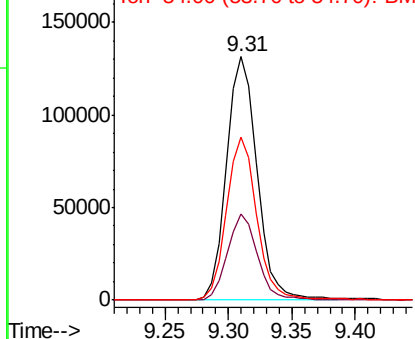

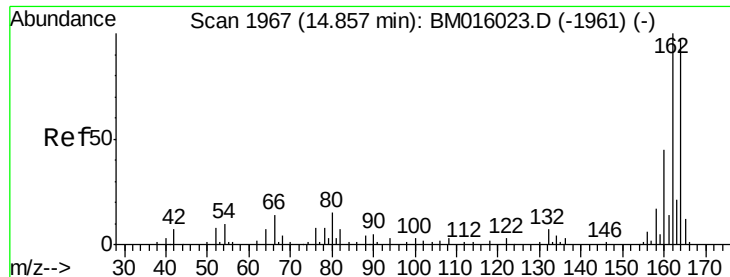

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.76 min Scan# 1950

Delta R.T. -0.01 min

Lab File: BM016324.D

Acq: 13 Aug 2018 13:59

Instrument :

BNA_M

ClientSampleId :

JC-03-080918-I


Tgt Ion:164 Resp: 37470

Ion Ratio Lower Upper

164 100

162 110.7 82.4 123.6




160 54.4 35.8 53.6#

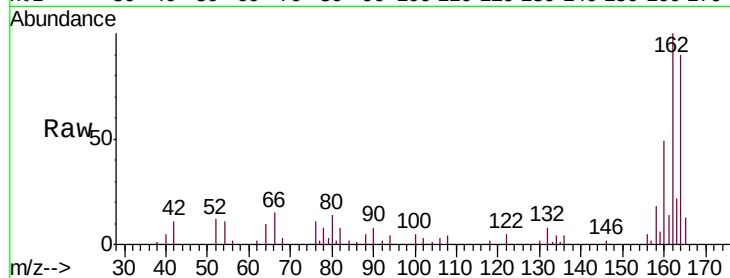

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

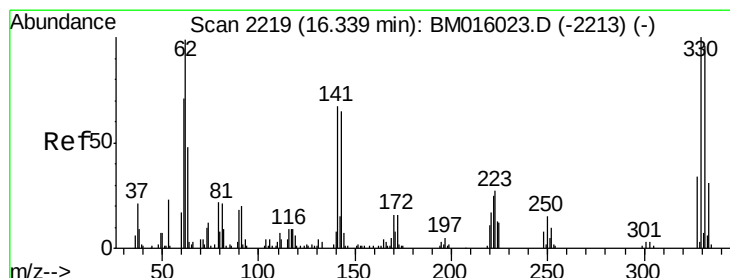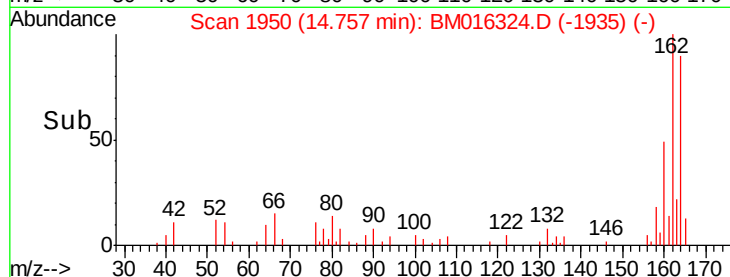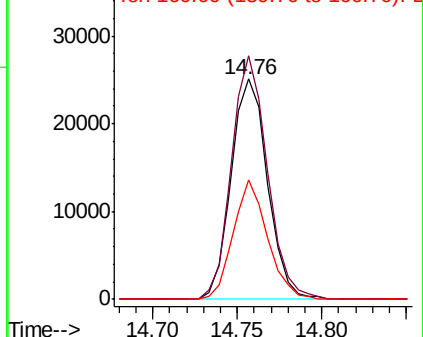

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.25 min Scan# 2204

Delta R.T. -0.01 min

Lab File: BM016324.D

Acq: 13 Aug 2018 13:59


Tgt Ion:330 Resp: 71552

Ion Ratio Lower Upper

330 100

332 98.8 0.0 0.0#



141 92.3 0.0 0.0#

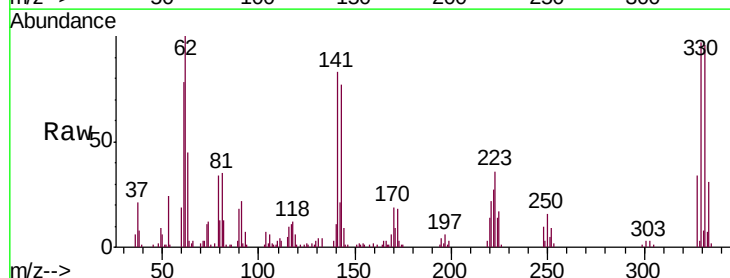


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



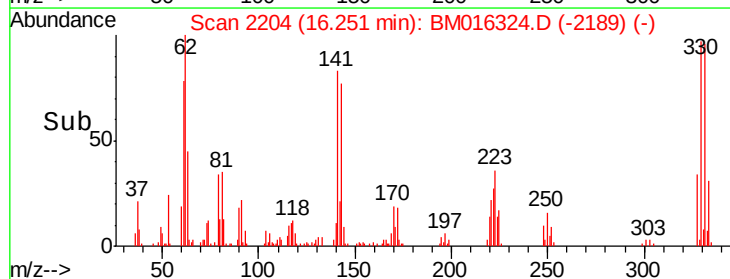
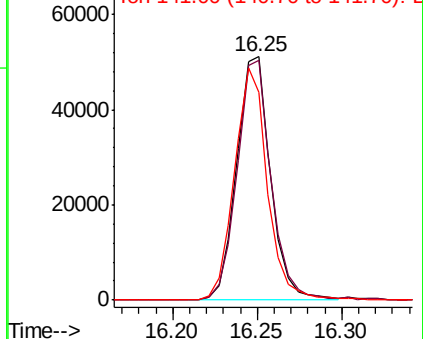


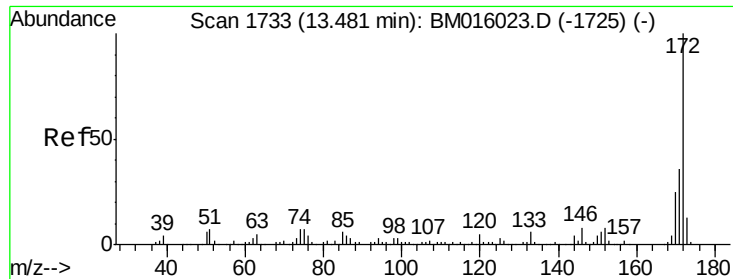

#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.38 min Scan# 1716
 Delta R.T. -0.01 min
 Lab File: BM016324.D
 Acq: 13 Aug 2018 13:59




Instrument :
 BNA_M
 ClientSampleId :
 JC-03-080918-I


Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.5	42.7
170	24.6	18.8	28.2

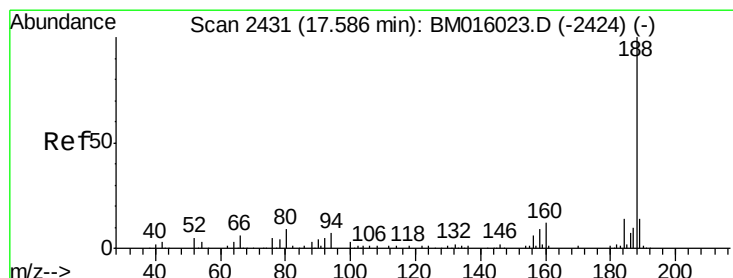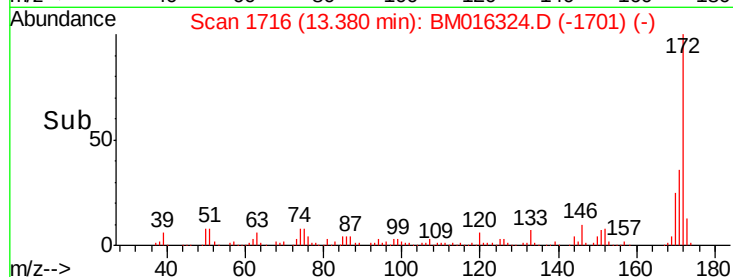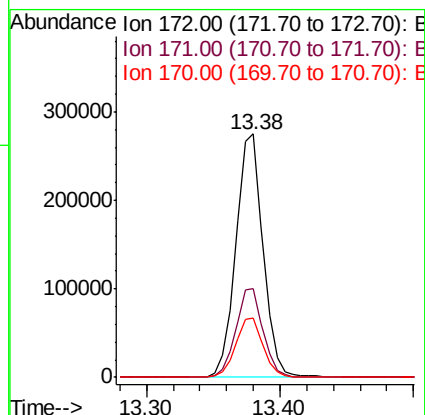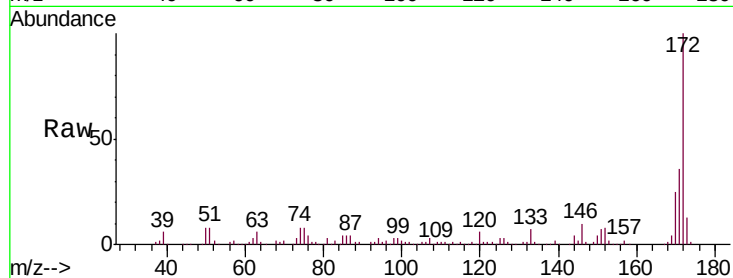

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.49 min Scan# 2415
 Delta R.T. -0.02 min
 Lab File: BM016324.D
 Acq: 13 Aug 2018 13:59

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.0	8.7	13.1#
80	6.9	9.3	13.9#

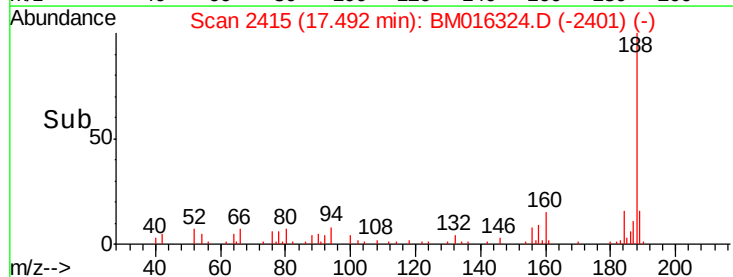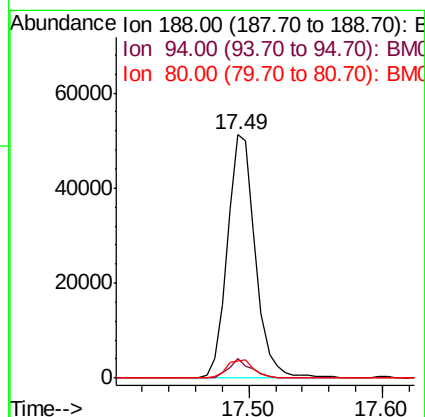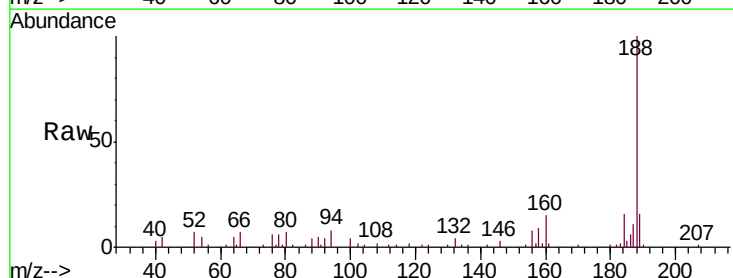

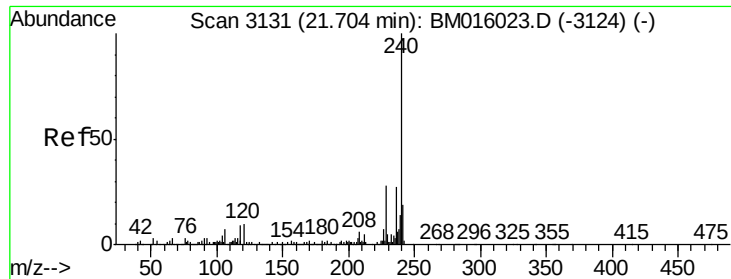

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.62 min Scan# 3117

Delta R.T. -0.02 min

Lab File: BM016324.D

Acq: 13 Aug 2018 13:59

Instrument :

BNA_M

ClientSampleId :

JC-03-080918-I


Tgt Ion:240 Resp: 88344

Ion Ratio Lower Upper

240 100

120 7.5 8.2 12.2#




236 29.9 20.0 30.0

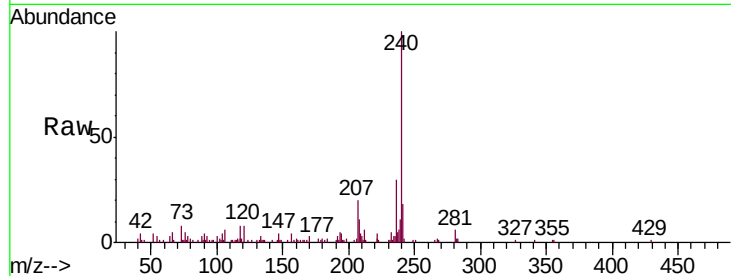

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

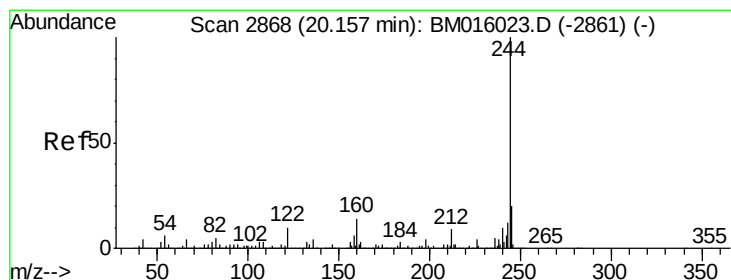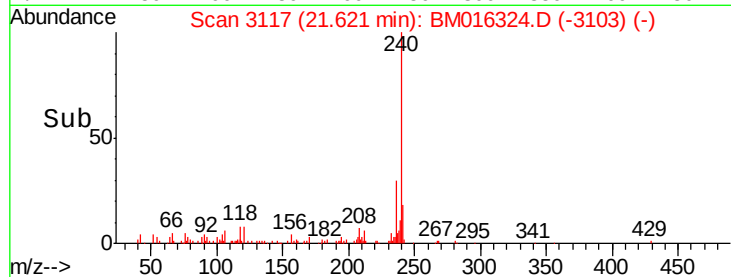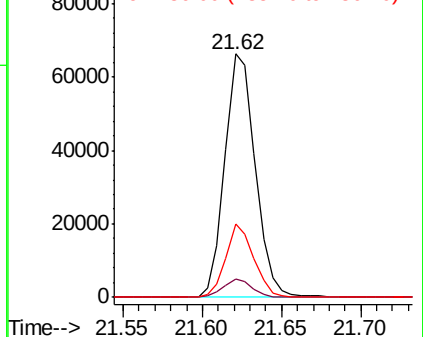

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.07 min Scan# 2854

Delta R.T. -0.01 min

Lab File: BM016324.D

Acq: 13 Aug 2018 13:59


Tgt Ion:244 Resp: 580658

Ion Ratio Lower Upper

244 100

212 11.4 4.9 7.3#



122 8.7 6.2 9.4

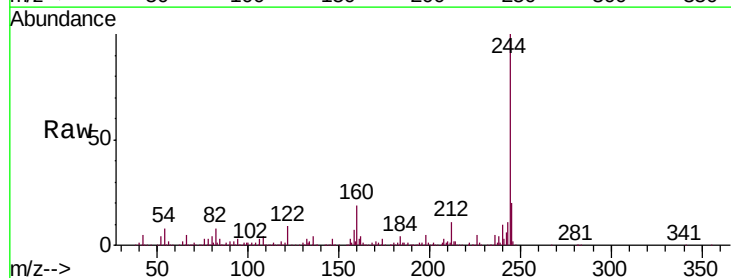


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

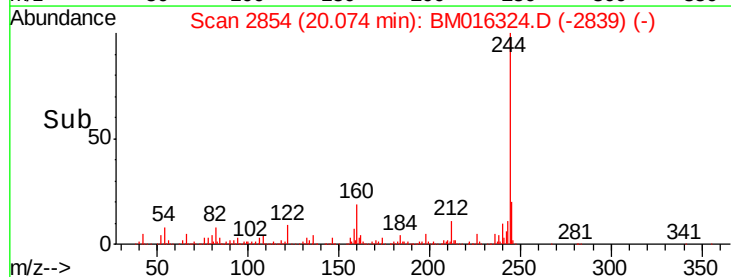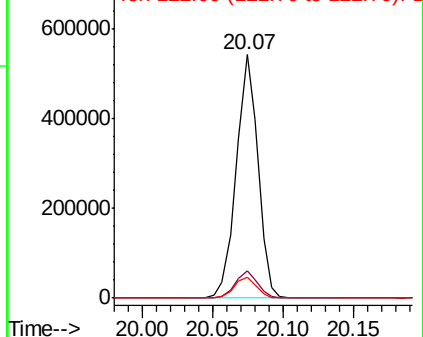

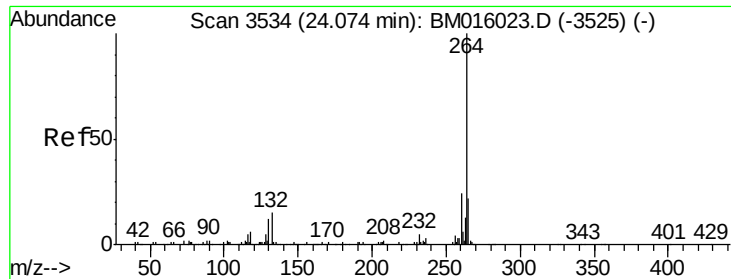

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.96 min Scan# 3514
Delta R.T. -0.02 min
Lab File: BM016324.D
Acq: 13 Aug 2018 13:59

Instrument :
BNA_M
ClientSampleId :
JC-03-080918-I

Tgt Ion:	264	Resp:	102944
Ion	Ratio	Lower	Upper
264	100		
260	23.8	18.6	27.8
265	21.7	17.3	25.9

