

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
 Data File : BM016330.D
 Acq On : 13 Aug 2018 17:59
 Operator : SJ/JU
 Sample : J4442-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-1

Quant Time: Aug 14 03:53:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 10 18:44:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	25611	20.00	ng	-0.01
21) Naphthalene-d8	10.94	136	84648	20.00	ng	-0.01
38) Acenaphthene-d10	14.76	164	38669	20.00	ng	-0.01
63) Phenanthrene-d10	17.49	188	74662	20.00	ng	-0.02
75) Chrysene-d12	21.62	240	90038	20.00	ng	-0.02
86) Perylene-d12	23.95	264	105866	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	198193	128.55	ng	0.00
7) Phenol-d6	7.29	99	190395	94.56	ng	-0.01
23) Nitrobenzene-d5	9.31	82	195428	107.38	ng	-0.01
41) 2,4,6-Tribromophenol	16.25	330	61174	124.73	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	334392	105.22	ng	-0.02
78) Terphenyl-d14	20.07	244	470478	109.38	ng	-0.01
Target Compounds						
15) Benzyl Alcohol	8.44	79	4444	2.772	ng	Qvalue # 30

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
Data File : BM016330.D
Acq On : 13 Aug 2018 17:59
Operator : SJ/JU
Sample : J4442-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-1

Quant Time: Aug 14 03:53:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 10 18:44:22 2018
Response via : Initial Calibration

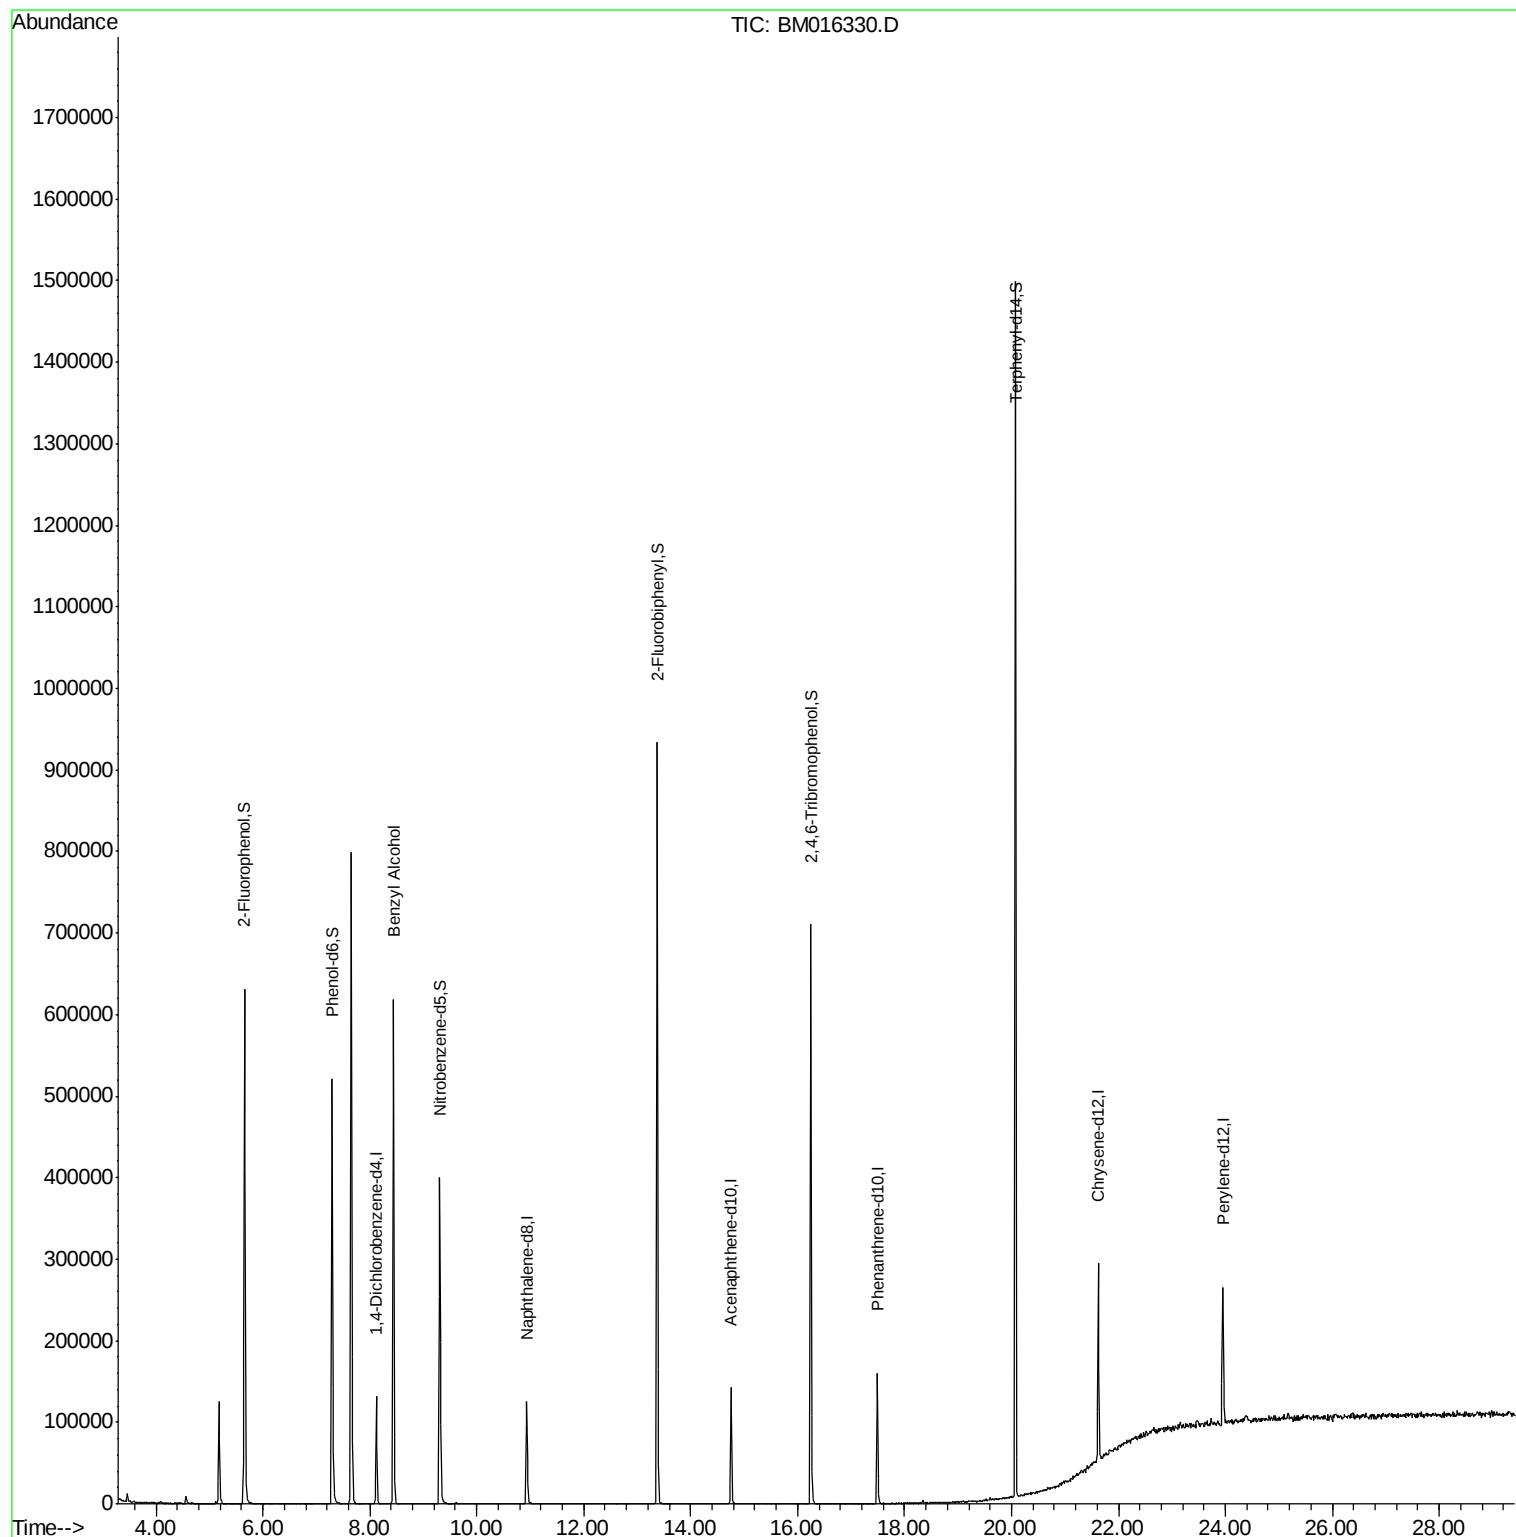







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.12 min Scan# 822
 Delta R.T. -0.01 min
 Lab File: BM016330.D
 Acq: 13 Aug 2018 17:59

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-1

Tgt Ion:152 Resp: 25611
 Ion Ratio Lower Upper
 152 100
 150 155.2 119.5 179.3
 115 74.0 43.0 64.4#

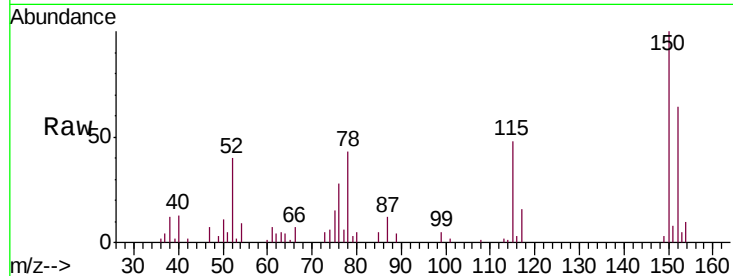


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

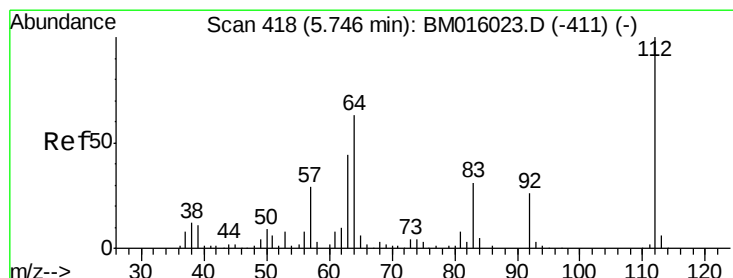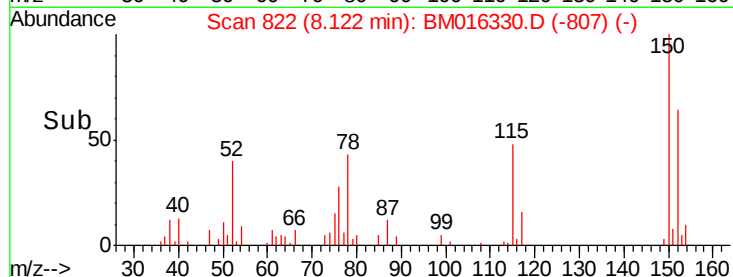
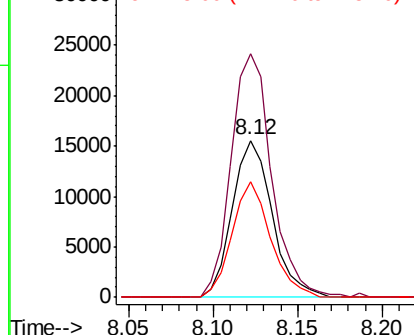


#5
 2-Fluorophenol
 Concen: Below ng
 RT: 5.66 min Scan# 403
 Delta R.T. -0.01 min
 Lab File: BM016330.D
 Acq: 13 Aug 2018 17:59

Tgt Ion:112 Resp: 198193
 Ion Ratio Lower Upper
 112 100
 64 57.6 38.6 57.8
 63 47.2 19.3 28.9#

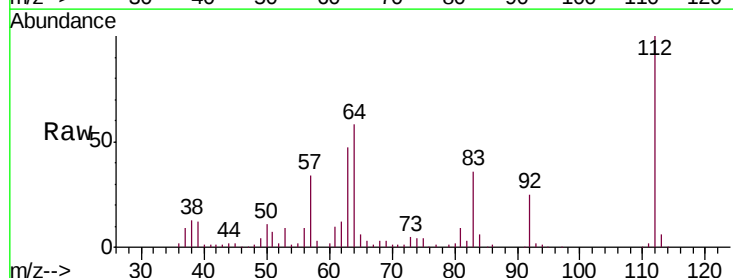

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

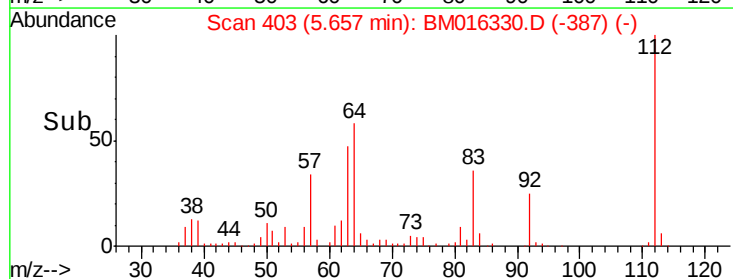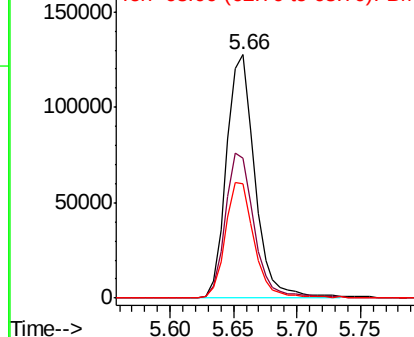



#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 681

Delta R.T. -0.01 min

Lab File: BM016330.D

Acq: 13 Aug 2018 17:59

Instrument :

BNA_M

ClientSampleId :

SP-1-1


Tgt Ion: 99 Resp: 190395

Ion Ratio Lower Upper

99 100

42 39.8 11.0 16.4#




71 59.7 23.4 35.2#

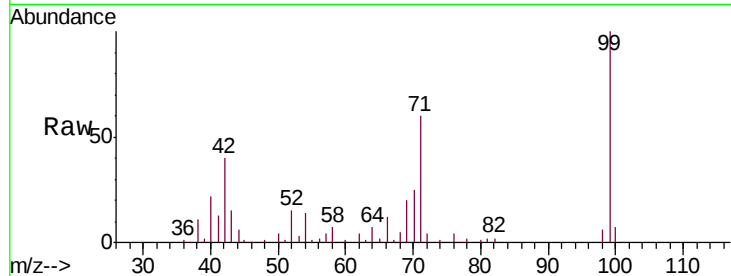

Abundance Ion 99.00 (98.70 to 99.70): BM016330.D (-690) (-)

Ion 42.00 (41.70 to 42.70): BM016330.D (-690) (-)

Ion 71.00 (70.70 to 71.70): BM016330.D (-690) (-)

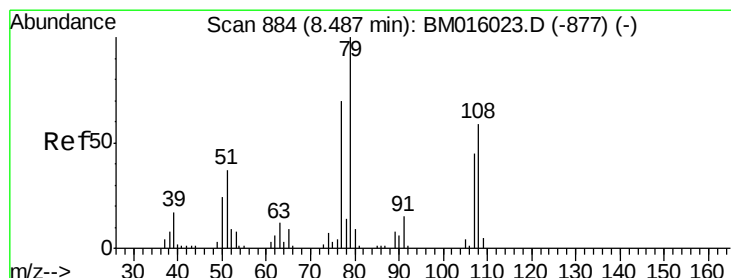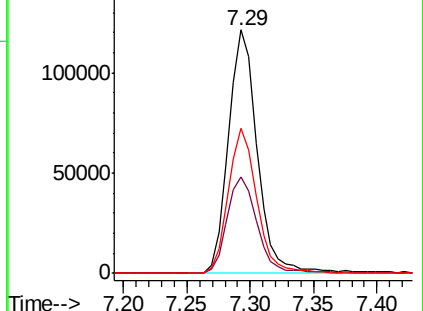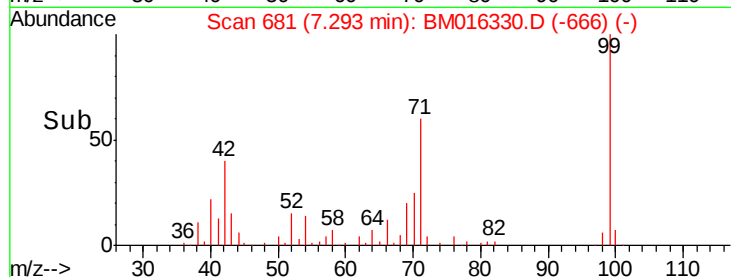

#15

Benzyl Alcohol

Concen: 2.772 ng

RT: 8.44 min Scan# 876

Delta R.T. 0.05 min

Lab File: BM016330.D

Acq: 13 Aug 2018 17:59


Tgt Ion: 79 Resp: 4444

Ion Ratio Lower Upper

79 100

108 91.6 65.0 97.4



77 178.2 53.0 79.6#

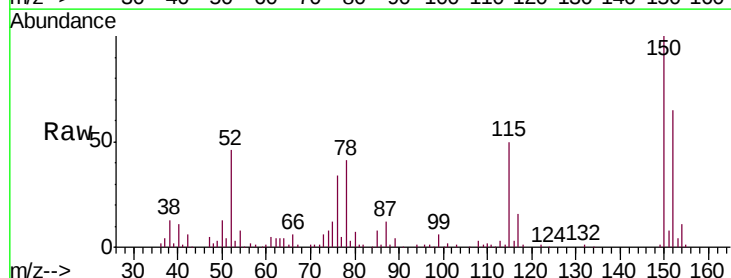

Abundance Ion 79.00 (78.70 to 79.70): BM016330.D (-877) (-)

Ion 108.00 (107.70 to 108.70): BM016330.D (-877) (-)

Ion 77.00 (76.70 to 77.70): BM016330.D (-877) (-)

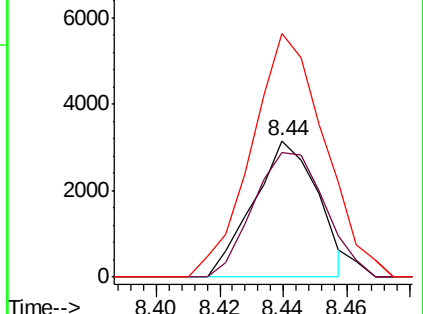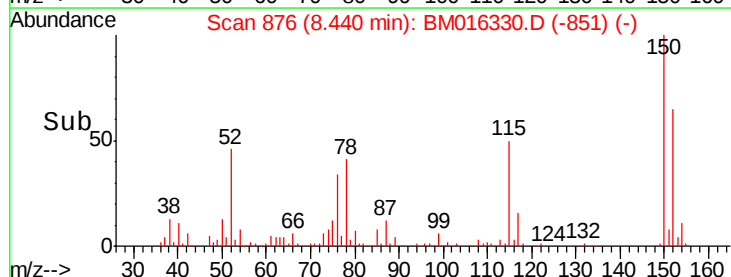







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.94 min Scan# 1301
Delta R.T. -0.01 min
Lab File: BM016330.D
Acq: 13 Aug 2018 17:59

Instrument :
BNA_M
ClientSampleId :
SP-1-1

Tgt Ion: 136 Resp: 84648
Ion Ratio Lower Upper
136 100
137 11.8 8.7 13.1
54 10.9 4.6 6.8#
68 3.9 3.7 5.5

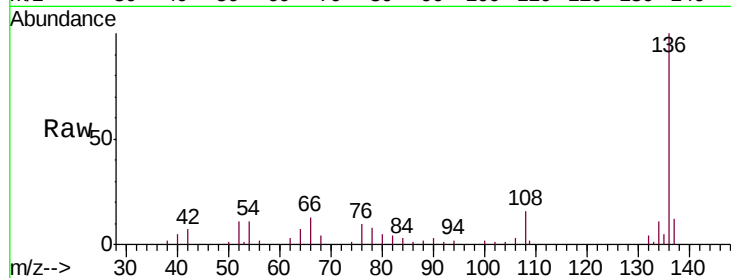


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

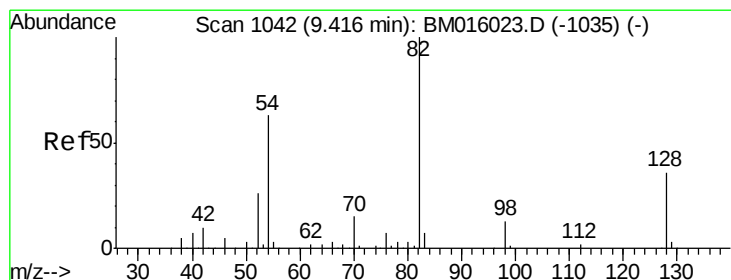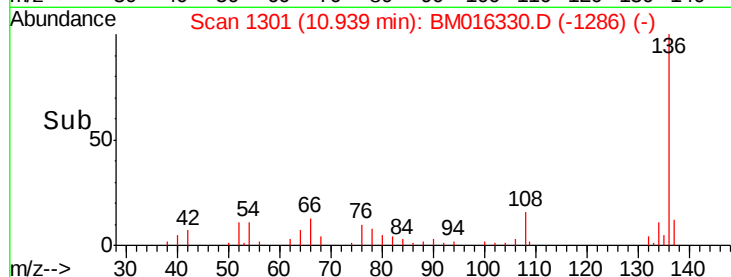
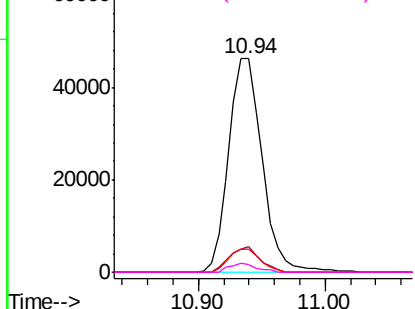


#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.31 min Scan# 1024
Delta R.T. -0.01 min
Lab File: BM016330.D
Acq: 13 Aug 2018 17:59

Tgt Ion: 82 Resp: 195428
Ion Ratio Lower Upper
82 100
128 36.0 32.8 49.2
54 68.0 40.6 60.8#

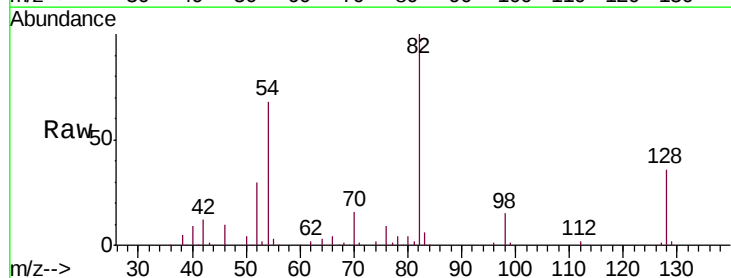

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

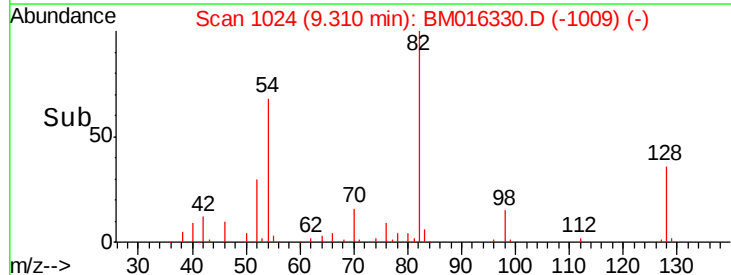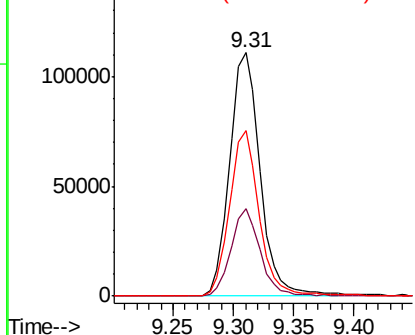



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.76 min Scan# 1950

Delta R.T. -0.01 min

Lab File: BM016330.D

Acq: 13 Aug 2018 17:59

Instrument :

BNA_M

ClientSampleId :

SP-1-1


Tgt Ion:164 Resp: 38669

Ion Ratio Lower Upper

164 100

162 111.3 82.4 123.6




160 48.7 35.8 53.6

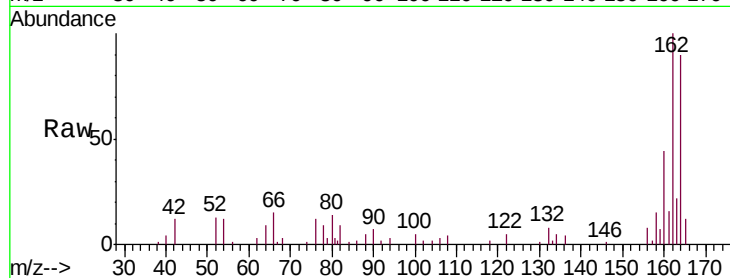

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

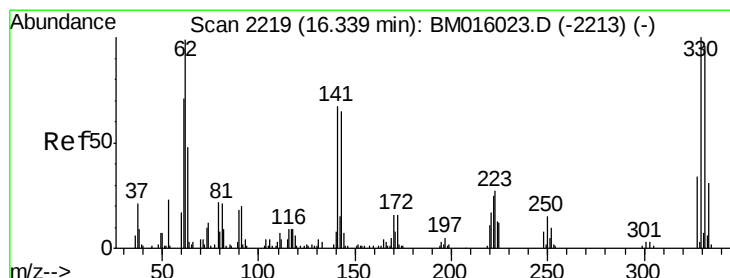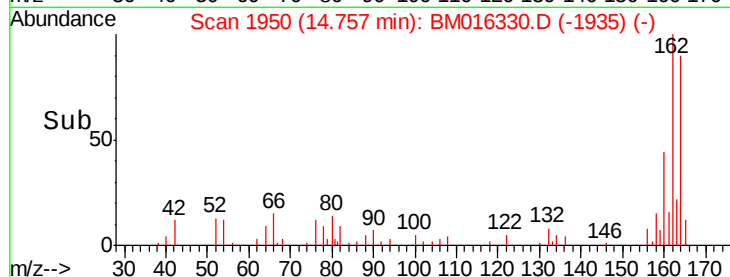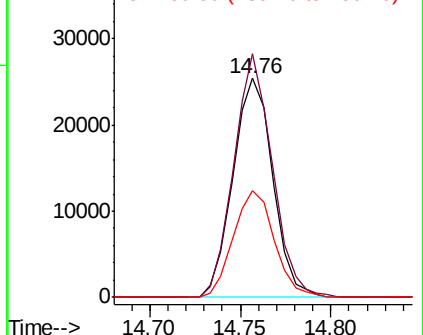

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.25 min Scan# 2203

Delta R.T. -0.02 min

Lab File: BM016330.D

Acq: 13 Aug 2018 17:59


Tgt Ion:330 Resp: 61174

Ion Ratio Lower Upper

330 100

332 96.5 0.0 0.0#



141 89.8 0.0 0.0#

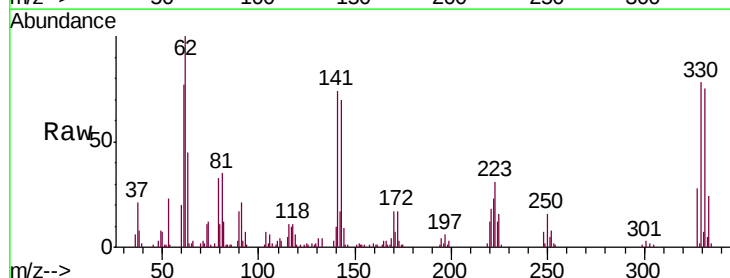

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



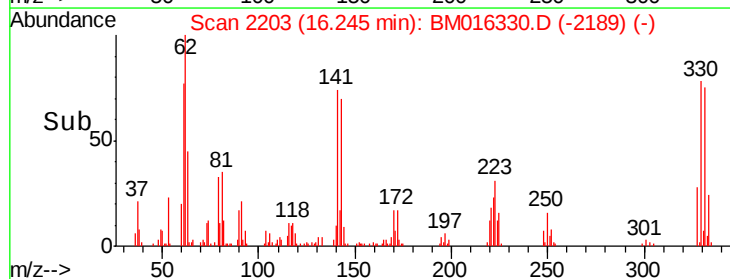
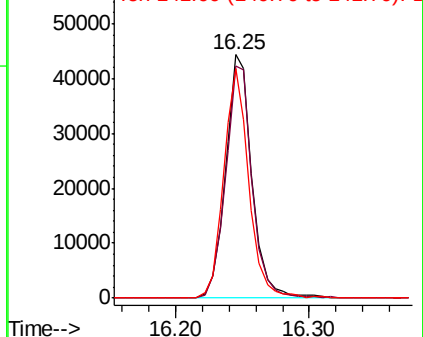




#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.37 min Scan# 1715
 Delta R.T. -0.02 min
 Lab File: BM016330.D
 Acq: 13 Aug 2018 17:59




Instrument :
 BNA_M
 ClientSampleId :
 SP-1-1

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.5	42.7
170	24.8	18.8	28.2

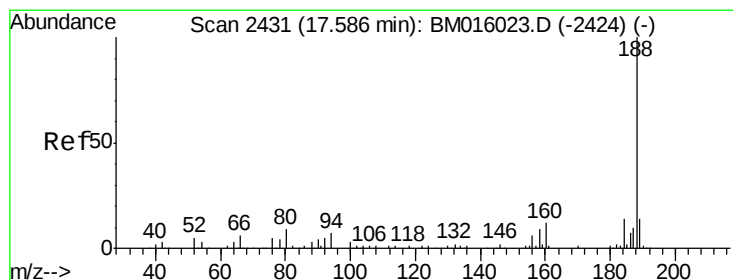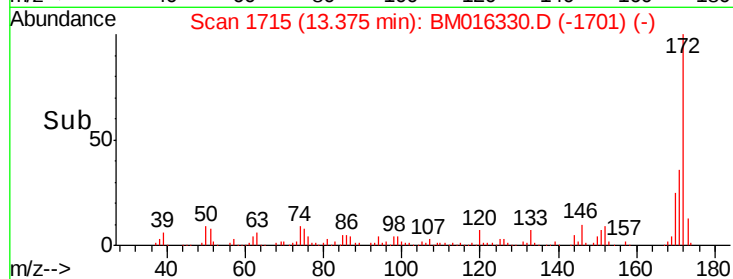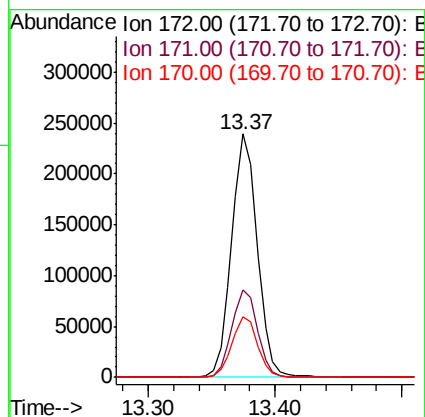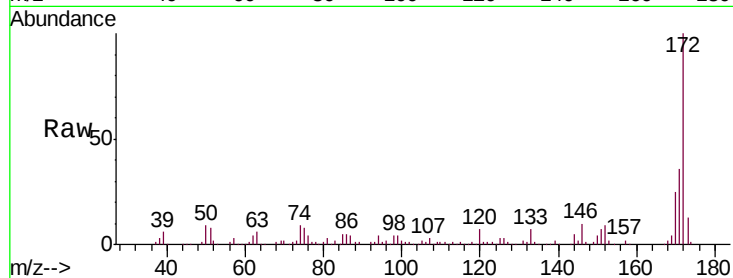

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.49 min Scan# 2415
 Delta R.T. -0.02 min
 Lab File: BM016330.D
 Acq: 13 Aug 2018 17:59

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.2	8.7	13.1#
80	7.6	9.3	13.9#

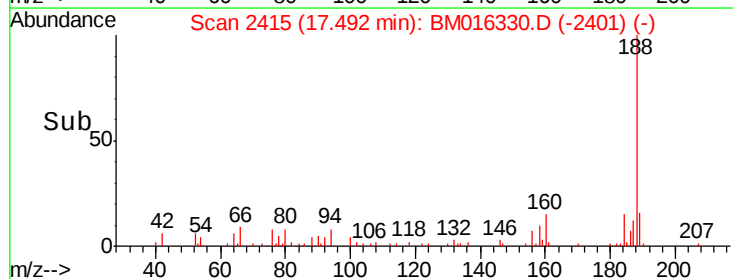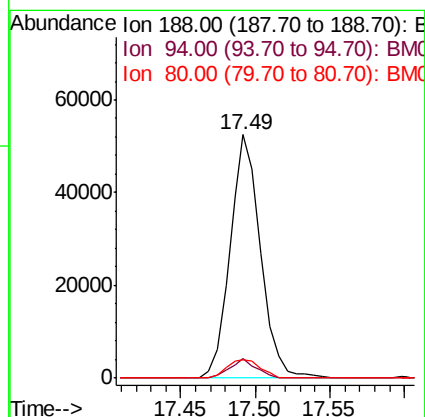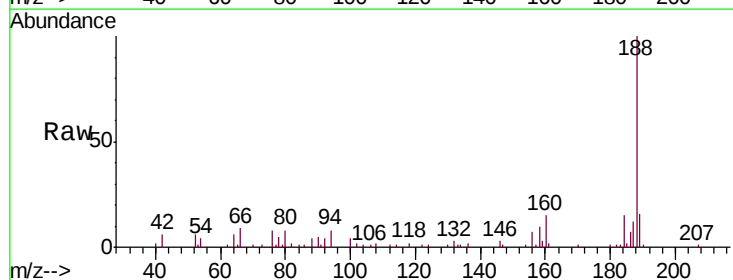



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.62 min Scan# 3117

Delta R.T. -0.02 min

Lab File: BM016330.D

Acq: 13 Aug 2018 17:59

Instrument :

BNA_M

ClientSampleId :

SP-1-1


Tgt Ion:240 Resp: 90038

Ion Ratio Lower Upper

240 100

120 7.1 8.2 12.2#




236 24.6 20.0 30.0

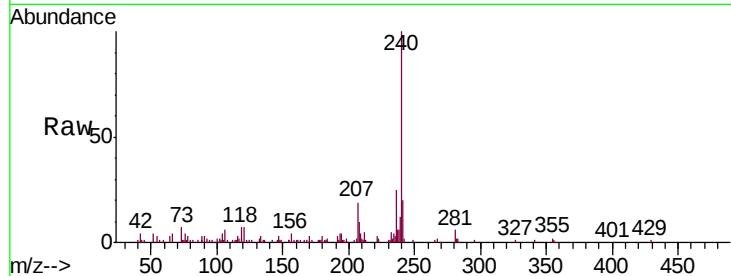

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

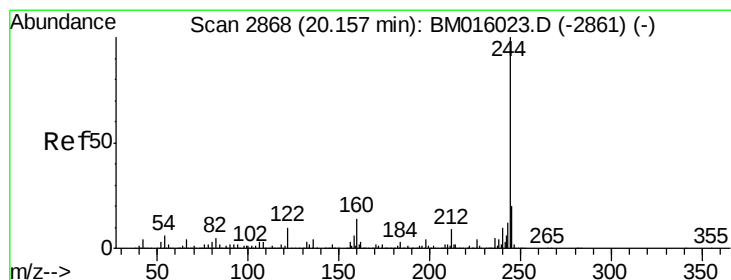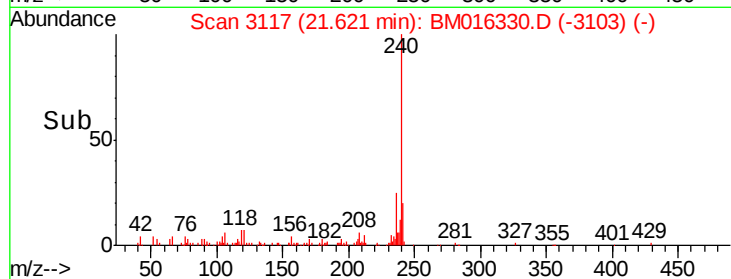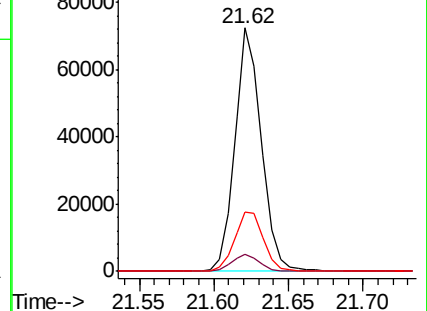

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.07 min Scan# 2854

Delta R.T. -0.01 min

Lab File: BM016330.D

Acq: 13 Aug 2018 17:59


Tgt Ion:244 Resp: 470478

Ion Ratio Lower Upper

244 100

212 10.8 4.9 7.3#



122 7.9 6.2 9.4

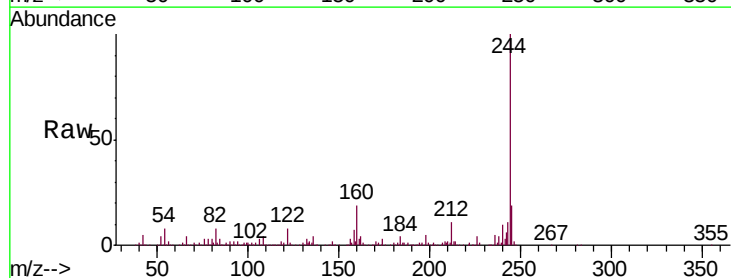


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

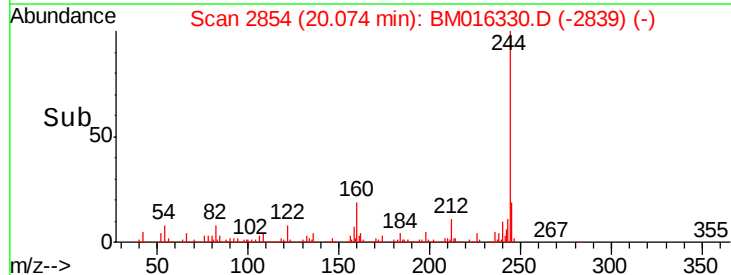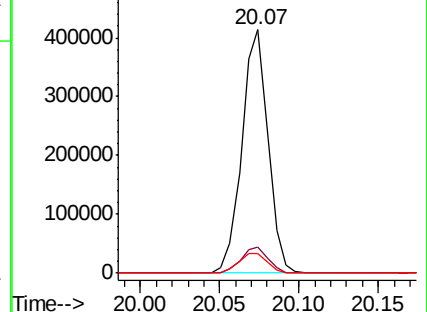


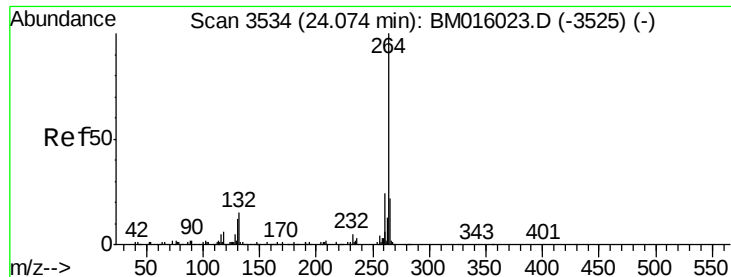

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.95 min Scan# 3513
Delta R.T. -0.02 min
Lab File: BM016330.D
Acq: 13 Aug 2018 17:59

Instrument :
BNA_M
ClientSampleId :
SP-1-1

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.4	18.6	27.8
265	22.5	17.3	25.9

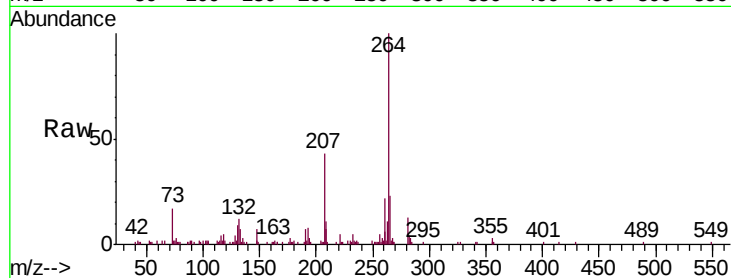

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

