

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
 Data File : BM016339.D
 Acq On : 14 Aug 2018 00:44
 Operator : SJ/JU
 Sample : J4442-50
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-5

Quant Time: Aug 14 03:55:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 10 18:44:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	26124	20.00	ng	-0.01
21) Naphthalene-d8	10.93	136	85470	20.00	ng	-0.02
38) Acenaphthene-d10	14.76	164	38718	20.00	ng	-0.01
63) Phenanthrene-d10	17.49	188	74751	20.00	ng	-0.02
75) Chrysene-d12	21.62	240	89308	20.00	ng	-0.02
86) Perylene-d12	23.95	264	107198	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	182693	116.17	ng	-0.01
7) Phenol-d6	7.29	99	180614	87.94	ng	-0.01
23) Nitrobenzene-d5	9.30	82	182719	99.43	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	56405	114.86	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	311832	97.99	ng	-0.02
78) Terphenyl-d14	20.07	244	449825	105.43	ng	-0.02
Target Compounds						
15) Benzyl Alcohol	8.44	79	4450	2.721	ng	Qvalue # 39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
Data File : BM016339.D
Acq On : 14 Aug 2018 00:44
Operator : SJ/JU
Sample : J4442-50
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-5

Quant Time: Aug 14 03:55:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 10 18:44:22 2018
Response via : Initial Calibration




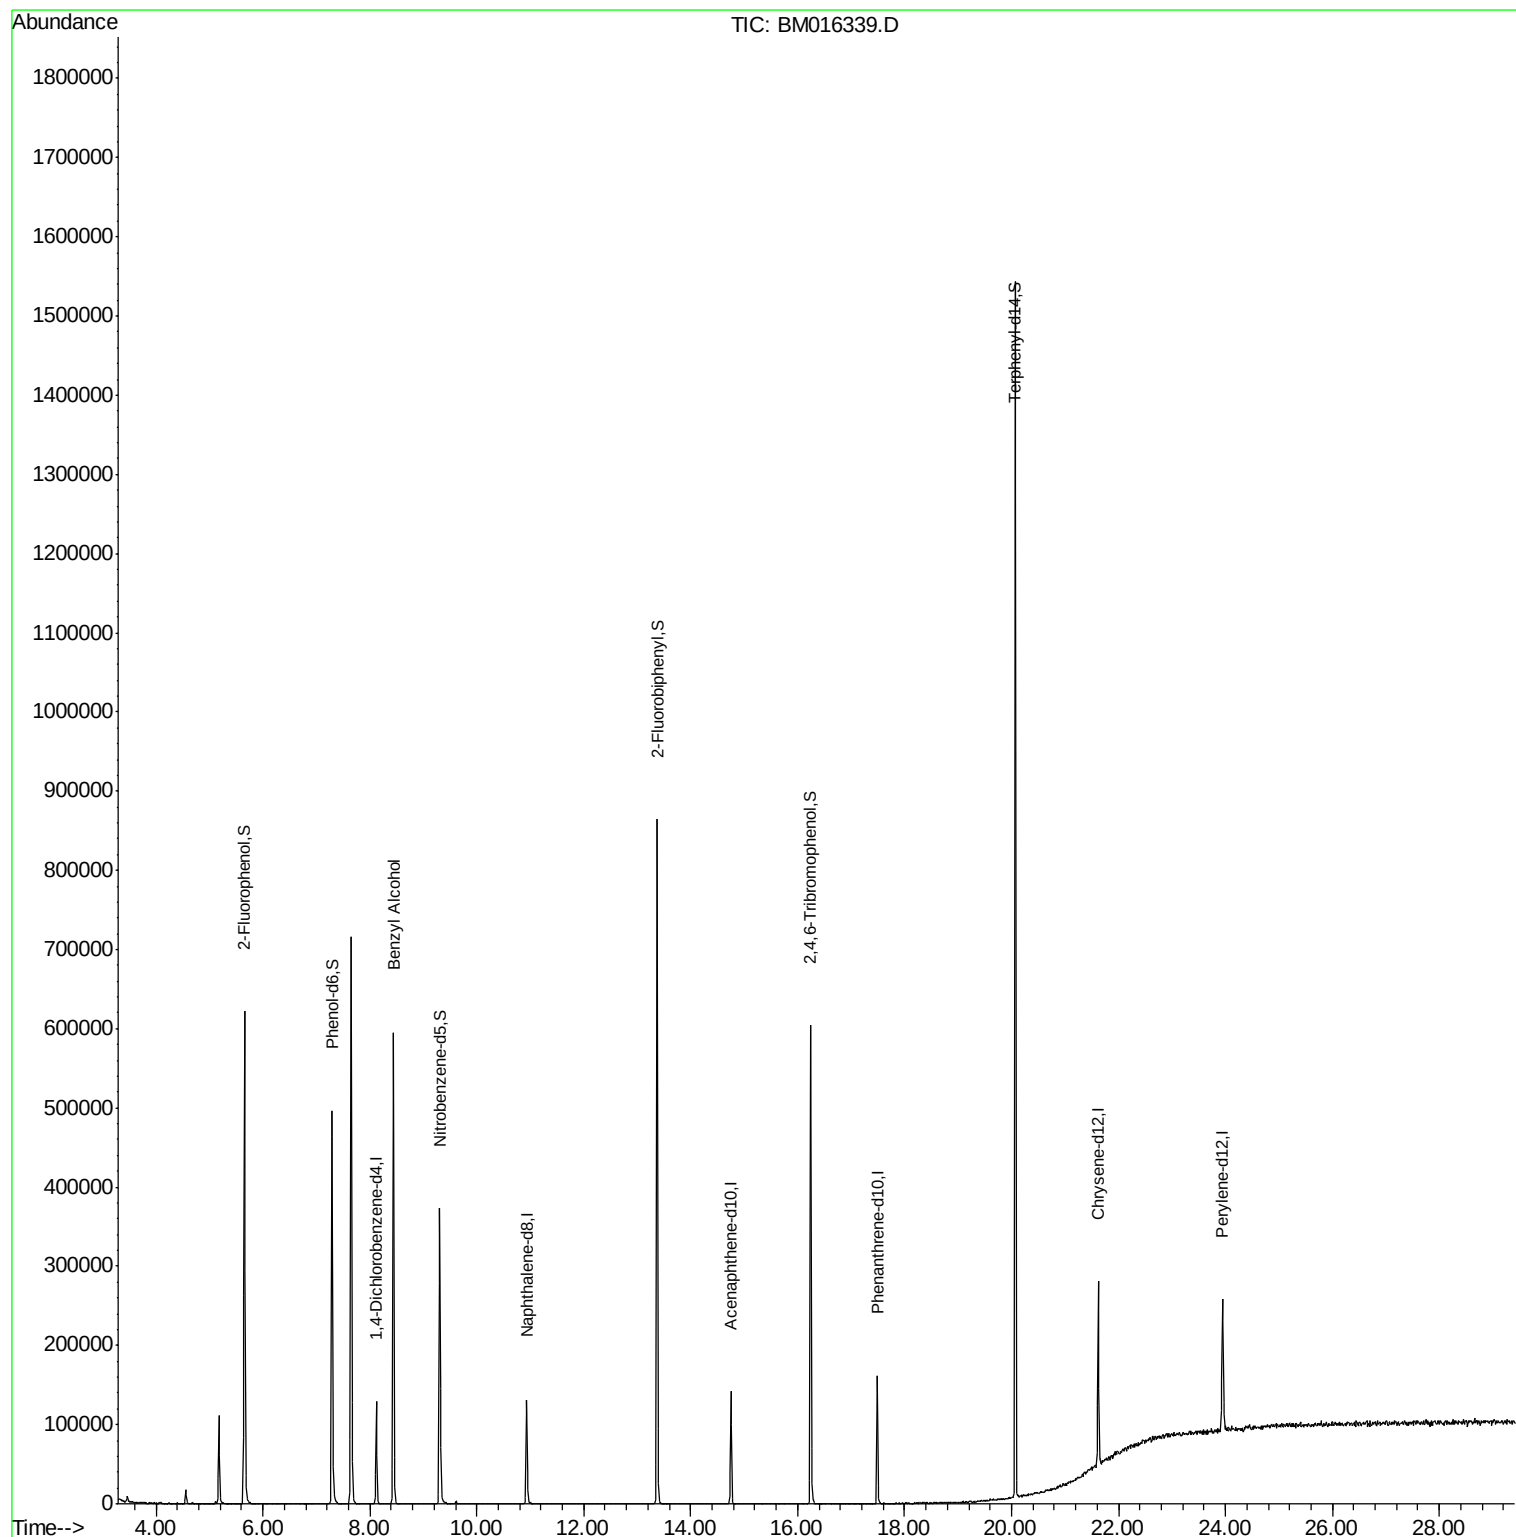


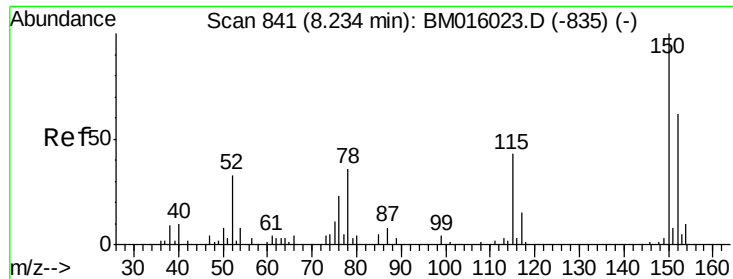

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.12 min Scan# 822
 Delta R.T. -0.01 min
 Lab File: BM016339.D
 Acq: 14 Aug 2018 00:44




Instrument :
 BNA_M
 ClientSampleId :
 SP-1-5


Tgt Ion:152 Resp: 26124
 Ion Ratio Lower Upper
 152 100
 150 149.3 119.5 179.3
 115 65.4 43.0 64.4#

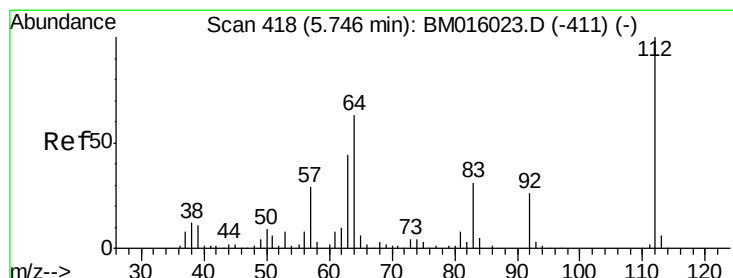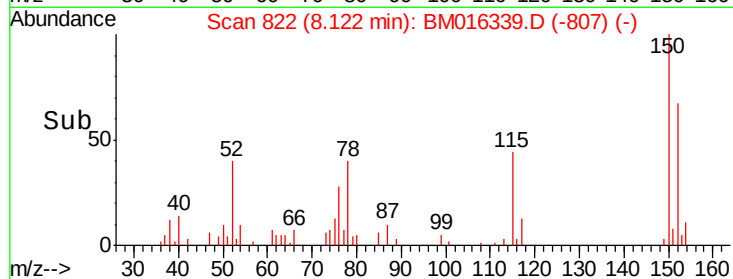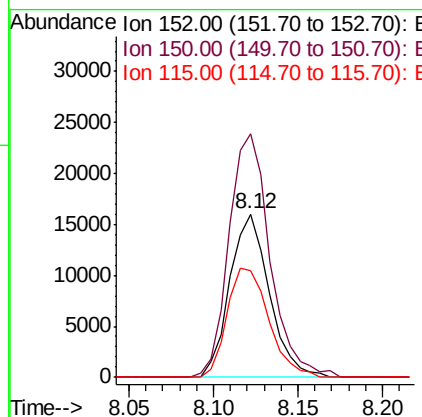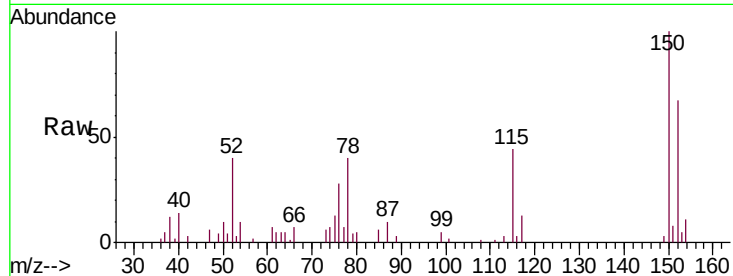

#5
 2-Fluorophenol
 Concen: N.D. ng
 RT: 5.65 min Scan# 402
 Delta R.T. -0.01 min
 Lab File: BM016339.D
 Acq: 14 Aug 2018 00:44

Tgt Ion:112 Resp: 182693
 Ion Ratio Lower Upper
 112 100
 64 62.7 38.6 57.8#
 63 50.0 19.3 28.9#

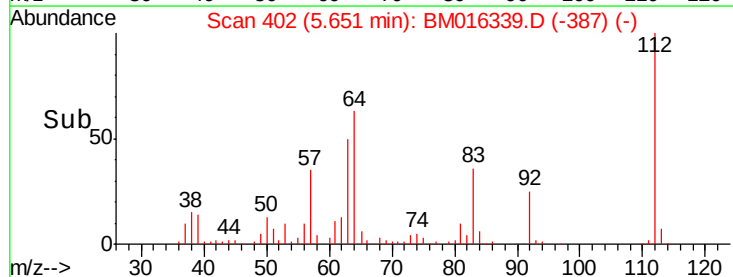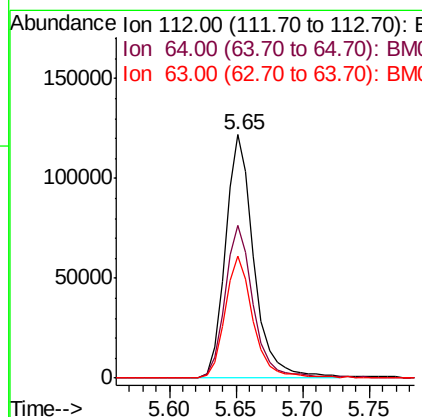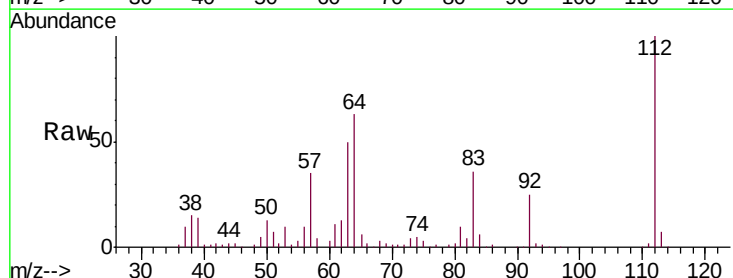

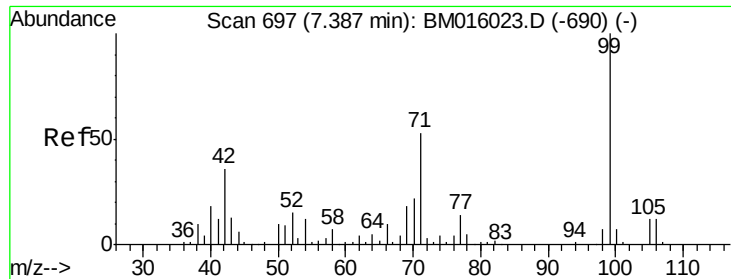

#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 681

Delta R.T. -0.01 min

Lab File: BM016339.D

Acq: 14 Aug 2018 00:44

Instrument :

BNA_M

ClientSampleId :

SP-1-5


Tgt Ion: 99 Resp: 180614

Ion Ratio Lower Upper

99 100

42 42.9 11.0 16.4#




71 61.5 23.4 35.2#

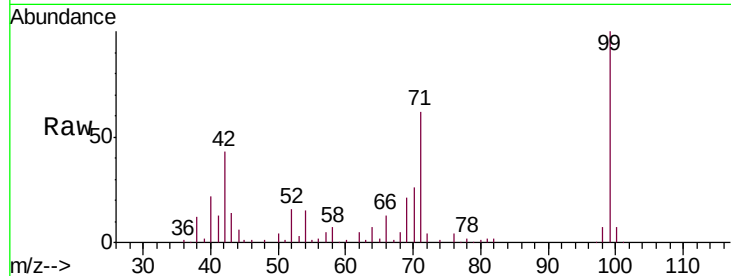

Abundance Ion 99.00 (98.70 to 99.70): BM016339.D (-666) (-)

Ion 42.00 (41.70 to 42.70): BM016339.D (-666) (-)

Ion 71.00 (70.70 to 71.70): BM016339.D (-666) (-)

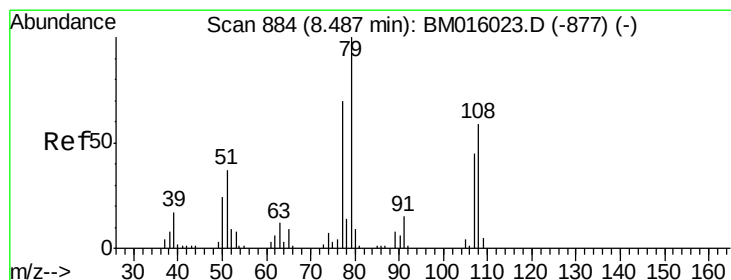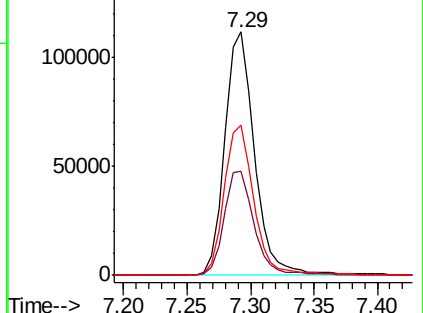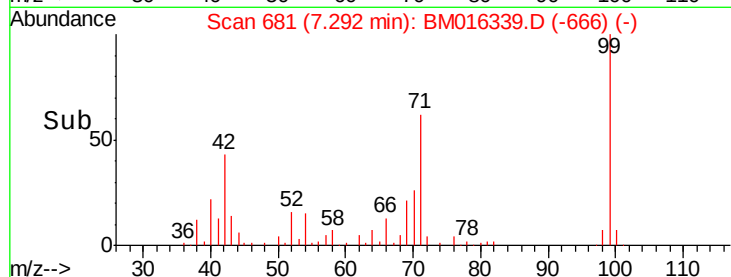

#15

Benzyl Alcohol

Concen: 2.721 ng

RT: 8.44 min Scan# 876

Delta R.T. 0.05 min

Lab File: BM016339.D

Acq: 14 Aug 2018 00:44


Tgt Ion: 79 Resp: 4450

Ion Ratio Lower Upper

79 100

108 80.1 65.0 97.4



77 173.9 53.0 79.6#

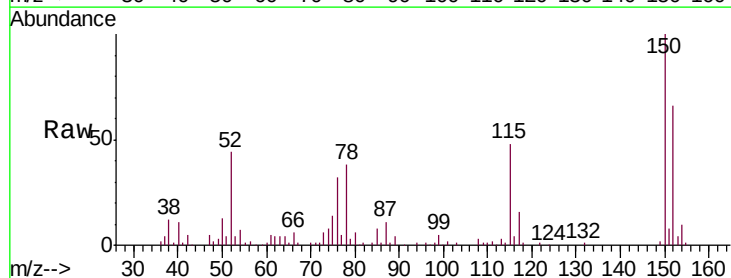


Abundance Ion 79.00 (78.70 to 79.70): BM016339.D (-851) (-)

Ion 108.00 (107.70 to 108.70): BM016339.D (-851) (-)

Ion 77.00 (76.70 to 77.70): BM016339.D (-851) (-)

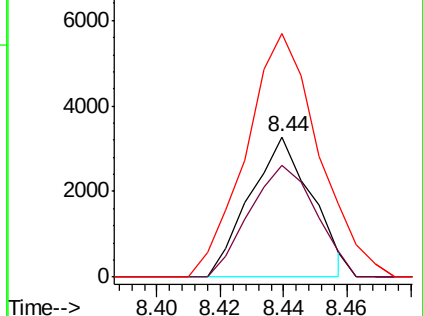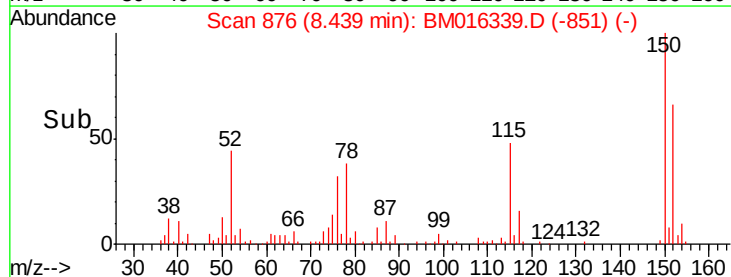


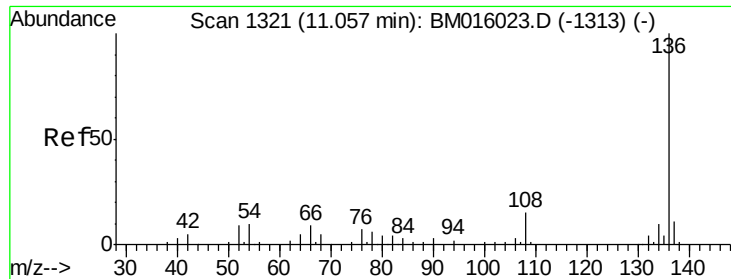




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1300
Delta R.T. -0.02 min
Lab File: BM016339.D
Acq: 14 Aug 2018 00:44

Instrument :
BNA_M
ClientSampleId :
SP-1-5

Tgt Ion: 136 Resp: 85470
Ion Ratio Lower Upper
136 100
137 10.9 8.7 13.1
54 10.7 4.6 6.8#
68 3.4 3.7 5.5#

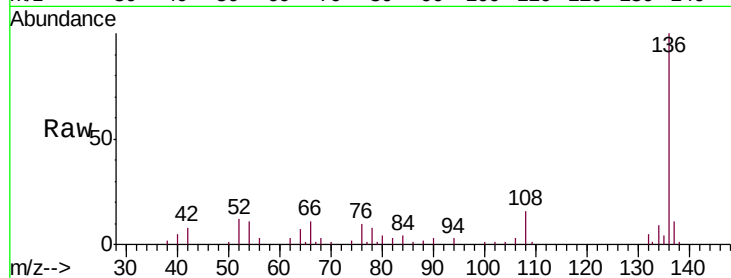


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

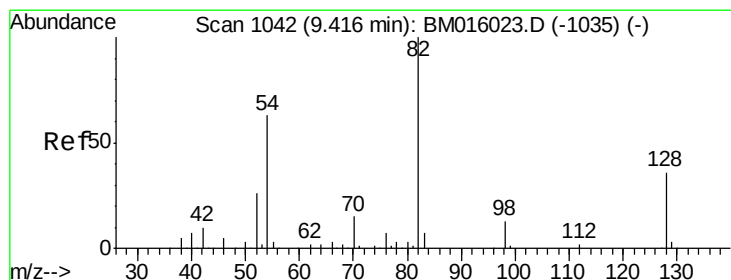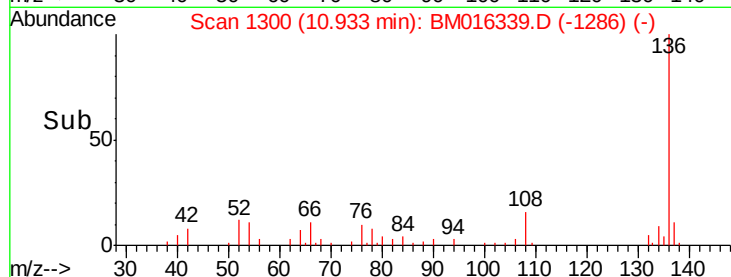
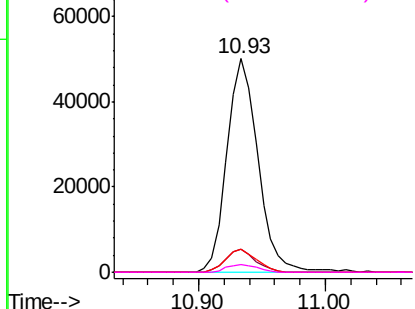



#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BM016339.D
Acq: 14 Aug 2018 00:44

Tgt Ion: 82 Resp: 182719
Ion Ratio Lower Upper
82 100
128 32.1 32.8 49.2#
54 66.0 40.6 60.8#

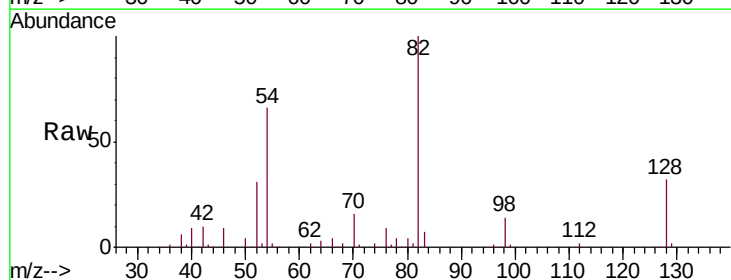

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

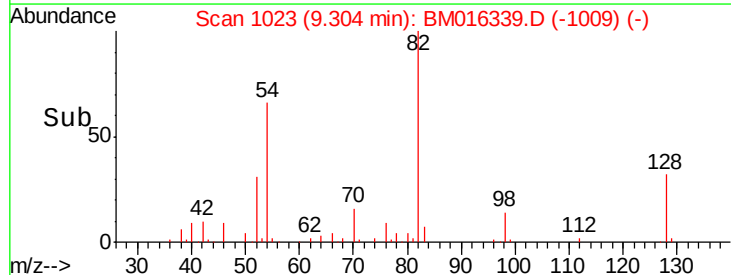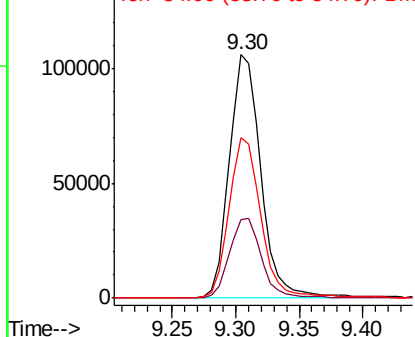

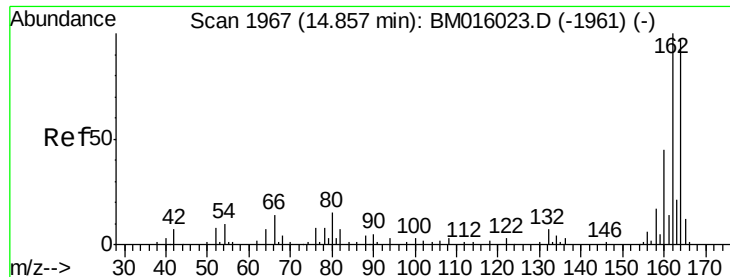

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.76 min Scan# 1950

Delta R.T. -0.01 min

Lab File: BM016339.D

Acq: 14 Aug 2018 00:44

Instrument :

BNA_M

ClientSampleId :

SP-1-5


Tgt Ion:164 Resp: 38718

Ion Ratio Lower Upper

164 100

162 111.3 82.4 123.6




160 50.3 35.8 53.6

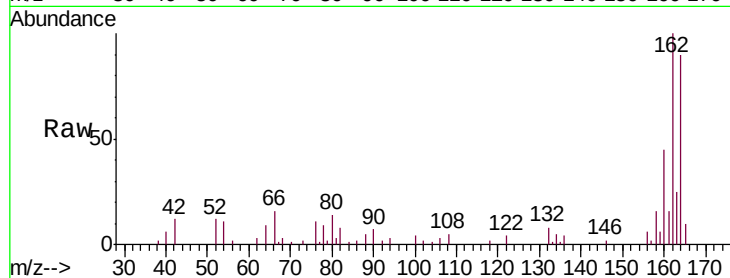

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

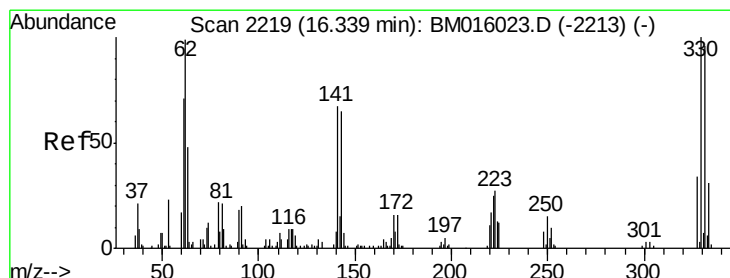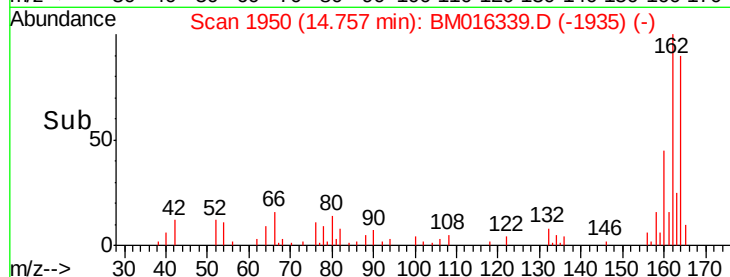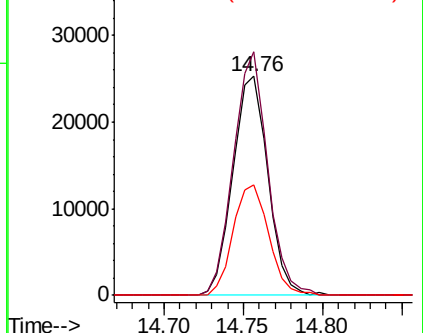

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.24 min Scan# 2203

Delta R.T. -0.02 min

Lab File: BM016339.D

Acq: 14 Aug 2018 00:44


Tgt Ion:330 Resp: 56405

Ion Ratio Lower Upper

330 100

332 95.8 0.0 0.0#



141 91.3 0.0 0.0#

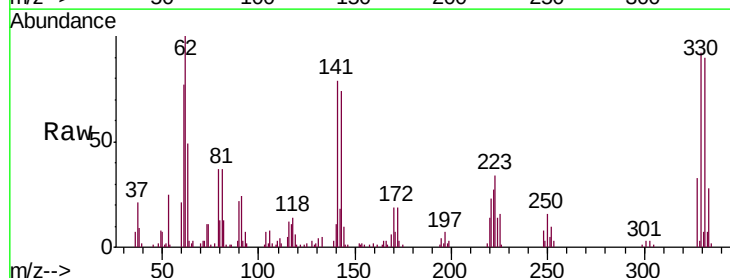


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



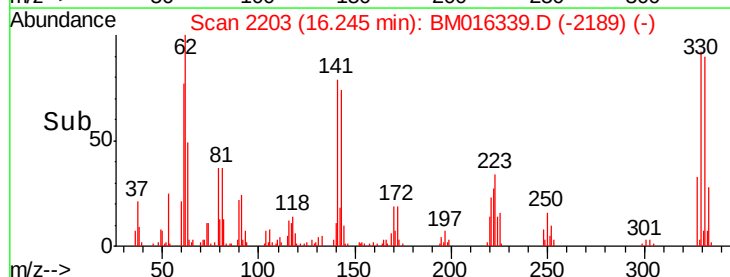
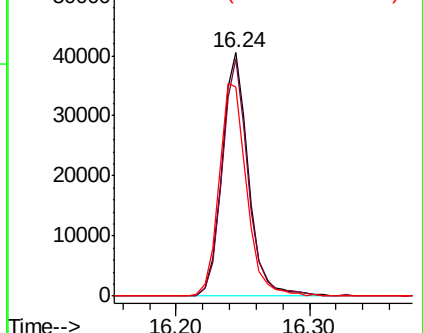


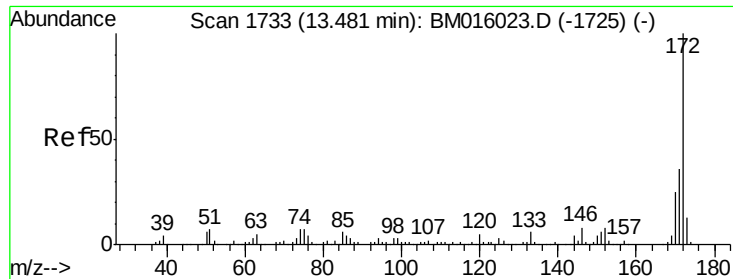

#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.37 min Scan# 1715
 Delta R.T. -0.02 min
 Lab File: BM016339.D
 Acq: 14 Aug 2018 00:44




Instrument :
 BNA_M
 ClientSampleId :
 SP-1-5


Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	28.5	42.7
170	24.2	18.8	28.2

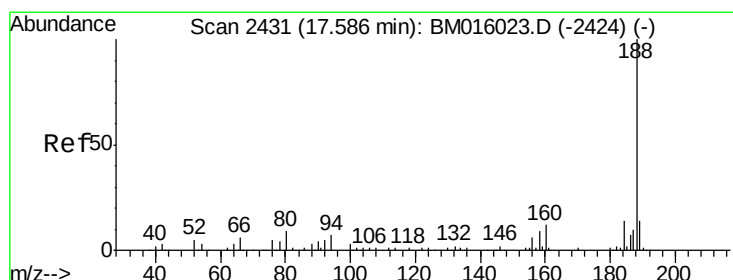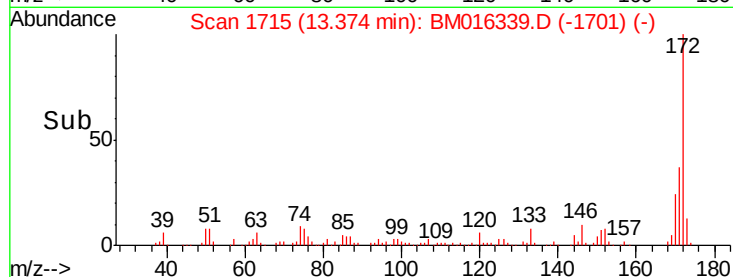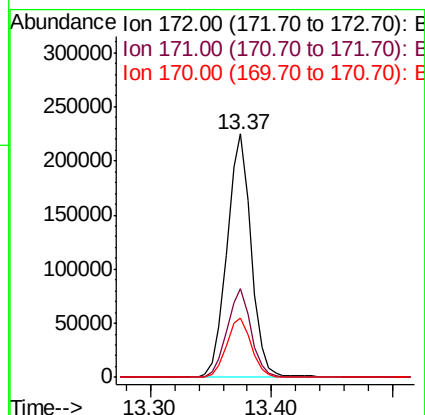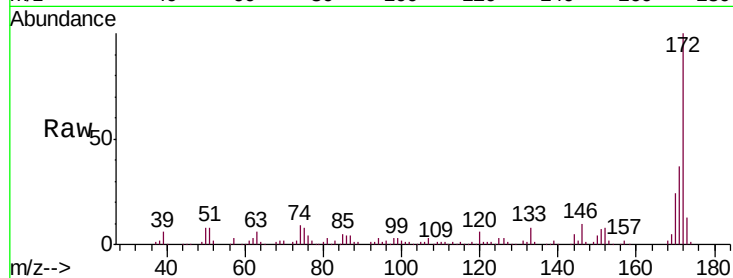

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.49 min Scan# 2415
 Delta R.T. -0.02 min
 Lab File: BM016339.D
 Acq: 14 Aug 2018 00:44

Tgt Ion	Ratio	Lower	Upper
188	100		
94	5.8	8.7	13.1#
80	7.4	9.3	13.9#


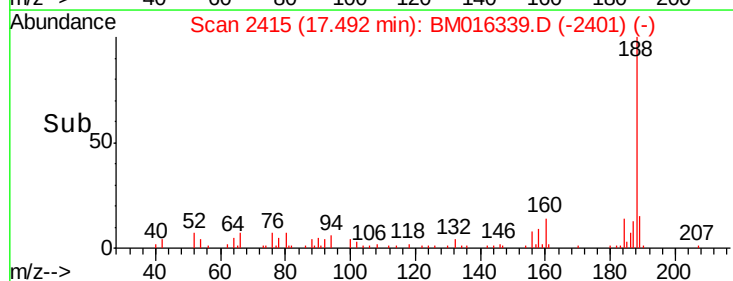
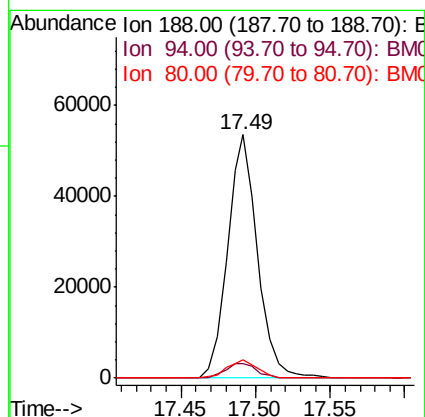
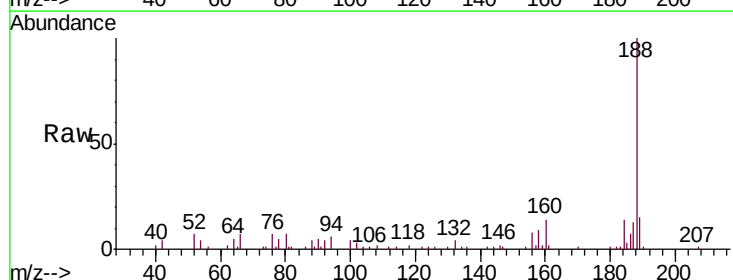


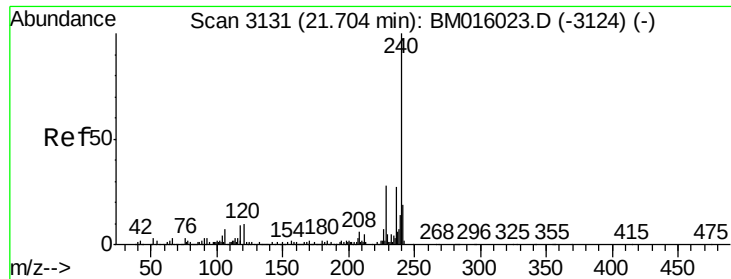

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.62 min Scan# 3117
Delta R.T. -0.02 min
Lab File: BM016339.D
Acq: 14 Aug 2018 00:44




Instrument :
BNA_M
ClientSampleId :
SP-1-5


Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.6	8.2	12.2#
236	27.2	20.0	30.0

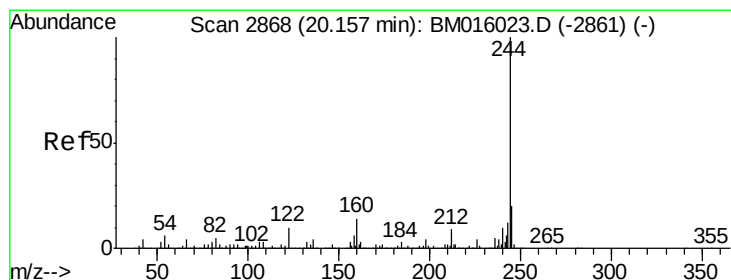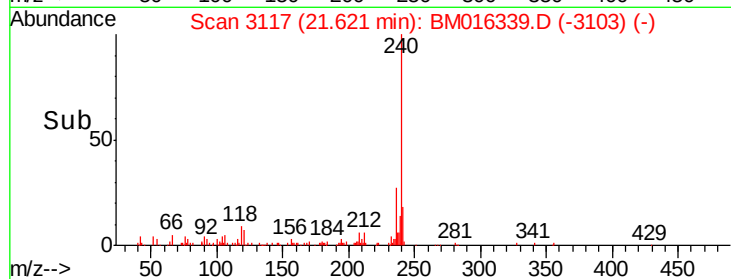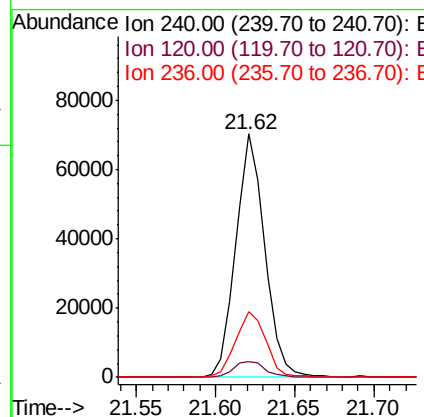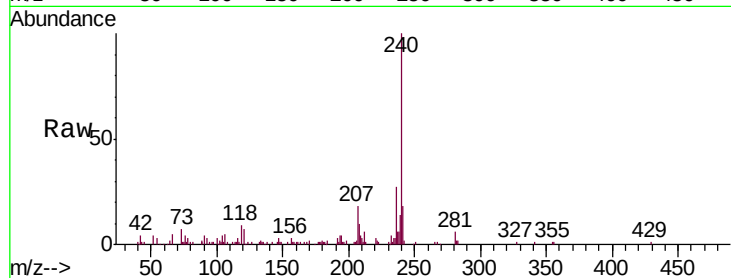

#78
Terphenyl-d14
Concen: N.D. ng
RT: 20.07 min Scan# 2853
Delta R.T. -0.02 min
Lab File: BM016339.D
Acq: 14 Aug 2018 00:44

Tgt Ion	Ratio	Lower	Upper
244	100		
212	11.1	4.9	7.3#
122	9.1	6.2	9.4

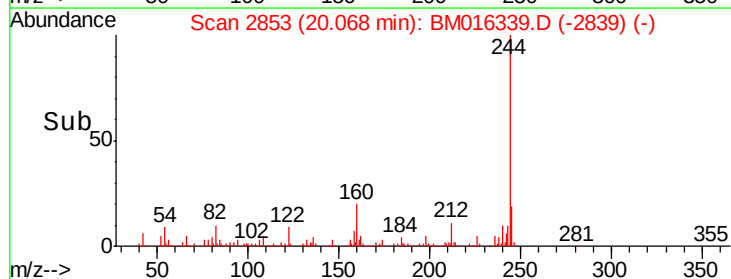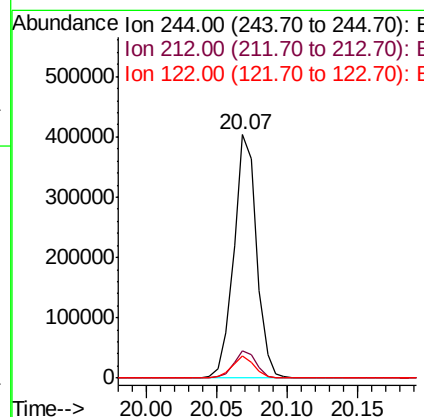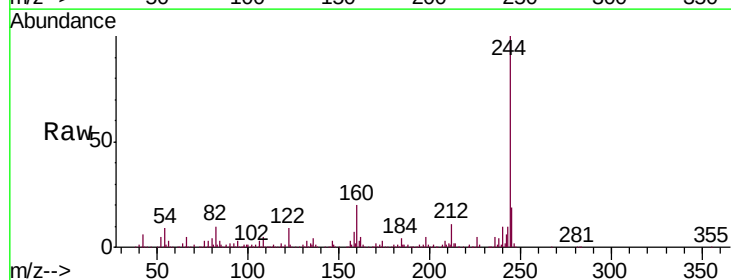


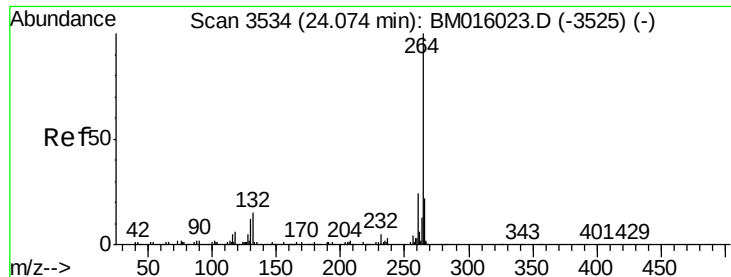

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.95 min Scan# 3513
Delta R.T. -0.02 min
Lab File: BM016339.D
Acq: 14 Aug 2018 00:44

Instrument :
BNA_M
ClientSampleId :
SP-1-5

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	18.6	27.8
265	23.0	17.3	25.9

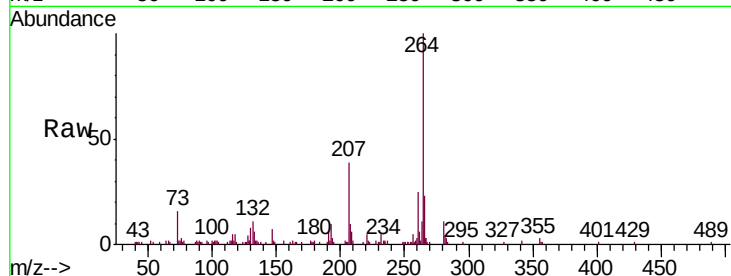

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

