
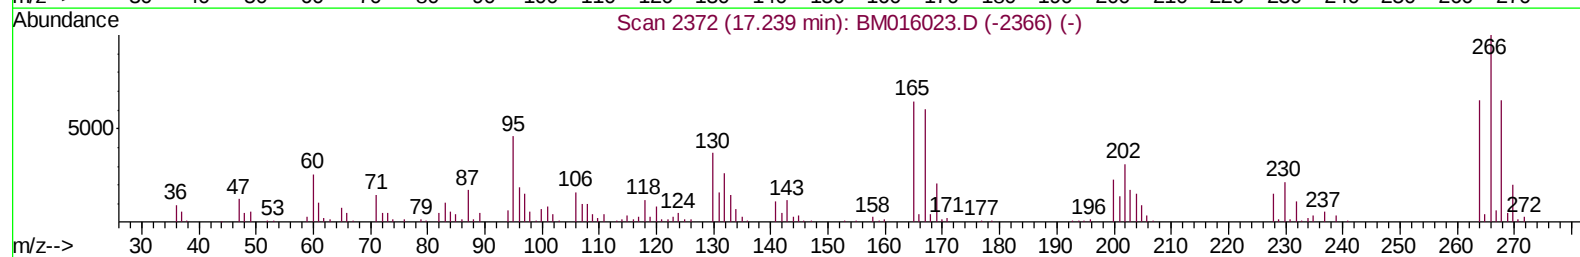
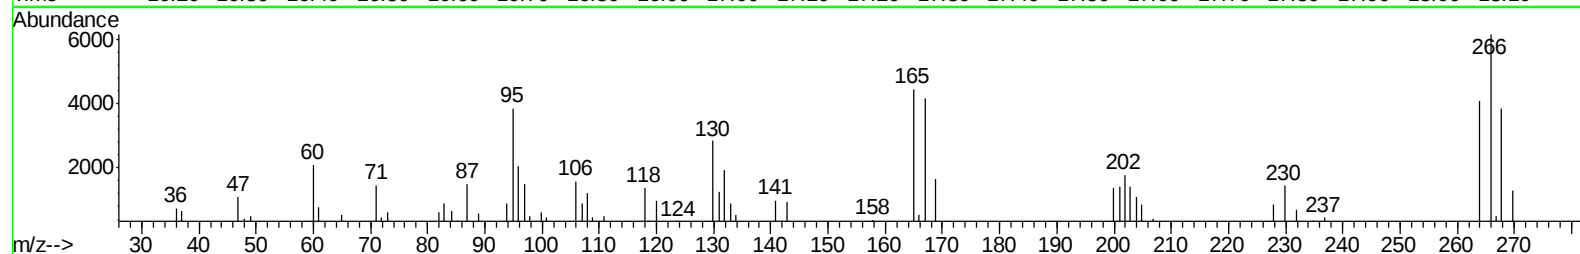


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
Data File : BM016317.D
Acq On : 13 Aug 2018 09:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 05:23:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 10 18:44:22 2018
Response via : Initial Calibration

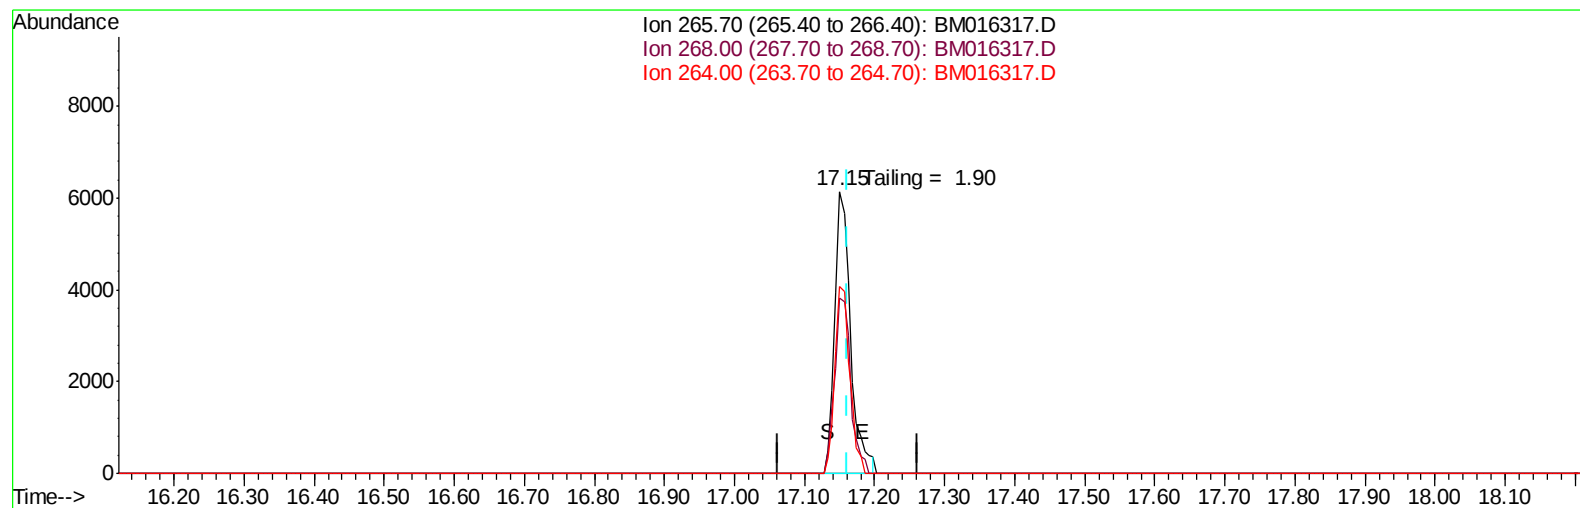

TIC: BM016317.D

(69) Pentachlorophenol (C)




17.151min (-0.012) 0.00ng

response 9653

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.47
264.00	61.20	66.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081318\
Data File : BM016317.D
Acq On : 13 Aug 2018 09:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 05:23:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 10 18:44:22 2018
Response via : Initial Calibration

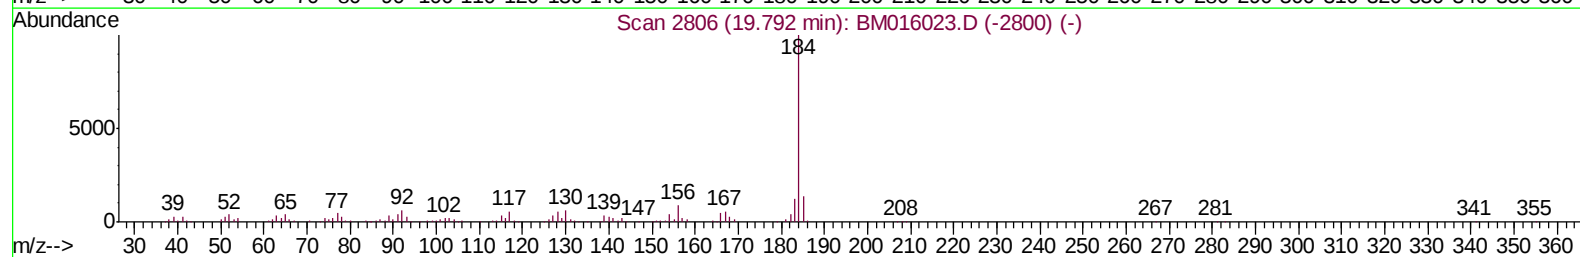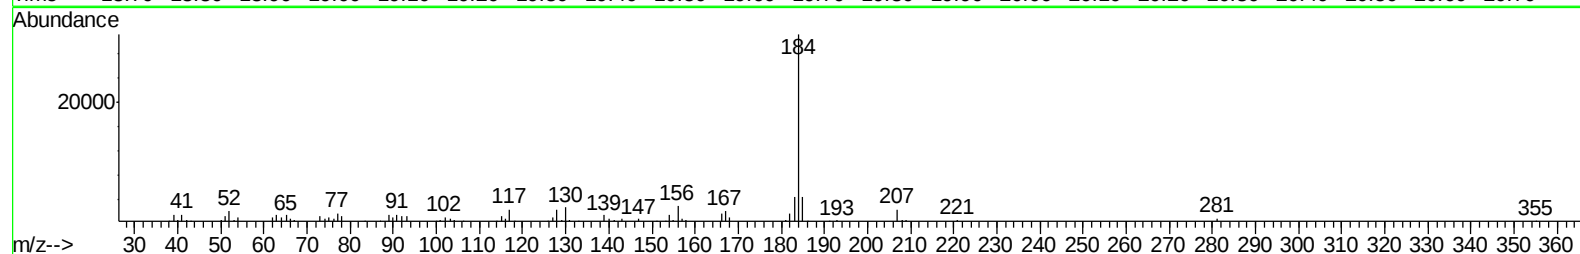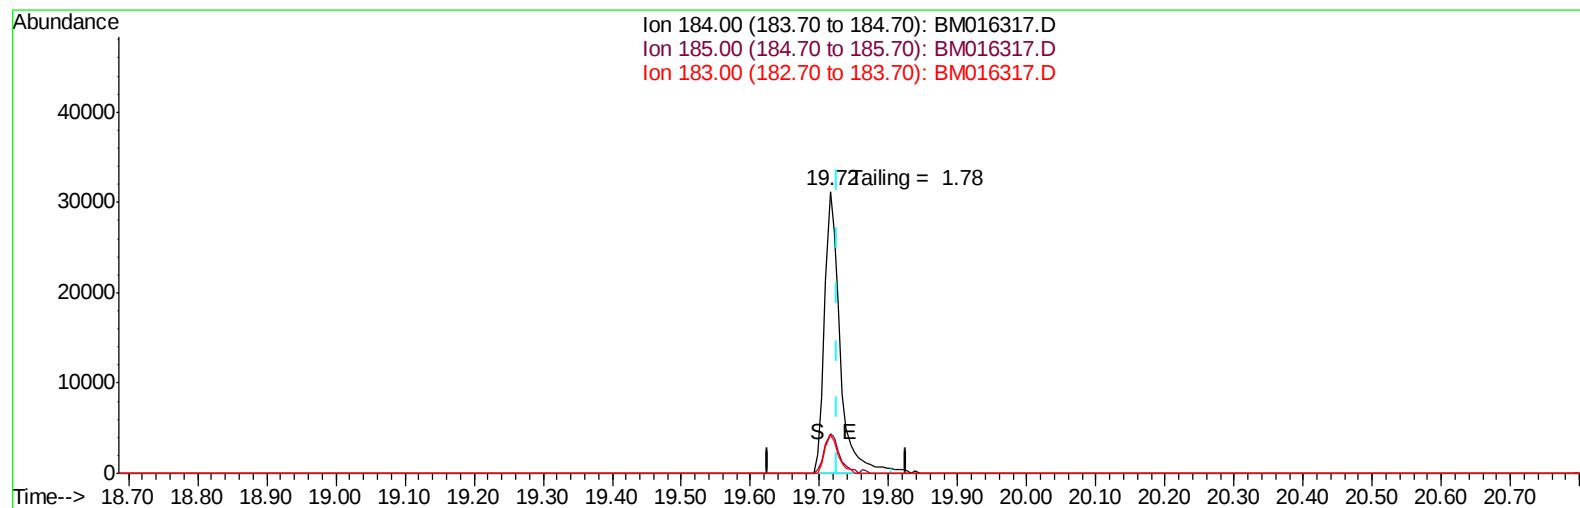

TIC: BM016317.D

(76) Benzidine

19.715min (-0.012) 0.00ng

response 47994

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.18
183.00	11.10	13.87#
0.00	0.00	0.00