


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081318\
 Data File : BM016317.D
 Acq On : 13 Aug 2018 09:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 10 18:44:22 2018

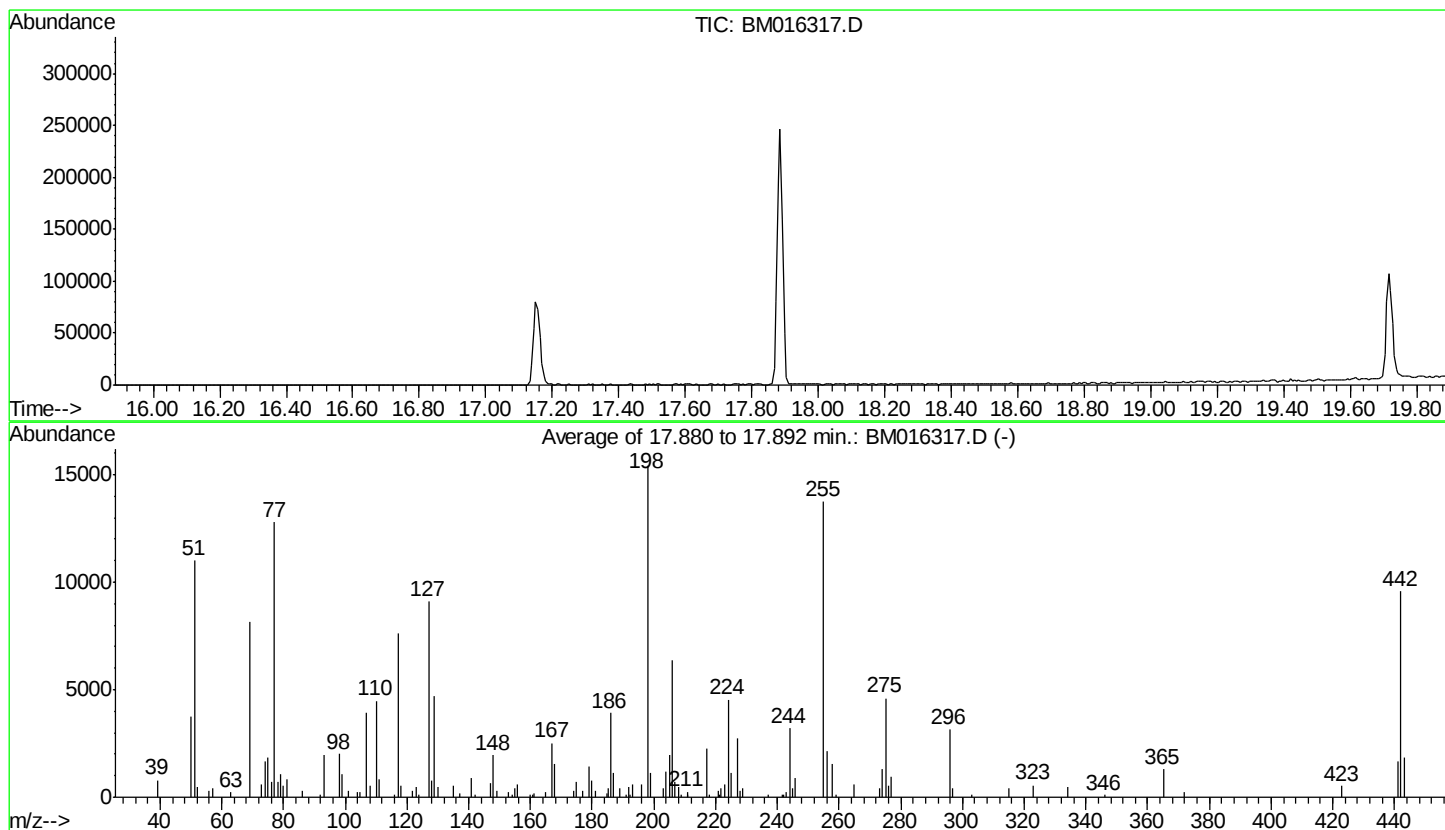

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.4	11010	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.0	8169	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.0	9096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15417	PASS
199	198	5	9	7.3	1119	PASS
275	198	10	60	29.7	4583	PASS
365	198	1	100	8.4	1290	PASS
441	198	0.01	100	10.8	1660	PASS
442	198	50	100	62.0	9561	PASS
443	442	15	24	19.6	1876	PASS