


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081318\
 Data File : BM016336.D
 Acq On : 13 Aug 2018 22:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 10 18:44:22 2018

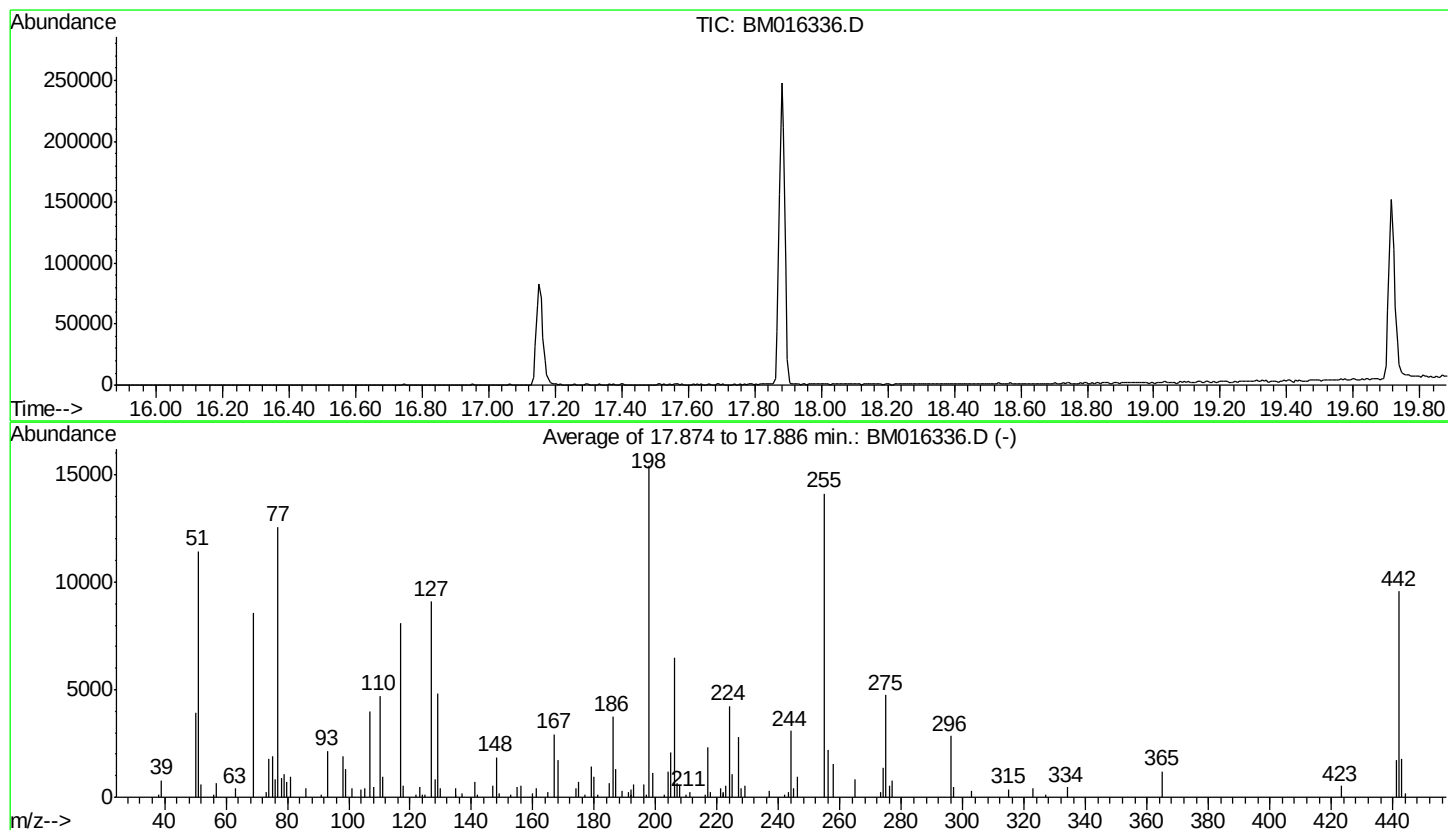

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	74.1	11421	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	55.5	8545	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.0	9097	PASS
197	198	0.00	2	0.6	100	PASS
198	198	100	100	100.0	15408	PASS
199	198	5	9	7.2	1117	PASS
275	198	10	60	30.8	4748	PASS
365	198	1	100	7.9	1212	PASS
441	198	0.01	100	11.0	1700	PASS
442	198	50	100	62.0	9555	PASS
443	442	15	24	18.8	1796	PASS