

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081418\
 Data File : BM016348.D
 Acq On : 14 Aug 2018 11:11
 Operator : SJ/JU
 Sample : J4447-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-7

Quant Time: Aug 15 11:29:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	22596	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	81745	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	40541	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	92241	20.00	ng	0.00
75) Chrysene-d12	21.62	240	110894	20.00	ng	0.00
86) Perylene-d12	23.95	264	115488	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	165294	121.51	ng	0.00
7) Phenol-d6	7.29	99	192466	108.34	ng	0.00
23) Nitrobenzene-d5	9.30	82	145603	82.85	ng	0.00
41) 2,4,6-Tribromophenol	16.24	330	59650	116.01	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	210050	63.04	ng	0.00
78) Terphenyl-d14	20.07	244	369557	69.76	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.44	79	3185	2.252	ng	Qvalue # 35
49) Dimethylphthalate	14.21	163	26591	7.495	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081418\
Data File : BM016348.D
Acq On : 14 Aug 2018 11:11
Operator : SJ/JU
Sample : J4447-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-7

Quant Time: Aug 15 11:29:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

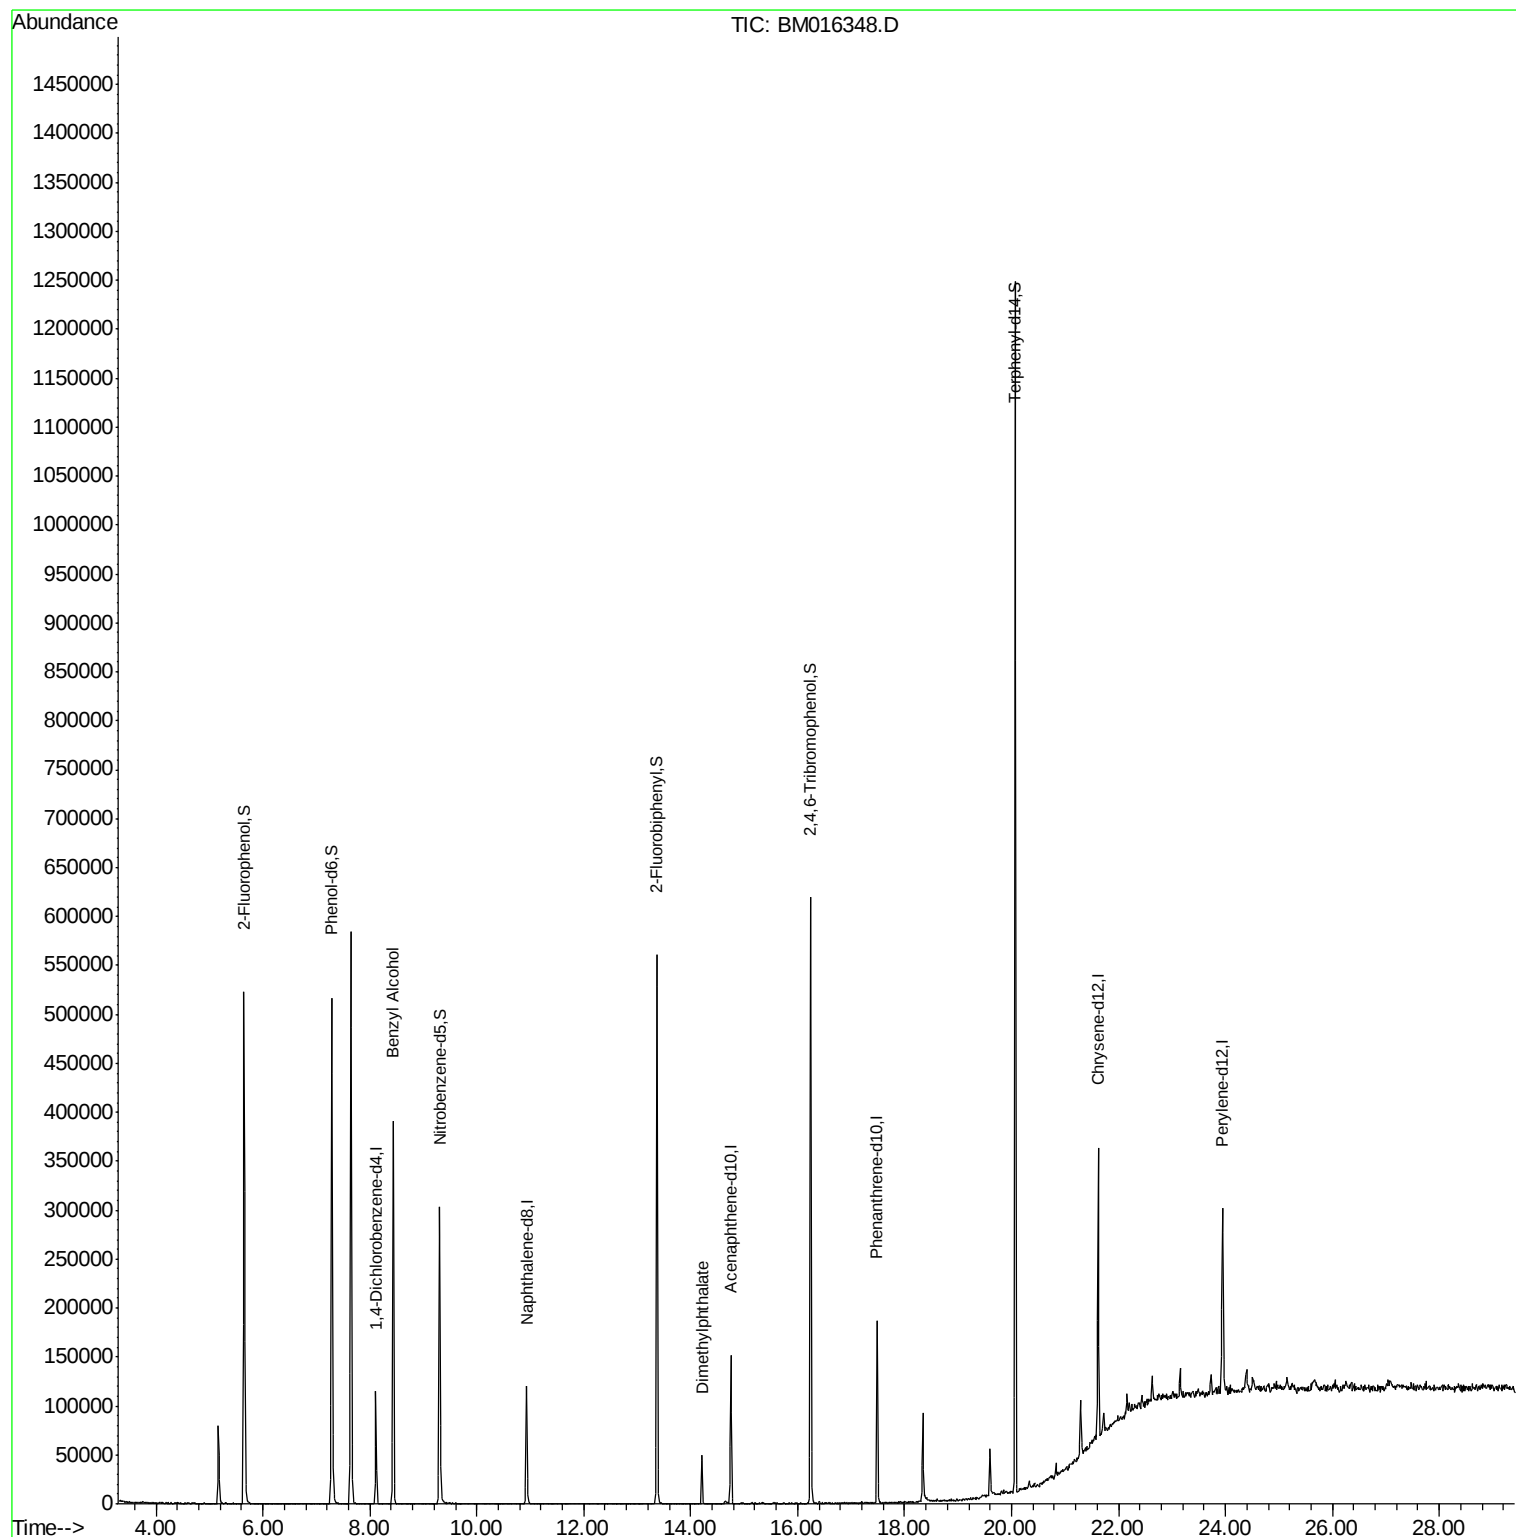

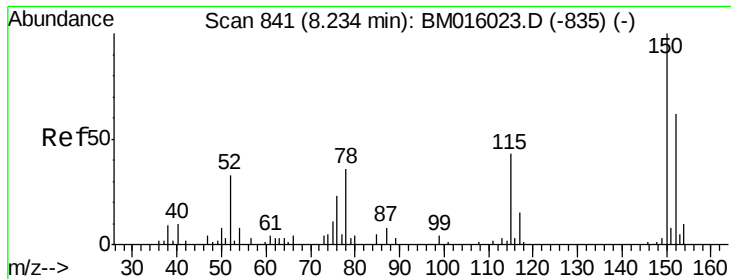


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 821
Delta R.T. -0.00 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Instrument :
BNA_M
ClientSampleId :
SP-1-7

Tgt Ion:152 Resp: 22596
Ion Ratio Lower Upper
152 100
150 155.8 119.5 179.3
115 70.5 43.0 64.4#

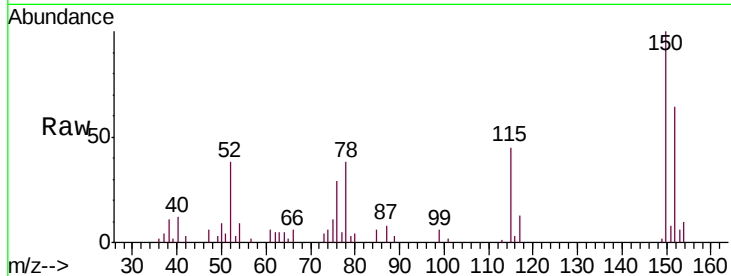


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

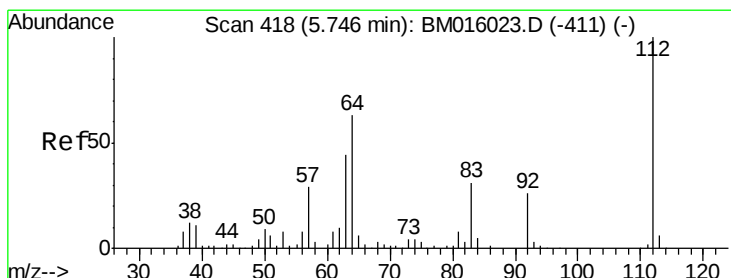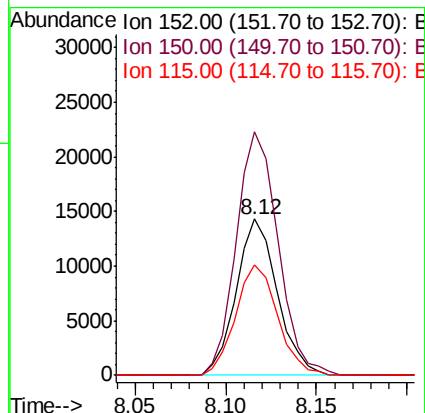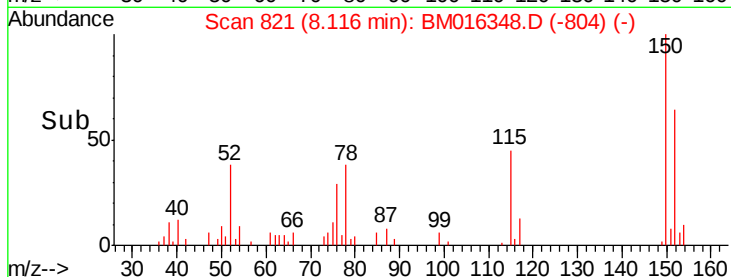



#5

2-Fluorophenol
Concen: N.D. ng
RT: 5.65 min Scan# 401
Delta R.T. -0.00 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Tgt Ion:112 Resp: 165294
Ion Ratio Lower Upper
112 100
64 61.9 38.6 57.8#
63 49.3 19.3 28.9#

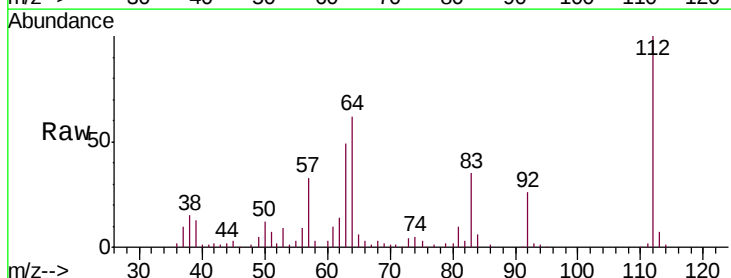

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM
Ion 63.00 (62.70 to 63.70): BM

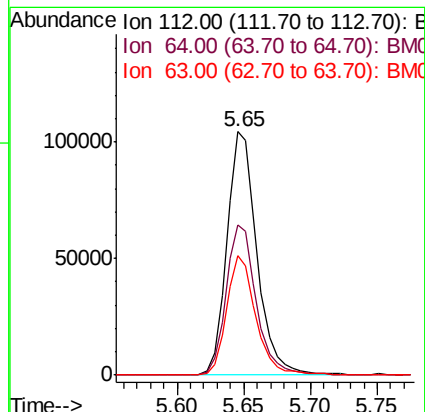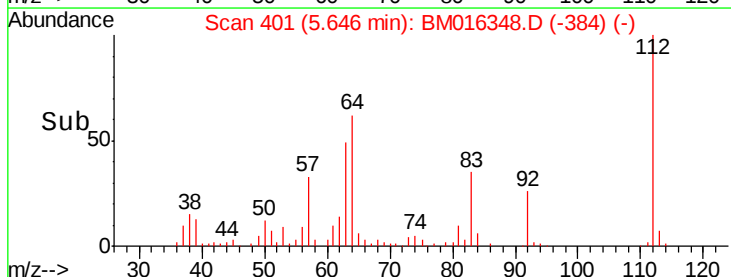



#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 680

Delta R.T. -0.00 min

Lab File: BM016348.D

Acq: 14 Aug 2018 11:11

Instrument :

BNA_M

ClientSampleId :

SP-1-7


Tgt Ion: 99 Resp: 192466

Ion Ratio Lower Upper

99 100

42 39.0 11.0 16.4#




71 58.4 23.4 35.2#

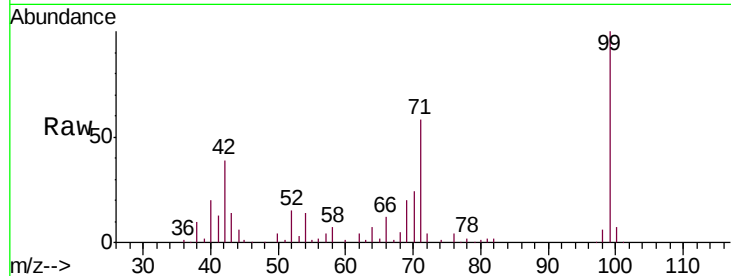

Abundance Ion 99.00 (98.70 to 99.70): BM016348.D (-663) (-)

Ion 42.00 (41.70 to 42.70): BM016348.D (-663) (-)

Ion 71.00 (70.70 to 71.70): BM016348.D (-663) (-)

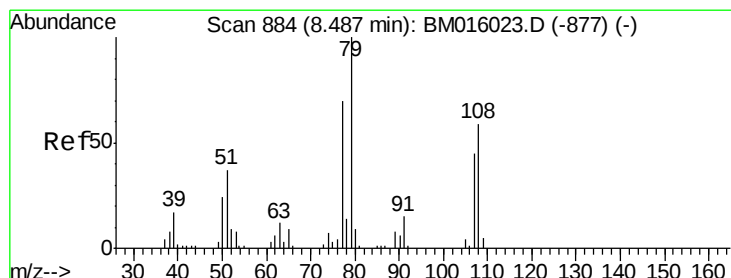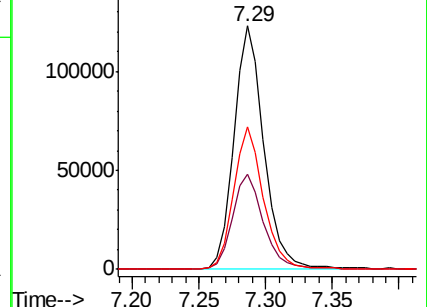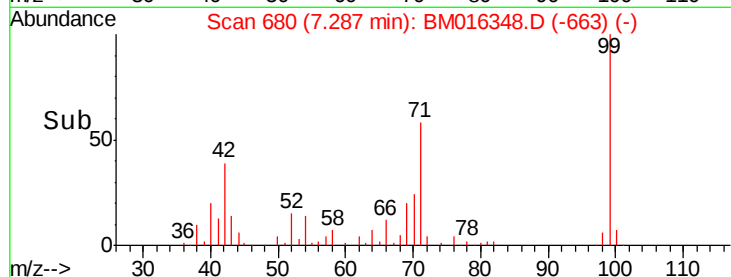

#15

Benzyl Alcohol

Concen: 2.252 ng

RT: 8.44 min Scan# 876

Delta R.T. 0.06 min

Lab File: BM016348.D

Acq: 14 Aug 2018 11:11


Tgt Ion: 79 Resp: 3185

Ion Ratio Lower Upper

79 100

108 84.4 65.0 97.4



77 177.6 53.0 79.6#

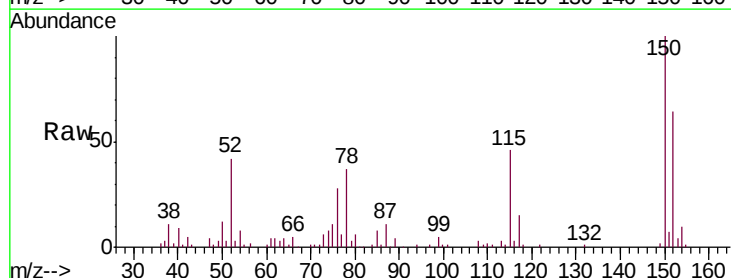

Abundance Ion 79.00 (78.70 to 79.70): BM016348.D (-848) (-)

Ion 108.00 (107.70 to 108.70): BM016348.D (-848) (-)

Ion 77.00 (76.70 to 77.70): BM016348.D (-848) (-)



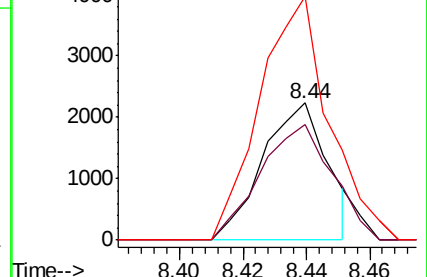
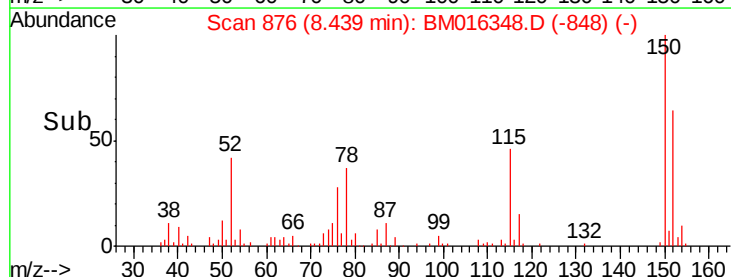




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1300
Delta R.T. 0.01 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11




Instrument :
BNA_M
ClientSampleId :
SP-1-7

Tgt Ion: 136 Resp: 81745
Ion Ratio Lower Upper
136 100
137 10.5 8.7 13.1
54 10.9 4.6 6.8#
68 3.4 3.7 5.5#

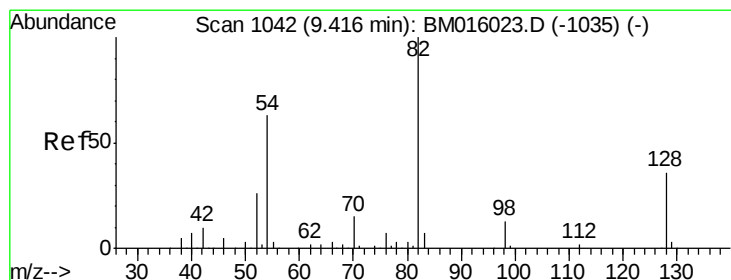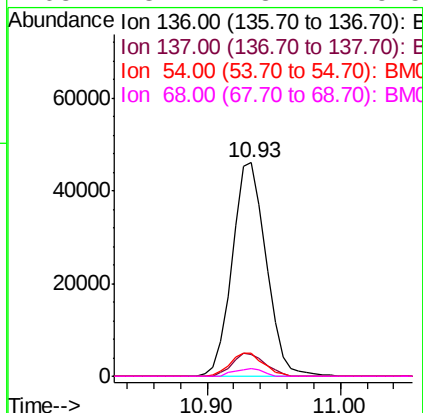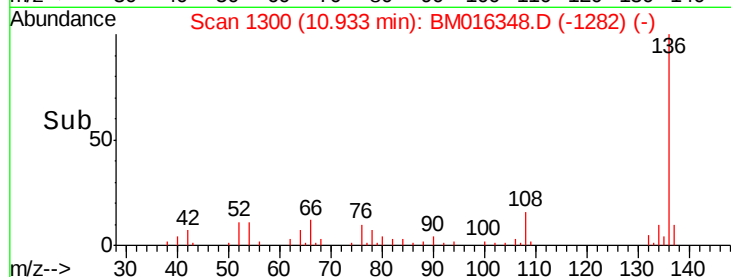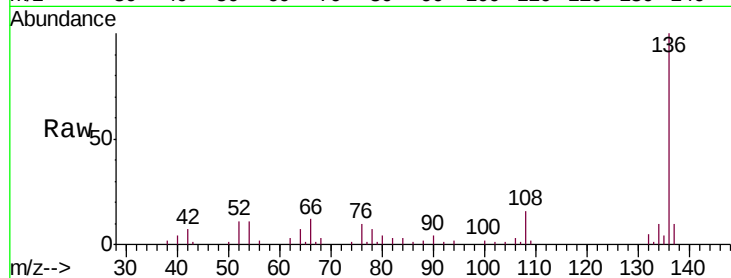

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.00 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Tgt Ion: 82 Resp: 145603
Ion Ratio Lower Upper
82 100
128 37.2 32.8 49.2
54 65.4 40.6 60.8#

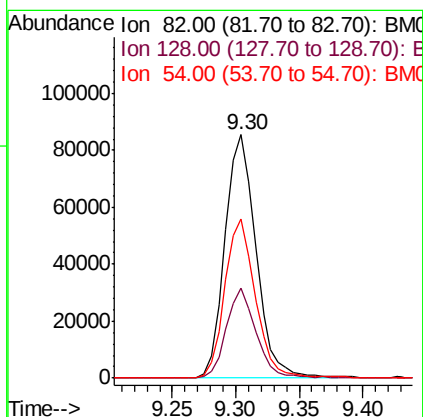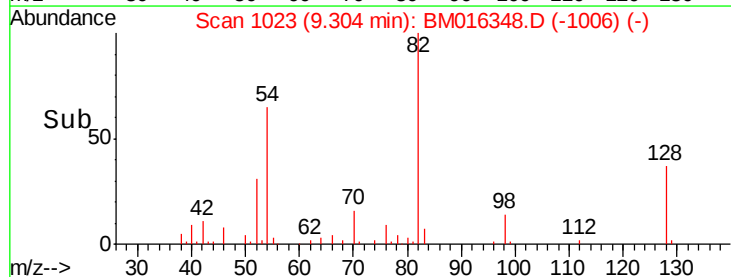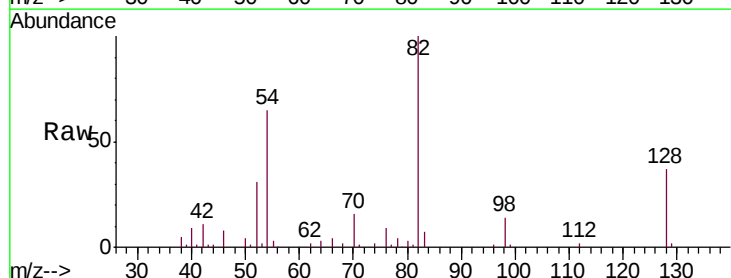



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.75 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BM016348.D

Acq: 14 Aug 2018 11:11

Instrument :

BNA_M

ClientSampleId :

SP-1-7


Tgt Ion:164 Resp: 40541

Ion Ratio Lower Upper

164 100

162 110.4 82.4 123.6




160 50.6 35.8 53.6

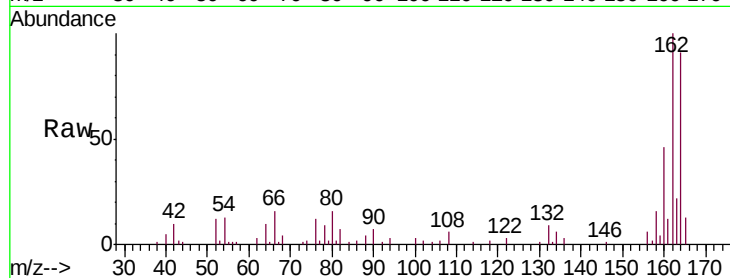

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

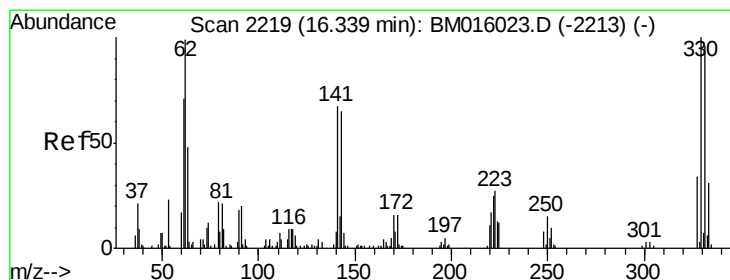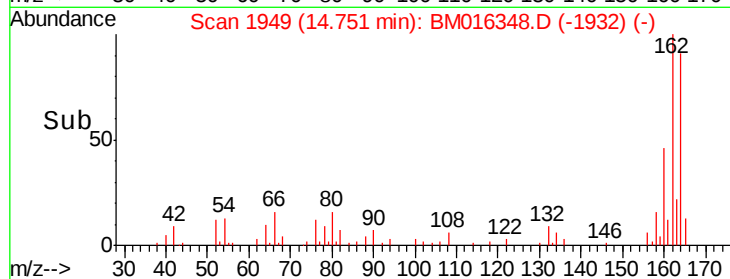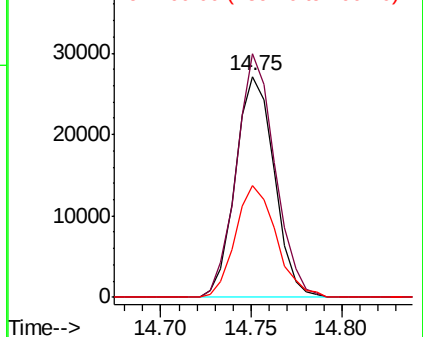

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.24 min Scan# 2203

Delta R.T. -0.00 min

Lab File: BM016348.D

Acq: 14 Aug 2018 11:11


Tgt Ion:330 Resp: 59650

Ion Ratio Lower Upper

330 100

332 96.2 0.0 0.0#



141 85.7 0.0 0.0#

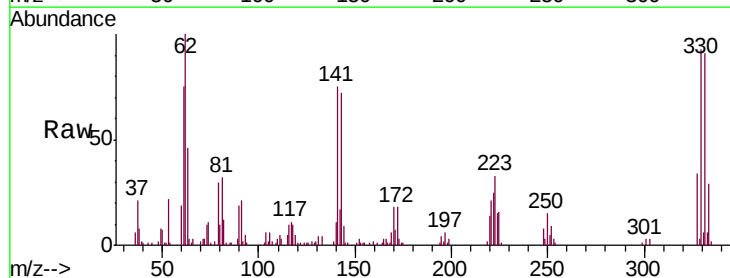

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

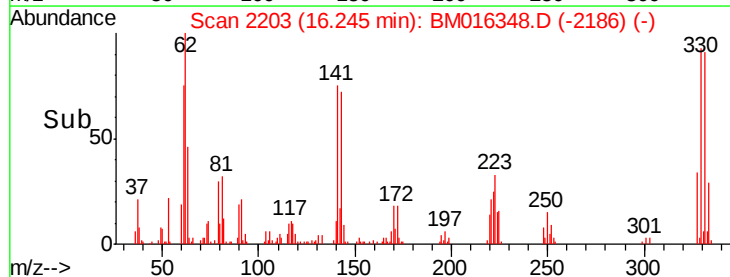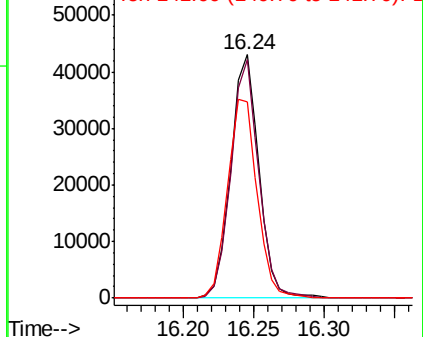







#44
2-Fluorobiphenyl
Concen: N.D. ng
RT: 13.37 min Scan# 1714
Delta R.T. -0.01 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Instrument :
BNA_M
ClientSampleId :
SP-1-7

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	28.5	42.7
170	24.3	18.8	28.2

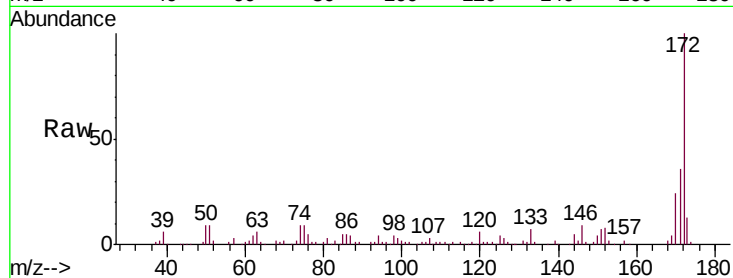


Abundance Ion 172.00 (171.70 to 172.70): E
200000
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

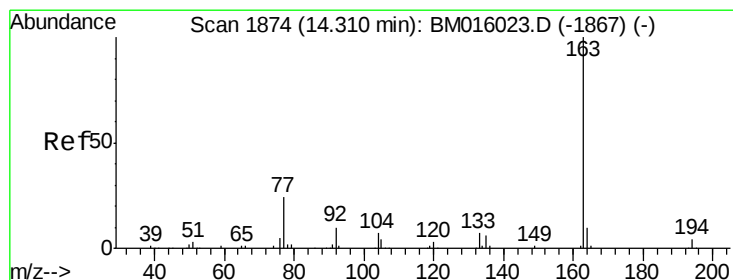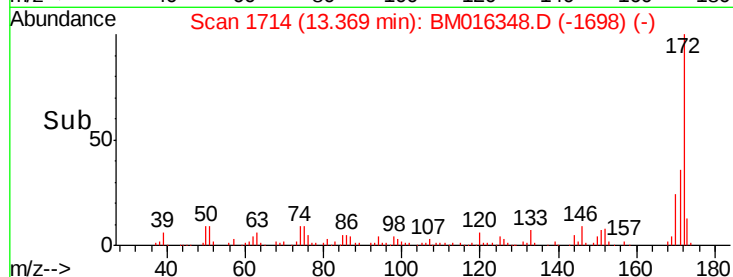
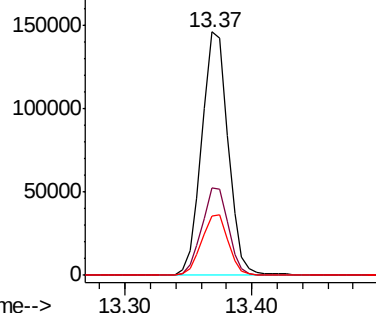



#49
Dimethylphthalate
Concen: 7.495 ng
RT: 14.21 min Scan# 1857
Delta R.T. -0.00 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Tgt Ion	Ratio	Lower	Upper
163	100		
194	2.6	2.7	4.1#
164	8.5	8.2	12.2

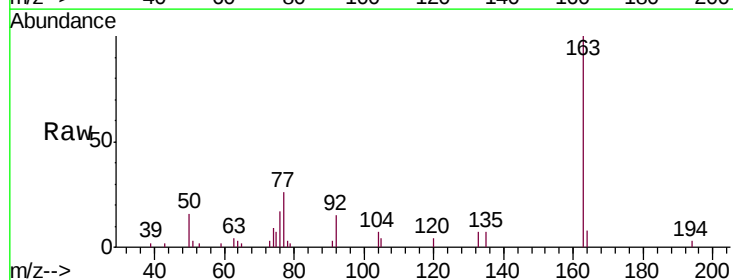

Abundance Ion 163.00 (162.70 to 163.70): E
25000
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

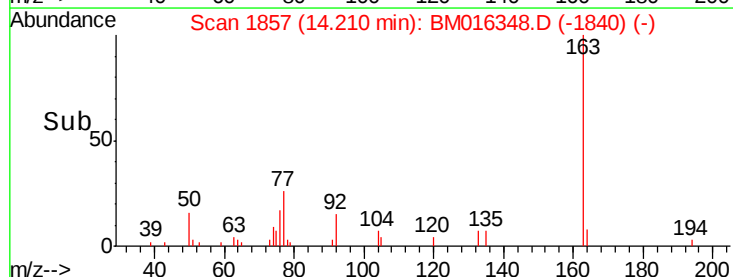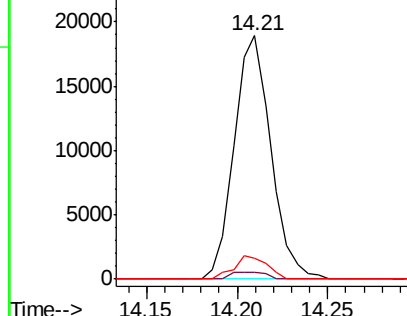


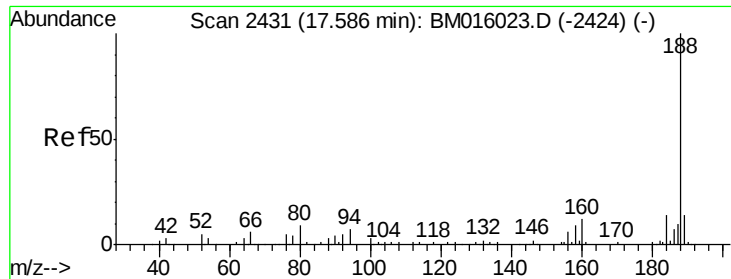




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.49 min Scan# 2414
Delta R.T. -0.01 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Instrument :
BNA_M
ClientSampleId :
SP-1-7

Tgt Ion:188 Resp: 92241
Ion Ratio Lower Upper
188 100
94 6.7 8.7 13.1#
80 7.1 9.3 13.9#

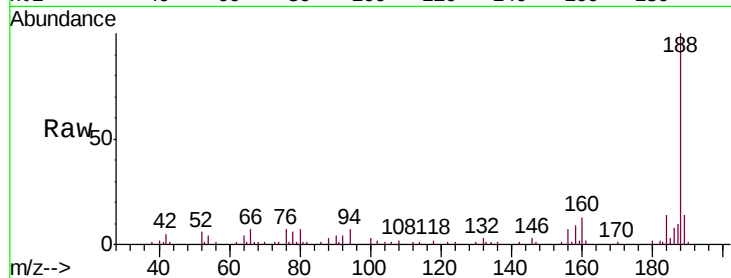


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

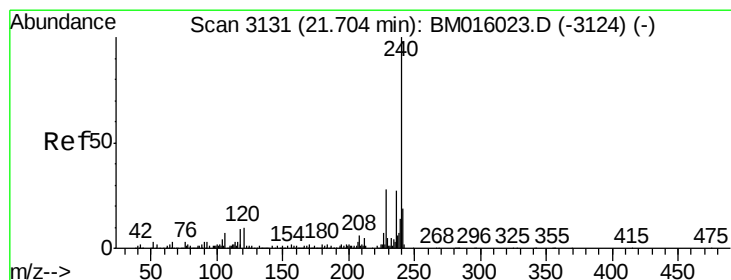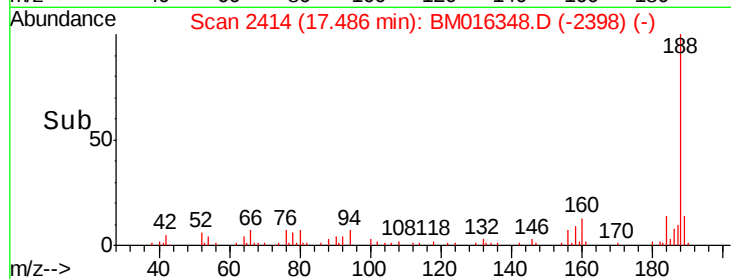
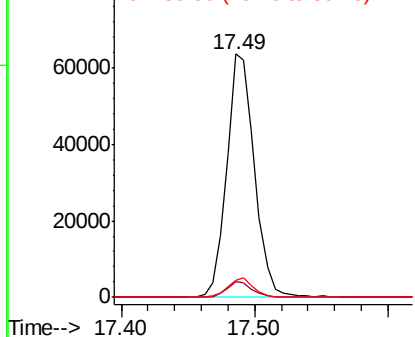



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.62 min Scan# 3117
Delta R.T. -0.00 min
Lab File: BM016348.D
Acq: 14 Aug 2018 11:11

Tgt Ion:240 Resp: 110894
Ion Ratio Lower Upper
240 100
120 7.5 8.2 12.2#
236 27.1 20.0 30.0

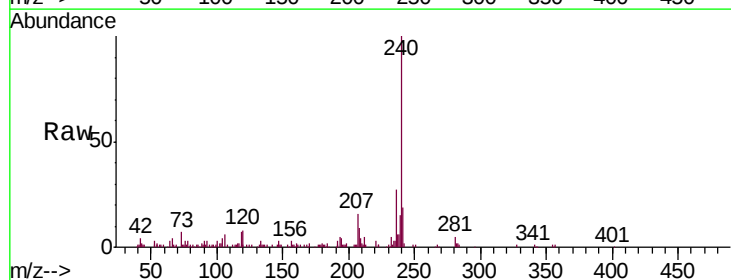

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

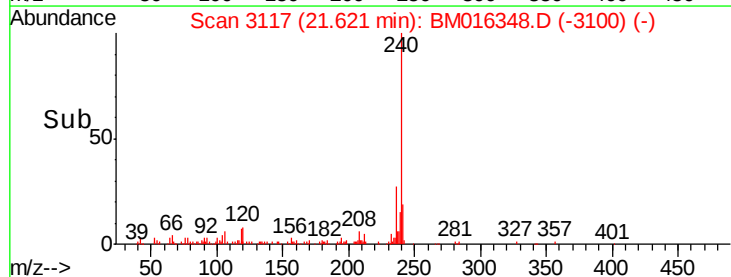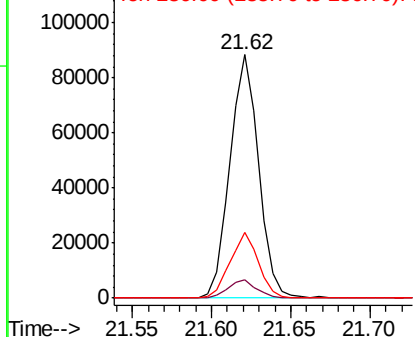

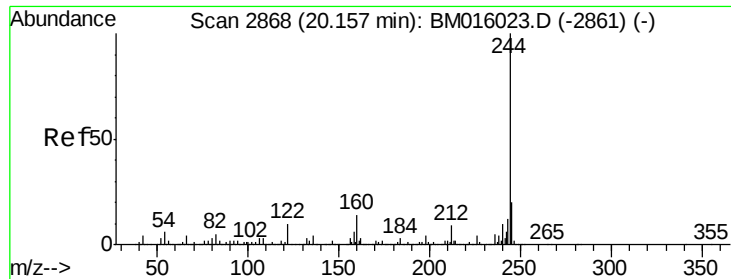

#78

Terphenyl-d14

Concen: Below ng

RT: 20.07 min Scan# 2853

Delta R.T. -0.00 min

Lab File: BM016348.D

Acq: 14 Aug 2018 11:11

Instrument :

BNA_M

ClientSampleId :

SP-1-7


Tgt Ion:244 Resp: 369557

Ion Ratio Lower Upper

244 100

212 10.6 4.9 7.3#




122 9.0 6.2 9.4

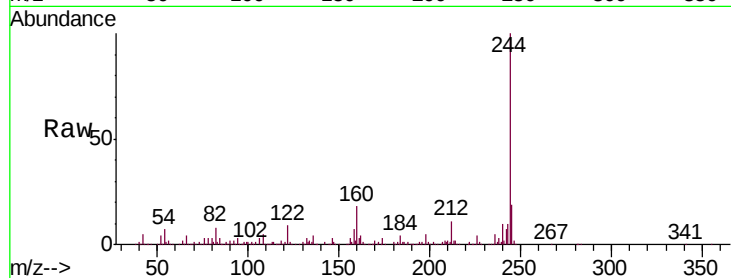

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

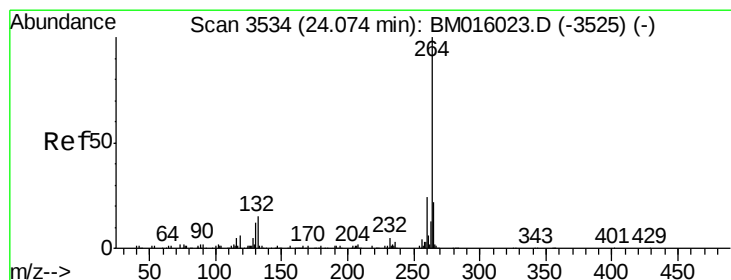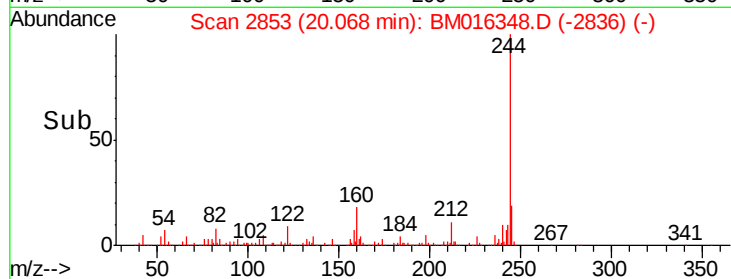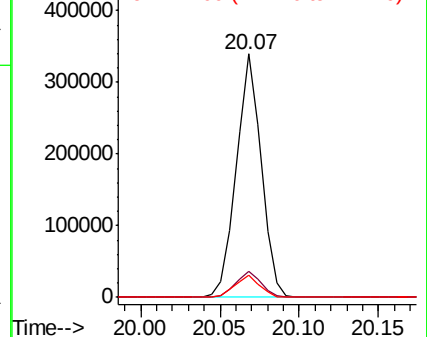

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.95 min Scan# 3513

Delta R.T. 0.01 min

Lab File: BM016348.D

Acq: 14 Aug 2018 11:11


Tgt Ion:264 Resp: 115488

Ion Ratio Lower Upper

264 100

260 24.7 18.6 27.8

265 21.7 17.3 25.9

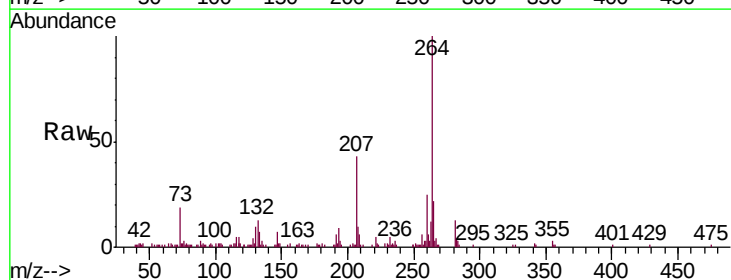

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

