

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081418\
 Data File : BM016362.D
 Acq On : 14 Aug 2018 19:39
 Operator : SJ/JU
 Sample : J4431-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GMW-1

Quant Time: Aug 15 11:31:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	31108	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	109697	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	55231	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	111964	20.00	ng	0.00
75) Chrysene-d12	21.62	240	123077	20.00	ng	0.00
86) Perylene-d12	23.95	264	135627	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	78304	41.81	ng	0.00
7) Phenol-d6	7.29	99	55099	22.53	ng	0.00
23) Nitrobenzene-d5	9.30	82	204091	86.53	ng	0.00
41) 2,4,6-Tribromophenol	16.24	330	57101	81.51	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	365544	80.53	ng	0.00
78) Terphenyl-d14	20.07	244	483527	82.24	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.43	79	4507	2.314	ng	Qvalue # 48
49) Dimethylphthalate	14.20	163	37730	7.806	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081418\
Data File : BM016362.D
Acq On : 14 Aug 2018 19:39
Operator : SJ/JU
Sample : J4431-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GMW-1

Quant Time: Aug 15 11:31:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

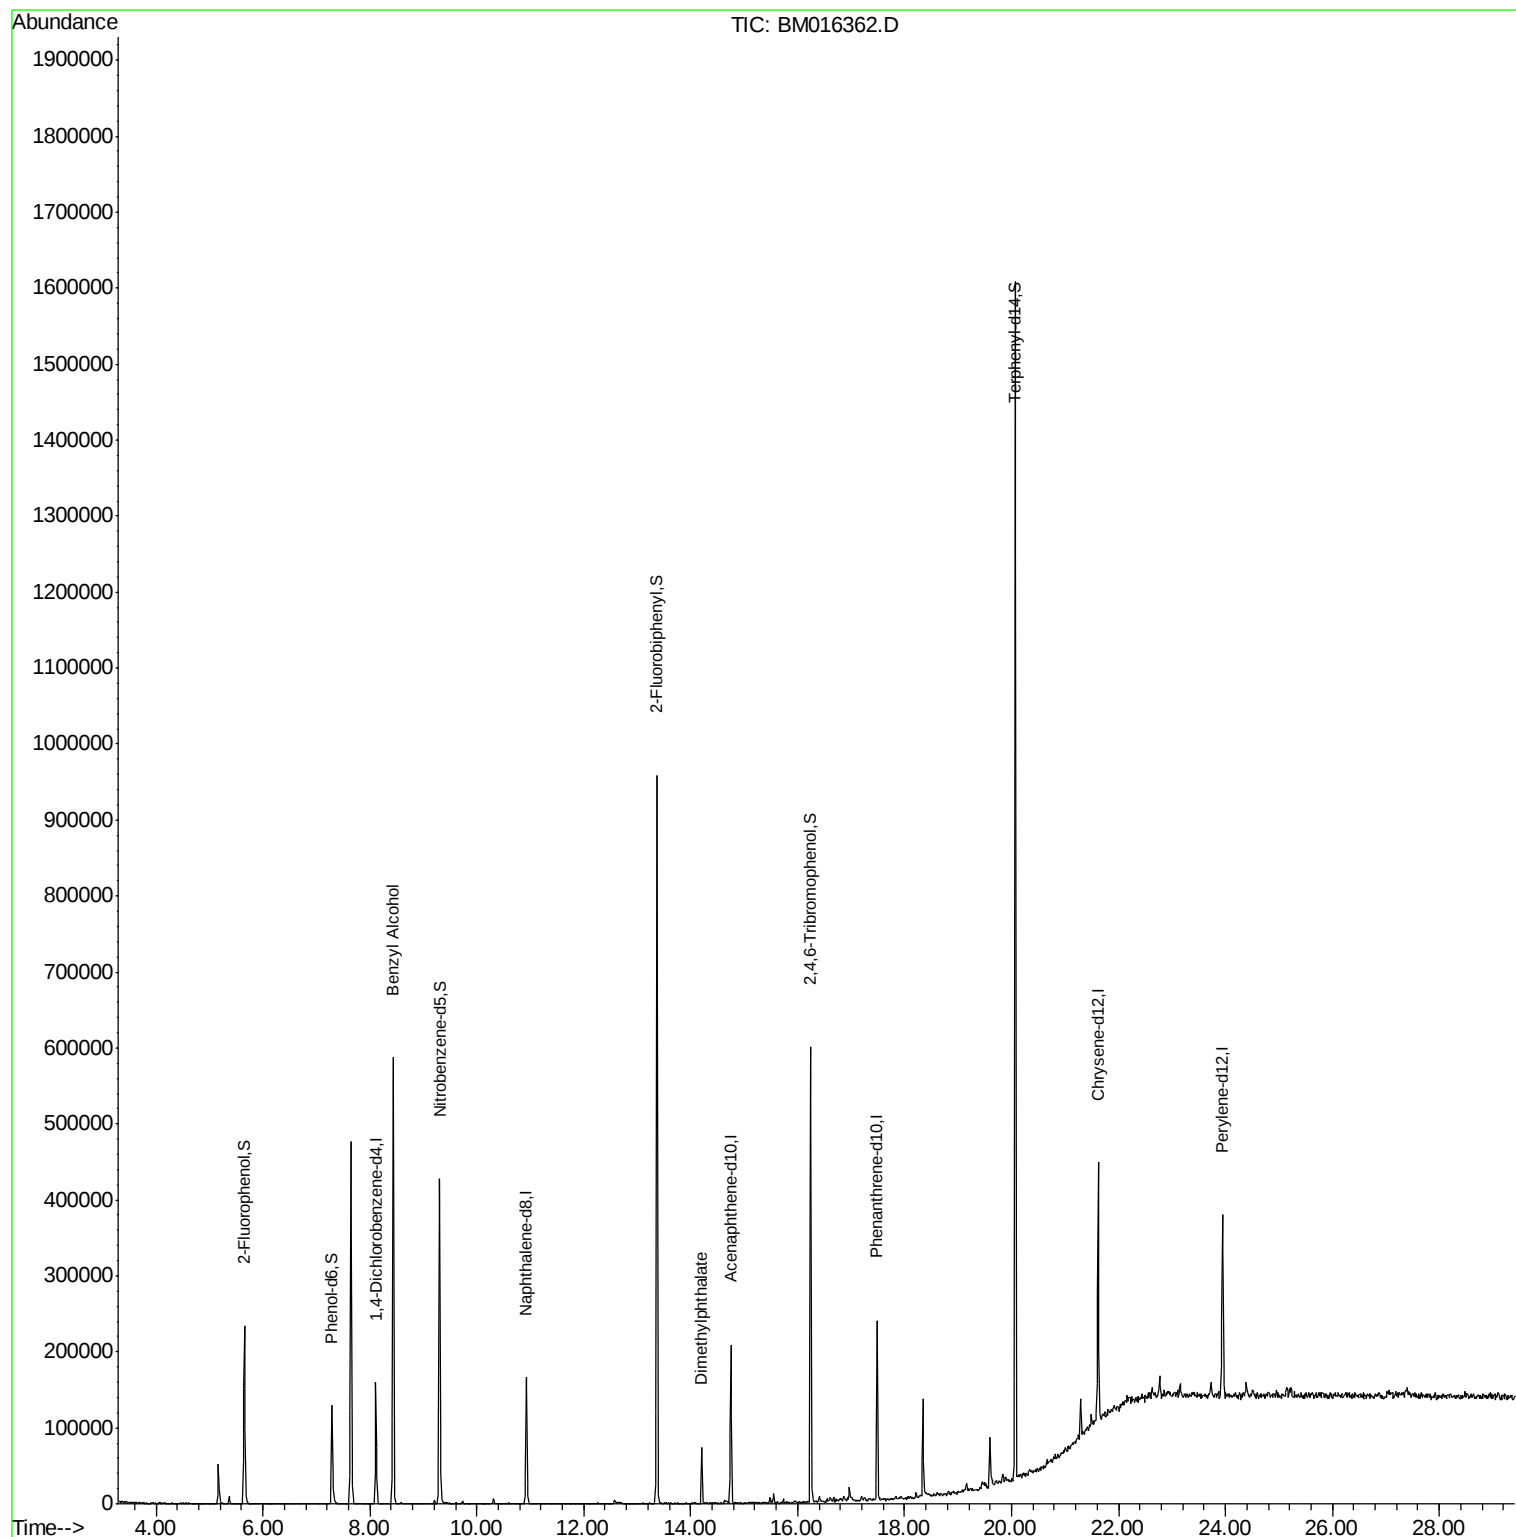

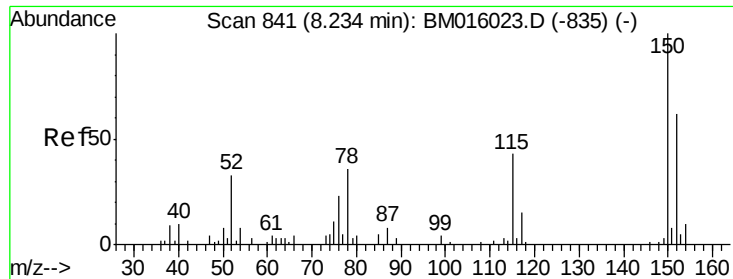


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 821
Delta R.T. -0.00 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39

Instrument :
BNA_M
ClientSampled :
GMW-1

Tgt Ion:152 Resp: 31108
Ion Ratio Lower Upper
152 100
150 155.9 119.5 179.3
115 69.7 43.0 64.4#

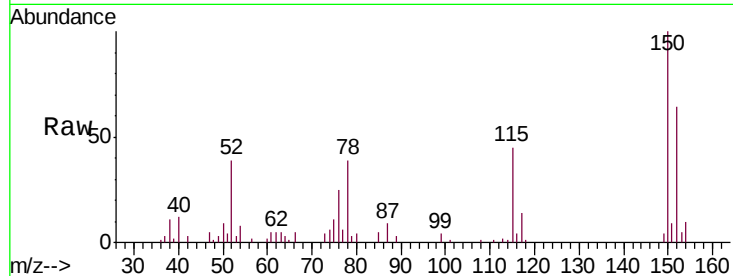


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

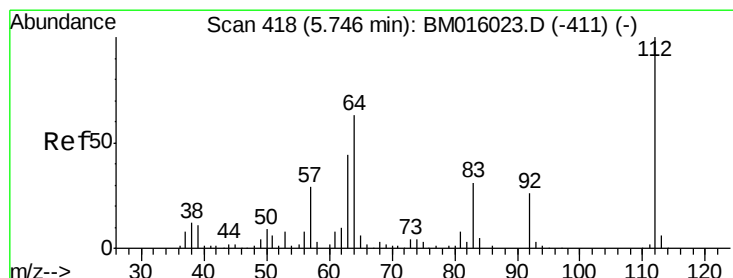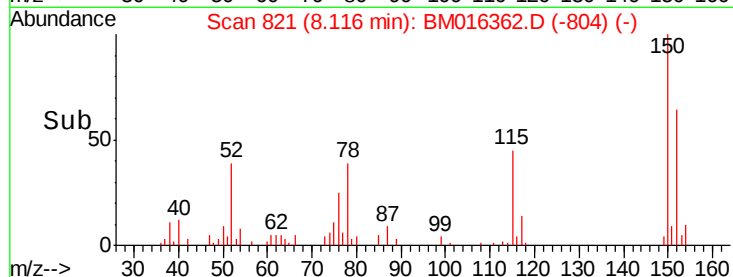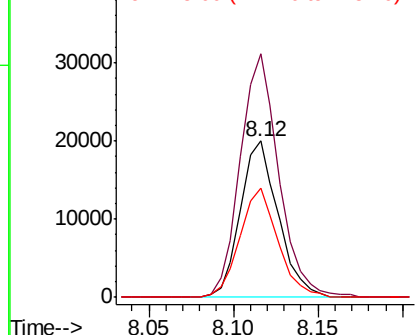



#5

2-Fluorophenol
Concen: N.D. ng
RT: 5.65 min Scan# 402
Delta R.T. 0.01 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39

Tgt Ion:112 Resp: 78304
Ion Ratio Lower Upper
112 100
64 61.7 38.6 57.8#
63 46.6 19.3 28.9#

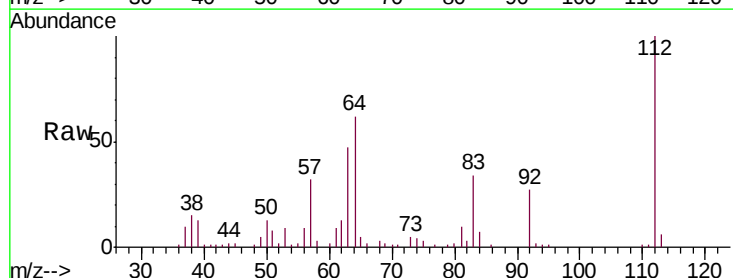

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

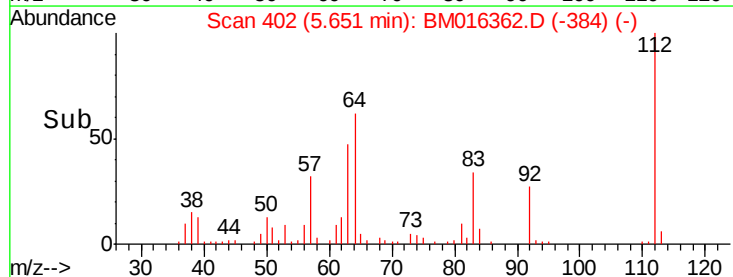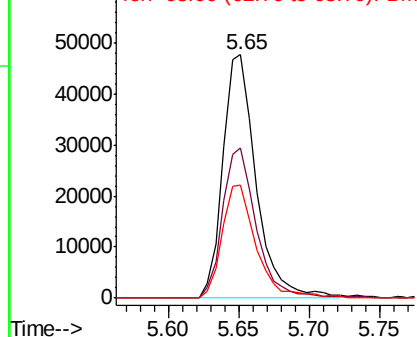



#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 680

Delta R.T. -0.00 min

Lab File: BM016362.D

Acq: 14 Aug 2018 19:39

Instrument :

BNA_M

ClientSampled :

GMW-1


Tgt Ion: 99 Resp: 55099

Ion Ratio Lower Upper




99 100

42 37.2 11.0 16.4#

71 56.1 23.4 35.2#

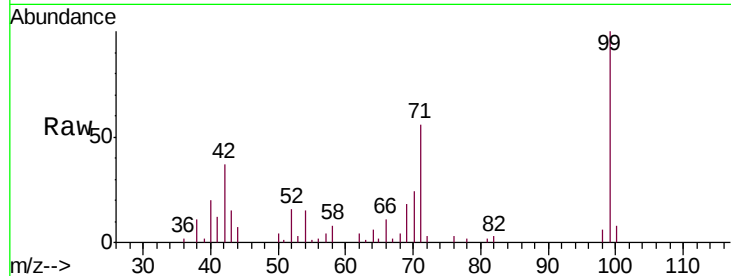

Abundance Ion 99.00 (98.70 to 99.70): BM016362.D (-663) (-)

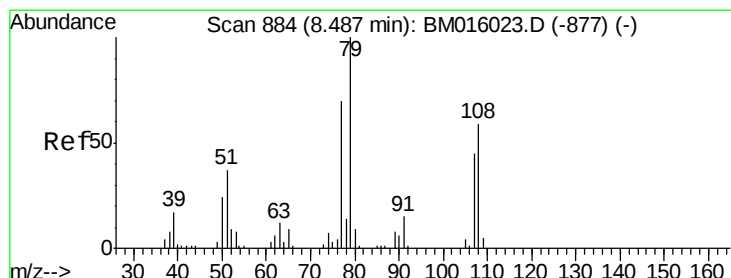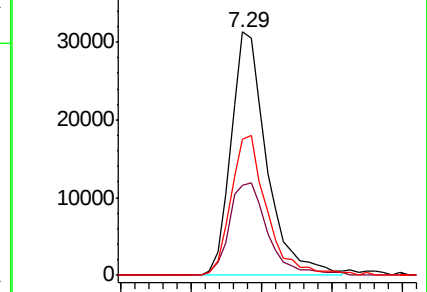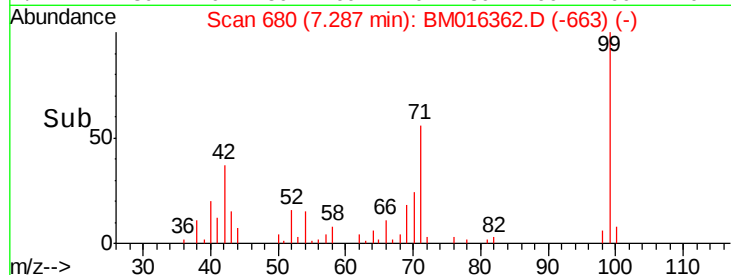

#15

Benzyl Alcohol

Concen: 2.314 ng

RT: 8.43 min Scan# 874

Delta R.T. 0.05 min

Lab File: BM016362.D

Acq: 14 Aug 2018 19:39


Tgt Ion: 79 Resp: 4507

Ion Ratio Lower Upper



79 100

108 65.8 65.0 97.4

77 141.6 53.0 79.6#

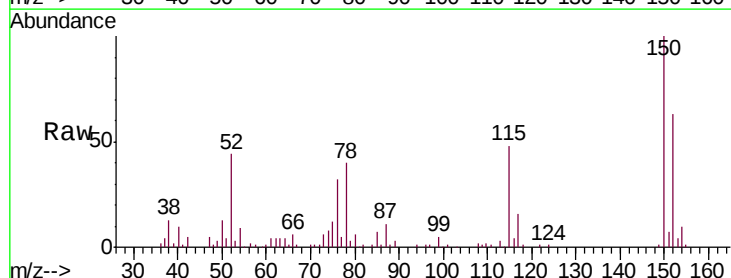

Abundance Ion 79.00 (78.70 to 79.70): BM016362.D (-848) (-)



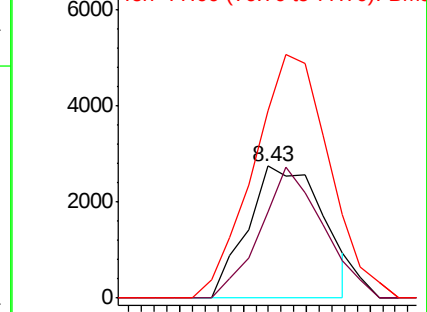
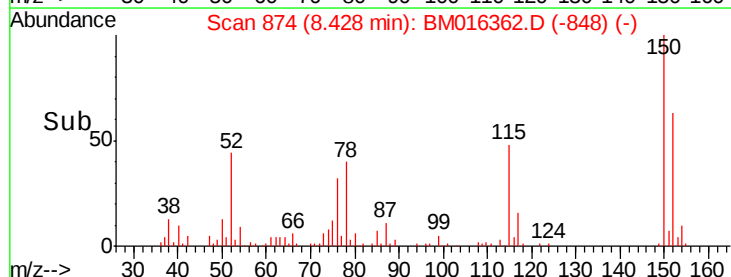




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1299
Delta R.T. -0.00 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39




Instrument :
BNA_M
ClientSampled :
GMW-1

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.5	8.7	13.1
54	9.8	4.6	6.8#
68	3.6	3.7	5.5#

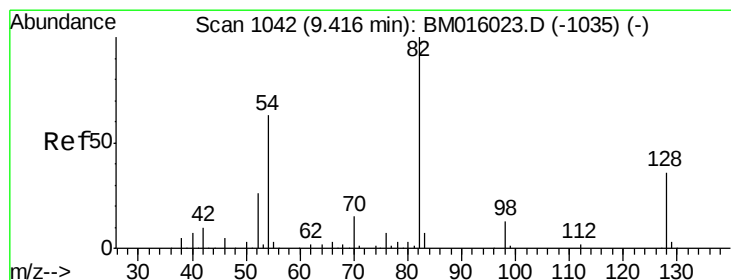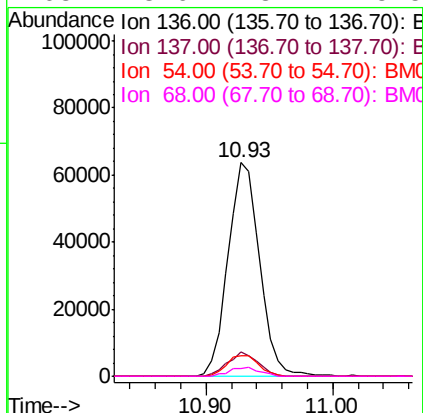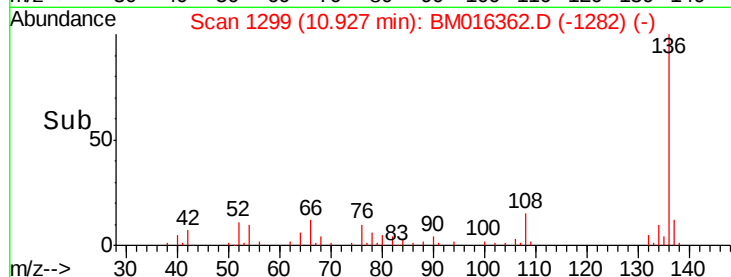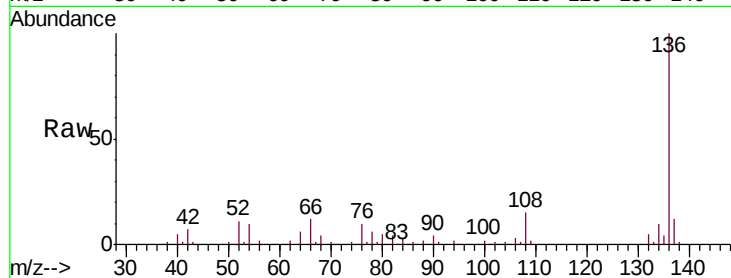

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.00 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39

Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.0	32.8	49.2
54	64.8	40.6	60.8#

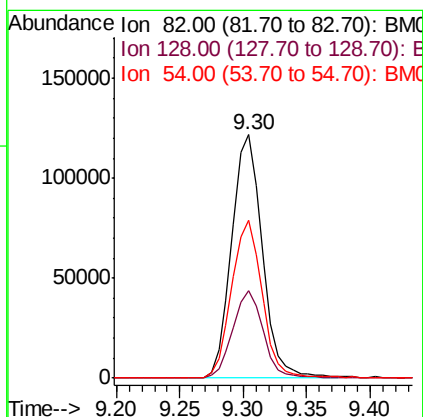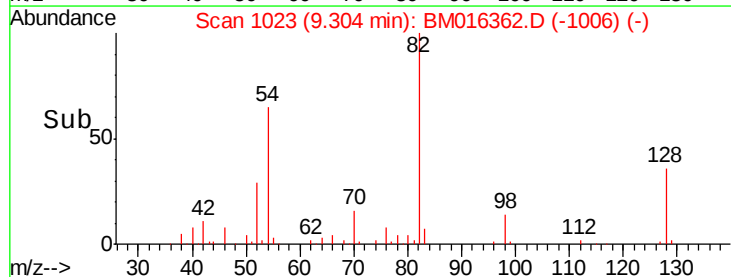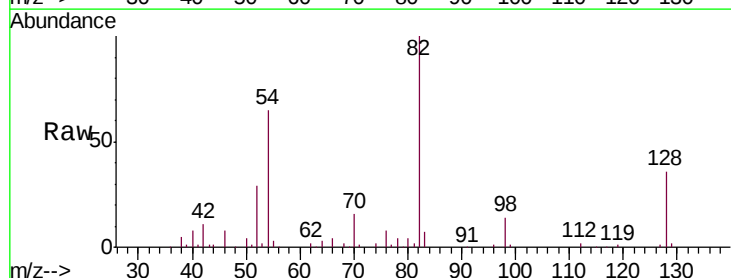



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.75 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BM016362.D

Acq: 14 Aug 2018 19:39

Instrument :

BNA_M

ClientSampleId :

GMW-1


Tgt Ion:164 Resp: 55231

Ion Ratio Lower Upper

164 100

162 104.7 82.4 123.6




160 48.3 35.8 53.6

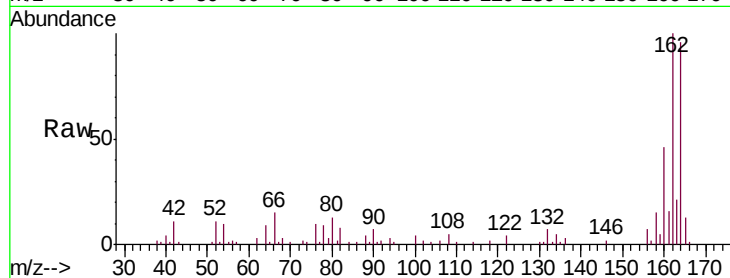

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

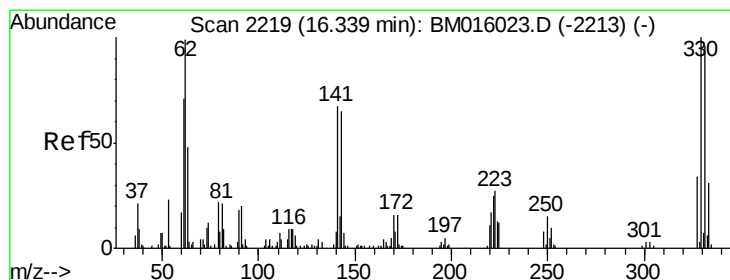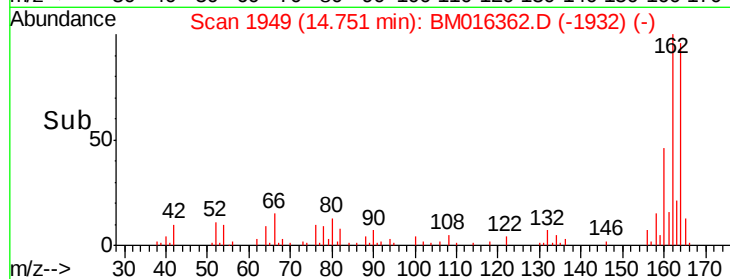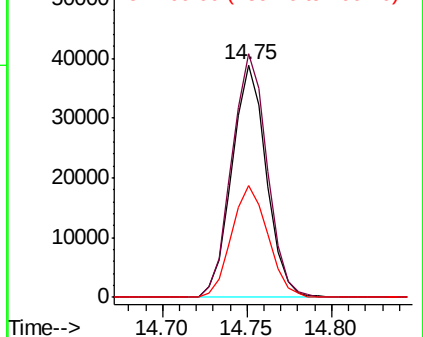

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.24 min Scan# 2203

Delta R.T. -0.00 min

Lab File: BM016362.D

Acq: 14 Aug 2018 19:39


Tgt Ion:330 Resp: 57101

Ion Ratio Lower Upper

330 100

332 96.1 0.0 0.0#



141 82.7 0.0 0.0#

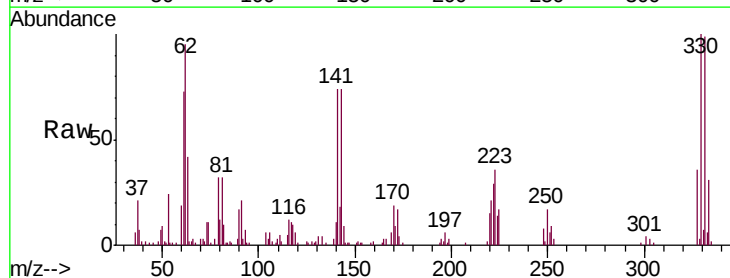

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



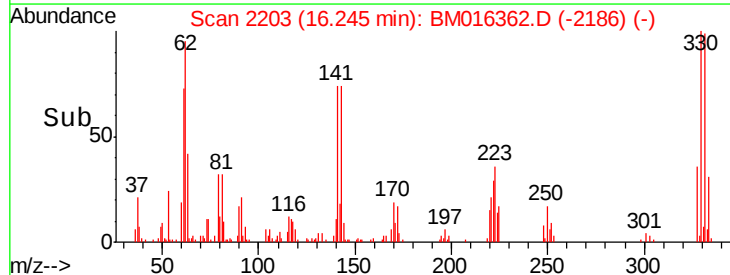
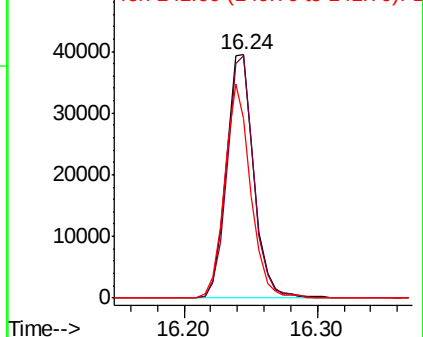




#44
2-Fluorobiphenyl
Concen: N.D. ng
RT: 13.37 min Scan# 1714
Delta R.T. -0.01 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39




Instrument :
BNA_M
ClientSampleId :
GMW-1


Tgt Ion:172 Resp: 365544
Ion Ratio Lower Upper
172 100
171 36.0 28.5 42.7
170 24.3 18.8 28.2

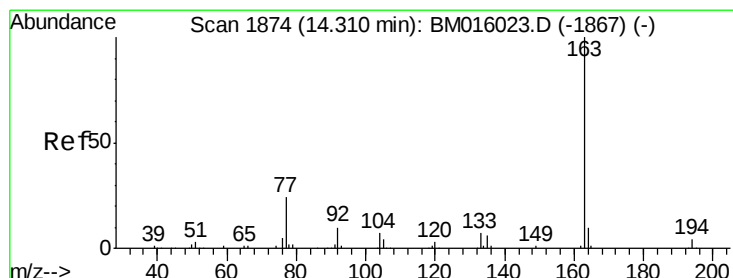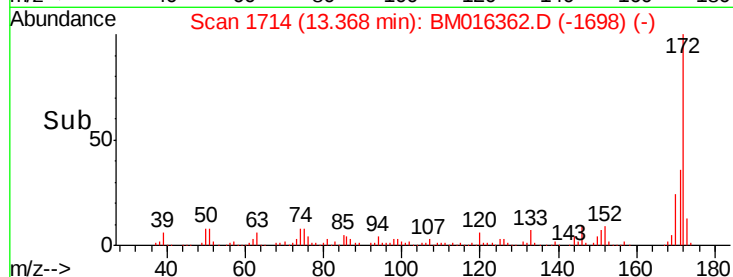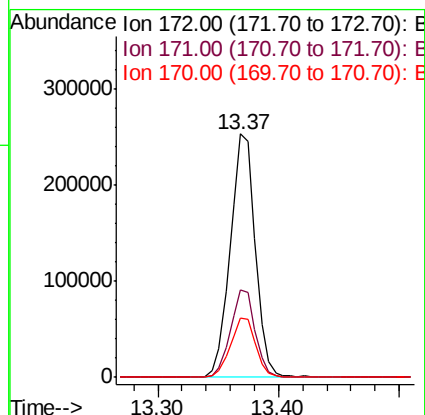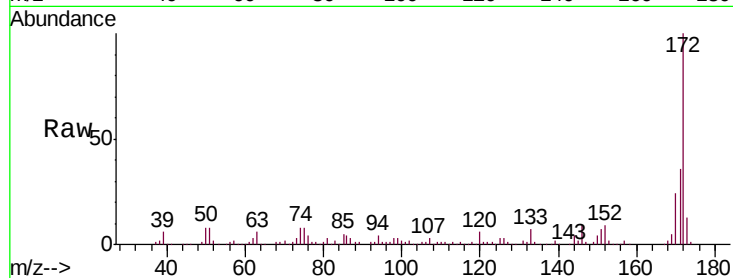

#49
Dimethylphthalate
Concen: 7.806 ng
RT: 14.20 min Scan# 1856
Delta R.T. -0.01 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39

Tgt Ion:163 Resp: 37730
Ion Ratio Lower Upper
163 100
194 4.4 2.7 4.1#
164 10.5 8.2 12.2


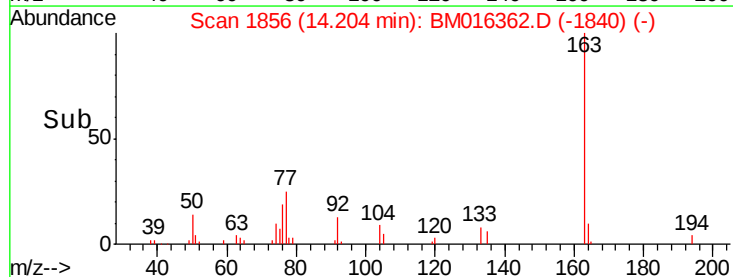
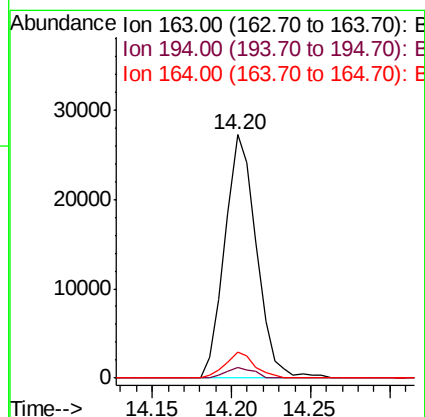
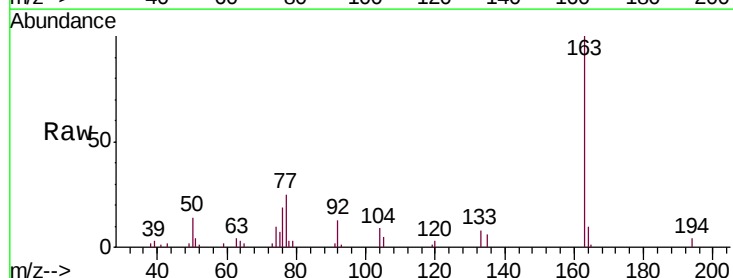


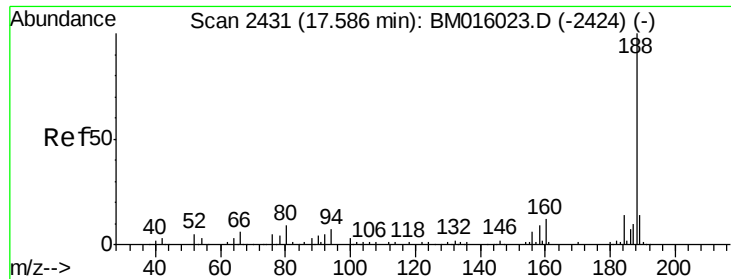

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.49 min Scan# 2414
Delta R.T. -0.01 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39




Instrument :
BNA_M
ClientSampleId :
GMW-1


Tgt Ion:188 Resp: 111964
Ion Ratio Lower Upper
188 100
94 6.2 8.7 13.1#
80 6.7 9.3 13.9#

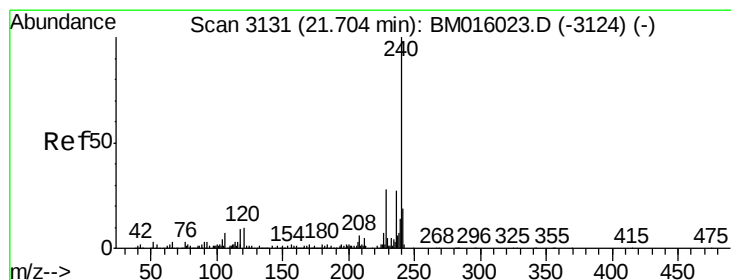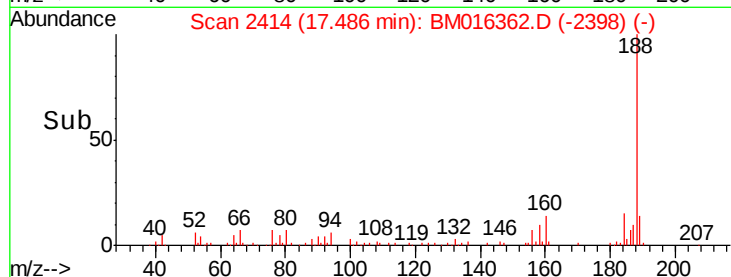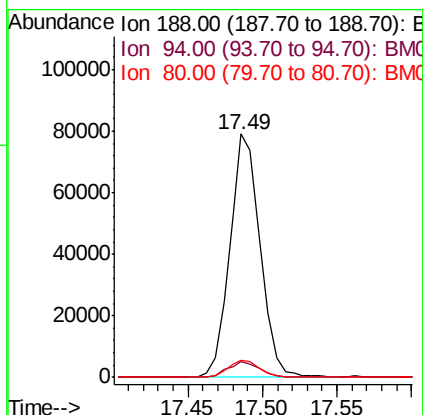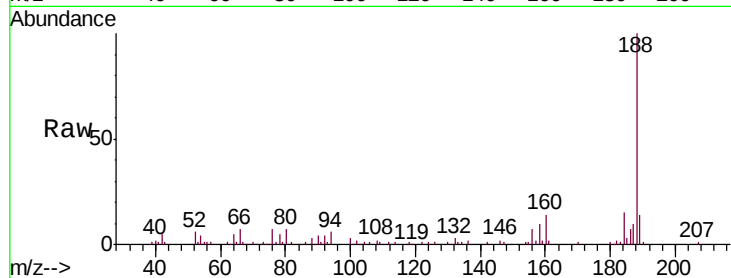

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.62 min Scan# 3117
Delta R.T. -0.00 min
Lab File: BM016362.D
Acq: 14 Aug 2018 19:39

Tgt Ion:240 Resp: 123077
Ion Ratio Lower Upper
240 100
120 7.1 8.2 12.2#
236 25.9 20.0 30.0

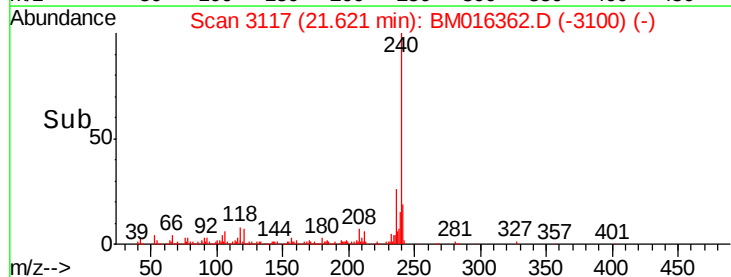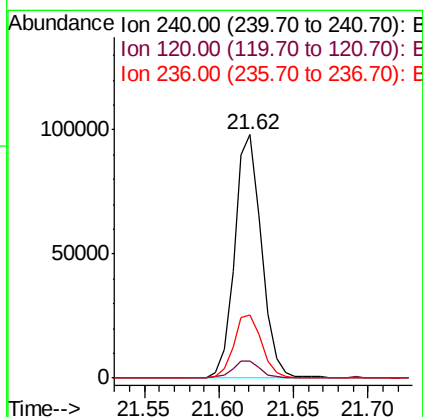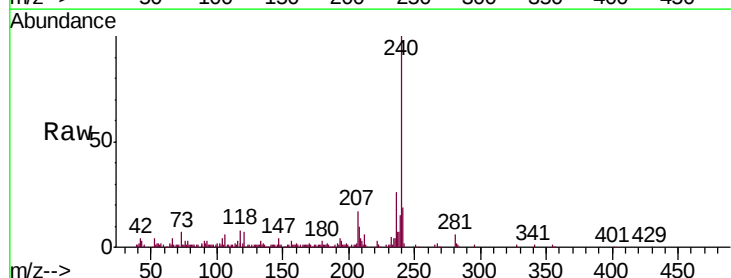

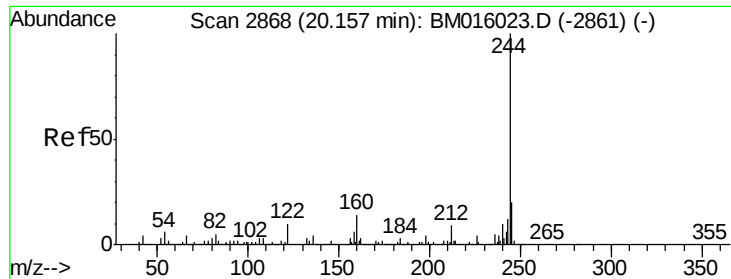

#78

Terphenyl-d14

Concen: Below ng

RT: 20.07 min Scan# 2853

Delta R.T. -0.00 min

Lab File: BM016362.D

Acq: 14 Aug 2018 19:39

Instrument :

BNA_M

ClientSampleID :

GMW-1


Tgt Ion:244 Resp: 483527

Ion Ratio Lower Upper

244 100

212 10.5 4.9 7.3#




122 9.0 6.2 9.4

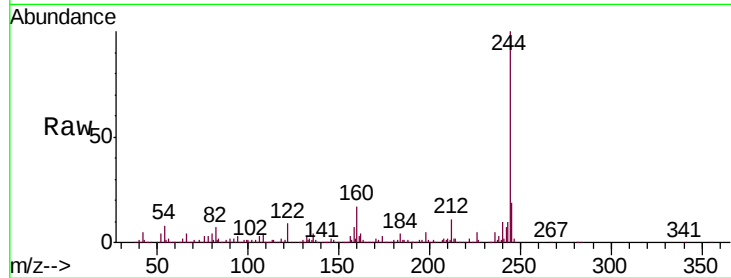

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

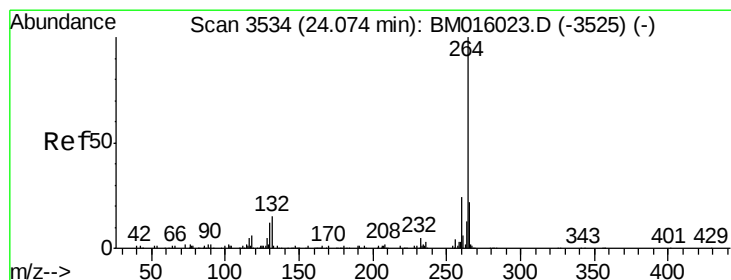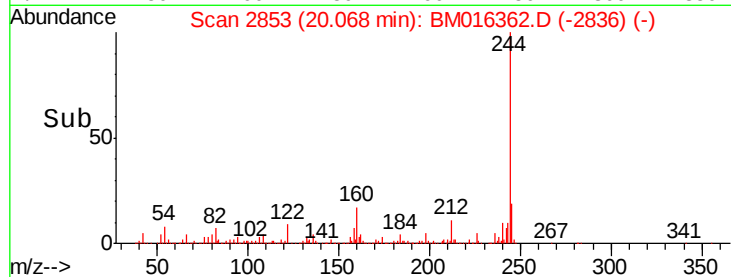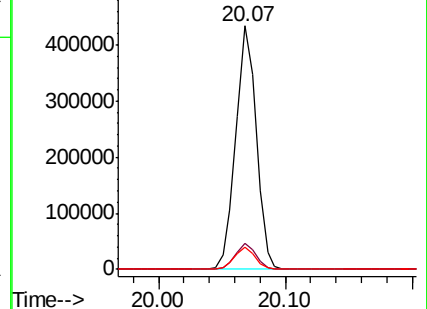

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.95 min Scan# 3513

Delta R.T. 0.01 min

Lab File: BM016362.D

Acq: 14 Aug 2018 19:39


Tgt Ion:264 Resp: 135627

Ion Ratio Lower Upper

264 100

260 23.5 18.6 27.8

265 21.4 17.3 25.9

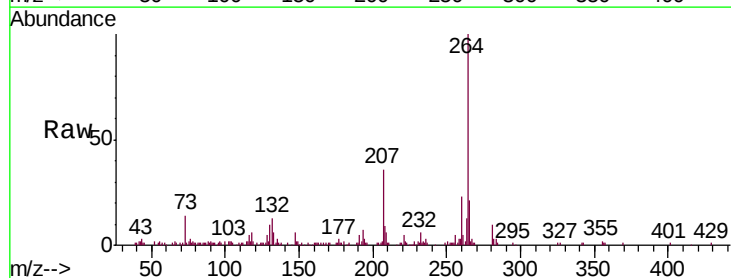

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

