

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081418\
 Data File : BM016363.D
 Acq On : 14 Aug 2018 20:15
 Operator : SJ/JU
 Sample : J4431-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GMW-5

Quant Time: Aug 15 11:31:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	31580	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	110990	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	52384	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	105231	20.00	ng	0.00
75) Chrysene-d12	21.62	240	119894	20.00	ng	0.00
86) Perylene-d12	23.95	264	135052	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	123582	65.00	ng	0.00
7) Phenol-d6	7.29	99	82352	33.17	ng	0.00
23) Nitrobenzene-d5	9.30	82	274849	115.18	ng	0.00
41) 2,4,6-Tribromophenol	16.24	330	99800	150.21	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	496555	115.34	ng	0.00
78) Terphenyl-d14	20.07	244	702666	122.68	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.43	79	5704	2.885	ng	Qvalue
49) Dimethylphthalate	14.21	163	21945	4.787	ng	# 42

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081418\
Data File : BM016363.D
Acq On : 14 Aug 2018 20:15
Operator : SJ/JU
Sample : J4431-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GMW-5

Quant Time: Aug 15 11:31:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

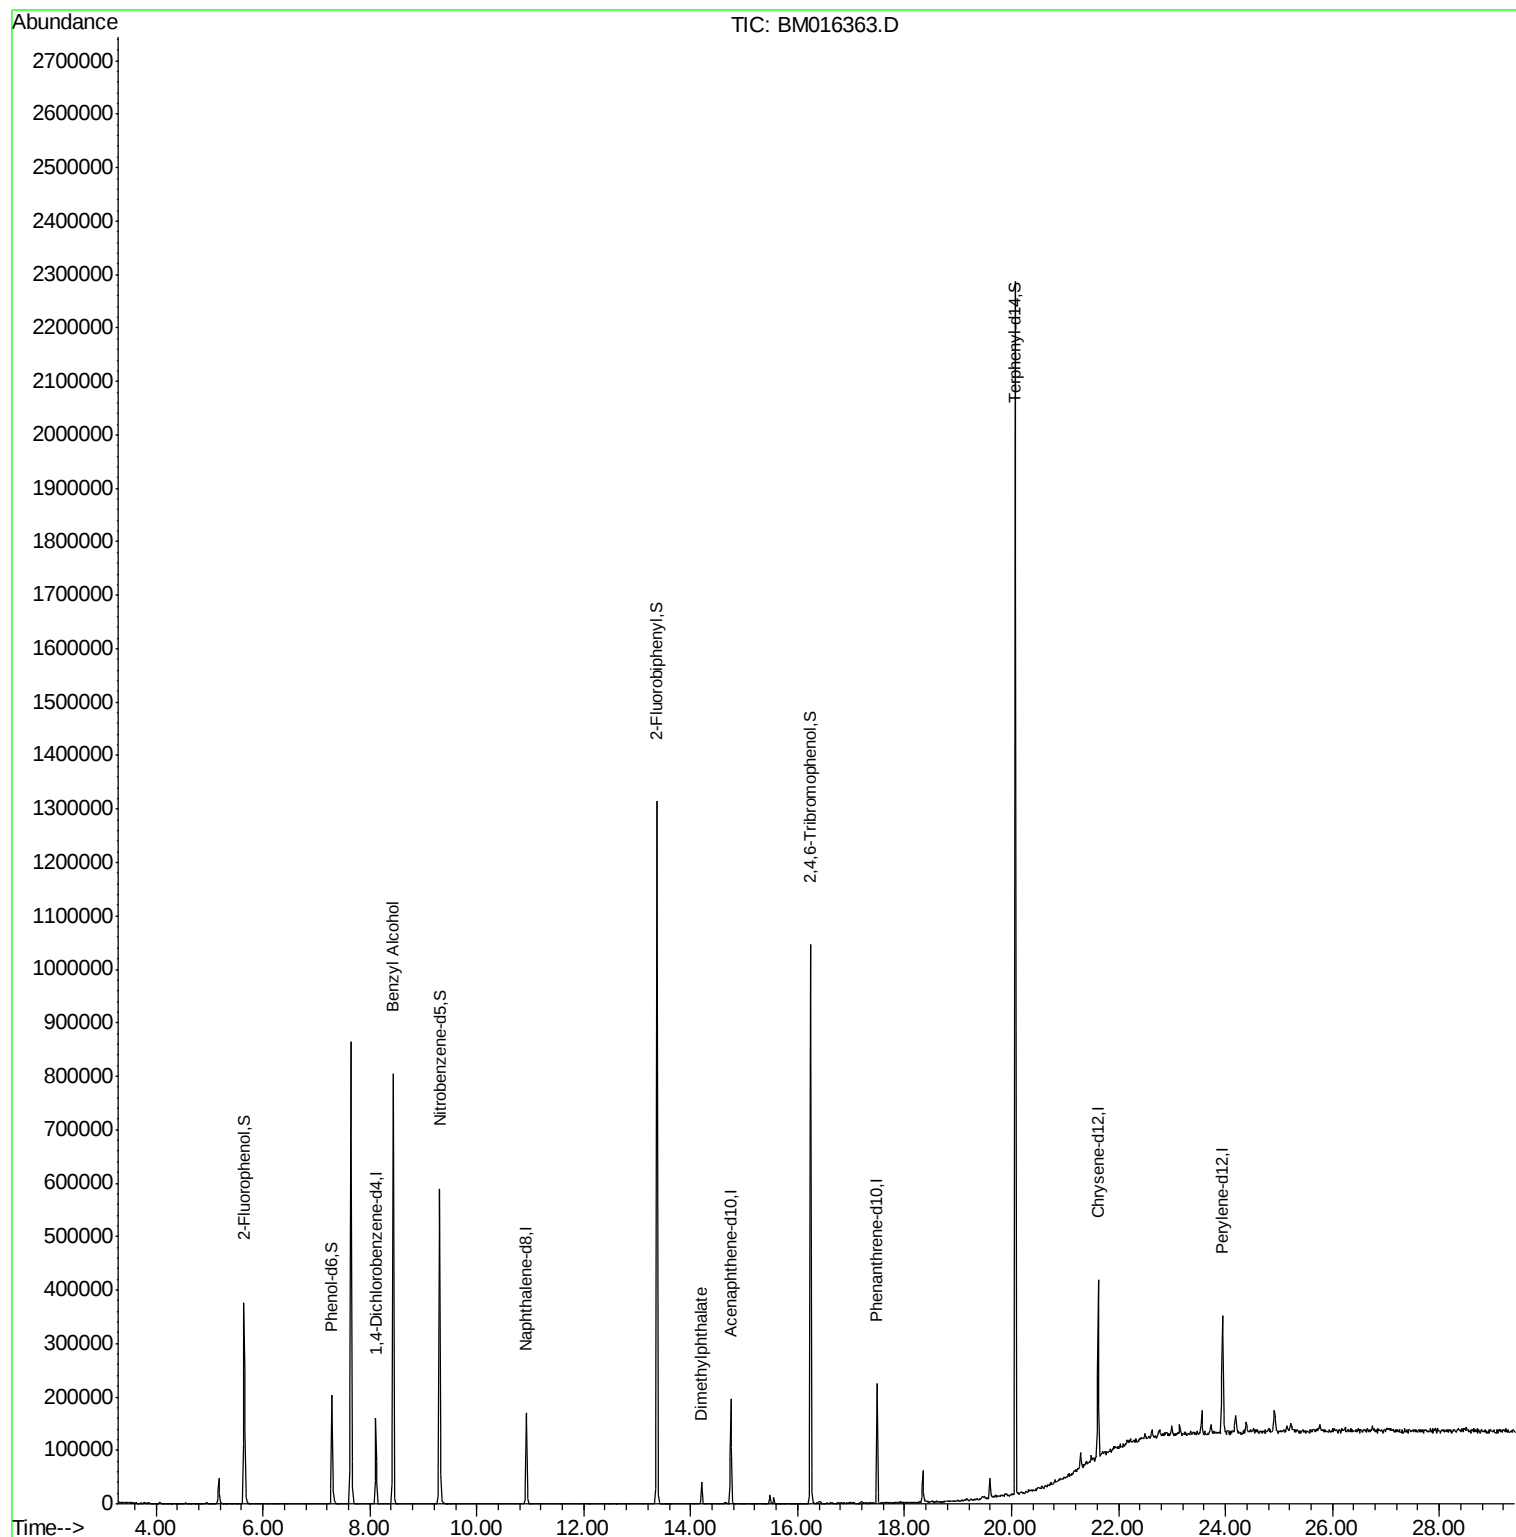




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 821
Delta R.T. -0.00 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15

Instrument :
BNA_M
ClientSampleId :
GMW-5

Tgt Ion:152 Resp: 31580
Ion Ratio Lower Upper
152 100
150 157.9 119.5 179.3
115 69.8 43.0 64.4#

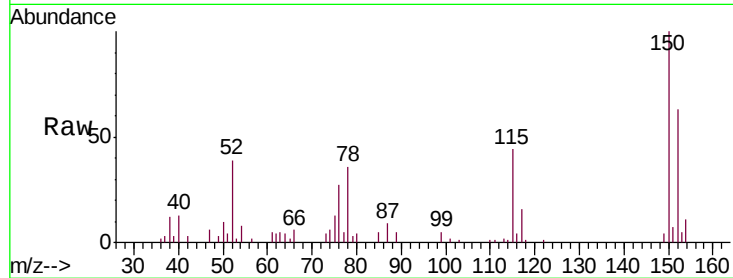


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

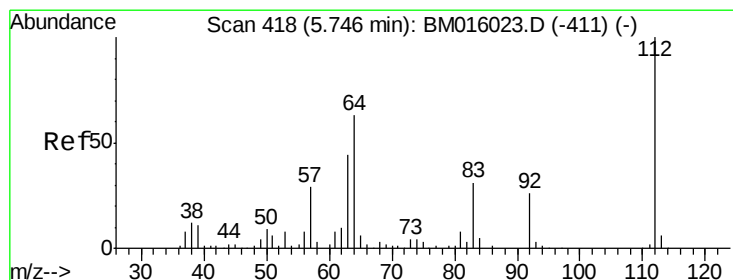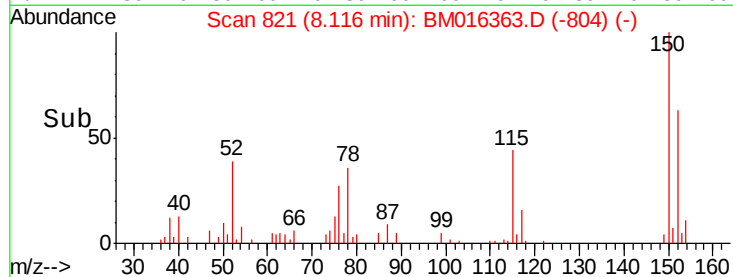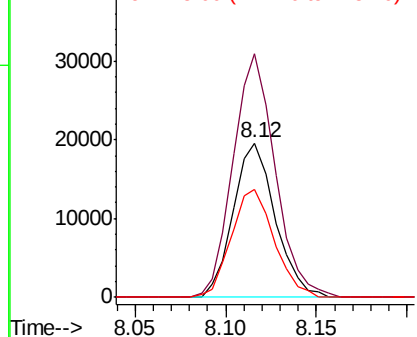



#5

2-Fluorophenol
Concen: N.D. ng
RT: 5.65 min Scan# 402
Delta R.T. 0.01 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15

Tgt Ion:112 Resp: 123582
Ion Ratio Lower Upper
112 100
64 60.1 38.6 57.8#
63 46.2 19.3 28.9#

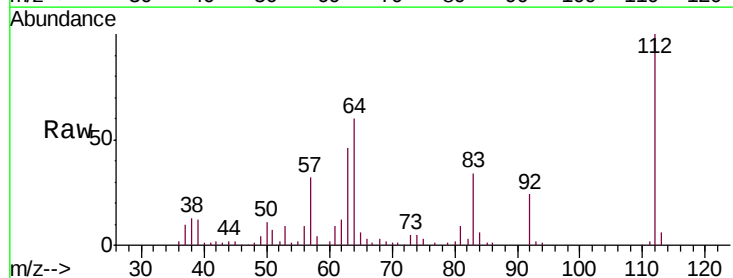

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

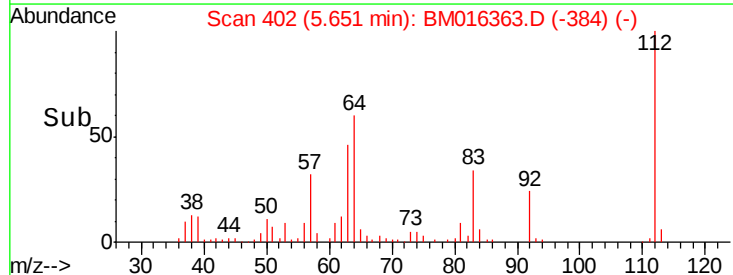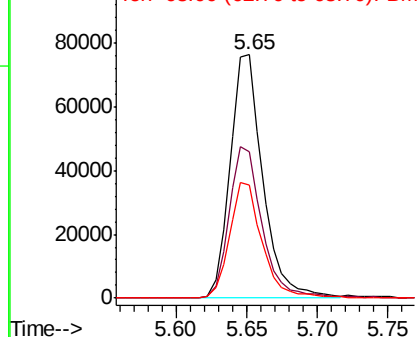



#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 680

Delta R.T. -0.00 min

Lab File: BM016363.D

Acq: 14 Aug 2018 20:15

Instrument :

BNA_M

ClientSampleId :

GMW-5





Tgt Ion: 99 Resp: 82352

Ion Ratio Lower Upper

99 100

42 40.6 11.0 16.4#

71 58.3 23.4 35.2#

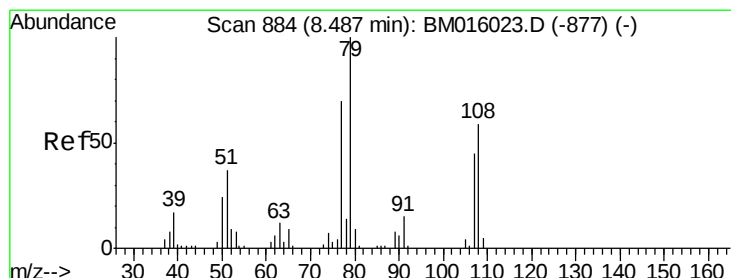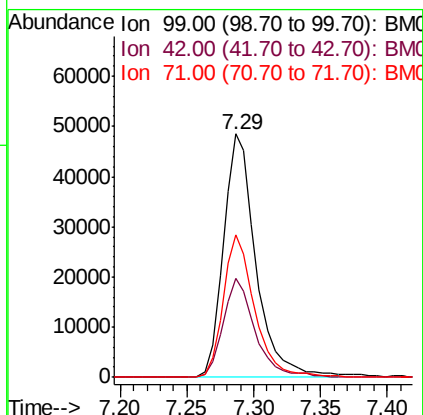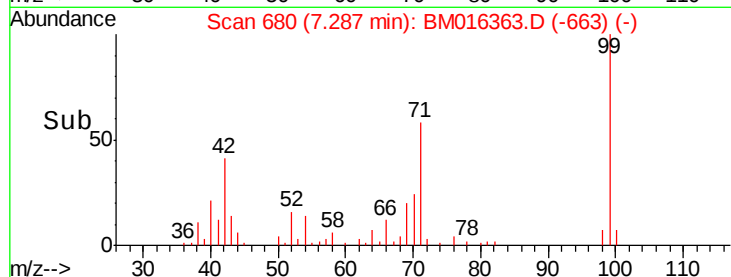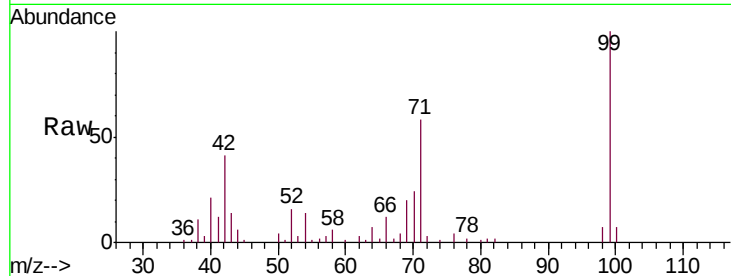

#15

Benzyl Alcohol

Concen: 2.885 ng

RT: 8.43 min Scan# 875

Delta R.T. 0.06 min

Lab File: BM016363.D

Acq: 14 Aug 2018 20:15




Tgt Ion: 79 Resp: 5704

Ion Ratio Lower Upper

79 100

108 85.3 65.0 97.4

77 165.5 53.0 79.6#


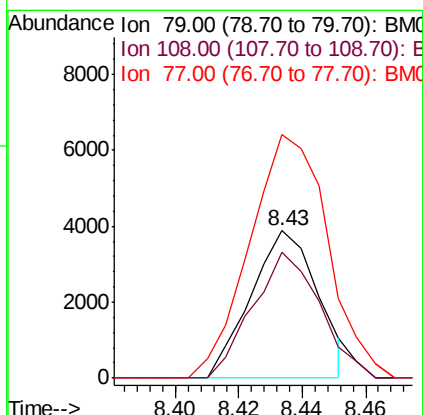
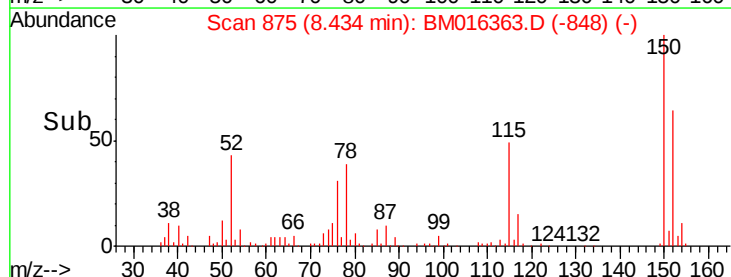
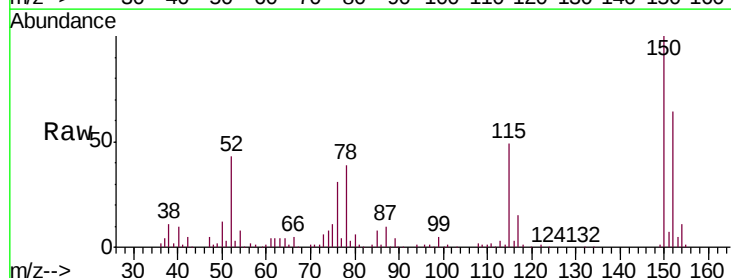




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1299
Delta R.T. -0.00 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15




Instrument :
BNA_M
ClientSampleID :
GMW-5

Tgt Ion:	136	Resp:	110990
Ion	Ratio	Lower	Upper
136	100		
137	11.5	8.7	13.1
54	9.4	4.6	6.8#
68	4.1	3.7	5.5

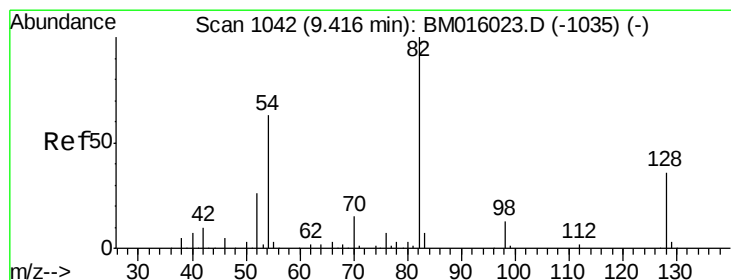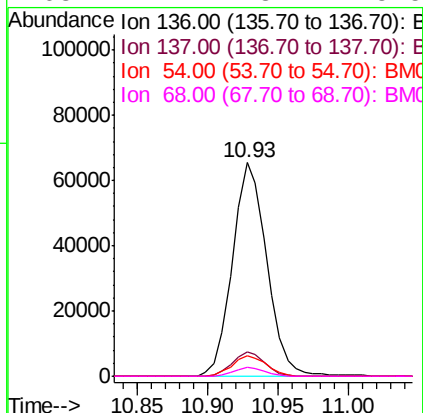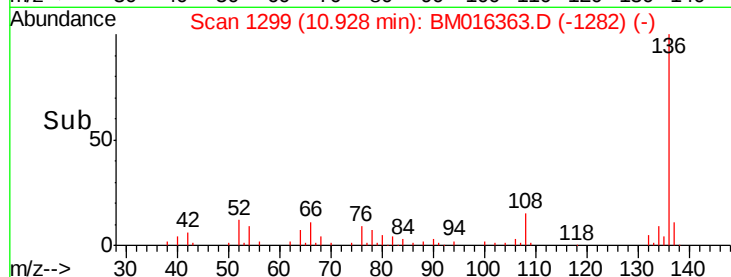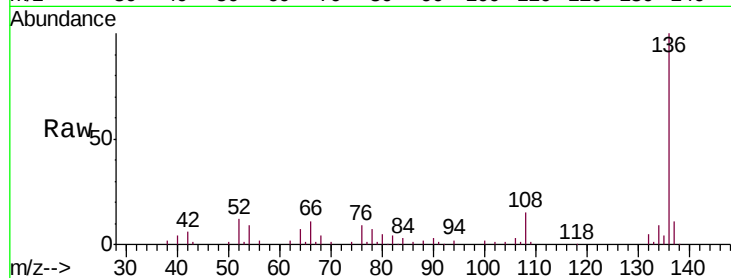

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.00 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15

Tgt Ion:	82	Resp:	274849
Ion	Ratio	Lower	Upper
82	100		
128	35.6	32.8	49.2
54	63.9	40.6	60.8#

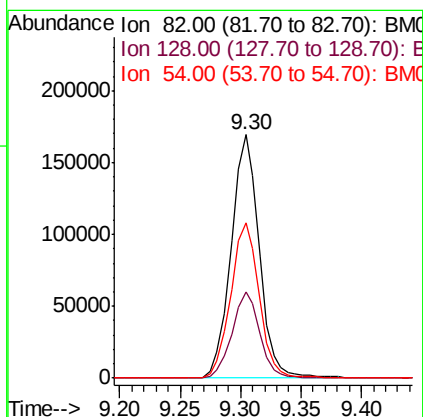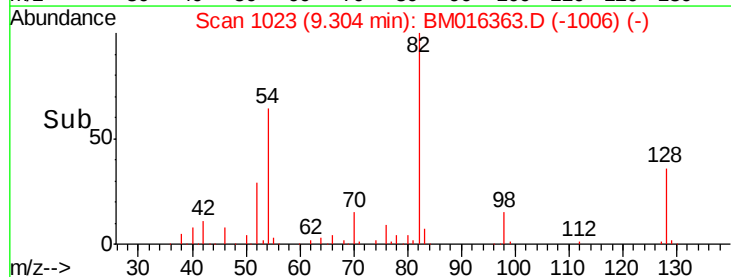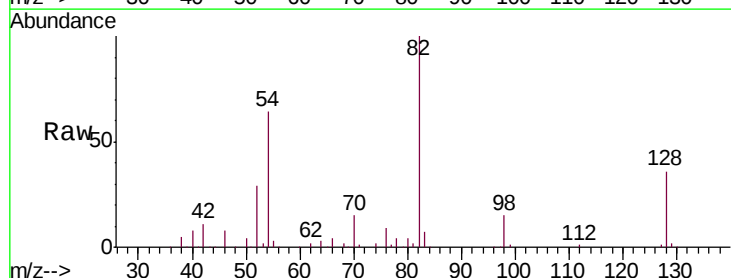



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.75 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BM016363.D

Acq: 14 Aug 2018 20:15

Instrument :

BNA_M

ClientSampled :

GMW-5


Tgt Ion:164 Resp: 52384

Ion Ratio Lower Upper

164 100

162 108.9 82.4 123.6




160 48.3 35.8 53.6

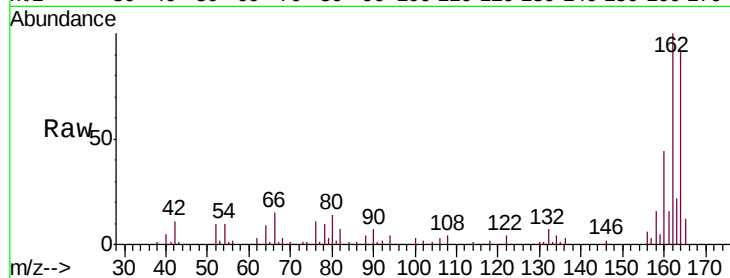

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

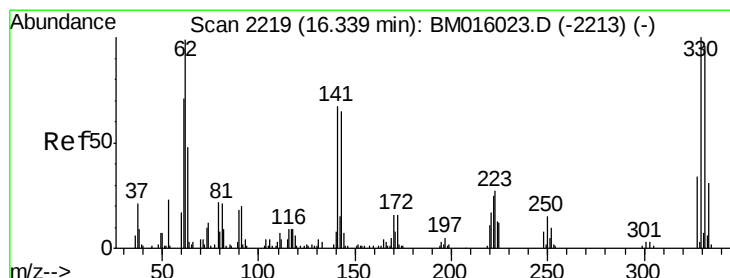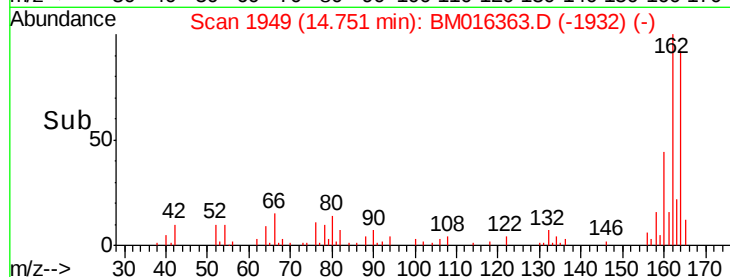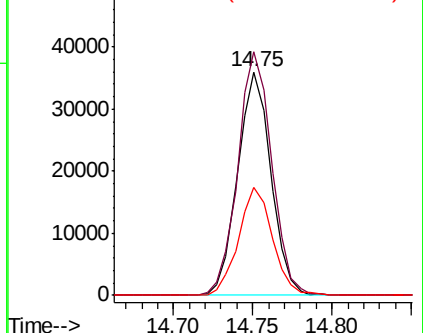

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.24 min Scan# 2203

Delta R.T. -0.00 min

Lab File: BM016363.D

Acq: 14 Aug 2018 20:15


Tgt Ion:330 Resp: 99800

Ion Ratio Lower Upper

330 100

332 97.3 0.0 0.0#



141 83.7 0.0 0.0#

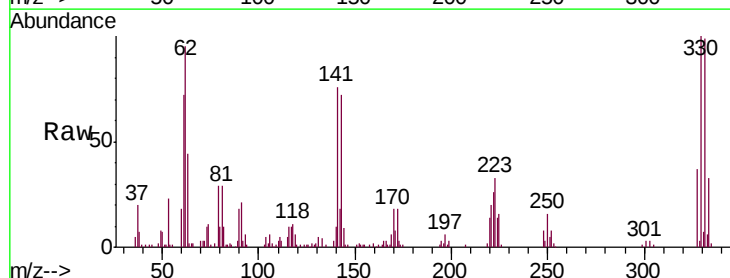

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



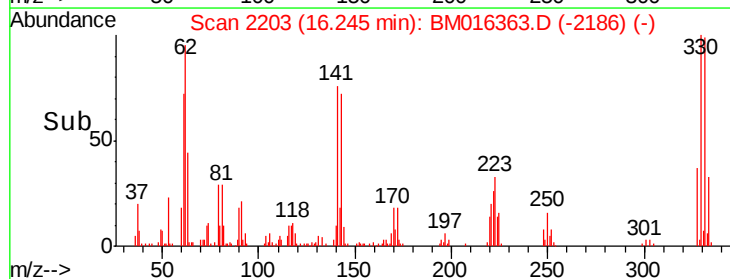
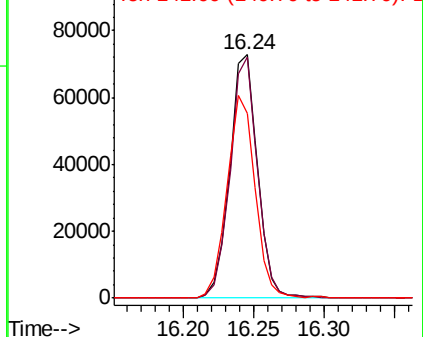




#44
2-Fluorobiphenyl
Concen: N.D. ng
RT: 13.37 min Scan# 1714
Delta R.T. -0.01 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15




Instrument :
BNA_M
ClientSampleId :
GMW-5


Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	28.5	42.7
170	24.0	18.8	28.2

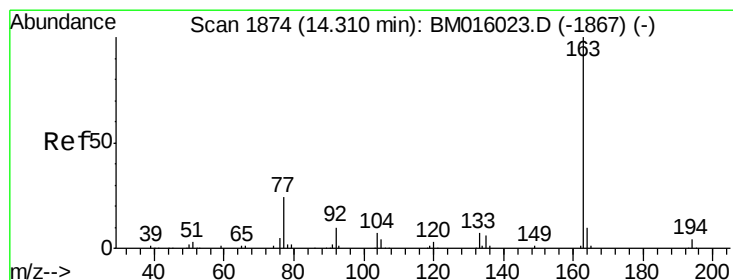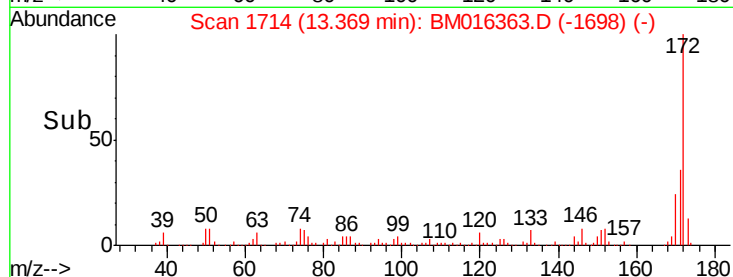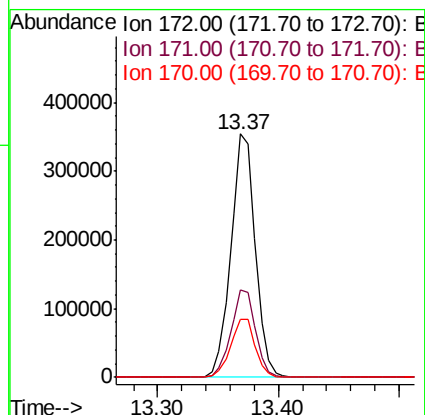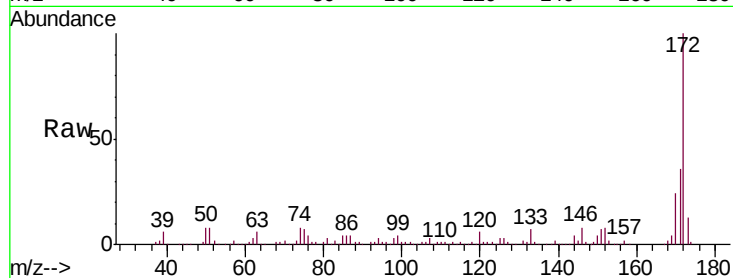

#49
Dimethylphthalate
Concen: 4.787 ng
RT: 14.21 min Scan# 1857
Delta R.T. -0.00 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.6	2.7	4.1
164	9.6	8.2	12.2

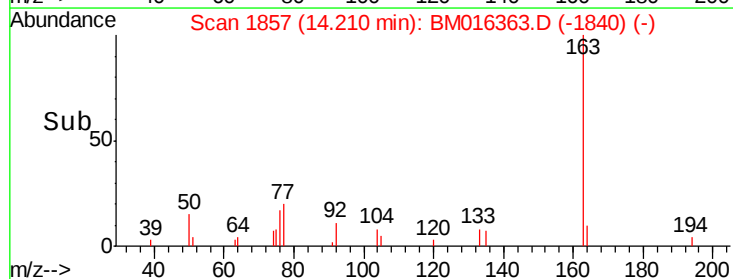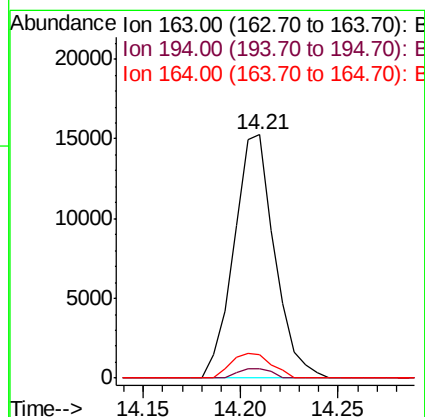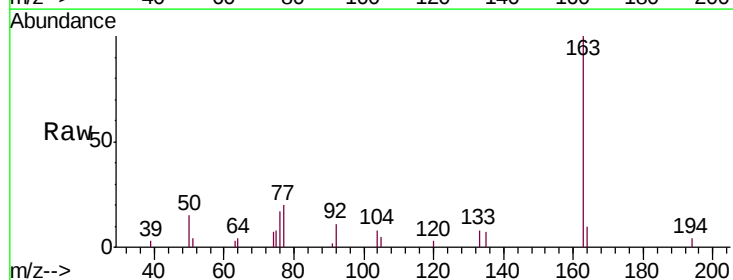


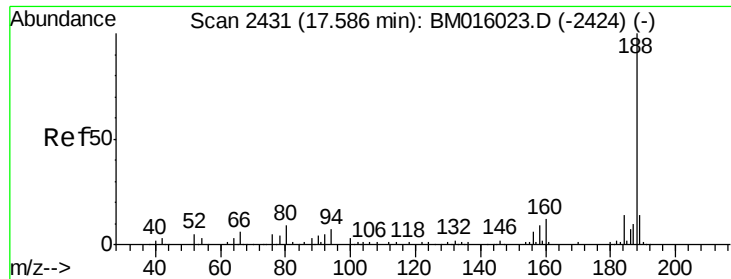




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.49 min Scan# 2414
Delta R.T. -0.01 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15

Instrument :
BNA_M
ClientSampled :
GMW-5

Tgt Ion:188 Resp: 105231
Ion Ratio Lower Upper
188 100
94 7.2 8.7 13.1#
80 7.1 9.3 13.9#

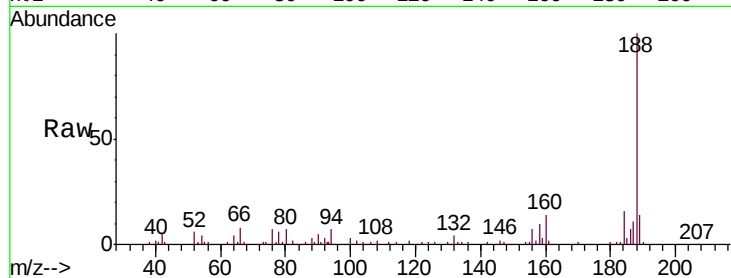


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

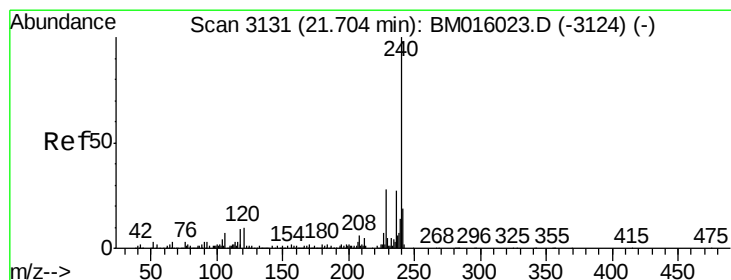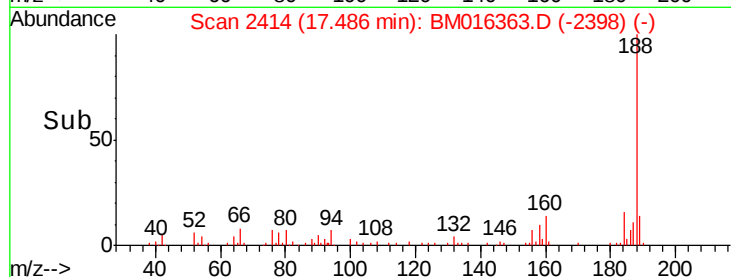
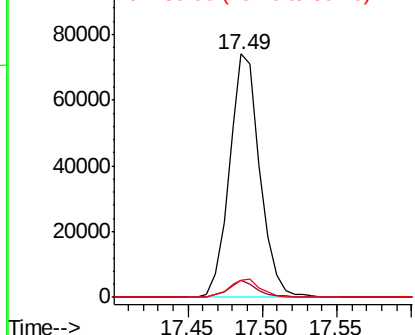



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.62 min Scan# 3117
Delta R.T. -0.00 min
Lab File: BM016363.D
Acq: 14 Aug 2018 20:15

Tgt Ion:240 Resp: 119894
Ion Ratio Lower Upper
240 100
120 6.1 8.2 12.2#
236 26.9 20.0 30.0

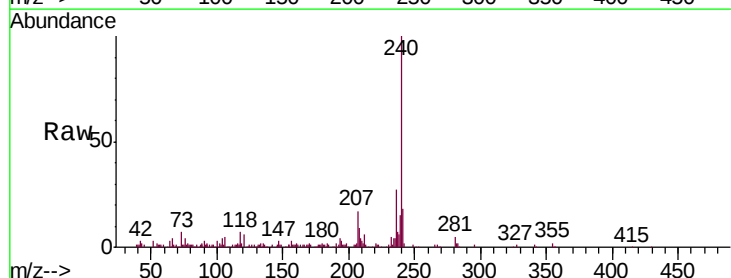

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

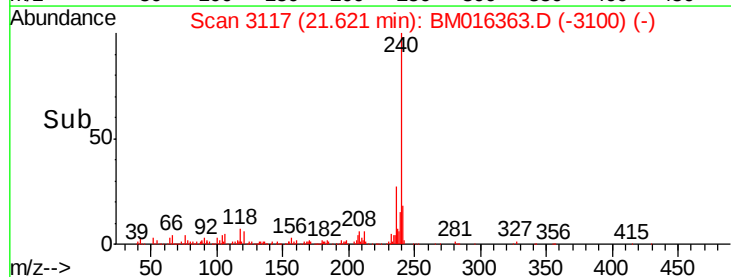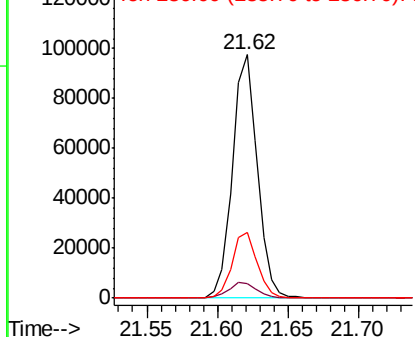

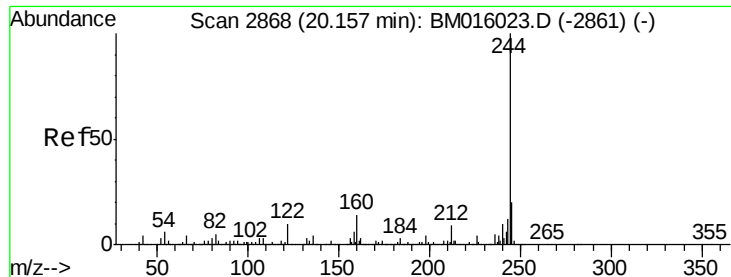

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.07 min Scan# 2853

Delta R.T. -0.00 min

Lab File: BM016363.D

Acq: 14 Aug 2018 20:15

Instrument :

BNA_M

ClientSampleId :

GMW-5


Tgt Ion:244 Resp: 702666

Ion Ratio Lower Upper

244 100

212 10.7 4.9 7.3#




122 8.6 6.2 9.4

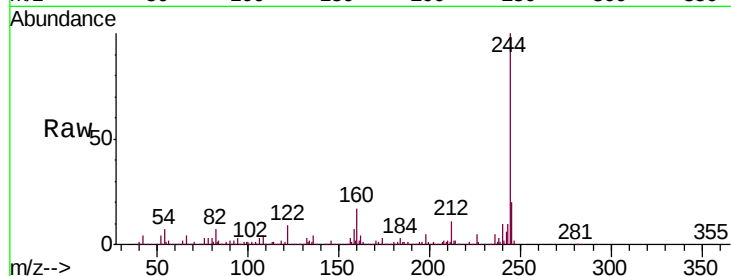

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

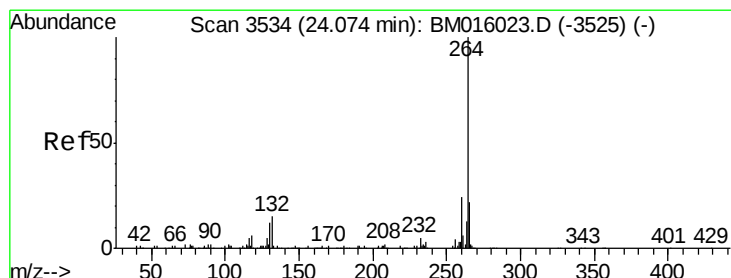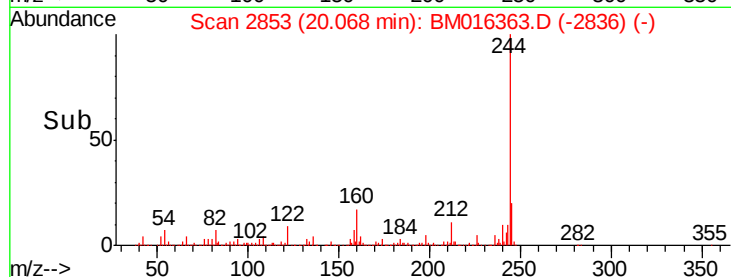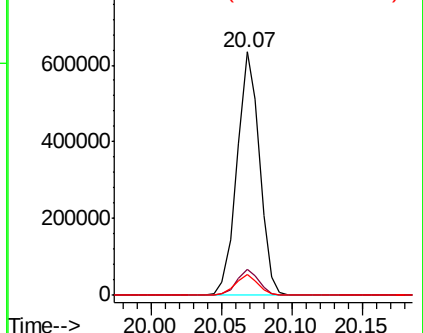

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.95 min Scan# 3513

Delta R.T. 0.01 min

Lab File: BM016363.D

Acq: 14 Aug 2018 20:15


Tgt Ion:264 Resp: 135052

Ion Ratio Lower Upper

264 100

260 23.8 18.6 27.8

265 22.4 17.3 25.9

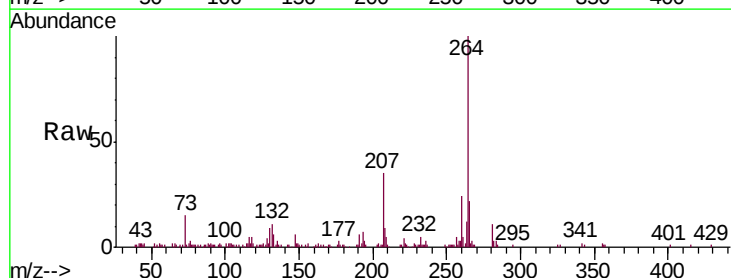

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

