

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081418\
 Data File : BM016353.D
 Acq On : 14 Aug 2018 14:12
 Operator : SJ/JU
 Sample : J4442-51
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-6

Quant Time: Aug 15 11:29:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	35551	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	134838	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	73204	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	148895	20.00	ng	0.00
75) Chrysene-d12	21.62	240	132835	20.00	ng	0.00
86) Perylene-d12	23.95	264	146504	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	248545	116.13	ng	0.00
7) Phenol-d6	7.29	99	299979	107.33	ng	0.00
23) Nitrobenzene-d5	9.30	82	219845	75.83	ng	0.00
41) 2,4,6-Tribromophenol	16.24	330	98539	106.13	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	397166	66.01	ng	0.00
78) Terphenyl-d14	20.07	244	494138	77.87	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.21	163	32906	5.136	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081418\
Data File : BM016353.D
Acq On : 14 Aug 2018 14:12
Operator : SJ/JU
Sample : J4442-51
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-6

Quant Time: Aug 15 11:29:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

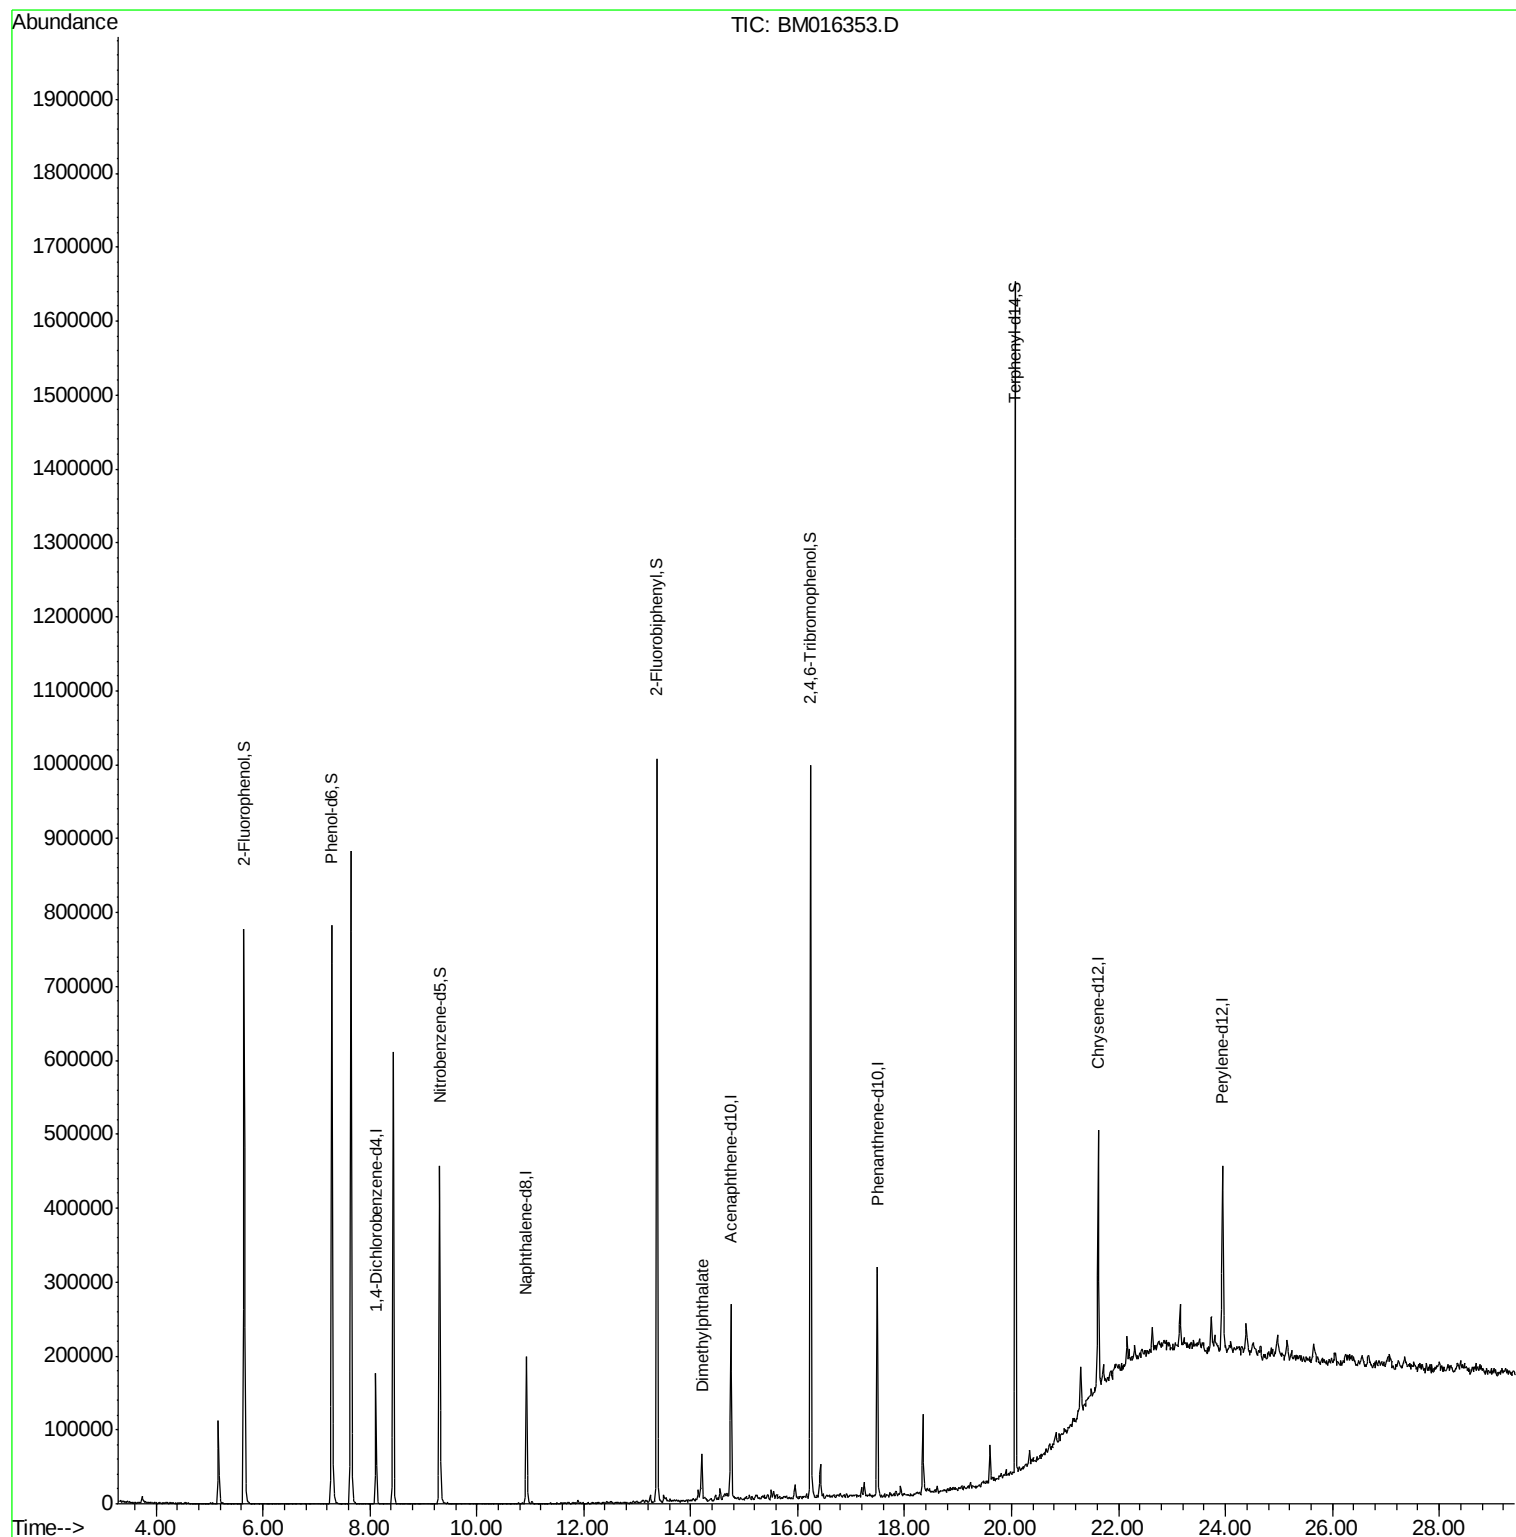

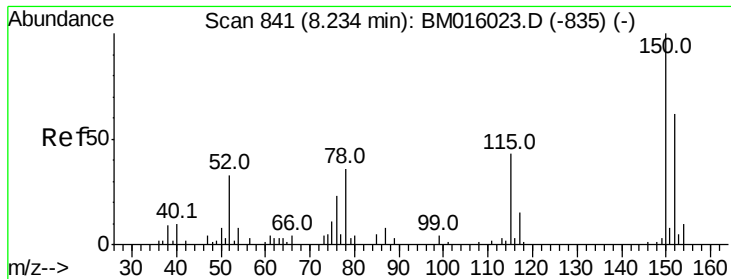


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.12 min Scan# 821
 Delta R.T. -0.00 min
 Lab File: BM016353.D
 Acq: 14 Aug 2018 14:12

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-6

Tot Ion:152 Resp: 35551
 Ion Ratio Lower Upper
 152 100
 150 160.5 119.5 179.3
 115 73.8 43.0 64.4#

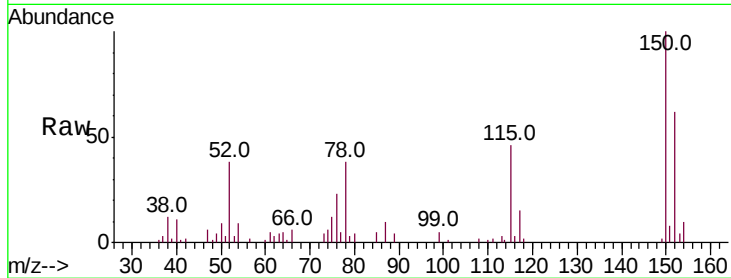


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

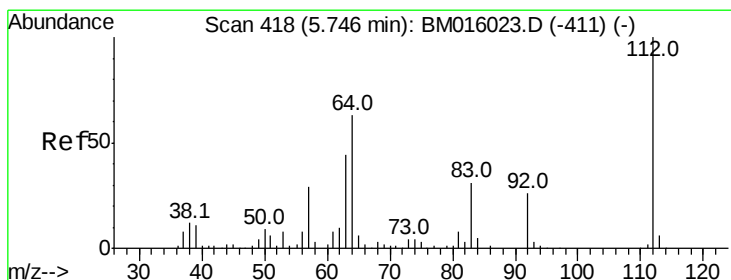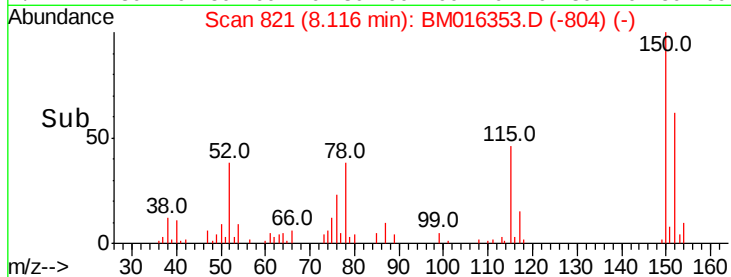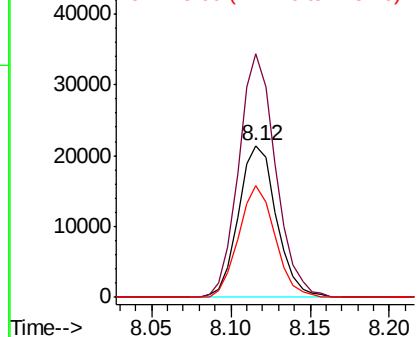



#5


2-Fluorophenol
 Concen: Below ng
 RT: 5.65 min Scan# 401
 Delta R.T. -0.00 min
 Lab File: BM016353.D
 Acq: 14 Aug 2018 14:12

Tgt Ion:112 Resp: 248545
 Ion Ratio Lower Upper
 112 100
 64 62.1 38.6 57.8#
 63 47.1 19.3 28.9#

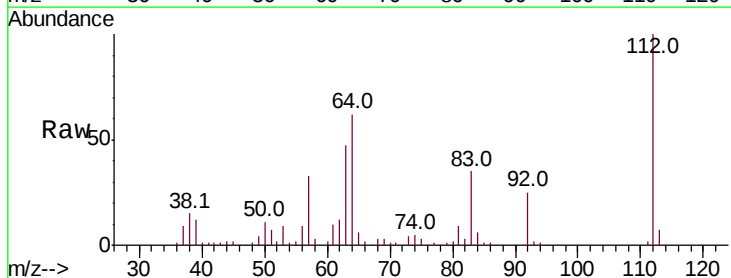

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

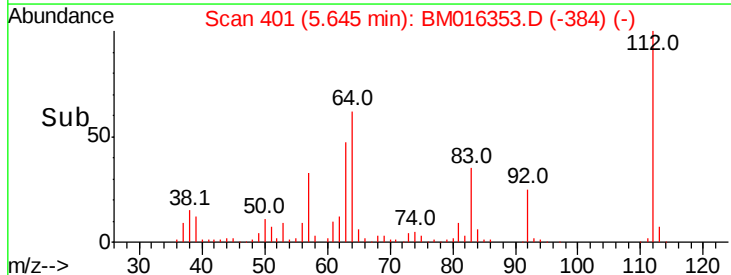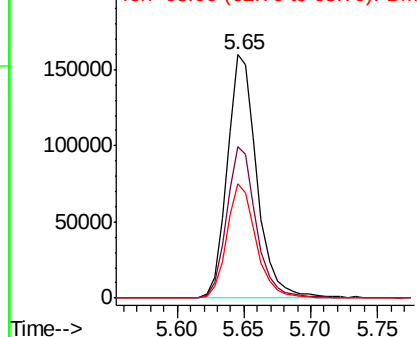

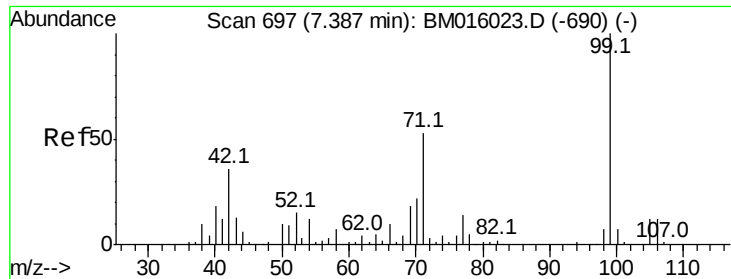

#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 680

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12

Instrument :

BNA_M

ClientSampleId :

SP-1-6


Tot Ion: 99 Resp: 299979

Ion Ratio Lower Upper

99 100

42 39.8 11.0 16.4#




71 58.3 23.4 35.2#

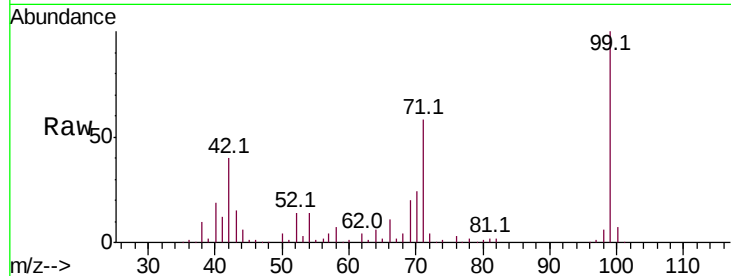

Abundance Ion 99.00 (98.70 to 99.70): BM016353.D (-663) (-)

Ion 42.00 (41.70 to 42.70): BM016353.D (-663) (-)

Ion 71.00 (70.70 to 71.70): BM016353.D (-663) (-)

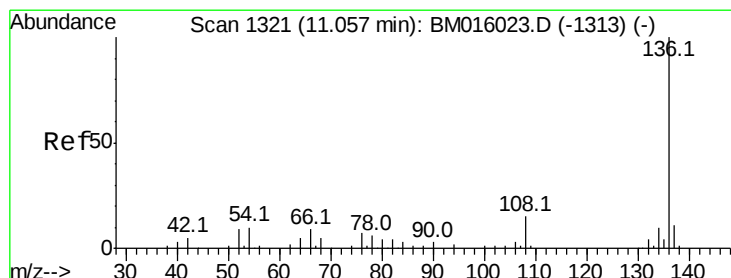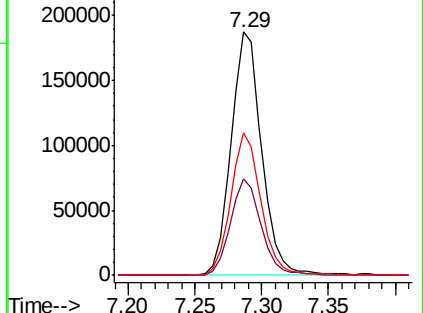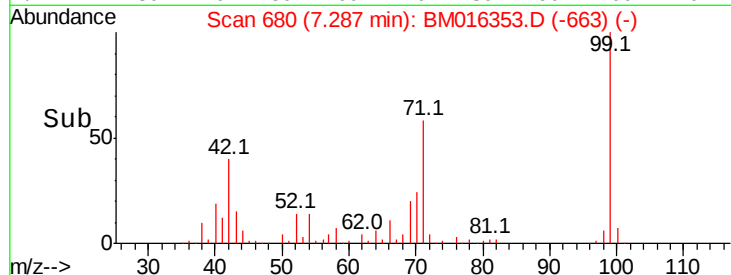

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.93 min Scan# 1300

Delta R.T. 0.01 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12

Tgt Ion: 136 Resp: 134838


Ion Ratio Lower Upper

136 100

137 11.0 8.7 13.1

54 10.3 4.6 6.8#

68 4.1 3.7 5.5


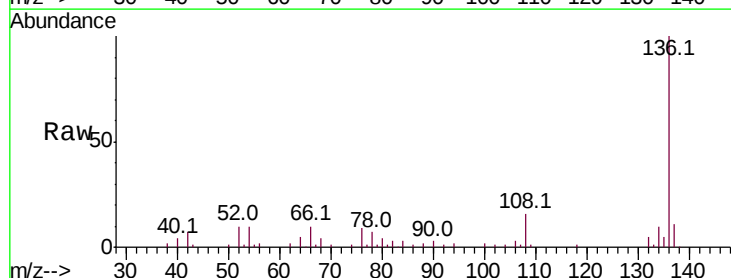



Abundance Ion 136.00 (135.70 to 136.70): BM016353.D (-1282) (-)

Ion 137.00 (136.70 to 137.70): BM016353.D (-1282) (-)

Ion 54.00 (53.70 to 54.70): BM016353.D (-1282) (-)

Ion 68.00 (67.70 to 68.70): BM016353.D (-1282) (-)

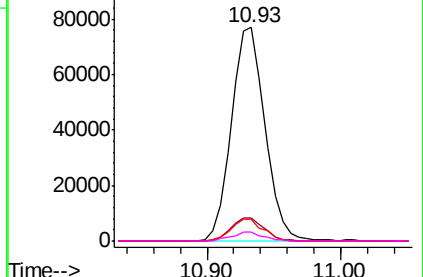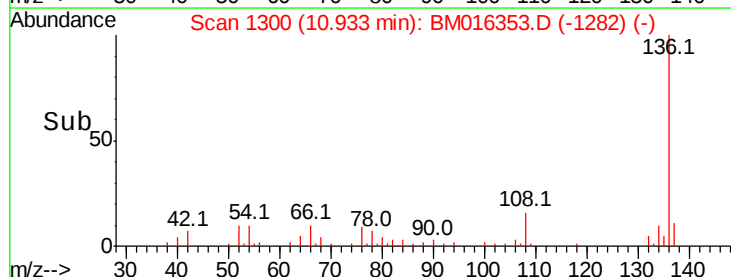

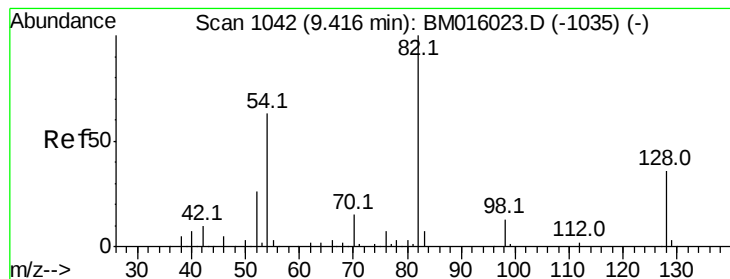

#23

Nitrobenzene-d5

Concen: N.D. ng

RT: 9.30 min Scan# 1023

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12

Instrument :

BNA_M

ClientSampleId :

SP-1-6


Tot Ion: 82 Resp: 219845

Ion Ratio Lower Upper

82 100

128 34.9 32.8 49.2




54 64.3 40.6 60.8#

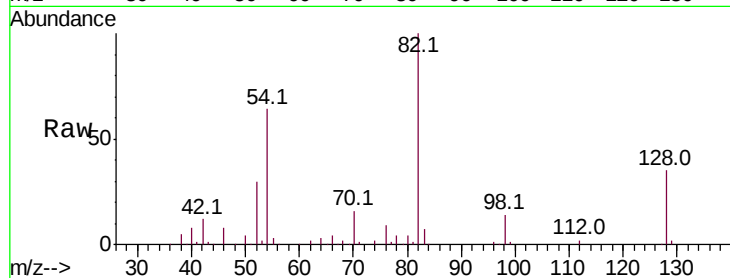

Abundance Ion 82.00 (81.70 to 82.70): BM016023.D (-1035) (-)

Ion 128.00 (127.70 to 128.70): BM016023.D (-1035) (-)

Ion 54.00 (53.70 to 54.70): BM016023.D (-1035) (-)

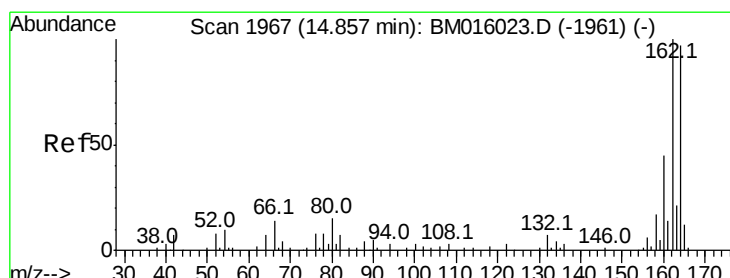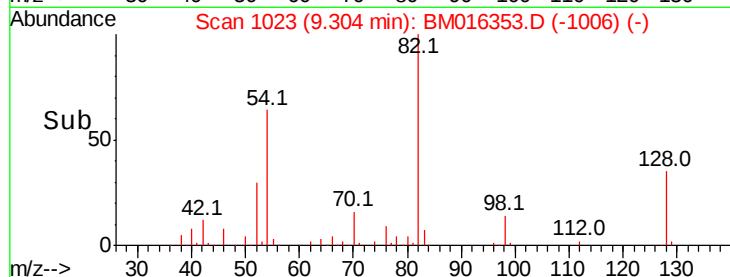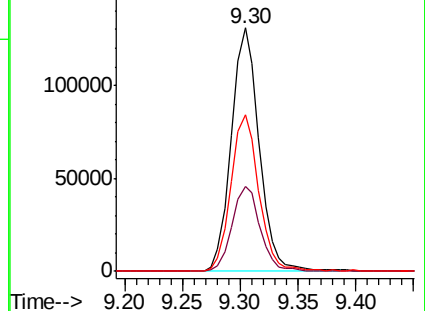

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.75 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12


Tgt Ion: 164 Resp: 73204

Ion Ratio Lower Upper

164 100

162 103.7 82.4 123.6



160 48.9 35.8 53.6

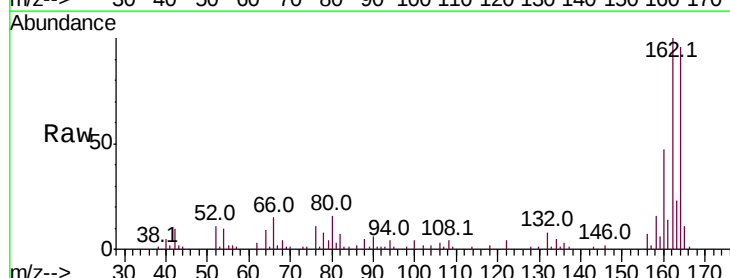


Abundance Ion 164.00 (163.70 to 164.70): BM016023.D (-1961) (-)

Ion 162.00 (161.70 to 162.70): BM016023.D (-1961) (-)

Ion 160.00 (159.70 to 160.70): BM016023.D (-1961) (-)

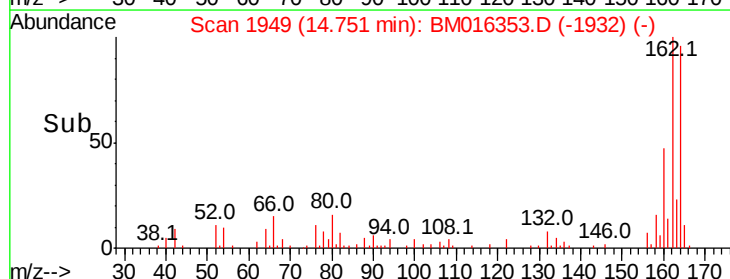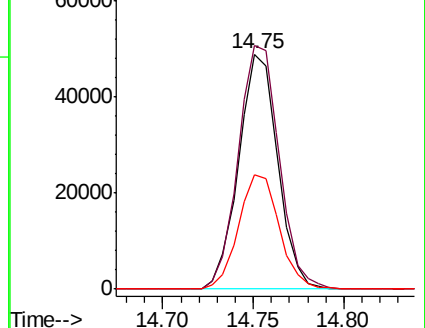


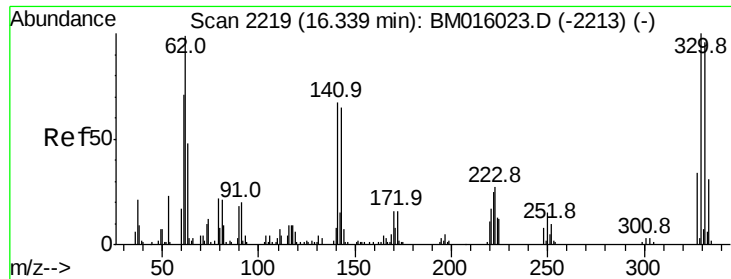




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.24 min Scan# 2203
 Delta R.T. -0.00 min
 Lab File: BM016353.D
 Acq: 14 Aug 2018 14:12

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-6

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	0.0	0.0#
141	80.4	0.0	0.0#

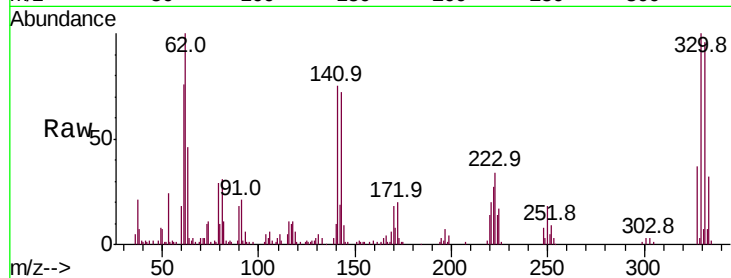


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

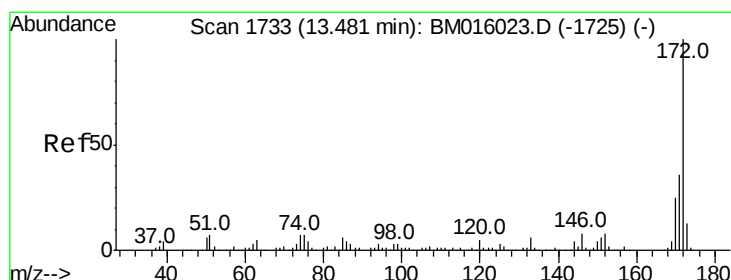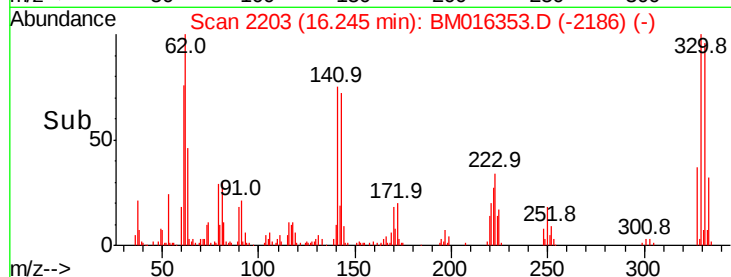
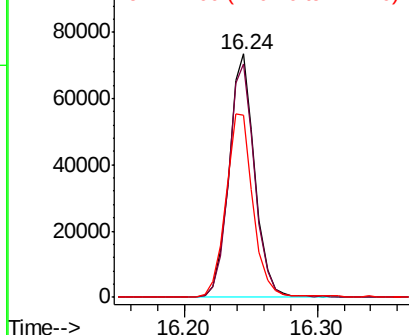



#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.37 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BM016353.D
 Acq: 14 Aug 2018 14:12

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.3	28.5	42.7
170	24.6	18.8	28.2

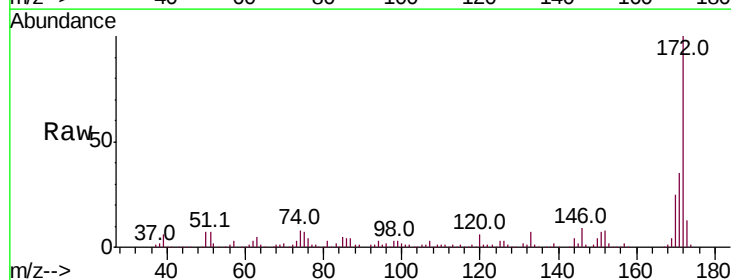

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

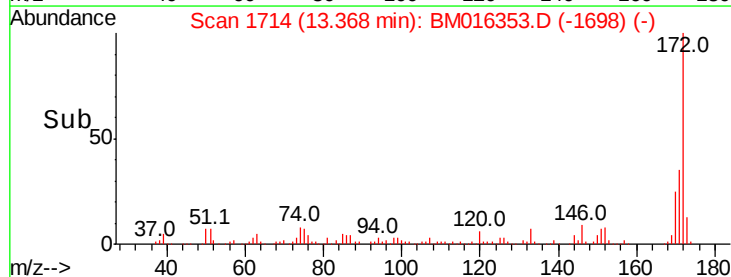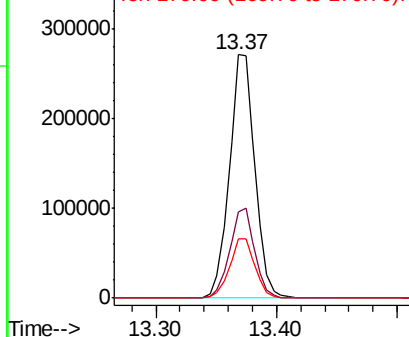

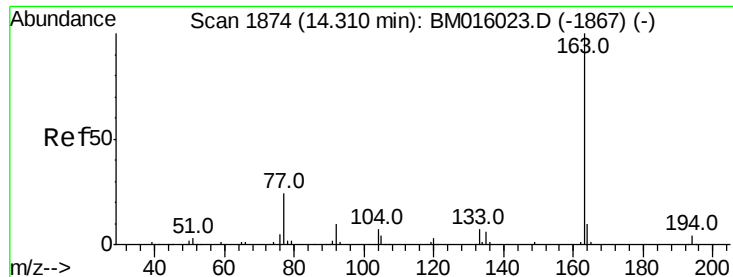

#49

Dimethylphthalate

Concen: 5.136 ng

RT: 14.21 min Scan# 1857

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12

Instrument :

BNA_M

ClientSampleId :

SP-1-6


Tot Ion:163 Resp: 32906

Ion Ratio Lower Upper




163 100

194 4.3 2.7 4.1#

164 10.5 8.2 12.2

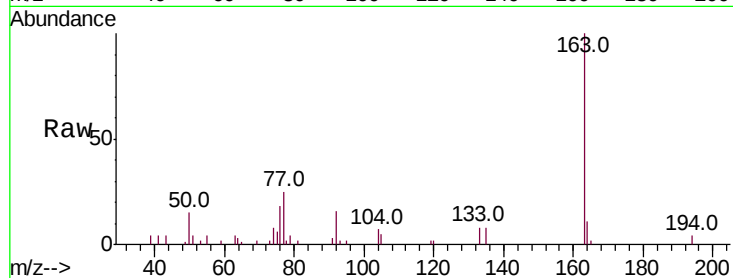

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

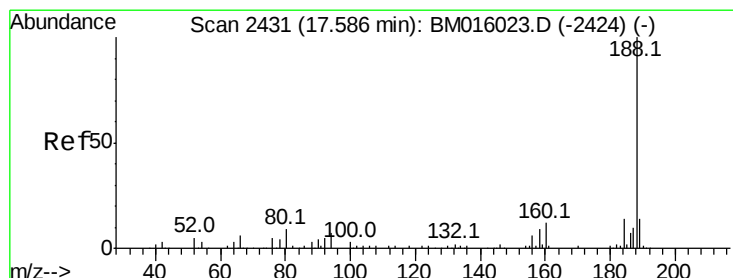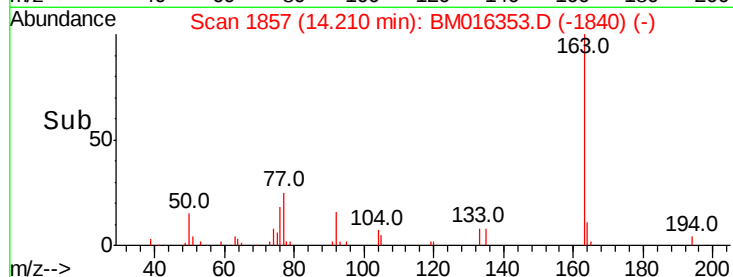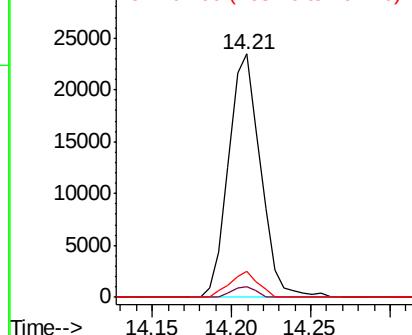

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.49 min Scan# 2415

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12


Tgt Ion:188 Resp: 148895

Ion Ratio Lower Upper



188 100


94 6.7 8.7 13.1#

80 8.6 9.3 13.9#

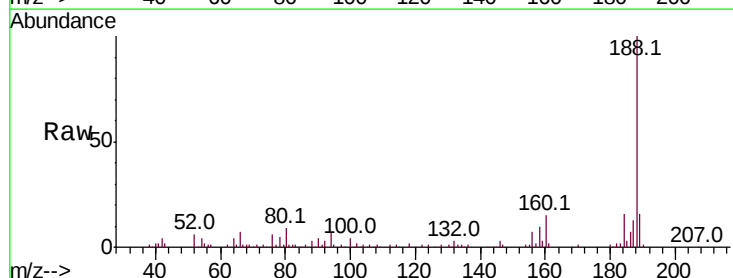

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

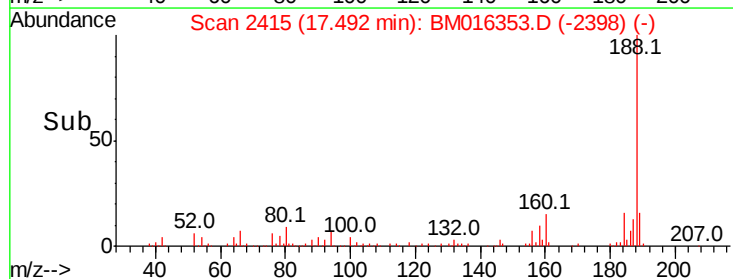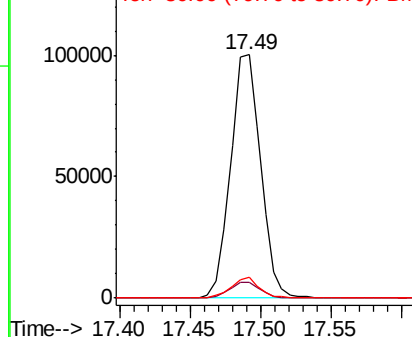

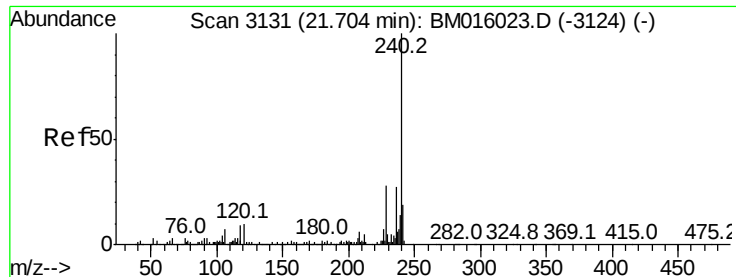

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.62 min Scan# 3117

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12

Instrument :

BNA_M

ClientSampleId :

SP-1-6


Tot Ion:240 Resp: 132835

Ion Ratio Lower Upper

240 100

120 8.7 8.2 12.2




236 29.0 20.0 30.0

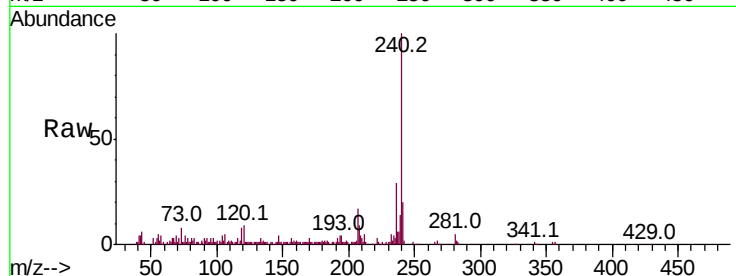

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

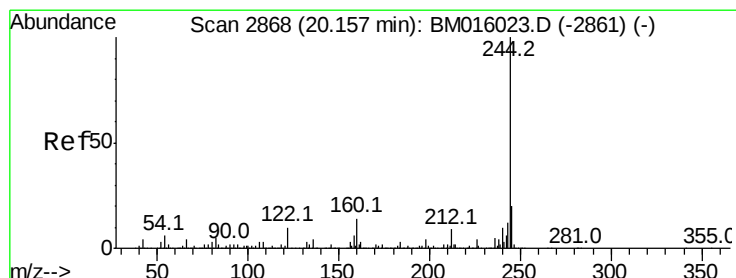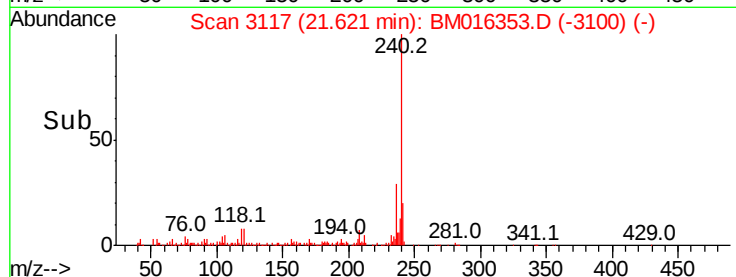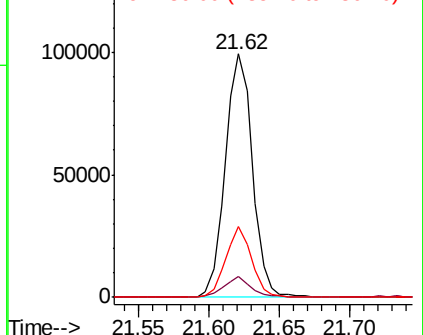

#78

Terphenyl-d14

Concen: Below ng

RT: 20.07 min Scan# 2853

Delta R.T. -0.00 min

Lab File: BM016353.D

Acq: 14 Aug 2018 14:12


Tgt Ion:244 Resp: 494138

Ion Ratio Lower Upper

244 100

212 10.5 4.9 7.3#



122 9.4 6.2 9.4#

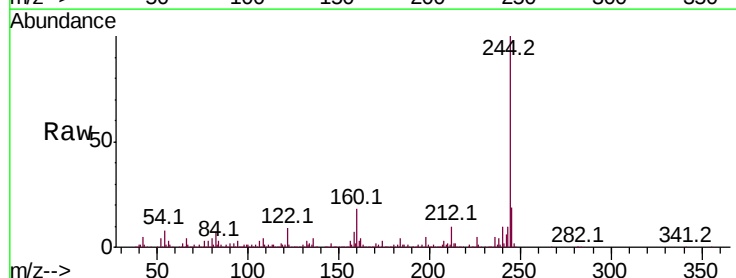


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

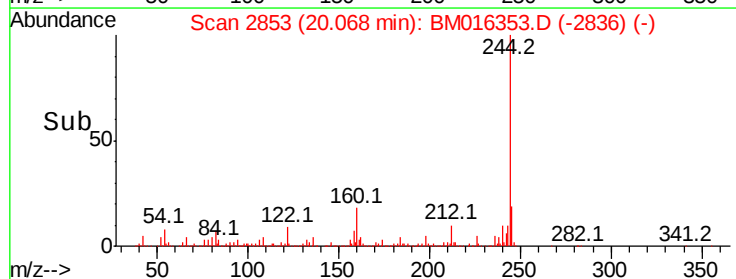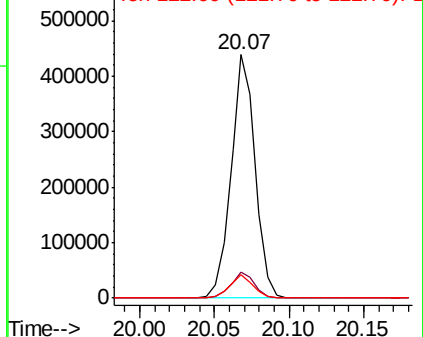

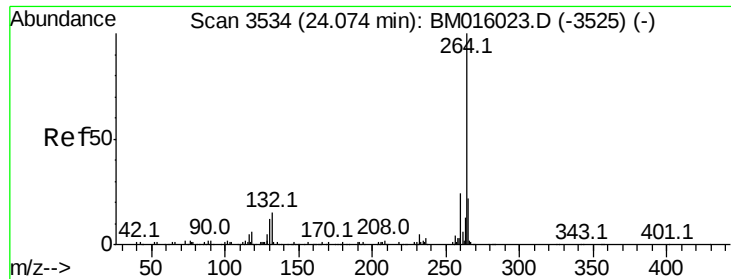

#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.95 min Scan# 3513
Delta R.T. 0.01 min
Lab File: BM016353.D
Acq: 14 Aug 2018 14:12

Instrument :
BNA_M
ClientSampleId :
SP-1-6

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.6	27.8
265	23.9	17.3	25.9

