


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081418\
 Data File : BM016346.D
 Acq On : 14 Aug 2018 09:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 15 11:23:48 2018

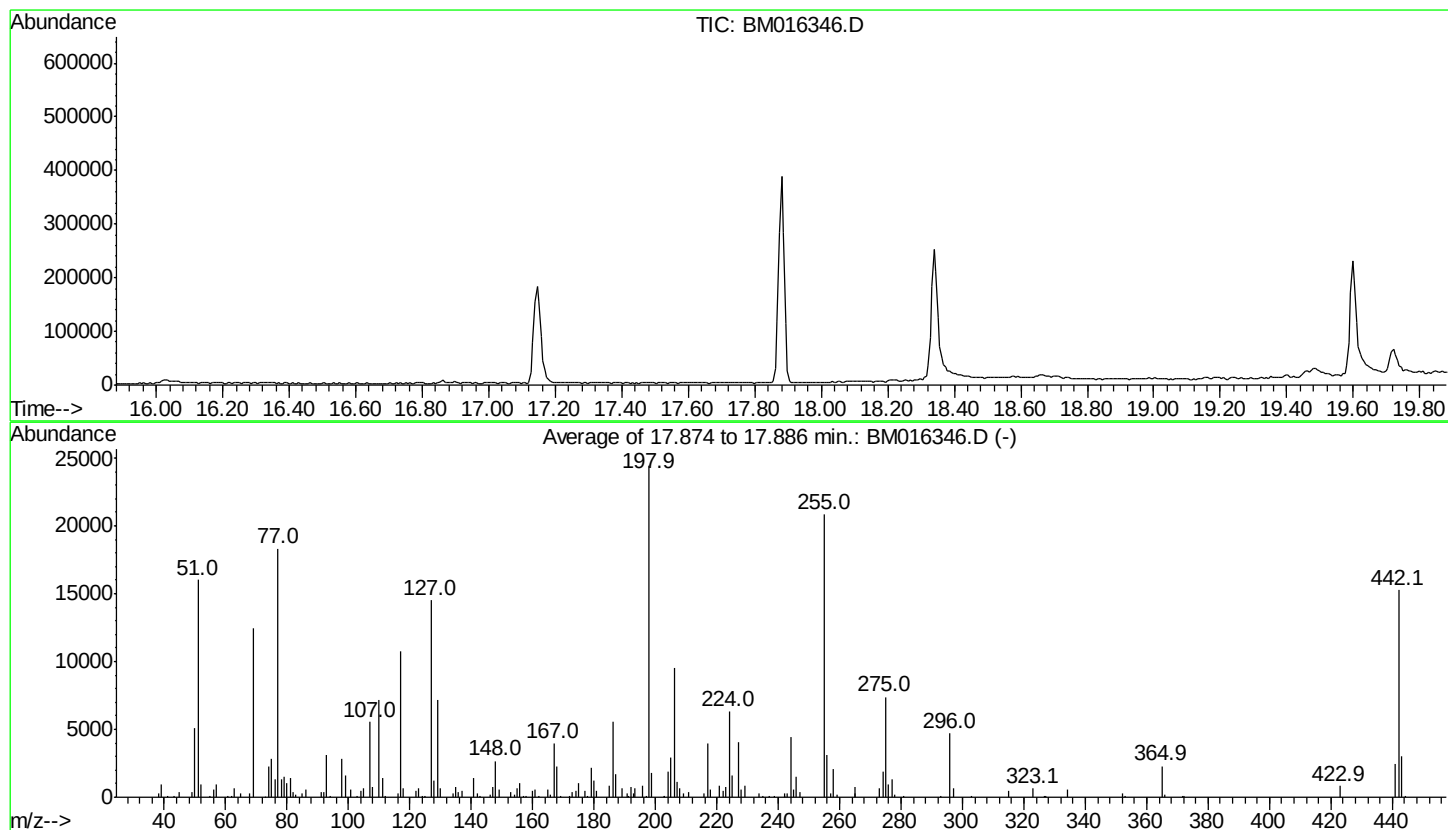

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.5	15999	PASS
68	69	0.00	2	1.9	242	PASS
69	198	0.00	100	51.0	12459	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.3	14501	PASS
197	198	0.00	2	0.4	109	PASS
198	198	100	100	100.0	24434	PASS
199	198	5	9	7.5	1829	PASS
275	198	10	60	30.2	7385	PASS
365	198	1	100	9.3	2267	PASS
441	198	0.01	100	10.1	2472	PASS
442	198	50	100	62.5	15277	PASS
443	442	15	24	19.9	3040	PASS