
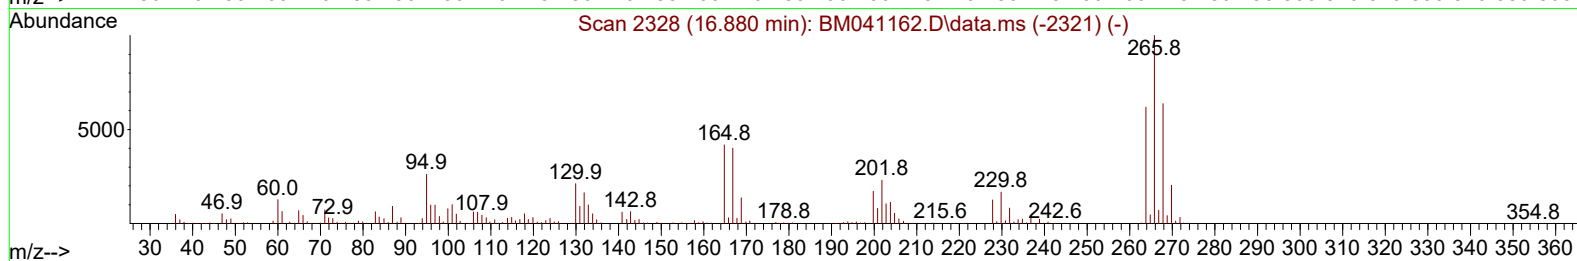
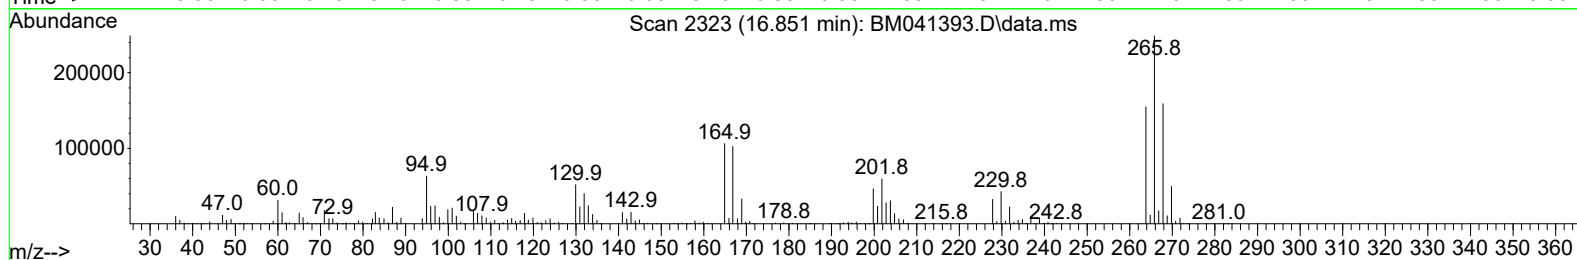


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041393.D
Acq On : 14 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 11:19:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 17:51:06 2023
Response via : Initial Calibration

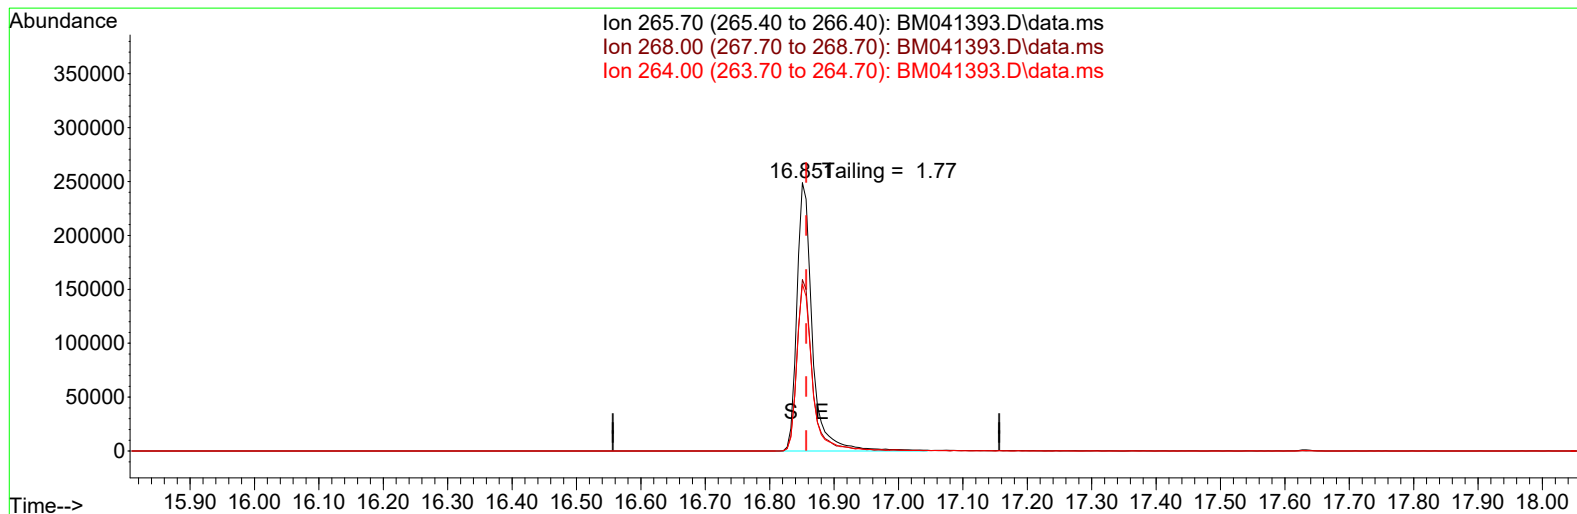

TIC: BM041393.D\data.ms

(70) Pentachlorophenol (C)




16.851min (-0.006) 0.00 ng

response 417716

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.88
264.00	61.80	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041393.D
Acq On : 14 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 11:19:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 17:51:06 2023
Response via : Initial Calibration

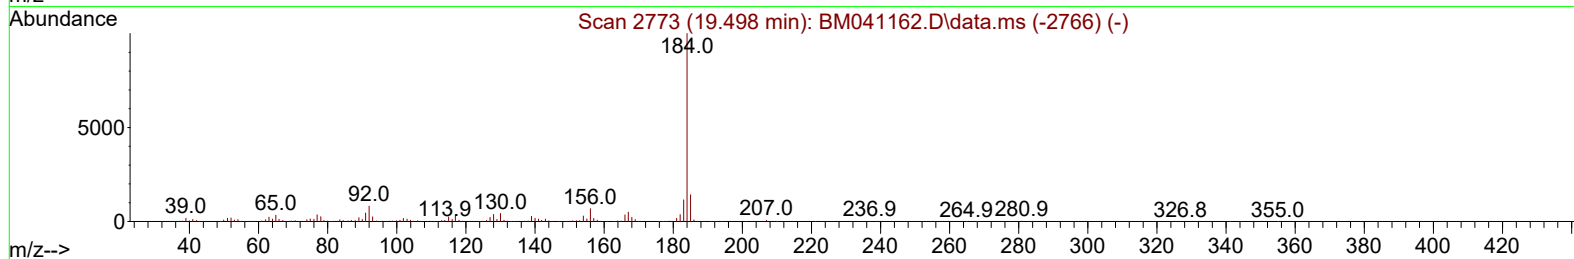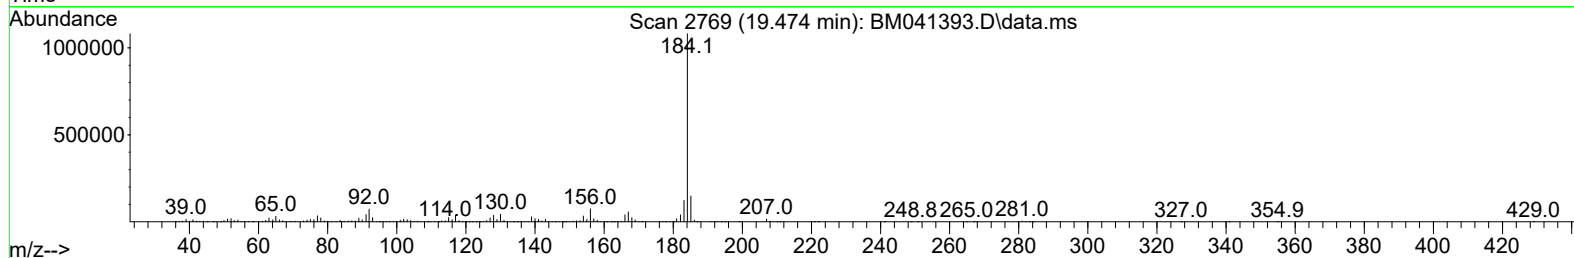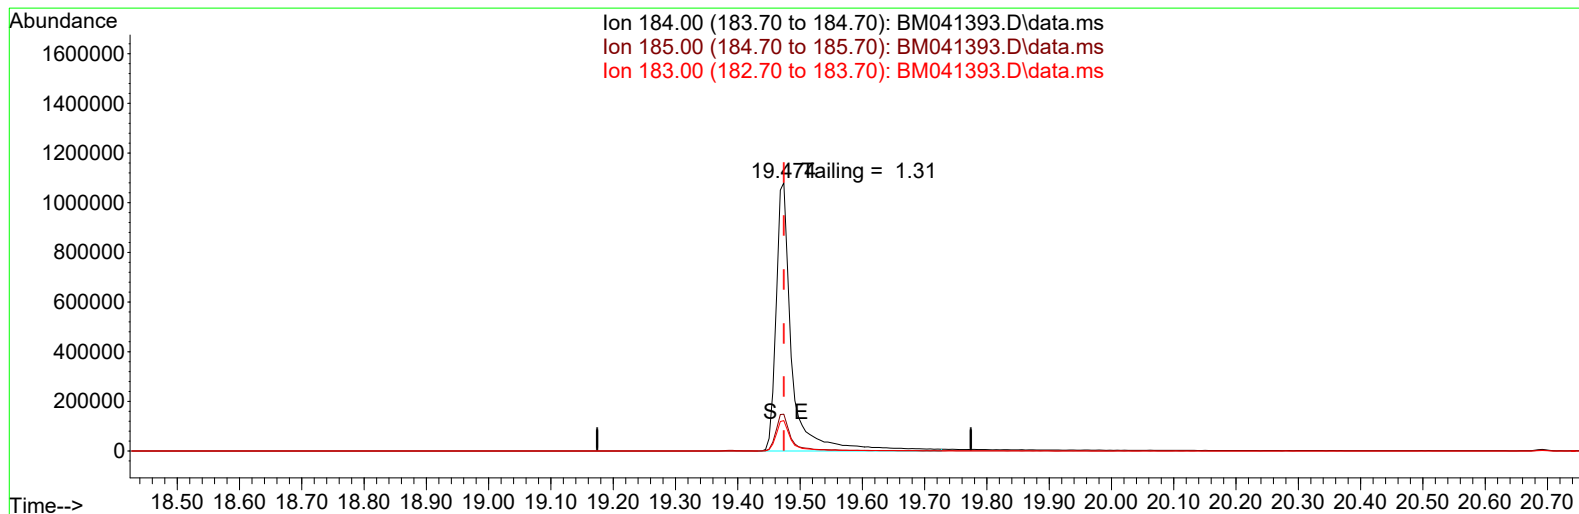

TIC: BM041393.D\data.ms

(77) Benzidine

19.474min (-0.000) 0.00 ng

response 1929102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.75
183.00	11.50	11.33
0.00	0.00	0.00