

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
 Data File : BM041395.D
 Acq On : 14 Aug 2023 10:33
 Operator : MA/JU
 Sample : PB154564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB154564BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.346	361	367	390	rBV	3147381	4806417	37.87%	9.625%
2	6.957	633	641	670	rBV	3039726	4901806	38.62%	9.816%
3	7.769	773	779	791	rBV	497448	804881	6.34%	1.612%
4	8.951	971	980	999	rBV	1743315	2982522	23.50%	5.973%
5	10.575	1249	1256	1268	rBV	638007	1141605	8.99%	2.286%
6	13.057	1671	1678	1705	rBV	4913512	7417092	58.43%	14.853%
7	14.439	1906	1913	1932	rBV	1024505	1621087	12.77%	3.246%
8	15.939	2161	2168	2197	rBV	4161020	6559938	51.68%	13.137%
9	17.198	2376	2382	2400	rBV	1341711	2045339	16.11%	4.096%
10	18.098	2530	2535	2547	rBV	71900	183701	1.45%	0.368%
11	19.839	2825	2831	2846	rBV	10569350	12693218	100.00%	25.419%
12	21.409	3093	3098	3109	rBV	1737437	2427696	19.13%	4.862%
13	23.774	3493	3500	3514	rBV	1052436	2351417	18.52%	4.709%




Sum of corrected areas: 49936719

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041395.D
Acq On : 14 Aug 2023 10:33
Operator : MA/JU
Sample : PB154564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154564BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

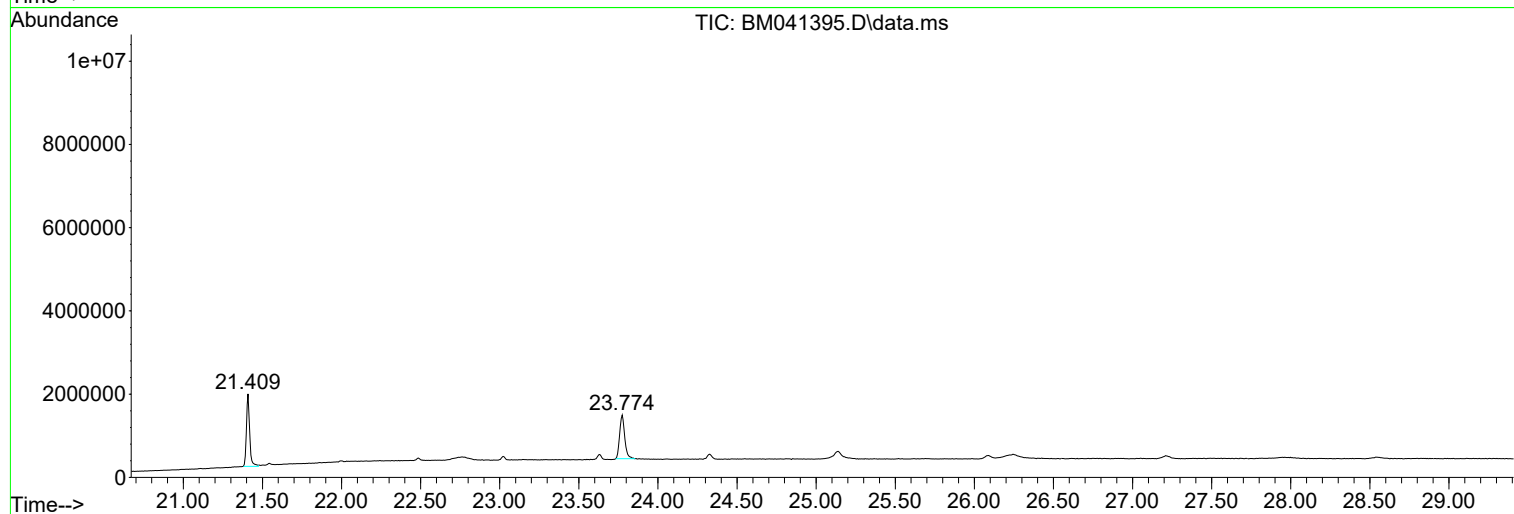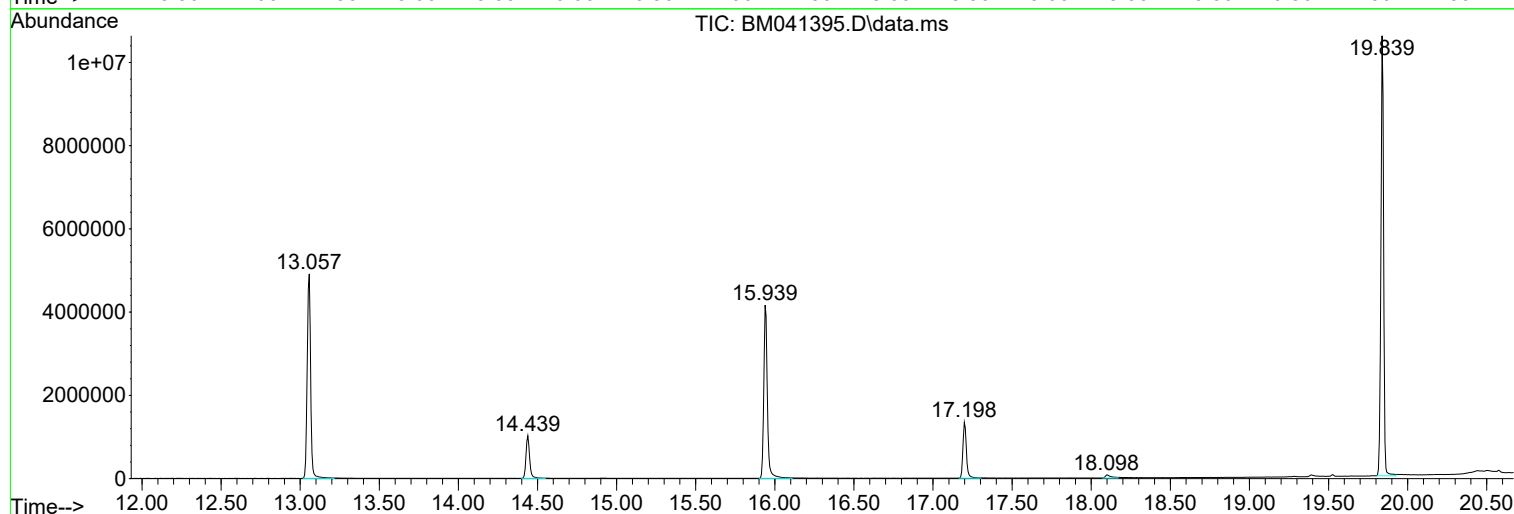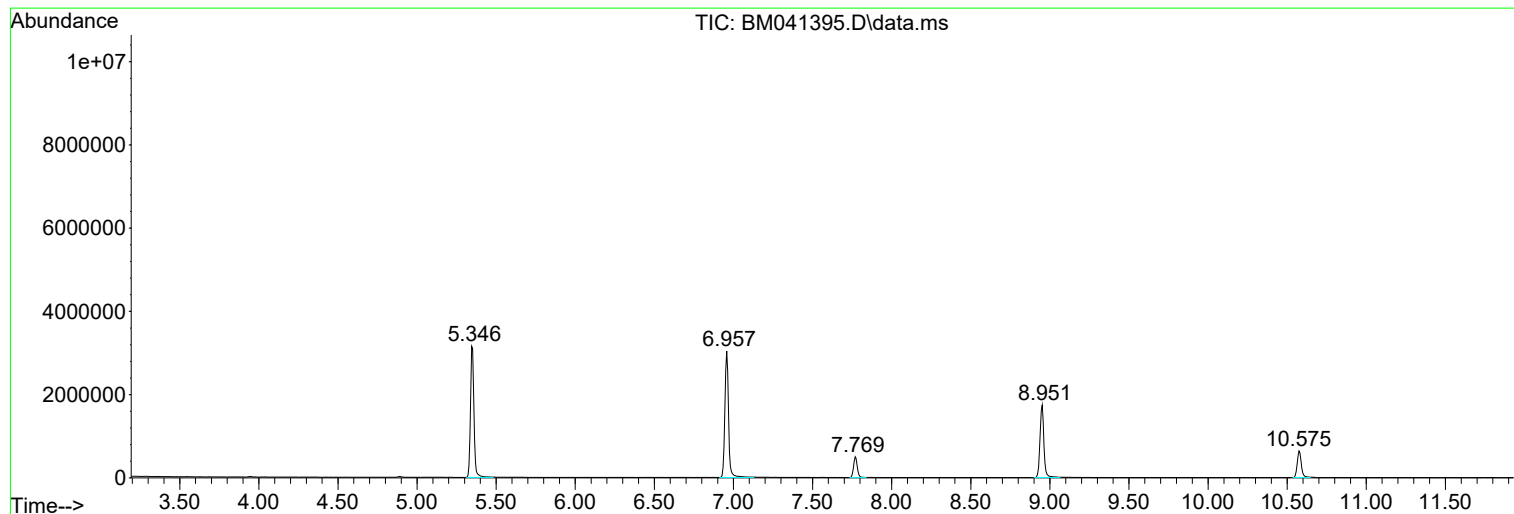

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041395.D
Acq On : 14 Aug 2023 10:33
Operator : MA/JU
Sample : PB154564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154564BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041395.D
Acq On : 14 Aug 2023 10:33
Operator : MA/JU
Sample : PB154564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154564BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------