


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041393.D
Acq On : 14 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 11 17:51:06 2023

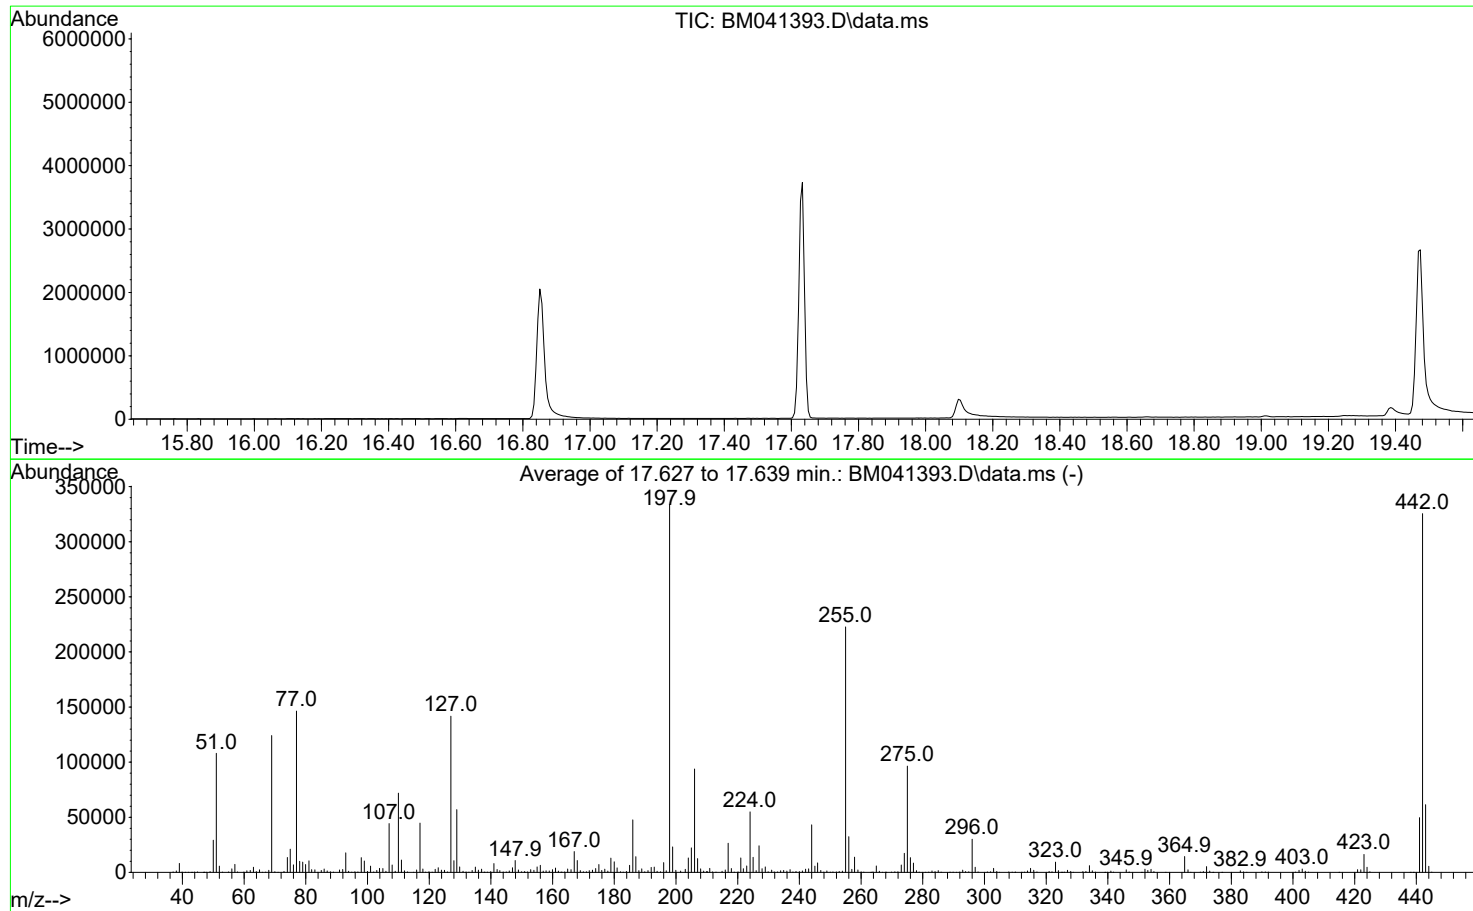




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	108008	PASS
68	69	0.00	2	1.5	1859	PASS
69	198	0.00	100	37.2	124177	PASS
70	69	0.00	2	0.5	628	PASS
127	198	10	80	42.5	141763	PASS
197	198	0.00	2	0.4	1457	PASS
198	198	100	100	100.0	333803	PASS
199	198	5	9	6.9	23096	PASS
275	198	10	60	28.9	96461	PASS
365	198	1	100	4.3	14438	PASS
441	198	0.01	100	14.9	49739	PASS
442	442	50	100	100.0	325589	PASS
443	442	15	24	18.9	61381	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
Data File : BM041393.D
Acq On : 14 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 14 11:19:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 17:51:06 2023
Response via : Initial Calibration

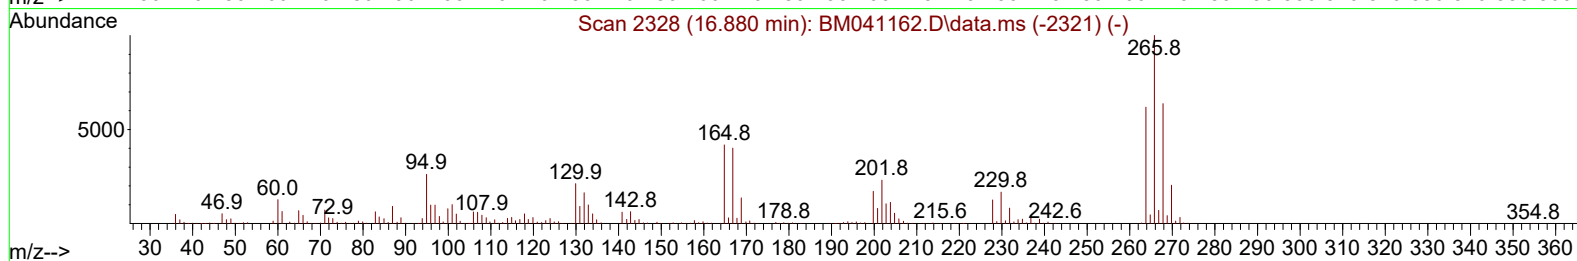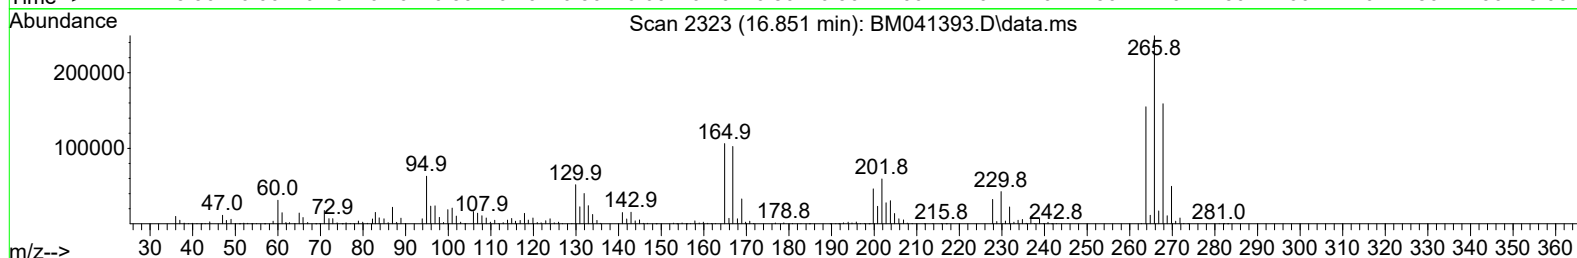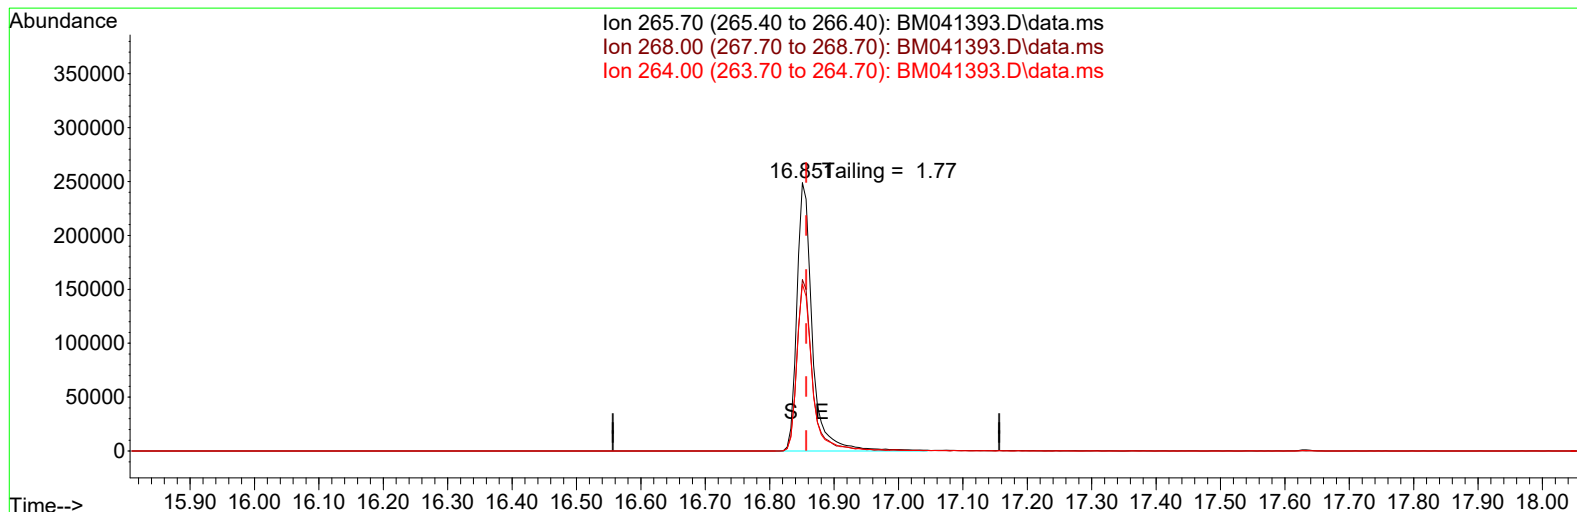

TIC: BM041393.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.006) 0.00 ng




response 417716

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.88
264.00	61.80	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081423\
 Data File : BM041393.D
 Acq On : 14 Aug 2023 08:20
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 14 11:19:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 17:51:06 2023
 Response via : Initial Calibration

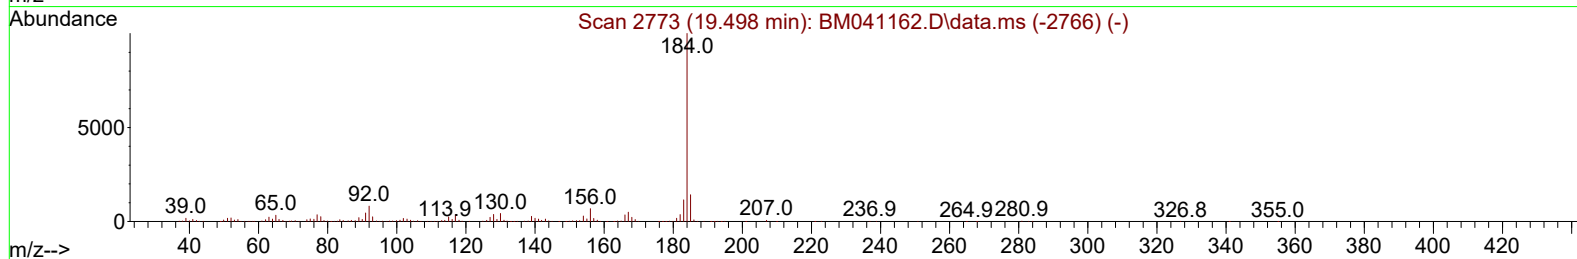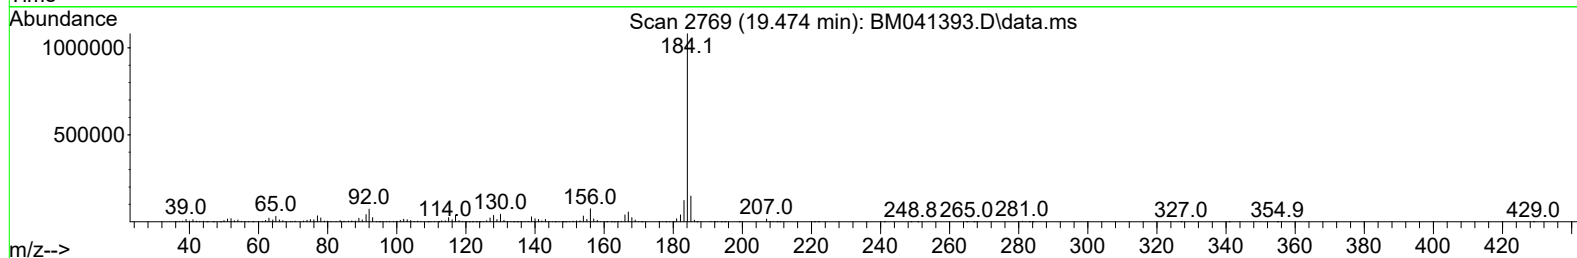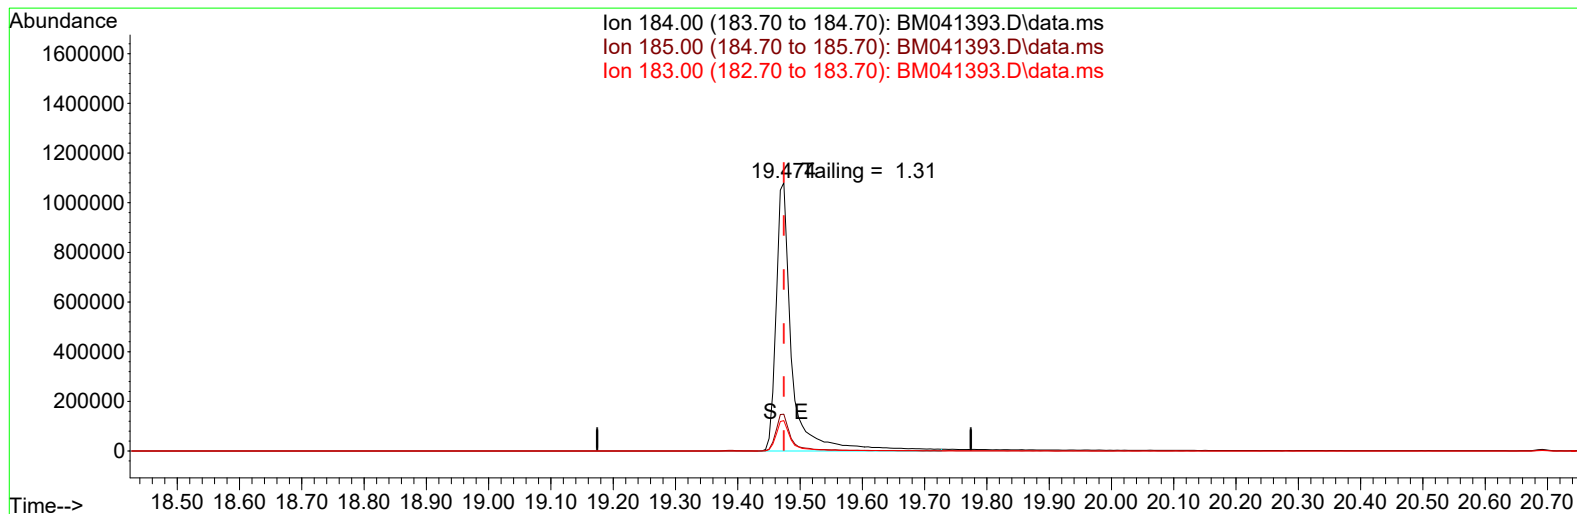

TIC: BM041393.D\data.ms

(77) Benzidine

19.474min (-0.000) 0.00 ng

response 1929102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.75
183.00	11.50	11.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/14/2023	BNA_M	<u>BM041393.D</u>
Compound Name	Response	Retention Time
DDT	1285929	20.692
DDD	23731	20.256
DDE	3980	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27711	1313640	2.11

Instrument :
BNA_M
ClientSampleId :
DFTPP