

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081518\
 Data File : BM016376.D
 Acq On : 15 Aug 2018 12:29
 Operator : SJ/JU
 Sample : PB112015BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112015BL

Quant Time: Aug 16 01:26:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	23696	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	84051	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	43442	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	96167	20.00	ng	0.00
75) Chrysene-d12	21.62	240	109596	20.00	ng	0.00
86) Perylene-d12	23.94	264	116638	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	166388	116.64	ng	0.00
7) Phenol-d6	7.29	99	193779	104.02	ng	0.00
23) Nitrobenzene-d5	9.30	82	151779	83.99	ng	0.00
41) 2,4,6-Tribromophenol	16.24	330	65806	119.43	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	291082	81.53	ng	0.00
78) Terphenyl-d14	20.07	244	495995	94.74	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.43	79	3445	2.322	ng	Qvalue # 34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081518\
Data File : BM016376.D
Acq On : 15 Aug 2018 12:29
Operator : SJ/JU
Sample : PB112015BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112015BL

Quant Time: Aug 16 01:26:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

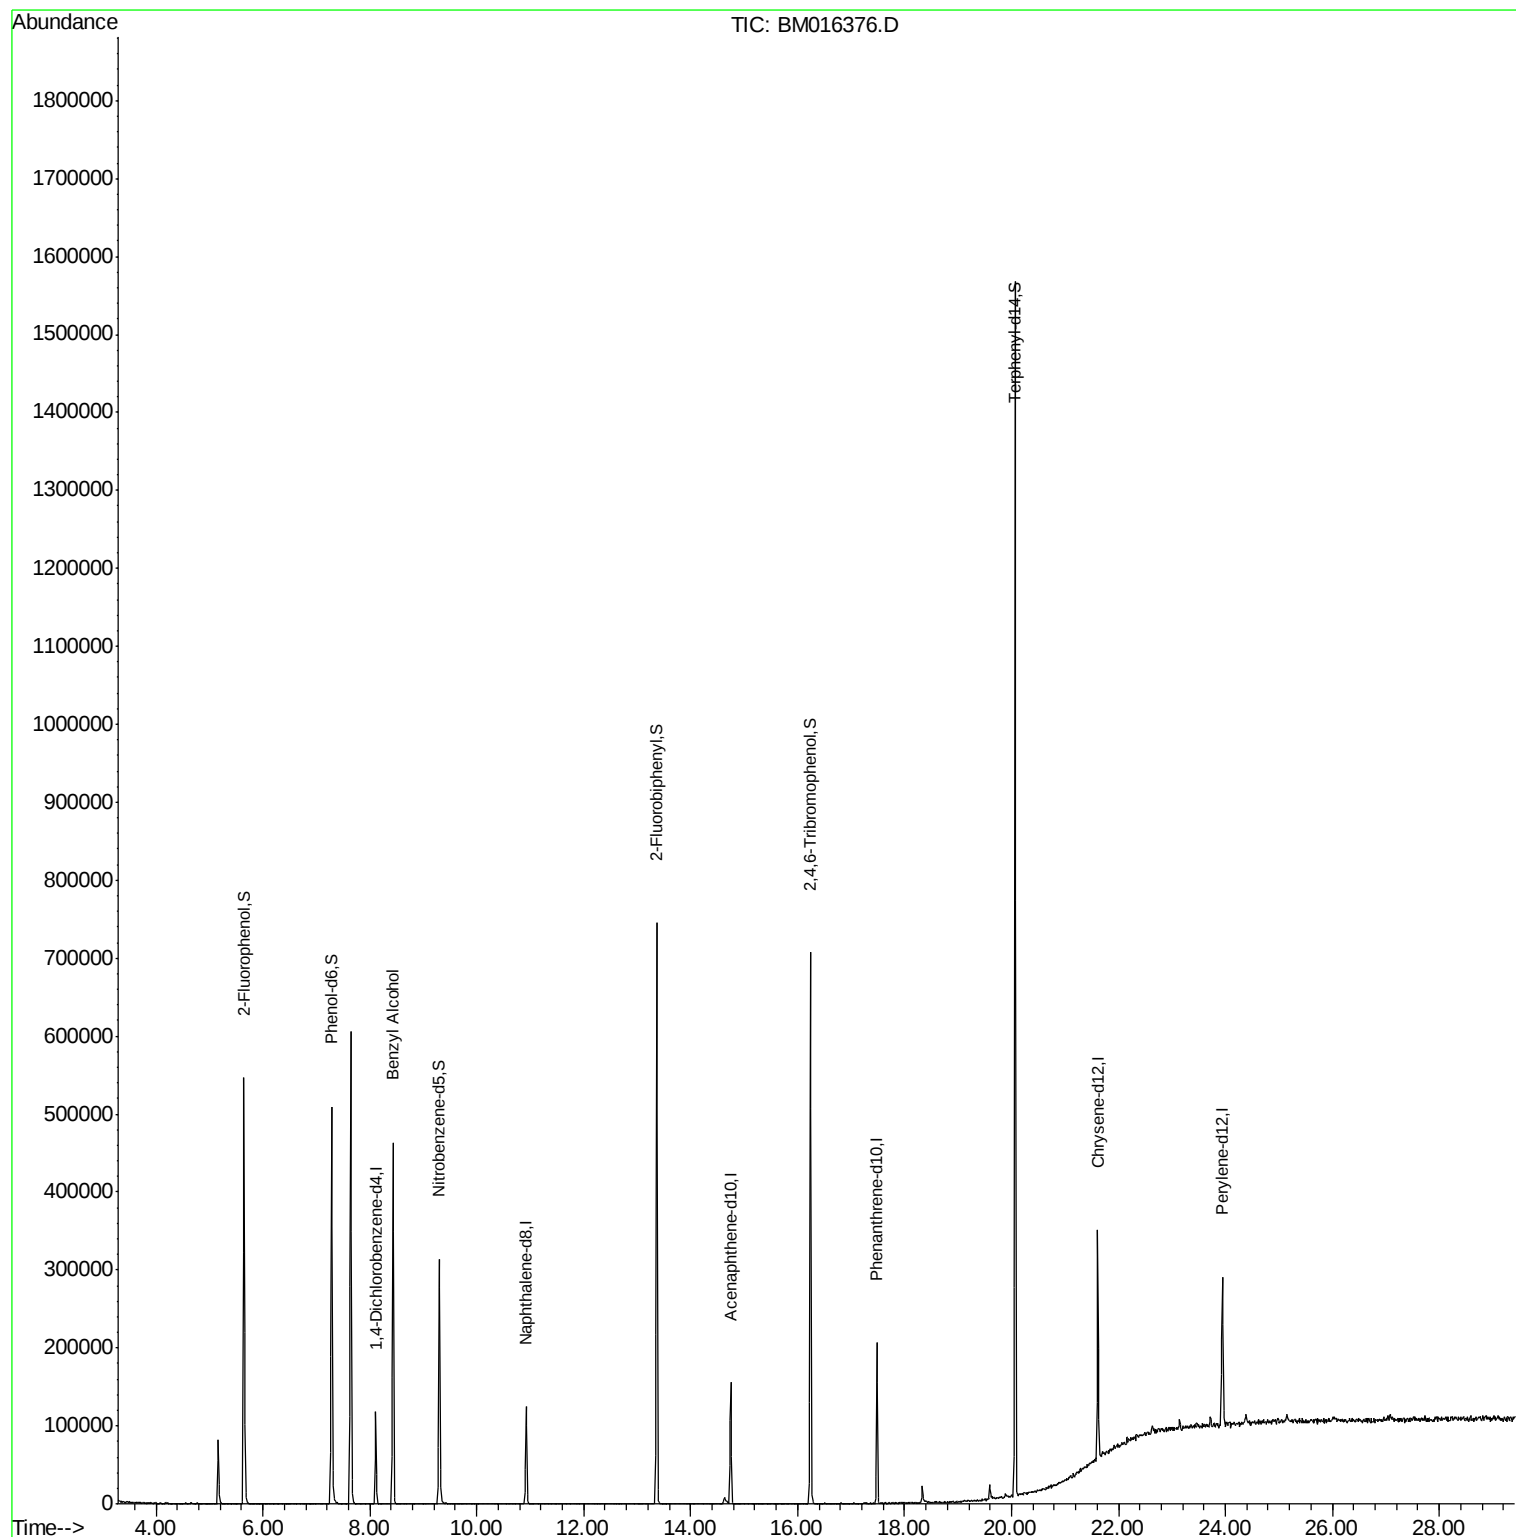


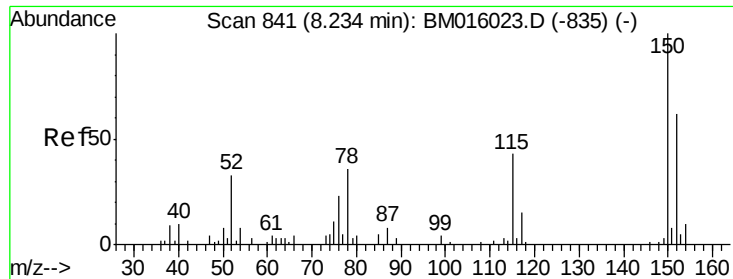




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.11 min Scan# 820
 Delta R.T. -0.01 min
 Lab File: BM016376.D
 Acq: 15 Aug 2018 12:29

Instrument :
 BNA_M
 ClientSampleId :
 PB112015BL

Tgt Ion:152 Resp: 23696
 Ion Ratio Lower Upper
 152 100
 150 148.8 119.5 179.3
 115 71.0 43.0 64.4#

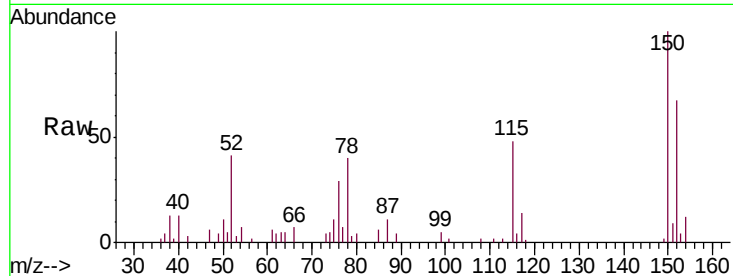


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

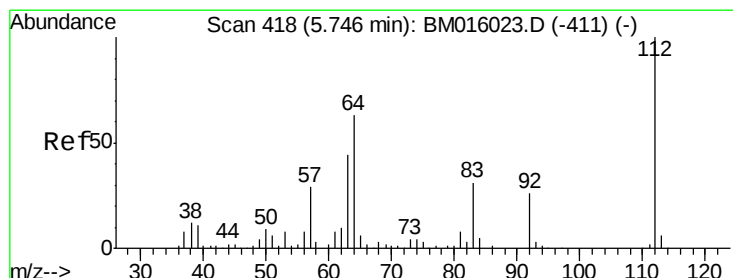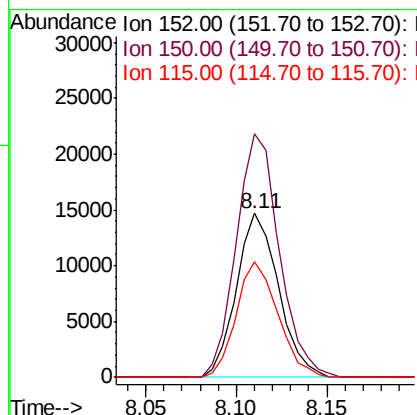
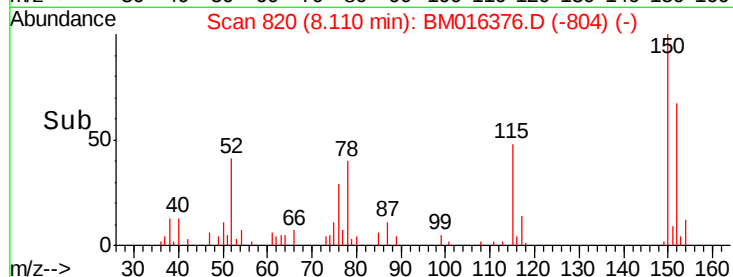


#5
 2-Fluorophenol
 Concen: N.D. ng
 RT: 5.65 min Scan# 401
 Delta R.T. 0.00 min
 Lab File: BM016376.D
 Acq: 15 Aug 2018 12:29

Tgt Ion:112 Resp: 166388
 Ion Ratio Lower Upper
 112 100
 64 62.8 38.6 57.8#
 63 47.0 19.3 28.9#

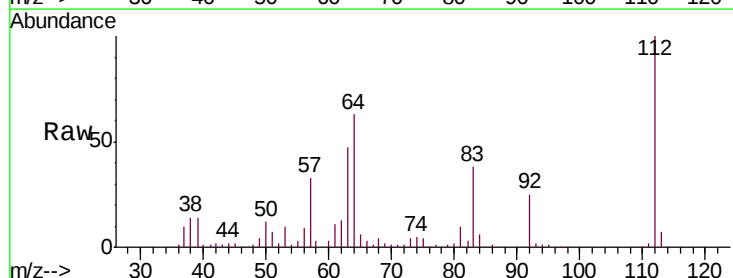

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

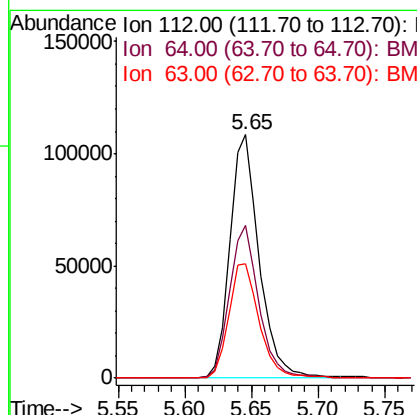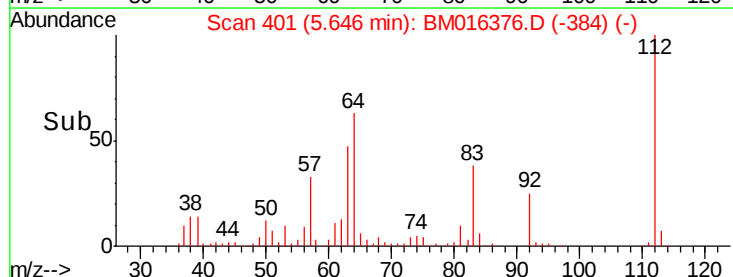



#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 680

Delta R.T. 0.00 min

Lab File: BM016376.D

Acq: 15 Aug 2018 12:29

Instrument :

BNA_M

ClientSampleId :

PB112015BL


Tgt Ion: 99 Resp: 193779

Ion Ratio Lower Upper

99 100

42 41.2 11.0 16.4#




71 58.5 23.4 35.2#

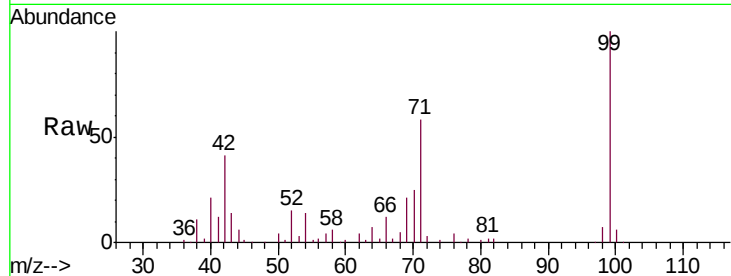

Abundance Ion 99.00 (98.70 to 99.70): BM016376.D (-690) (-)

Ion 42.00 (41.70 to 42.70): BM016376.D (-690) (-)

Ion 71.00 (70.70 to 71.70): BM016376.D (-690) (-)

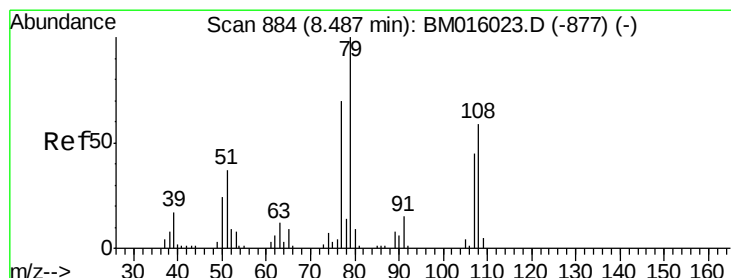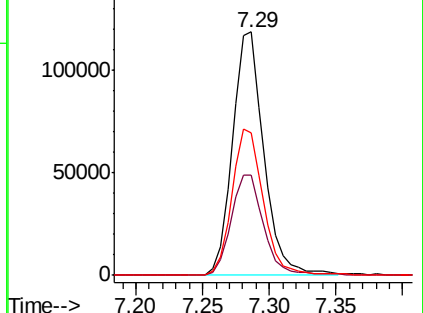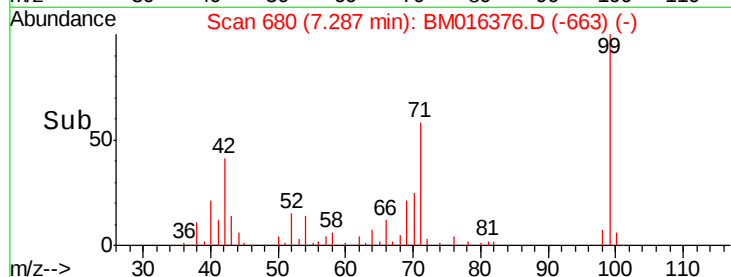

#15

Benzyl Alcohol

Concen: 2.322 ng

RT: 8.43 min Scan# 875

Delta R.T. 0.06 min

Lab File: BM016376.D

Acq: 15 Aug 2018 12:29


Tgt Ion: 79 Resp: 3445

Ion Ratio Lower Upper

79 100

108 89.7 65.0 97.4



77 174.3 53.0 79.6#

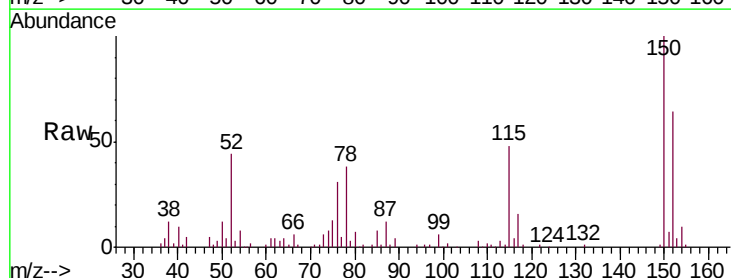

Abundance Ion 79.00 (78.70 to 79.70): BM016376.D (-848) (-)

Ion 108.00 (107.70 to 108.70): BM016376.D (-848) (-)

Ion 77.00 (76.70 to 77.70): BM016376.D (-848) (-)

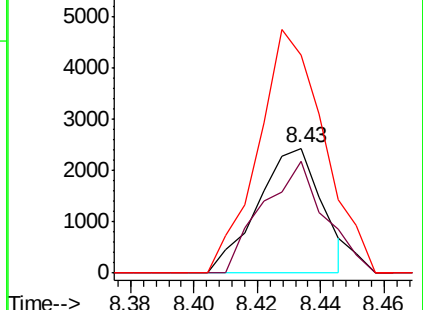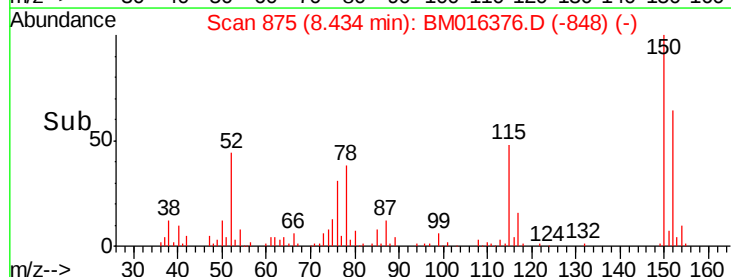







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1298
Delta R.T. -0.01 min
Lab File: BM016376.D
Acq: 15 Aug 2018 12:29

Instrument :
BNA_M
ClientSampleId :
PB112015BL

Tgt Ion:	136	Resp:	84051
Ion	Ratio	Lower	Upper
136	100		
137	11.9	8.7	13.1
54	10.2	4.6	6.8#
68	3.2	3.7	5.5#

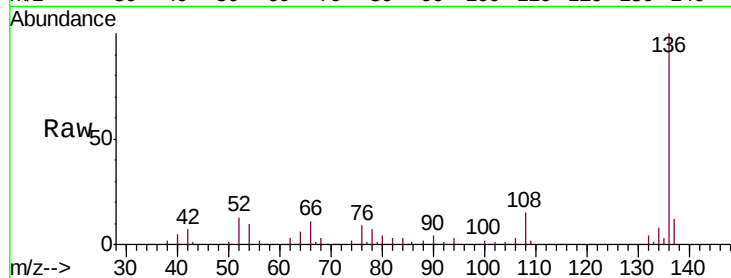


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

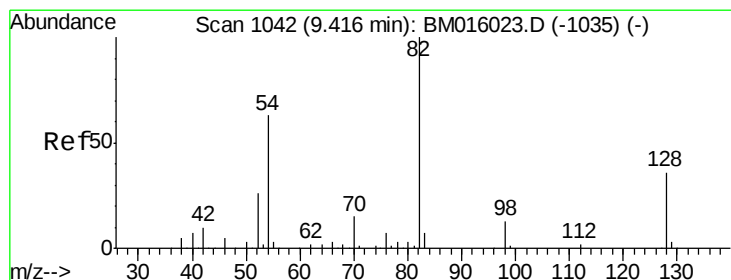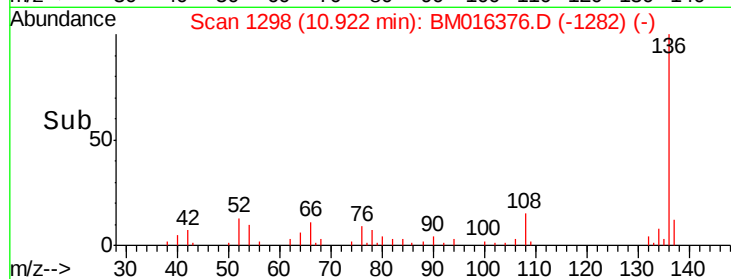
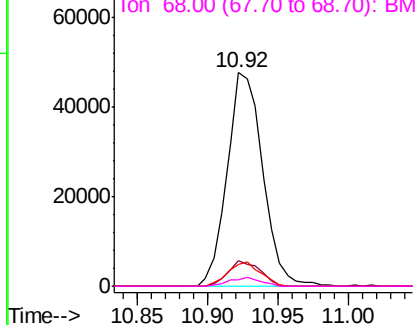


#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.30 min Scan# 1022
Delta R.T. -0.01 min
Lab File: BM016376.D
Acq: 15 Aug 2018 12:29

Tgt Ion:	82	Resp:	151779
Ion	Ratio	Lower	Upper
82	100		
128	33.0	32.8	49.2
54	63.3	40.6	60.8#

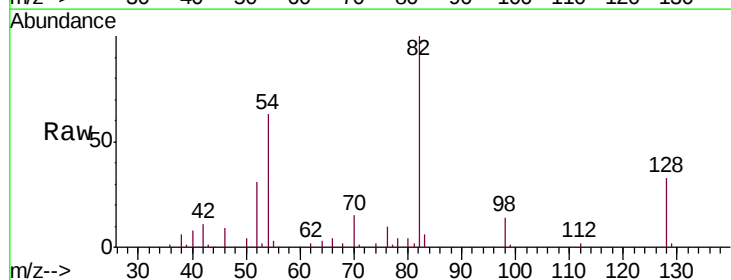

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

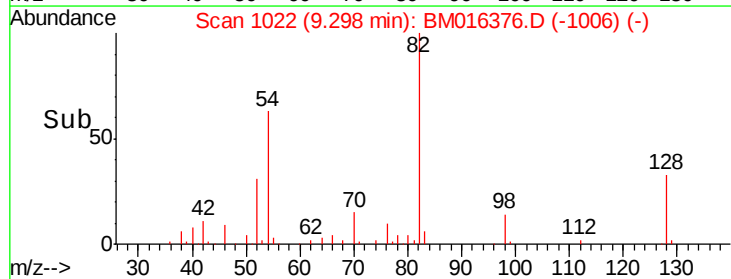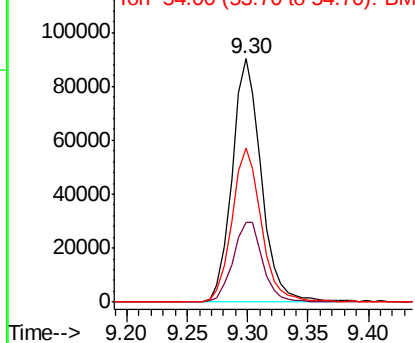



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.75 min Scan# 1948

Delta R.T. -0.01 min

Lab File: BM016376.D

Acq: 15 Aug 2018 12:29

Instrument :

BNA_M

ClientSampleId :

PB112015BL


Tgt Ion:164 Resp: 43442

Ion Ratio Lower Upper

164 100

162 104.4 82.4 123.6




160 49.9 35.8 53.6

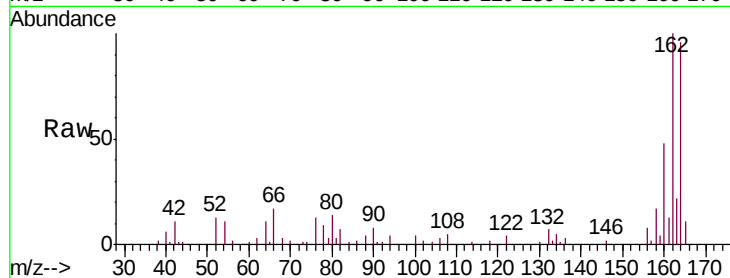

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

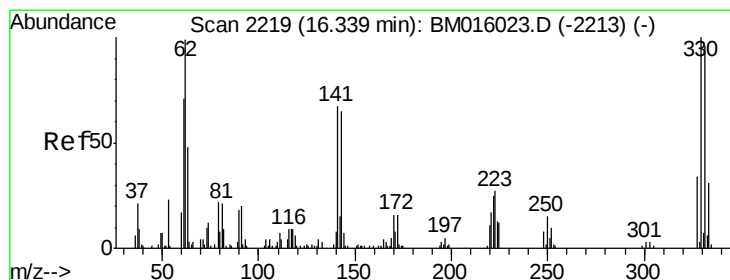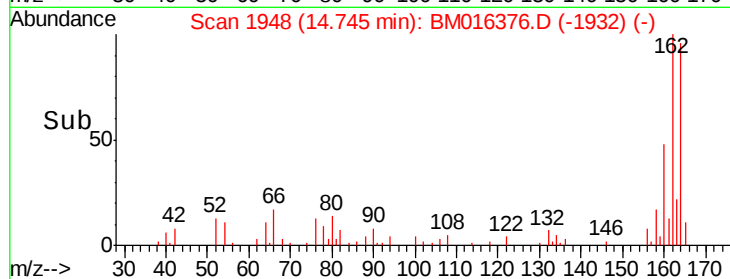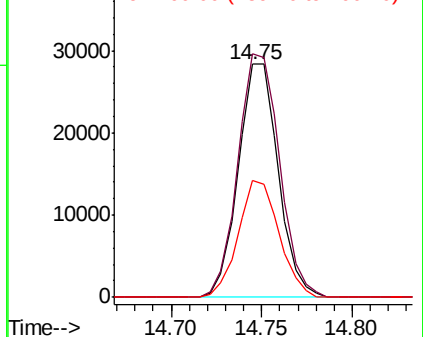

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.24 min Scan# 2202

Delta R.T. -0.01 min

Lab File: BM016376.D

Acq: 15 Aug 2018 12:29


Tgt Ion:330 Resp: 65806

Ion Ratio Lower Upper

330 100

332 97.2 0.0 0.0#



141 84.6 0.0 0.0#

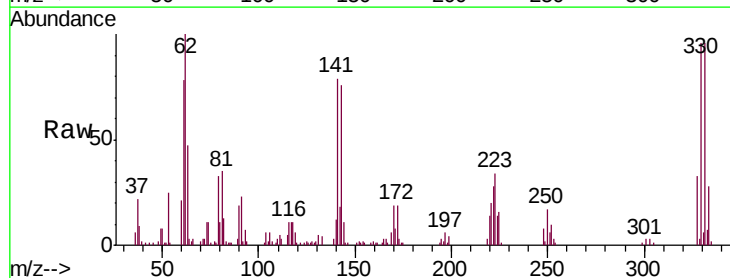

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



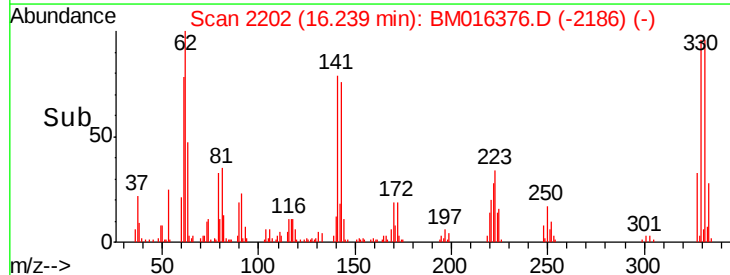
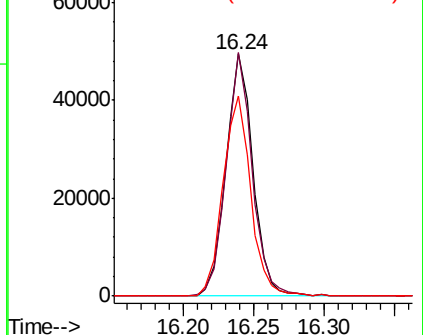




#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.37 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BM016376.D
 Acq: 15 Aug 2018 12:29




Instrument :
 BNA_M
 ClientSampleId :
 PB112015BL

Tgt Ion:172 Resp: 291082
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.5 42.7
 170 24.8 18.8 28.2

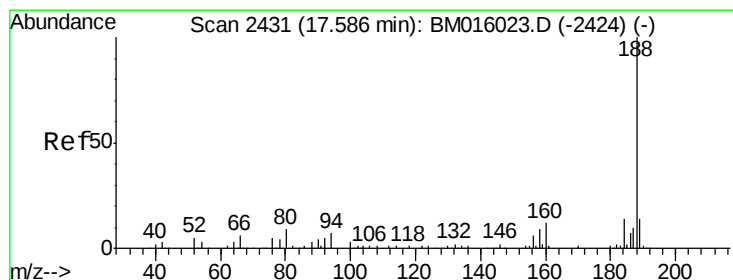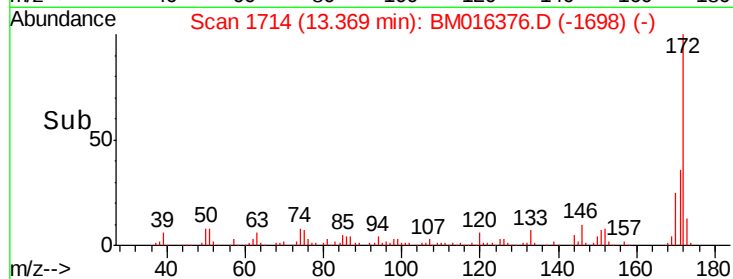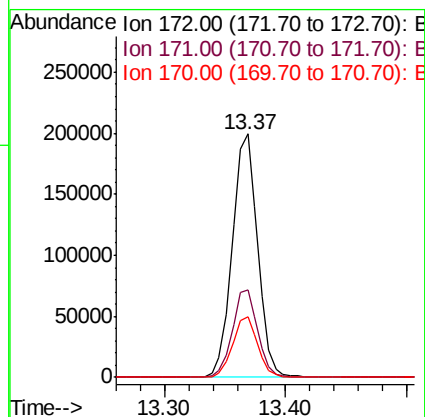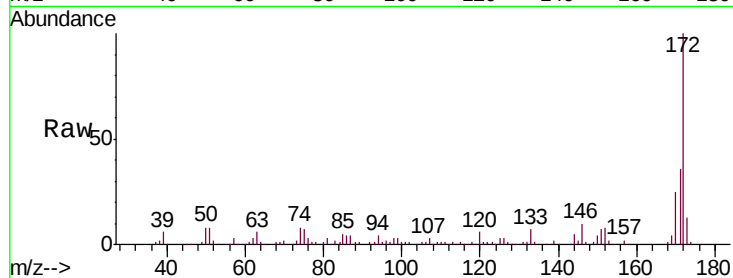

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.49 min Scan# 2414
 Delta R.T. -0.01 min
 Lab File: BM016376.D
 Acq: 15 Aug 2018 12:29

Tgt Ion:188 Resp: 96167
 Ion Ratio Lower Upper
 188 100
 94 6.3 8.7 13.1#
 80 7.1 9.3 13.9#

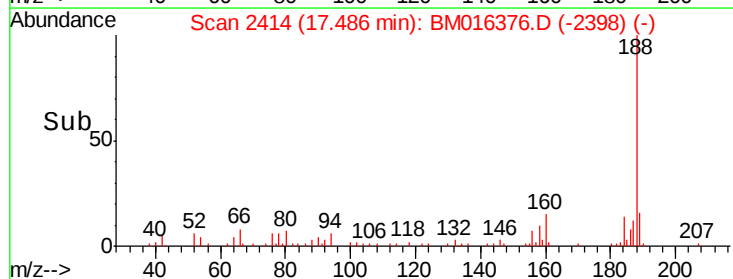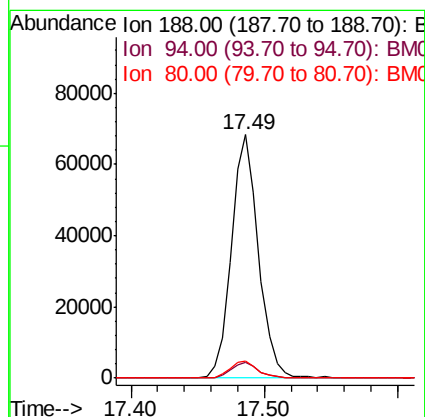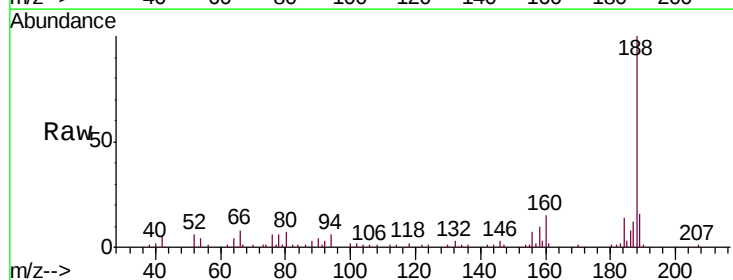



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.62 min Scan# 3116

Delta R.T. -0.01 min

Lab File: BM016376.D

Acq: 15 Aug 2018 12:29

Instrument :

BNA_M

ClientSampleId :

PB112015BL


Tgt Ion:240 Resp: 109596

Ion Ratio Lower Upper

240 100

120 6.9 8.2 12.2#




236 28.5 20.0 30.0

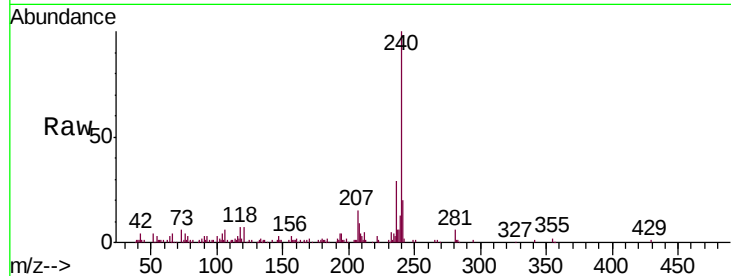

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

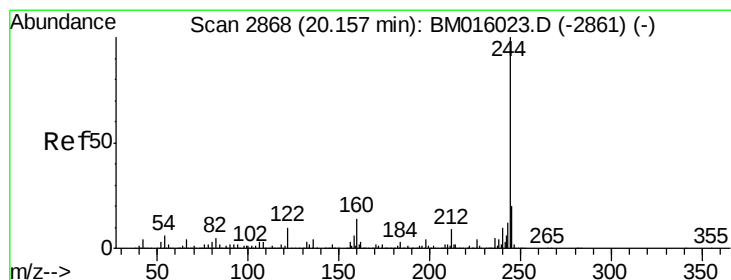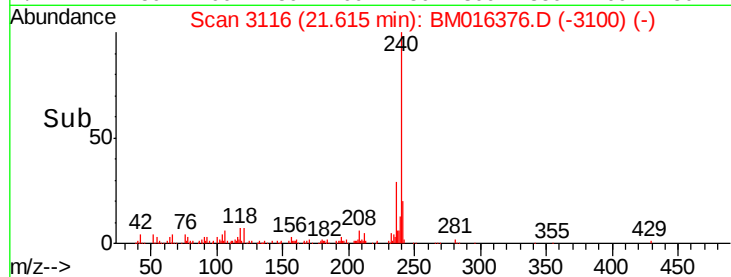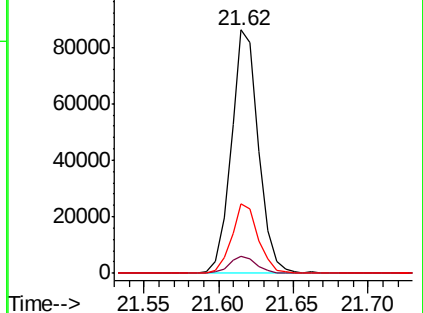

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.07 min Scan# 2853

Delta R.T. 0.00 min

Lab File: BM016376.D

Acq: 15 Aug 2018 12:29


Tgt Ion:244 Resp: 495995

Ion Ratio Lower Upper

244 100

212 10.2 4.9 7.3#



122 7.6 6.2 9.4

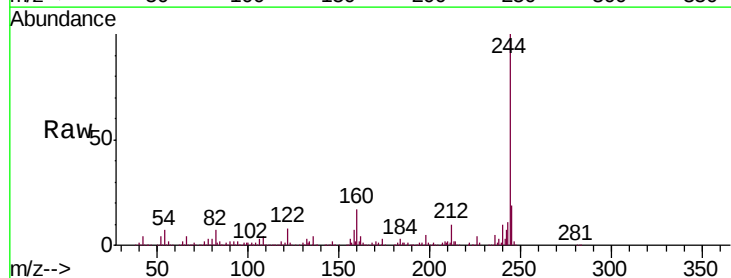


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

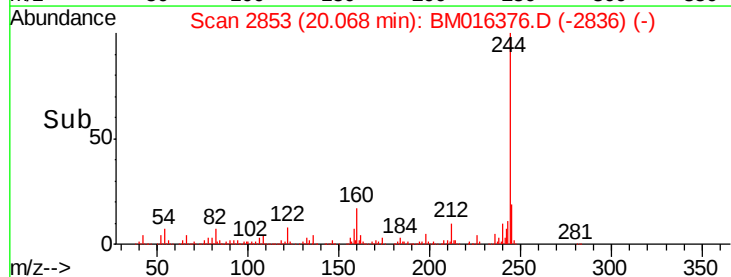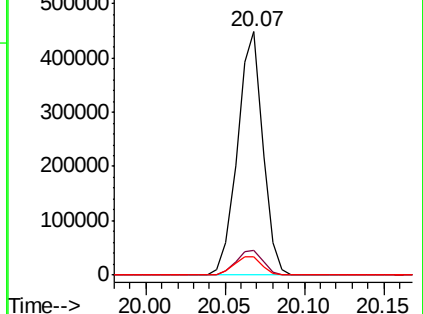

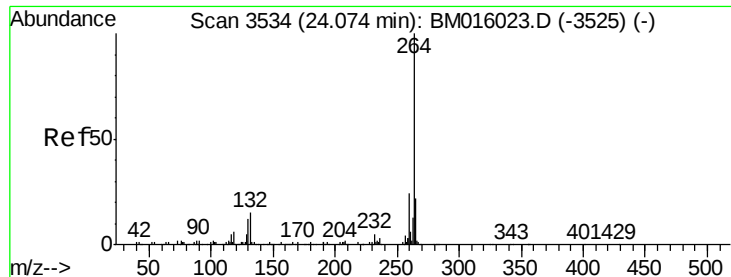

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.94 min Scan# 3512
Delta R.T. 0.00 min
Lab File: BM016376.D
Acq: 15 Aug 2018 12:29

Instrument :
BNA_M
ClientSampleId :
PB112015BL

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	18.6	27.8
265	21.7	17.3	25.9

