

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081518\
 Data File : BM016409.D
 Acq On : 16 Aug 2018 09:50
 Operator : SJ/JU
 Sample : J4462-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 16 11:48:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	17106	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	57650	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	31001	20.00	ng	0.00
63) Phenanthrene-d10	17.48	188	70078	20.00	ng	-0.01
75) Chrysene-d12	21.62	240	89943	20.00	ng	0.00
86) Perylene-d12	23.94	264	100720	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	38395	37.28	ng	0.00
7) Phenol-d6	7.29	99	25308	18.82	ng	0.00
23) Nitrobenzene-d5	9.29	82	136989	110.52	ng	-0.01
41) 2,4,6-Tribromophenol	16.23	330	34270	87.16	ng	-0.01
44) 2-Fluorobiphenyl	13.36	172	262869	103.17	ng	-0.01
78) Terphenyl-d14	20.06	244	420192	97.79	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.43	79	3398	3.173	ng	# 1
49) Dimethylphthalate	14.20	163	5538	2.041	ng	# 77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081518\
Data File : BM016409.D
Acq On : 16 Aug 2018 09:50
Operator : SJ/JU
Sample : J4462-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 16 11:48:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

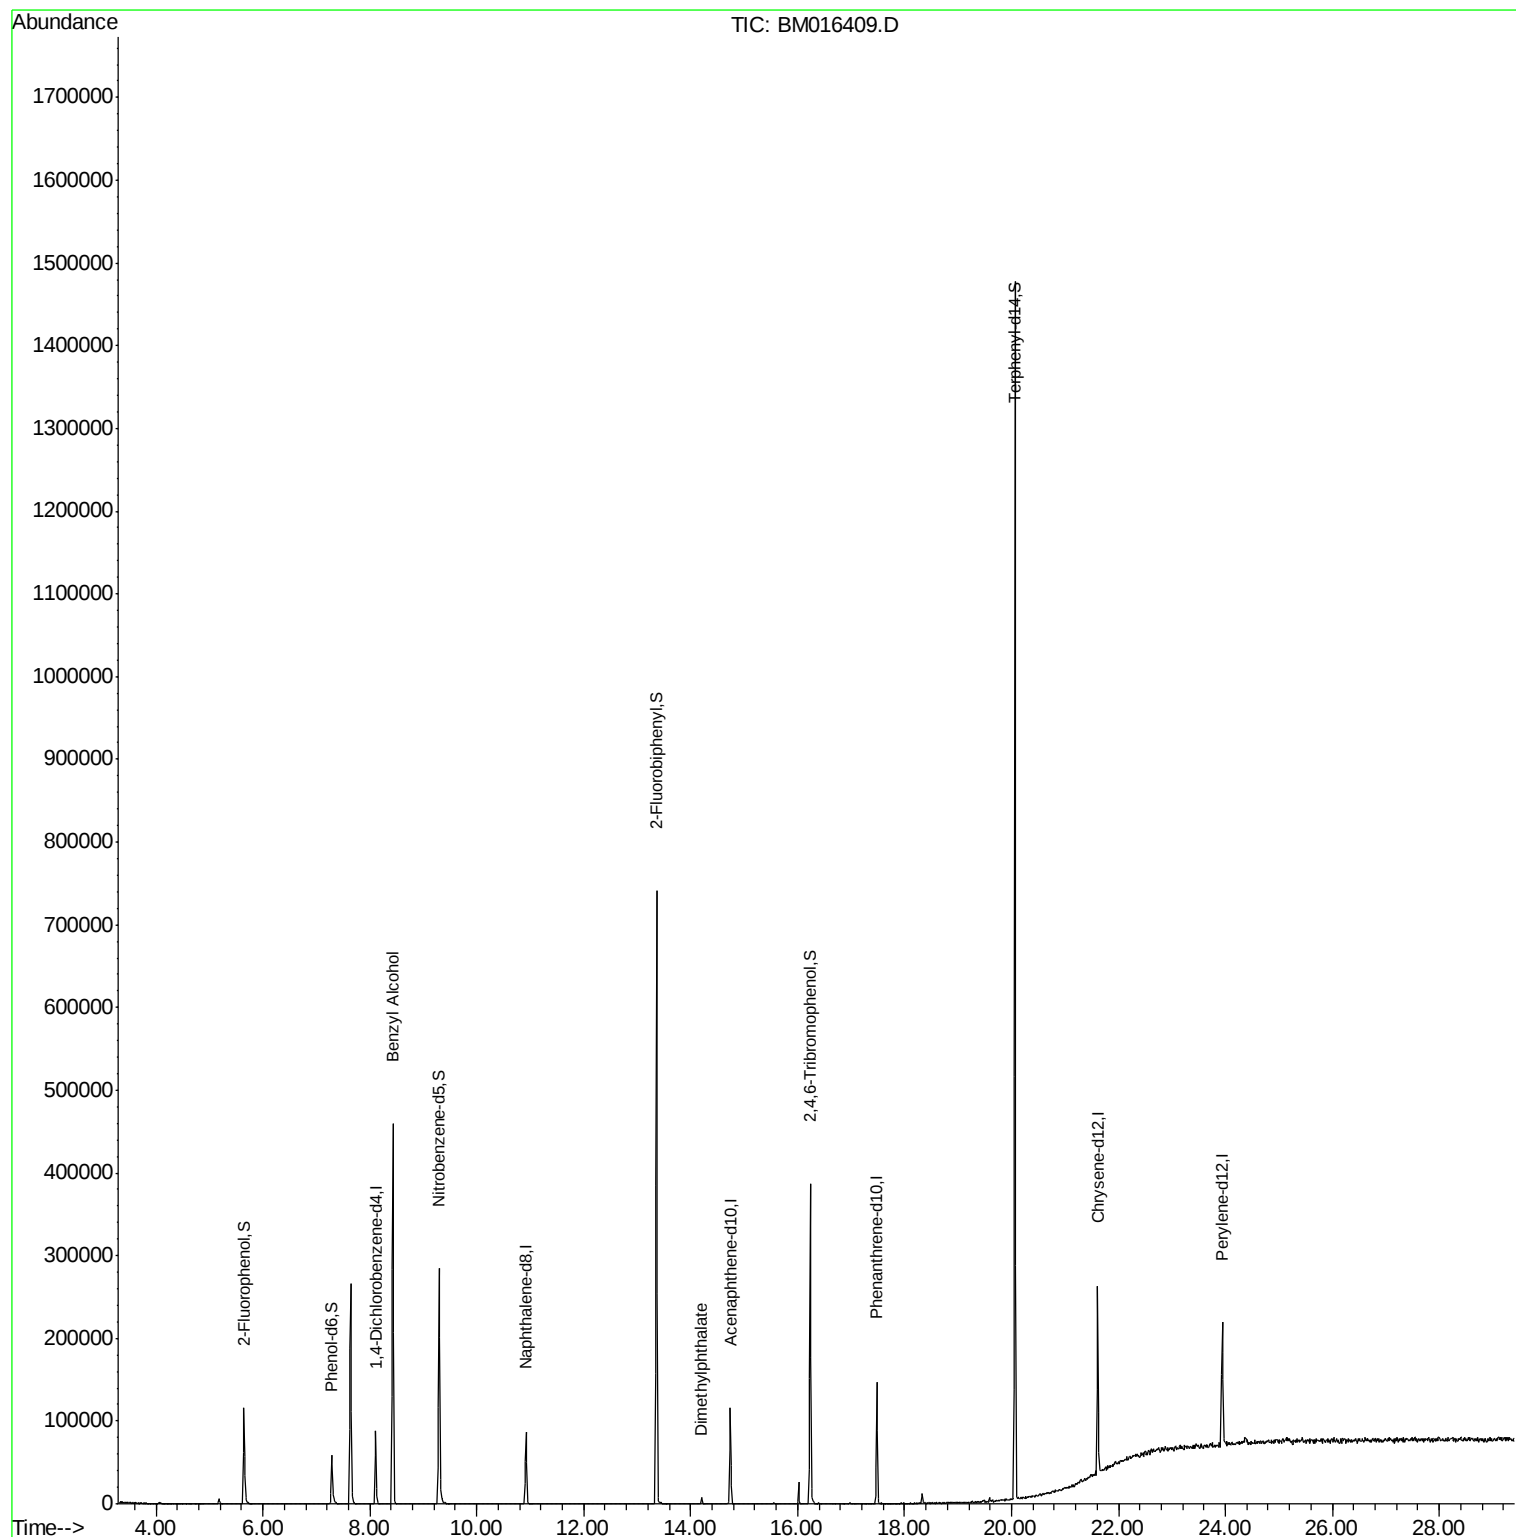







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.11 min Scan# 820
 Delta R.T. -0.01 min
 Lab File: BM016409.D
 Acq: 16 Aug 2018 09:50

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:152 Resp: 17106
 Ion Ratio Lower Upper
 152 100
 150 154.7 119.5 179.3
 115 70.6 43.0 64.4#

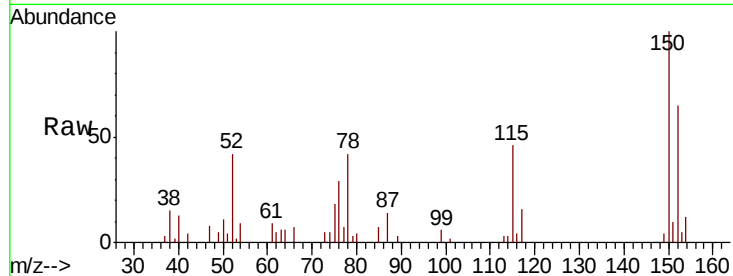


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

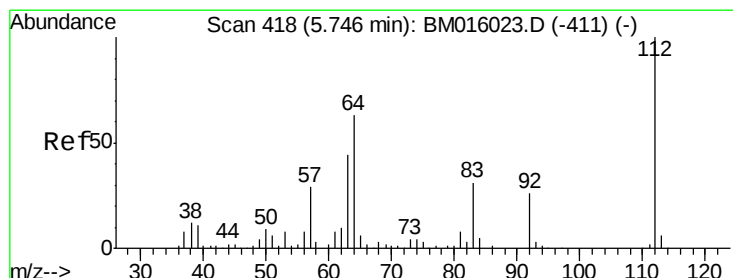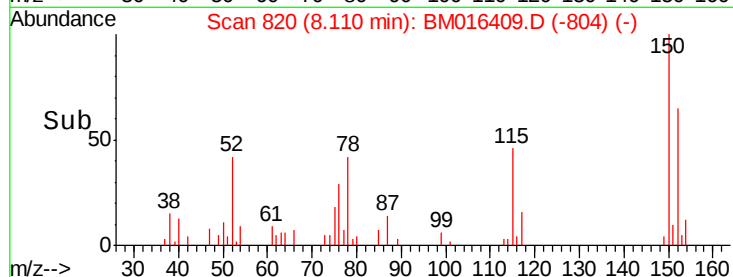
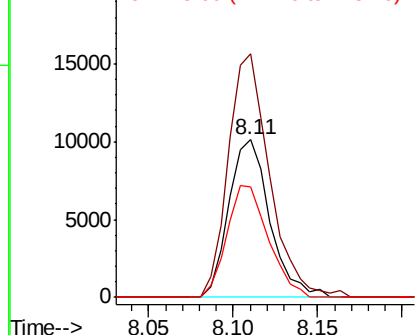


#5
 2-Fluorophenol
 Concen: N.D. ng
 RT: 5.65 min Scan# 401
 Delta R.T. 0.00 min
 Lab File: BM016409.D
 Acq: 16 Aug 2018 09:50

Tgt Ion:112 Resp: 38395
 Ion Ratio Lower Upper
 112 100
 64 62.8 38.6 57.8#
 63 55.9 19.3 28.9#

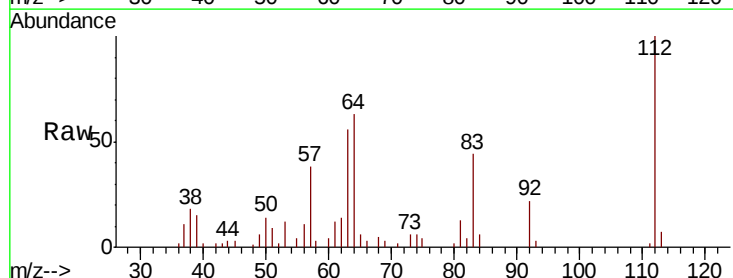

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

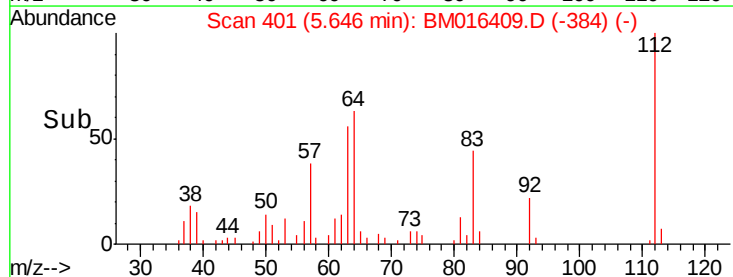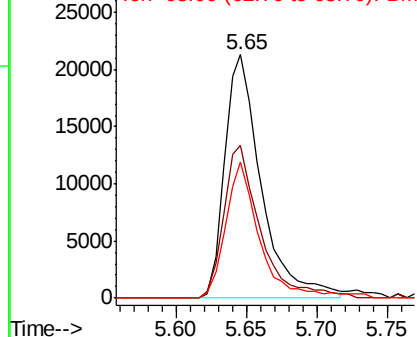



#7

Phenol-d6

Concen: N.D. ng

RT: 7.29 min Scan# 680

Delta R.T. 0.00 min

Lab File: BM016409.D

Acq: 16 Aug 2018 09:50

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 25308

Ion Ratio Lower Upper

99 100

42 46.3 11.0 16.4#




71 61.5 23.4 35.2#

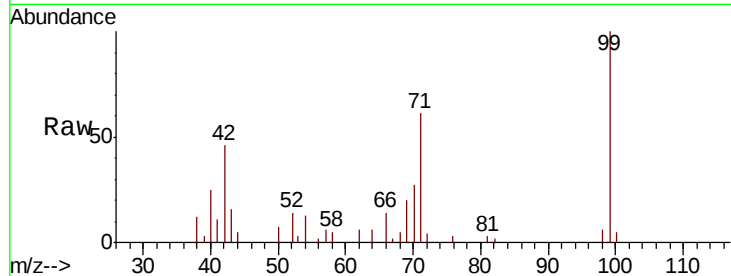

Abundance Ion 99.00 (98.70 to 99.70): BM016409.D (-663) (-)

Ion 42.00 (41.70 to 42.70): BM016409.D (-663) (-)

Ion 71.00 (70.70 to 71.70): BM016409.D (-663) (-)

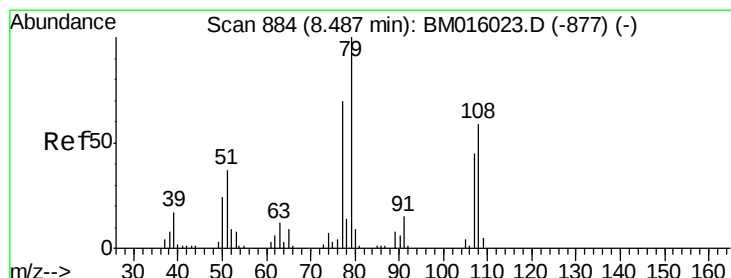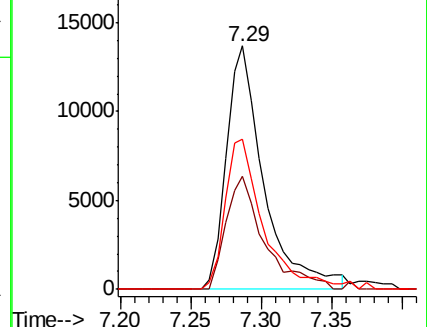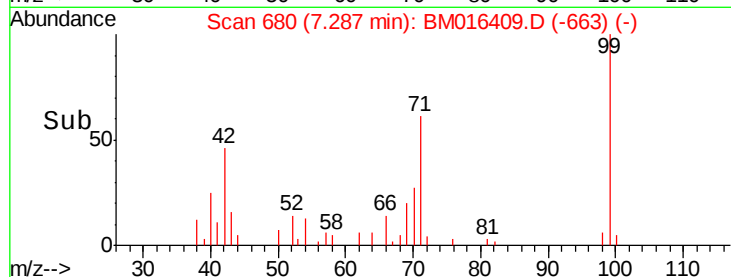

#15

Benzyl Alcohol

Concen: 3.173 ng

RT: 8.43 min Scan# 874

Delta R.T. 0.05 min

Lab File: BM016409.D

Acq: 16 Aug 2018 09:50


Tgt Ion: 79 Resp: 3398

Ion Ratio Lower Upper

79 100

108 114.5 65.0 97.4#



77 248.9 53.0 79.6#

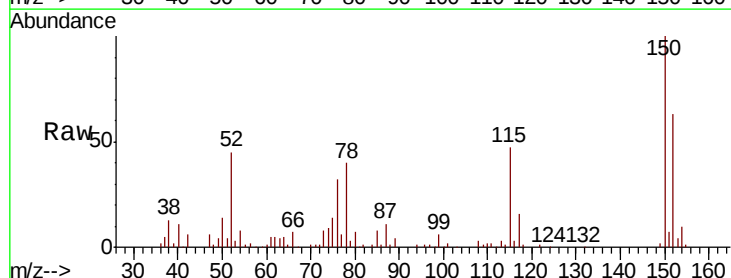

Abundance Ion 79.00 (78.70 to 79.70): BM016409.D (-848) (-)

Ion 108.00 (107.70 to 108.70): BM016409.D (-848) (-)

Ion 77.00 (76.70 to 77.70): BM016409.D (-848) (-)



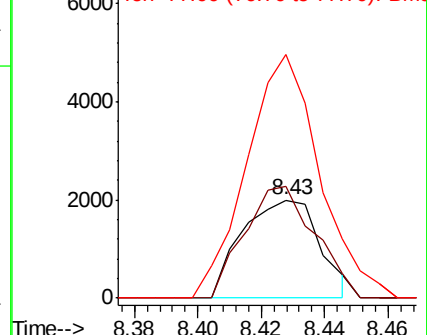
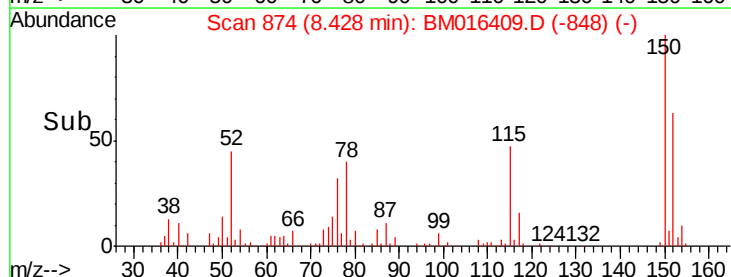




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1298
Delta R.T. -0.01 min
Lab File: BM016409.D
Acq: 16 Aug 2018 09:50




Instrument :
BNA_M
ClientSampleId :

Tot Ion:136	Resp:	57650
Ion	Ratio	Lower Upper
136	100	
137	11.2	8.7 13.1
54	12.4	4.6 6.8#
68	3.8	3.7 5.5

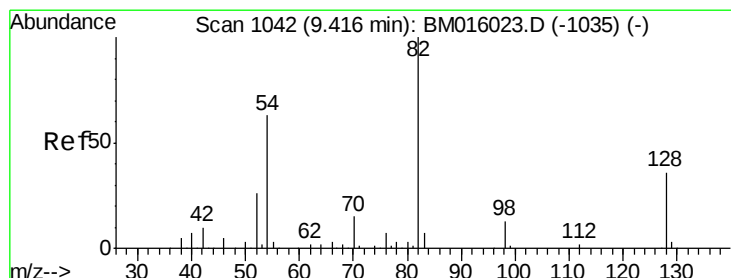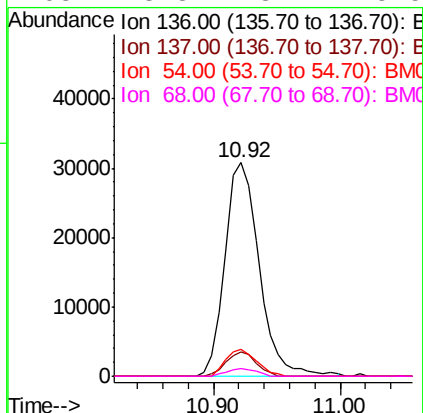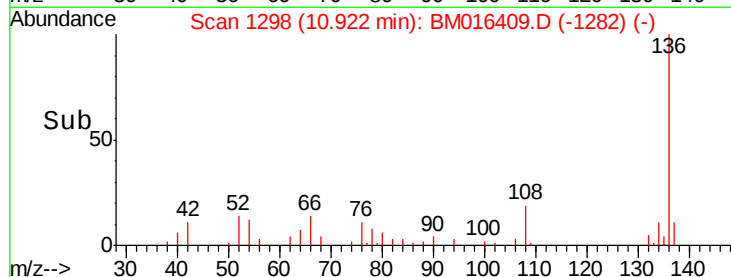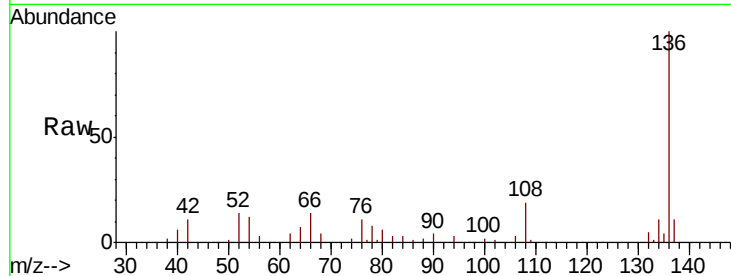

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.29 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BM016409.D
Acq: 16 Aug 2018 09:50

Tgt Ion: 82	Resp:	136989
Ion	Ratio	Lower Upper
82	100	
128	33.2	32.8 49.2
54	69.9	40.6 60.8#

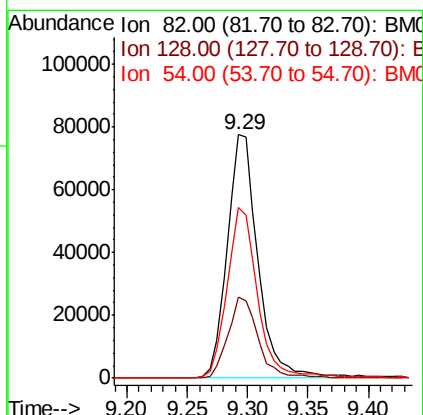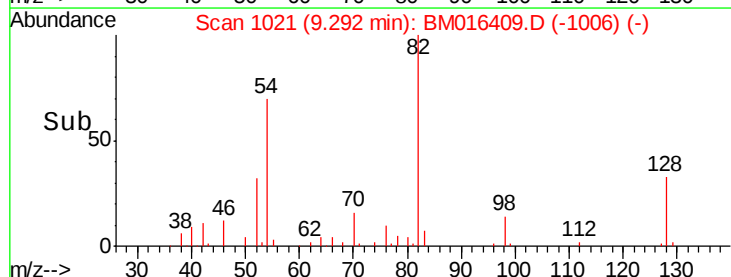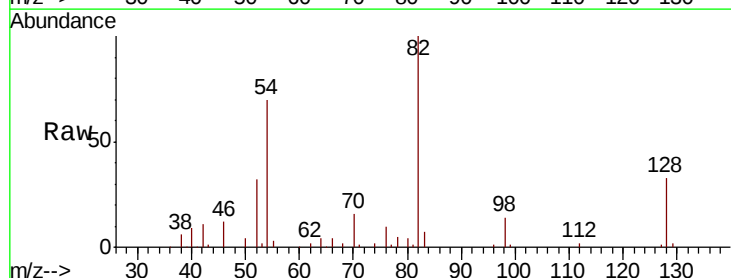



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.75 min Scan# 1948

Delta R.T. -0.01 min

Lab File: BM016409.D

Acq: 16 Aug 2018 09:50

Instrument :

BNA_M

ClientSampled :


Tot Ion:164 Resp: 31001

Ion Ratio Lower Upper




164 100

162 105.0 82.4 123.6

160 51.4 35.8 53.6

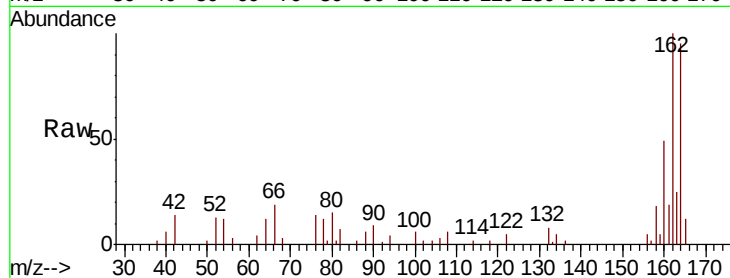

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

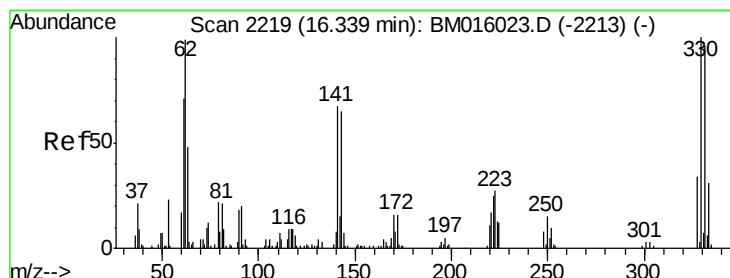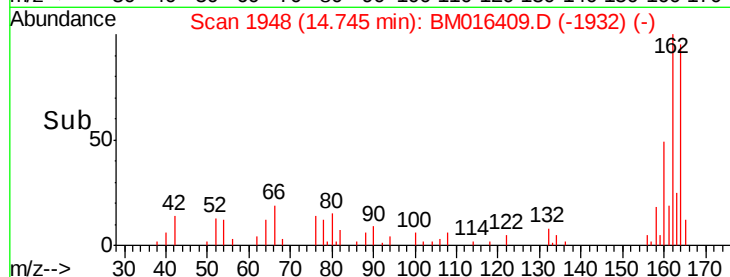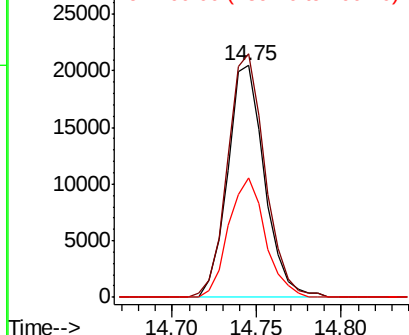

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.23 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BM016409.D

Acq: 16 Aug 2018 09:50


Tgt Ion:330 Resp: 34270

Ion Ratio Lower Upper



330 100

332 93.5 0.0 0.0#

141 94.5 0.0 0.0#

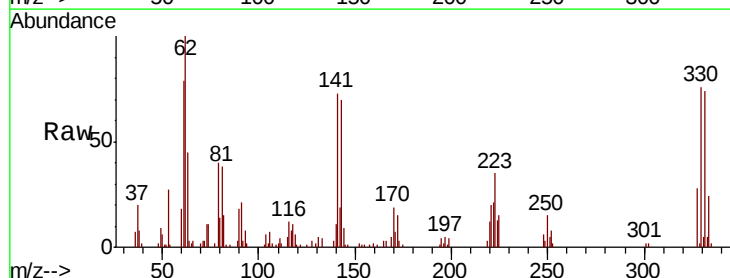

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



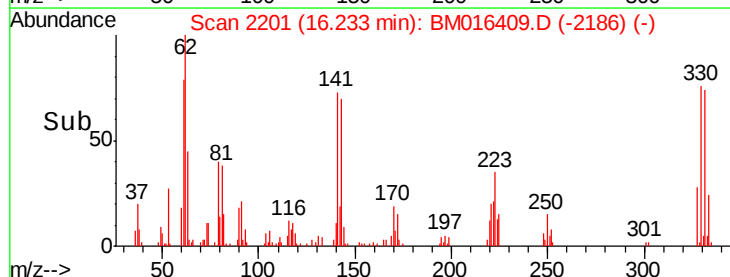
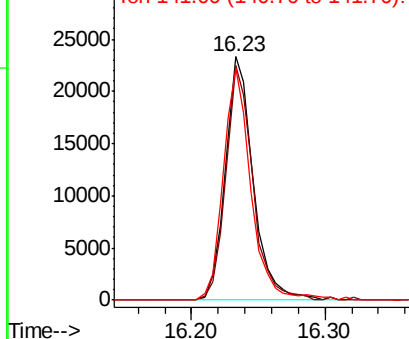




#44
2-Fluorobiphenyl
Concen: N.D. na
RT: 13.36 min Scan# 1713
Delta R.T. -0.01 min
Lab File: BM016409.D
Acq: 16 Aug 2018 09:50




Instrument :
BNA_M
ClientSampleId :


Tot Ion:172 Resp: 262869
Ion Ratio Lower Upper
172 100
171 36.1 28.5 42.7
170 25.4 18.8 28.2

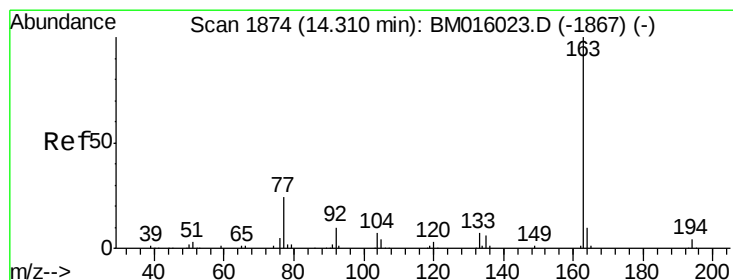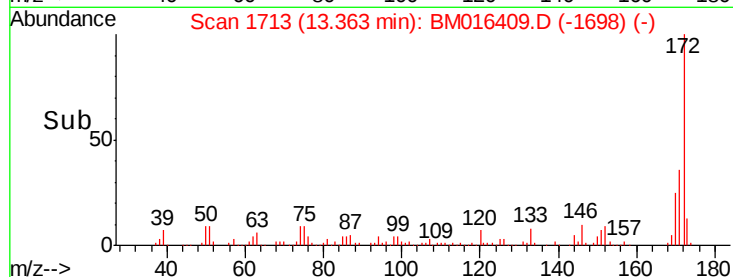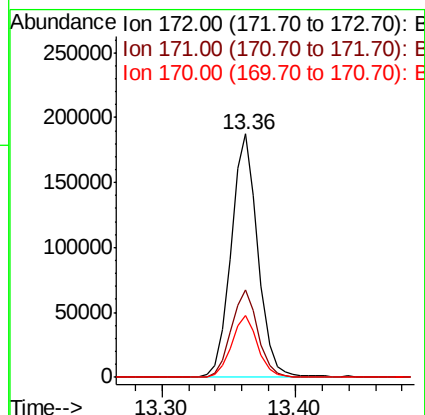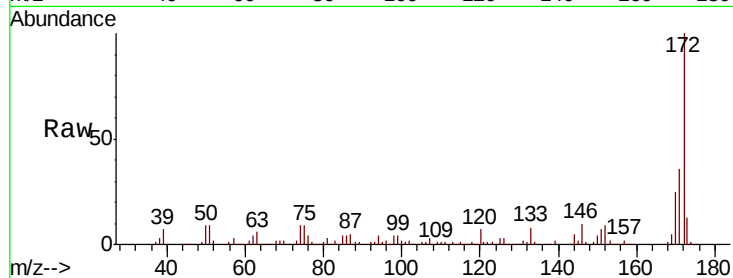

#49
Dimethylphthalate
Concen: 2.041 ng
RT: 14.20 min Scan# 1856
Delta R.T. -0.01 min
Lab File: BM016409.D
Acq: 16 Aug 2018 09:50

Tgt Ion:163 Resp: 5538
Ion Ratio Lower Upper
163 100
194 0.0 2.7 4.1#
164 0.0 8.2 12.2#

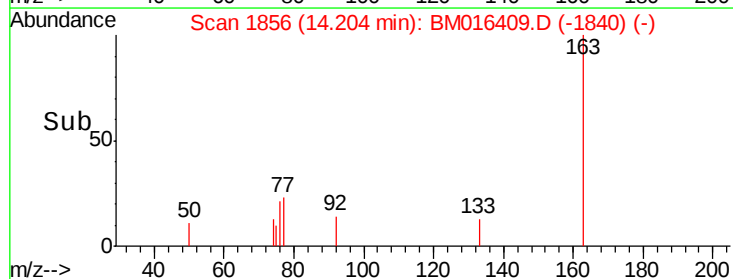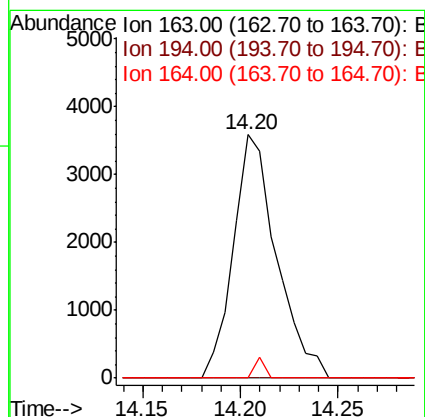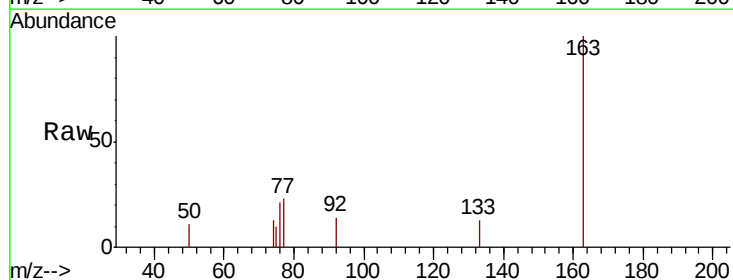


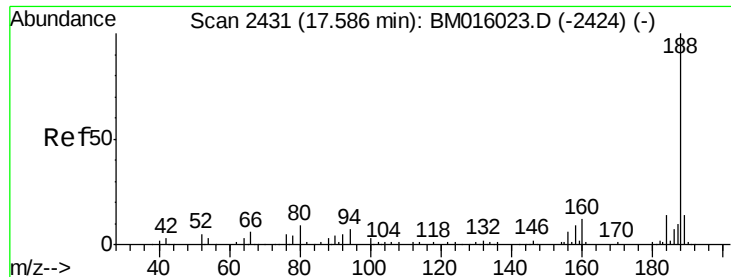




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.48 min Scan# 2413
Delta R.T. -0.01 min
Lab File: BM016409.D
Acq: 16 Aug 2018 09:50

Instrument :
BNA_M
ClientSampleId :

Tot Ion:188 Resp: 70078
Ion Ratio Lower Upper
188 100
94 6.1 8.7 13.1#
80 7.0 9.3 13.9#

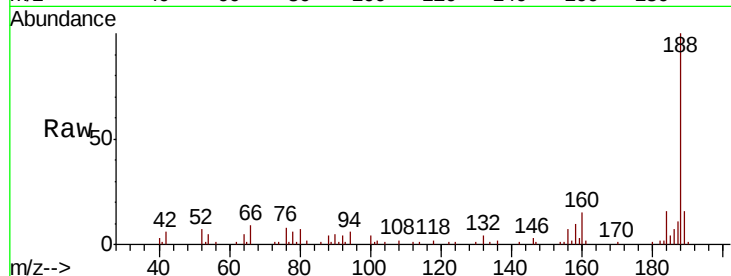


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM016409.D (-2398) (-)
Ion 80.00 (79.70 to 80.70): BM016409.D (-2398) (-)

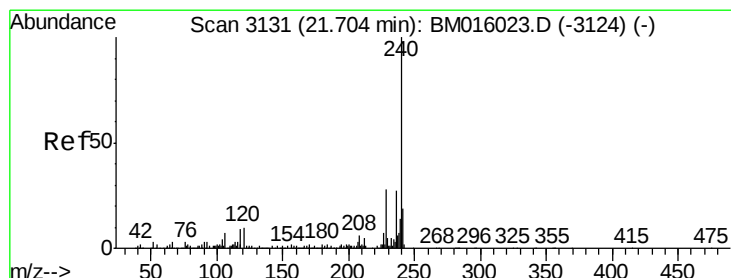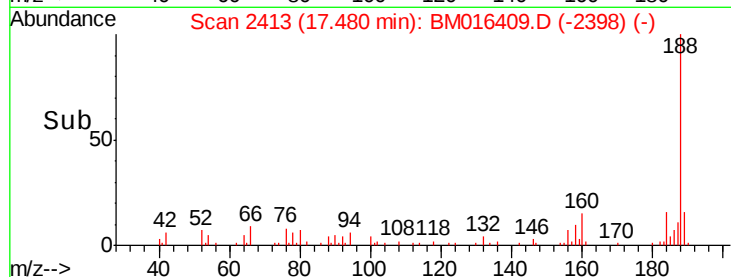
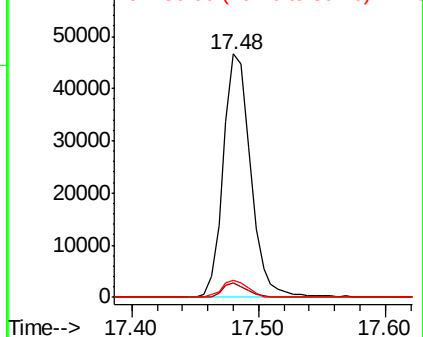



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.62 min Scan# 3116
Delta R.T. -0.01 min
Lab File: BM016409.D
Acq: 16 Aug 2018 09:50

Tgt Ion:240 Resp: 89943
Ion Ratio Lower Upper
240 100
120 5.9 8.2 12.2#
236 26.9 20.0 30.0

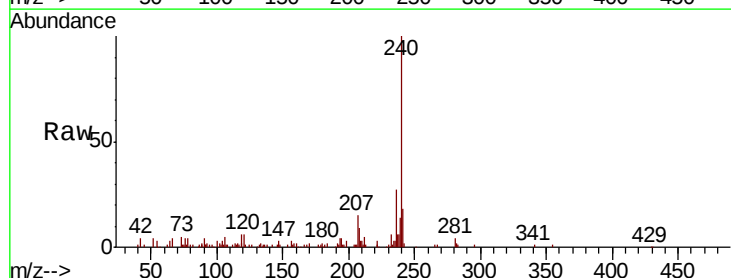

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



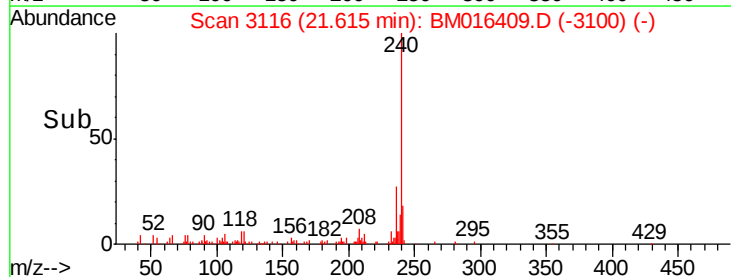
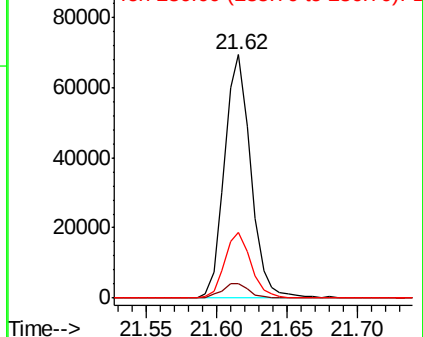


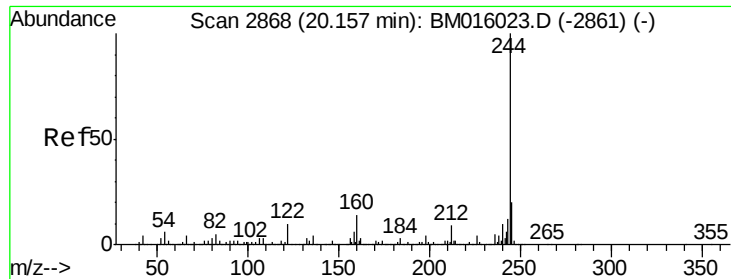

#78
 Terphenyl-d14
 Concen: N.D. ng
 RT: 20.06 min Scan# 2852
 Delta R.T. -0.01 min
 Lab File: BM016409.D
 Acq: 16 Aug 2018 09:50

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
244	100		
212	10.9	4.9	7.3#
122	7.7	6.2	9.4

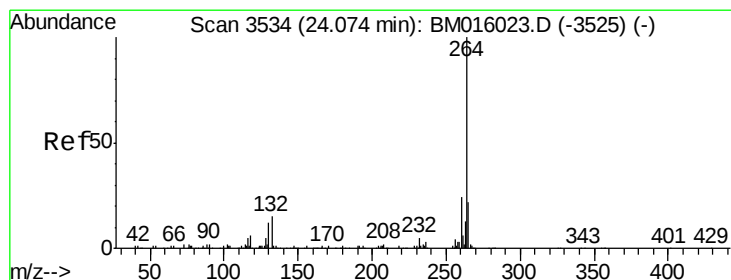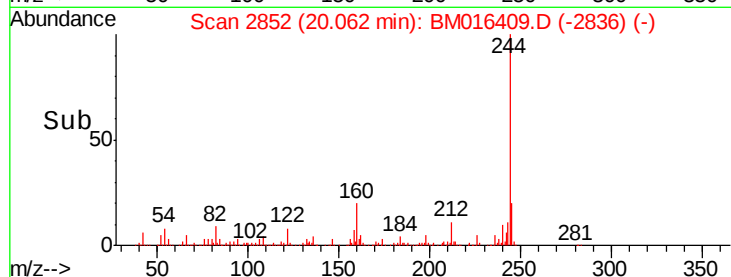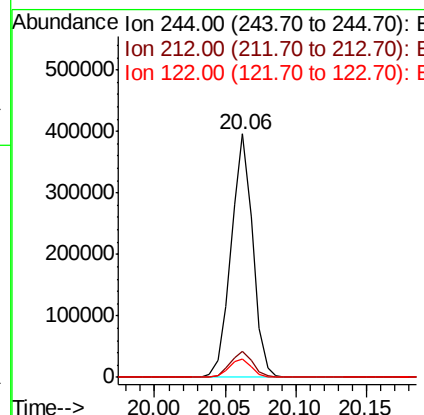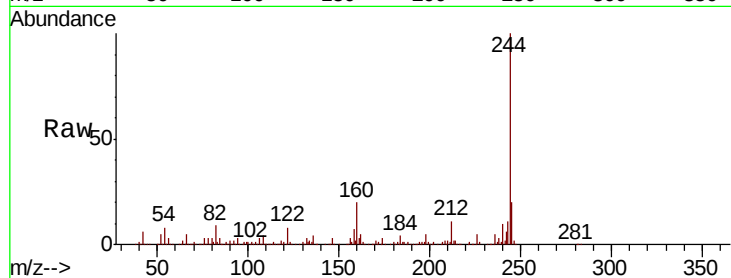

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.94 min Scan# 3511
 Delta R.T. -0.01 min
 Lab File: BM016409.D
 Acq: 16 Aug 2018 09:50

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.6	27.8
265	22.1	17.3	25.9

