

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081518\
 Data File : BM016410.D
 Acq On : 16 Aug 2018 10:26
 Operator : SJ/JU
 Sample : J4445-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DSN-001A-081018

Quant Time: Aug 16 12:07:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 15 11:23:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	18812	20.00	ng	-0.01
21) Naphthalene-d8	10.92	136	65747	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	33957	20.00	ng	0.00
63) Phenanthrene-d10	17.48	188	74486	20.00	ng	-0.01
75) Chrysene-d12	21.62	240	92991	20.00	ng	0.00
86) Perylene-d12	23.94	264	99470	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	69433	61.31	ng	0.00
7) Phenol-d6	7.28	99	44047	29.78	ng	0.00
23) Nitrobenzene-d5	9.30	82	168948	119.52	ng	0.00
41) 2,4,6-Tribromophenol	16.23	330	68930	160.05	ng	-0.01
44) 2-Fluorobiphenyl	13.36	172	323538	115.93	ng	-0.01
78) Terphenyl-d14	20.06	244	591900	133.24	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081518\
Data File : BM016410.D
Acq On : 16 Aug 2018 10:26
Operator : SJ/JU
Sample : J4445-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DSN-001A-081018

Quant Time: Aug 16 12:07:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 15 11:23:48 2018
Response via : Initial Calibration

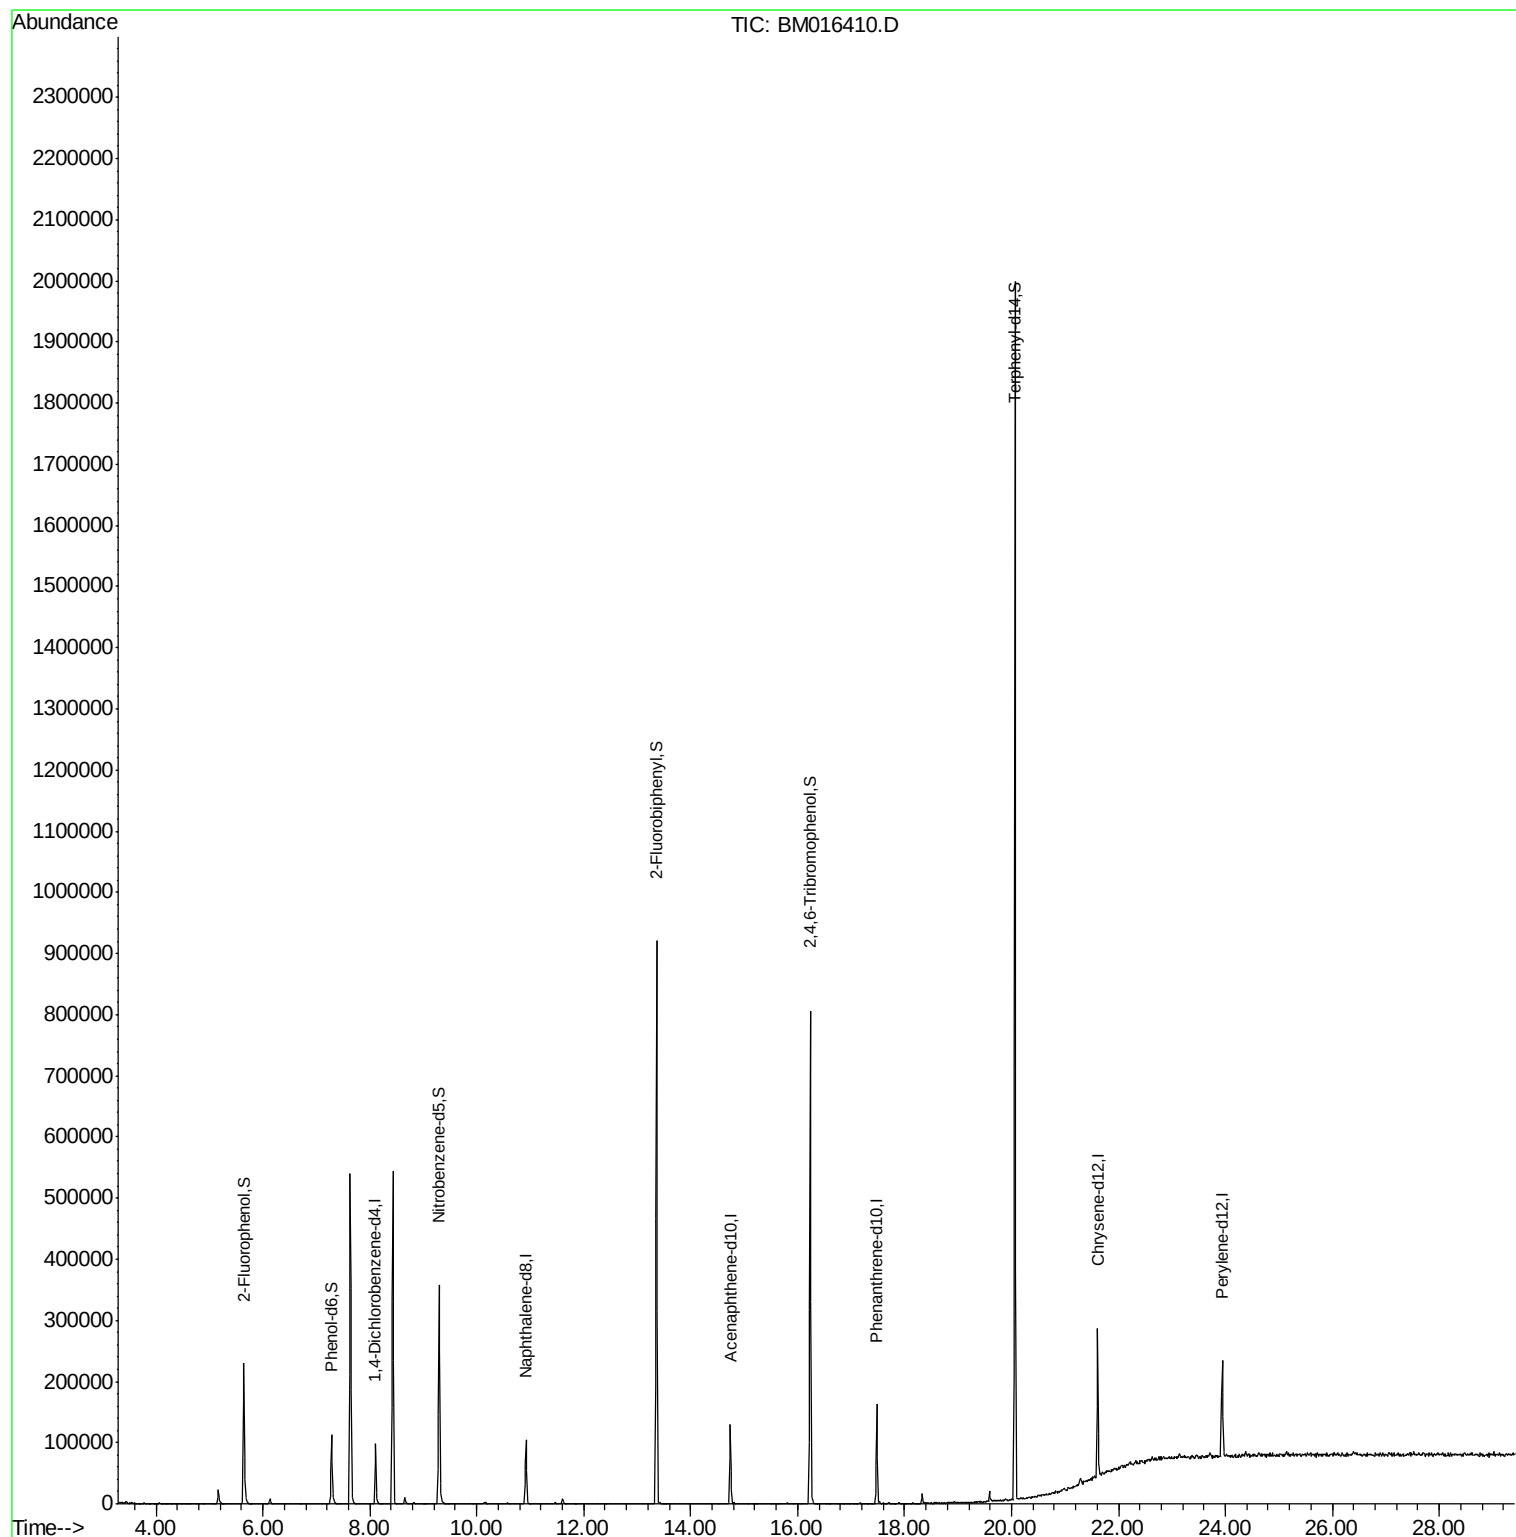

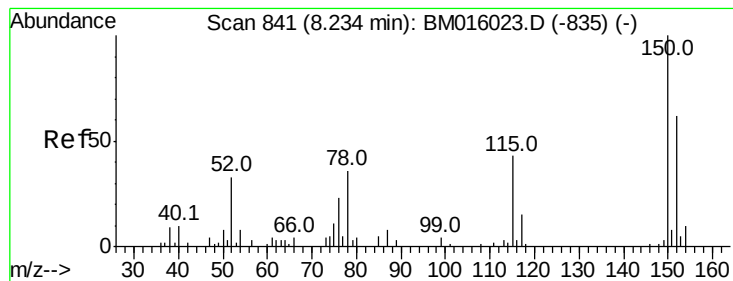

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.10 min Scan# 819

Delta R.T. -0.01 min

Lab File: BM016410.D

Acq: 16 Aug 2018 10:26

Instrument :

BNA_M

ClientSampleId :

DSN-001A-081018


Tot Ion:152 Resp: 18812

Ion Ratio Lower Upper

152 100

150 152.2 119.5 179.3




115 75.3 43.0 64.4#

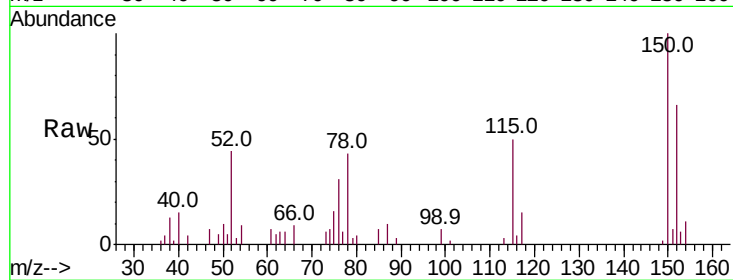

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

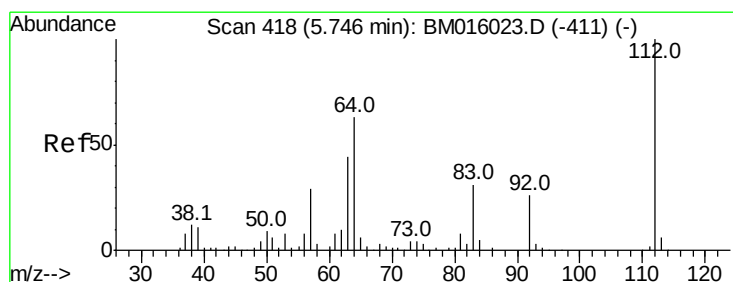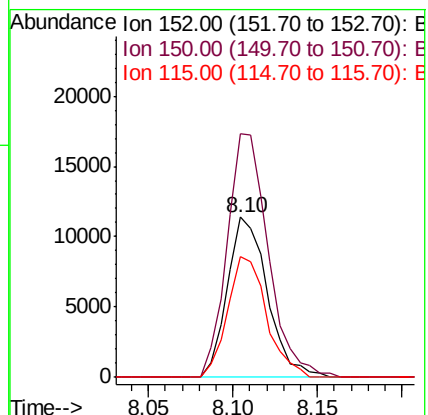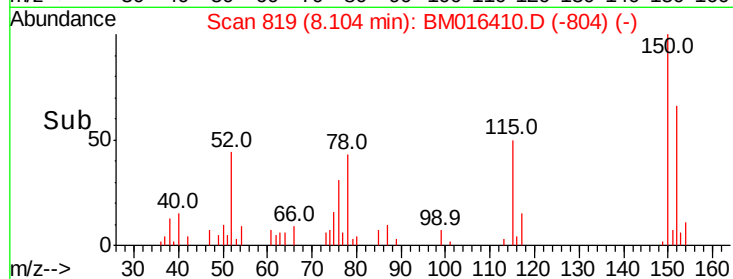

#5

2-Fluorophenol

Concen: N.D. ng

RT: 5.64 min Scan# 400

Delta R.T. -0.01 min

Lab File: BM016410.D

Acq: 16 Aug 2018 10:26


Tgt Ion:112 Resp: 69433

Ion Ratio Lower Upper

112 100

64 61.5 38.6 57.8#



63 49.7 19.3 28.9#

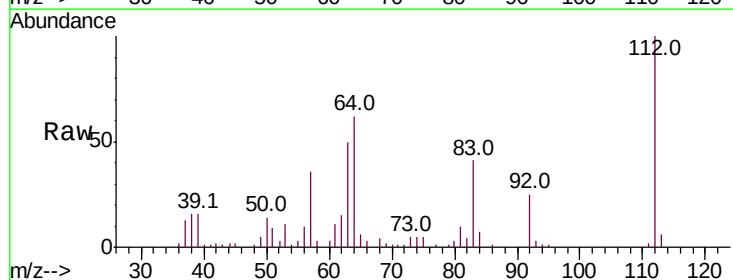


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

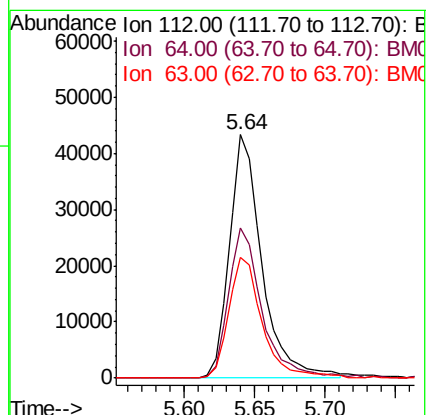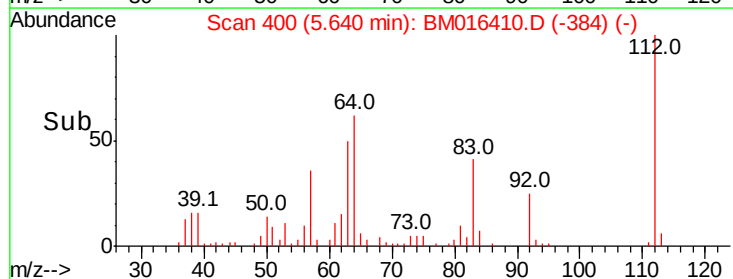

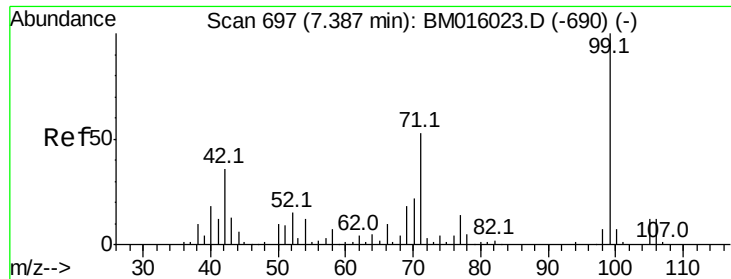

#7

Phenol-d6

Concen: N.D. ng

RT: 7.28 min Scan# 679

Delta R.T. -0.01 min

Lab File: BM016410.D

Acq: 16 Aug 2018 10:26

Instrument :

BNA_M

ClientSampleId :

DSN-001A-081018


Tot Ion: 99 Resp: 44047

Ion Ratio Lower Upper

99 100

42 47.5 11.0 16.4#




71 59.9 23.4 35.2#

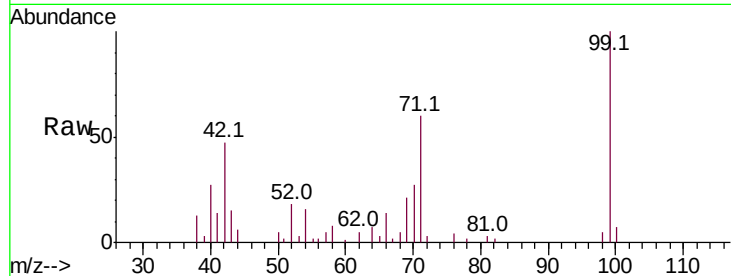

Abundance Ion 99.00 (98.70 to 99.70): BM016410.D (-663) (-)

Ion 42.00 (41.70 to 42.70): BM016410.D (-663) (-)

Ion 71.00 (70.70 to 71.70): BM016410.D (-663) (-)

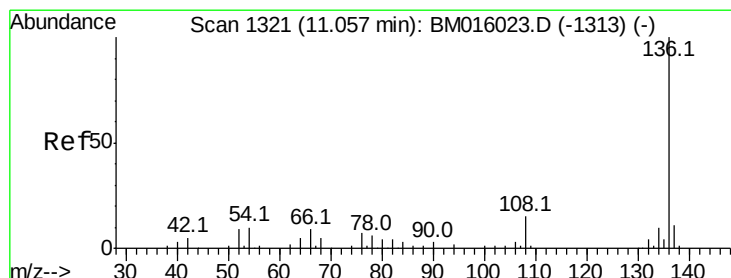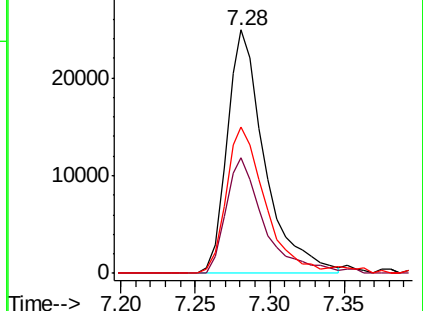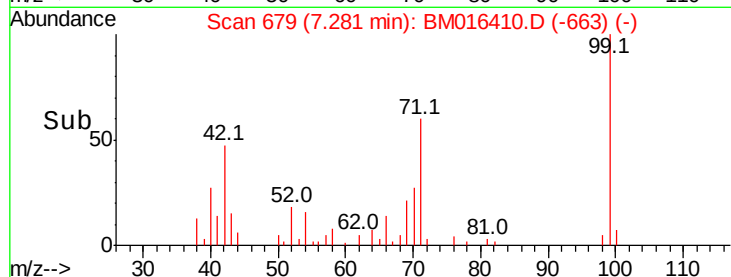

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BM016410.D

Acq: 16 Aug 2018 10:26

Tgt Ion: 136 Resp: 65747


Ion Ratio Lower Upper

136 100

137 10.0 8.7 13.1

54 11.5 4.6 6.8#

68 2.7 3.7 5.5#


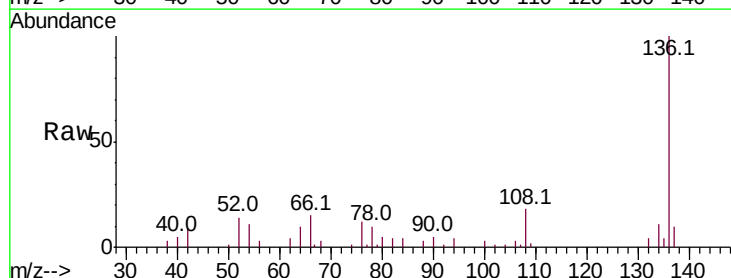



Abundance Ion 136.00 (135.70 to 136.70): BM016410.D (-1282) (-)

Ion 137.00 (136.70 to 137.70): BM016410.D (-1282) (-)

Ion 54.00 (53.70 to 54.70): BM016410.D (-1282) (-)

Ion 68.00 (67.70 to 68.70): BM016410.D (-1282) (-)



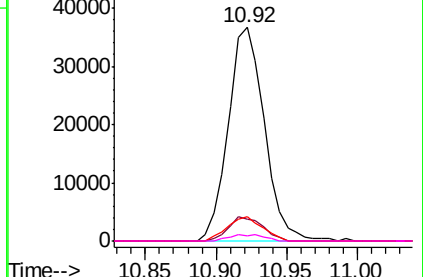
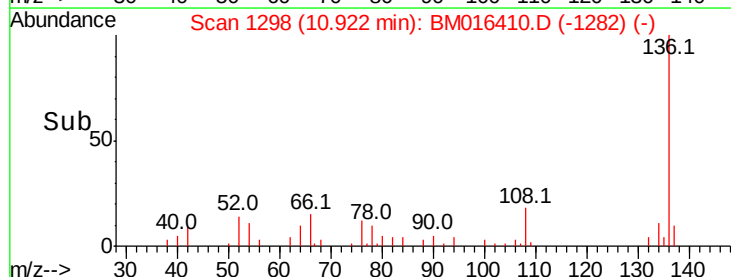


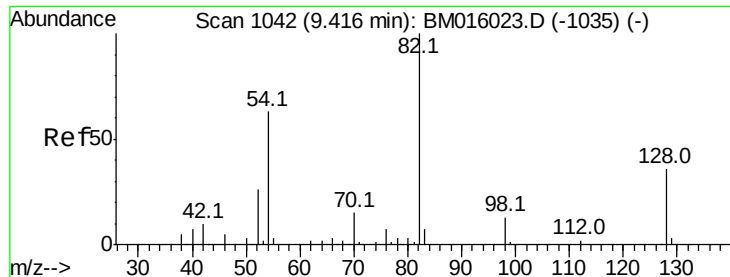

#23
 Nitrobenzene-d5
 Concen: Below na
 RT: 9.30 min Scan# 1022
 Delta R.T. -0.01 min
 Lab File: BM016410.D
 Acq: 16 Aug 2018 10:26




Instrument :
 BNA_M
 ClientSampleId :
 DSN-001A-081018


Tot Ion	Ratio	Lower	Upper
82	100		
128	33.9	32.8	49.2
54	67.2	40.6	60.8#

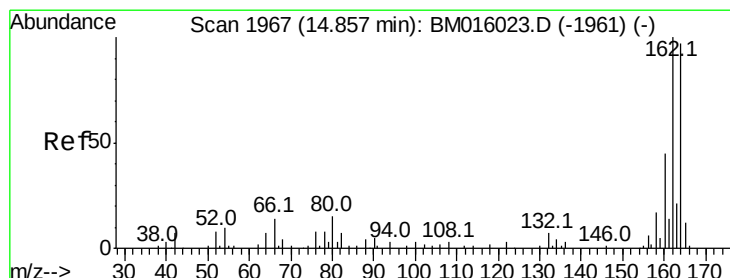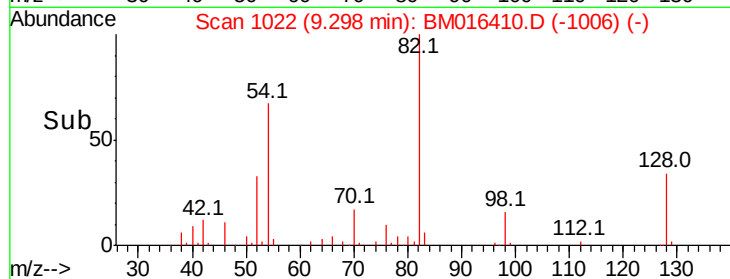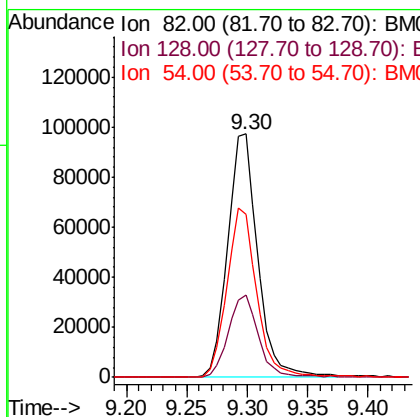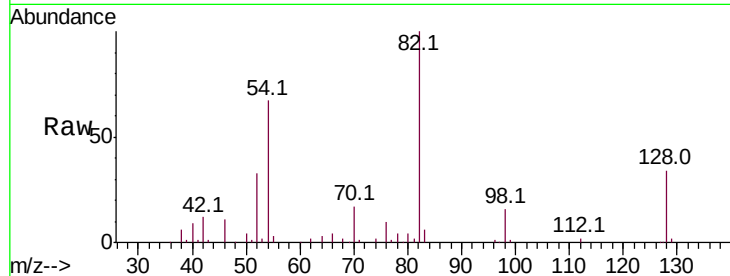

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.75 min Scan# 1948
 Delta R.T. -0.01 min
 Lab File: BM016410.D
 Acq: 16 Aug 2018 10:26

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.3	82.4	123.6
160	47.7	35.8	53.6

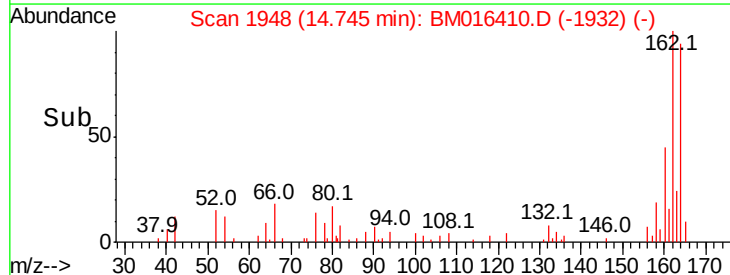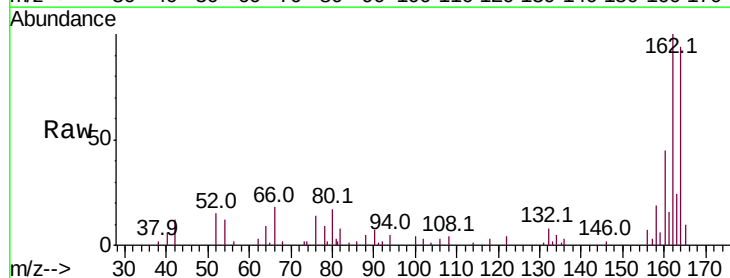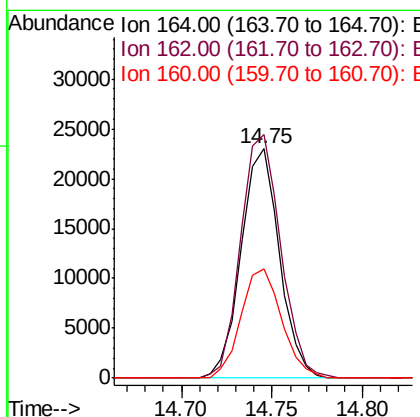


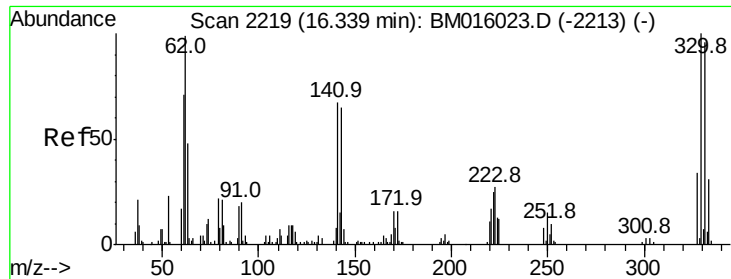




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.23 min Scan# 2201
 Delta R.T. -0.01 min
 Lab File: BM016410.D
 Acq: 16 Aug 2018 10:26

Instrument :
 BNA_M
 ClientSampleId :
 DSN-001A-081018

Tot Ion:330 Resp: 68930
 Ion Ratio Lower Upper
 330 100
 332 97.0 0.0 0.0#
 141 93.5 0.0 0.0#

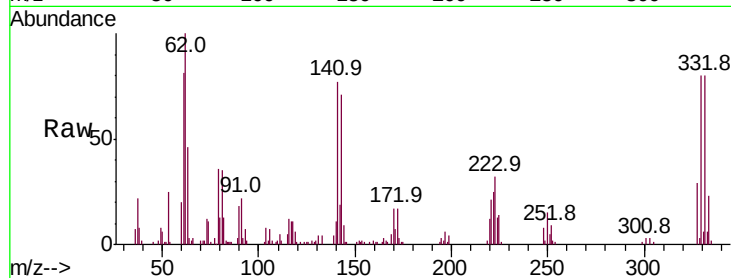


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

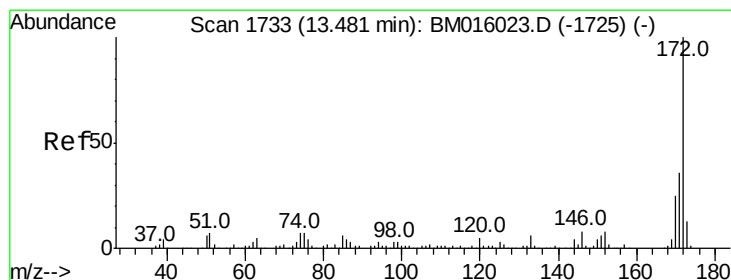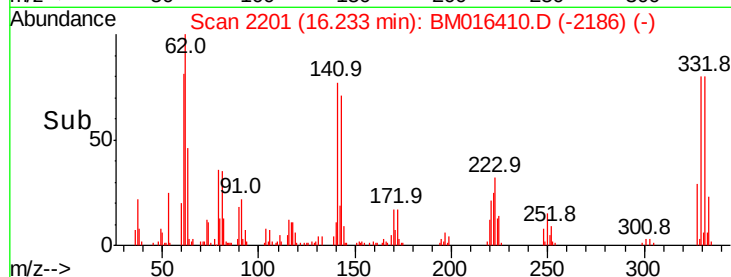
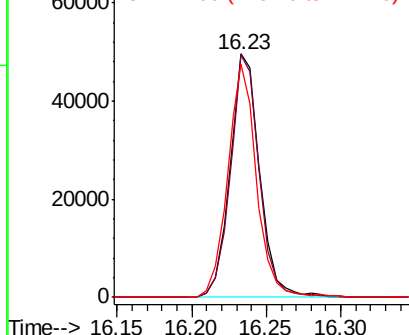



#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.36 min Scan# 1713
 Delta R.T. -0.01 min
 Lab File: BM016410.D
 Acq: 16 Aug 2018 10:26

Tgt Ion:172 Resp: 323538
 Ion Ratio Lower Upper
 172 100
 171 37.0 28.5 42.7
 170 25.3 18.8 28.2

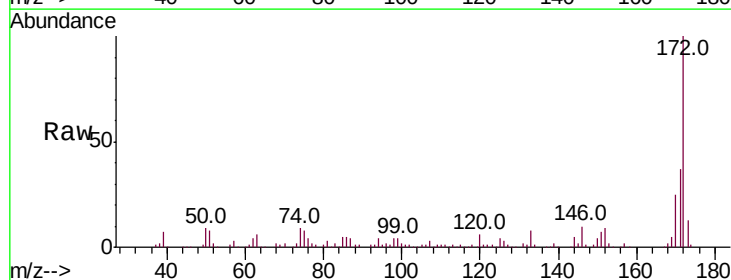

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



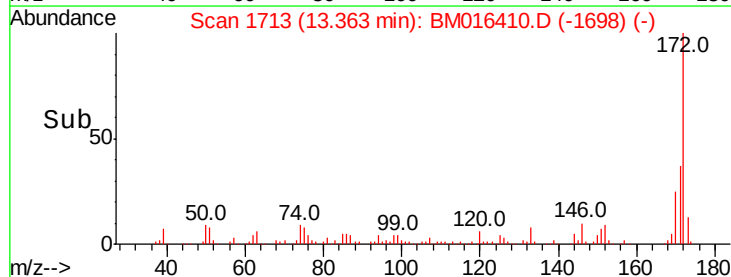
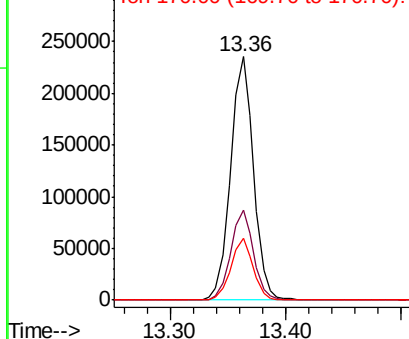


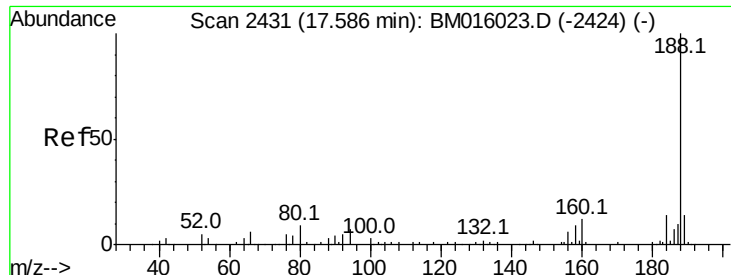

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.48 min Scan# 2413
Delta R.T. -0.01 min
Lab File: BM016410.D
Acq: 16 Aug 2018 10:26




Instrument :
BNA_M
ClientSampleId :
DSN-001A-081018


Tot Ion:188 Resp: 74486
Ion Ratio Lower Upper
188 100
94 6.0 8.7 13.1#
80 7.3 9.3 13.9#

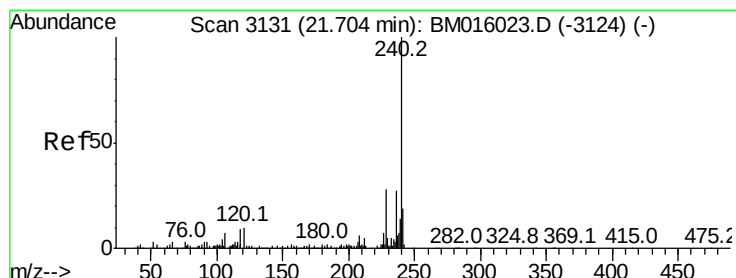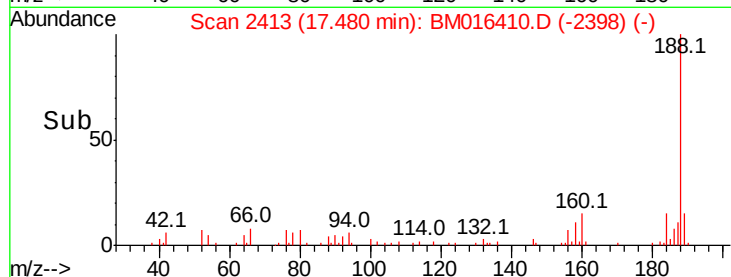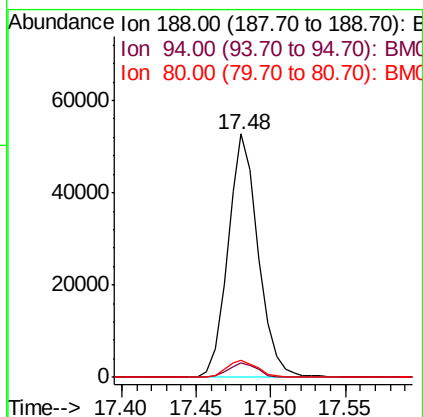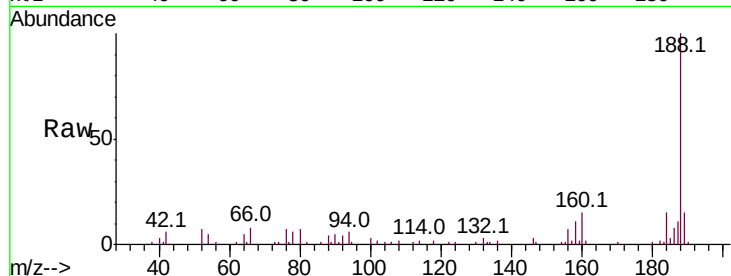

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.62 min Scan# 3116
Delta R.T. -0.01 min
Lab File: BM016410.D
Acq: 16 Aug 2018 10:26

Tgt Ion:240 Resp: 92991
Ion Ratio Lower Upper
240 100
120 6.4 8.2 12.2#
236 26.1 20.0 30.0

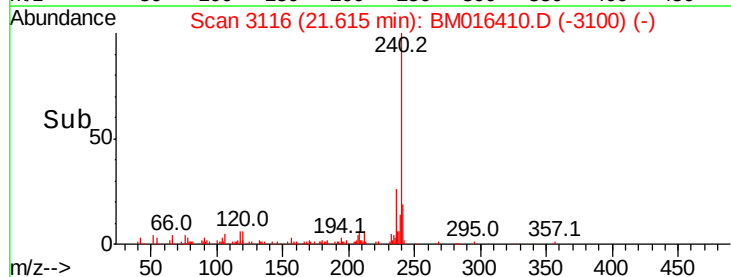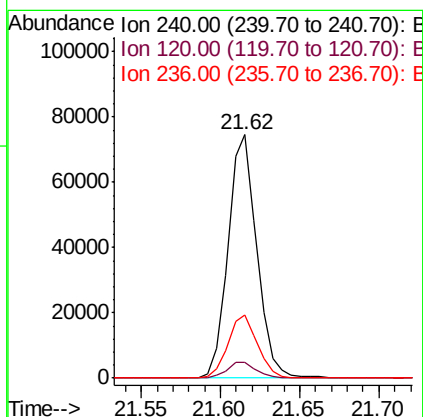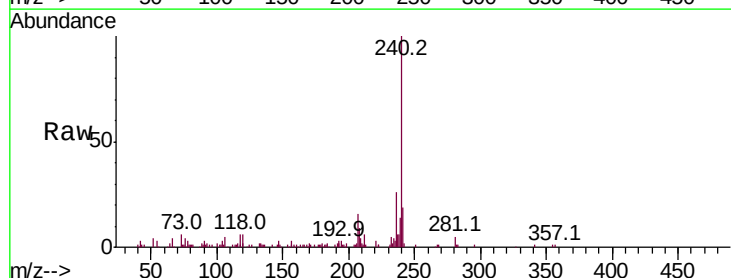


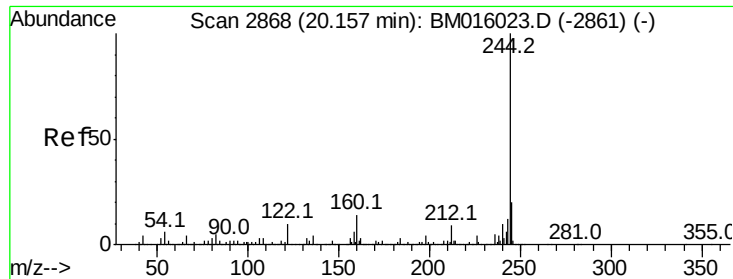




#78
 Terphenyl-d14
 Concen: Below na
 RT: 20.06 min Scan# 2852
 Delta R.T. -0.01 min
 Lab File: BM016410.D
 Acq: 16 Aug 2018 10:26

Instrument :
 BNA_M
 ClientSampleId :
 DSN-001A-081018

Tot Ion	Ratio	Lower	Upper
244	100		
212	10.5	4.9	7.3#
122	7.8	6.2	9.4

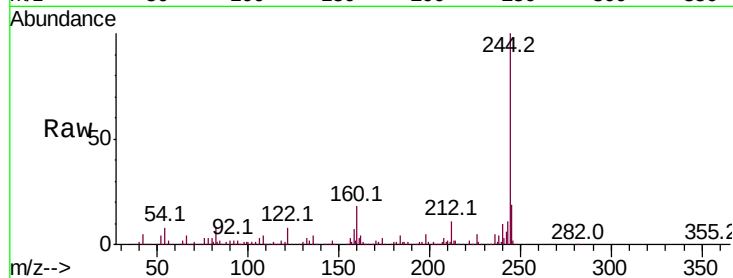


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

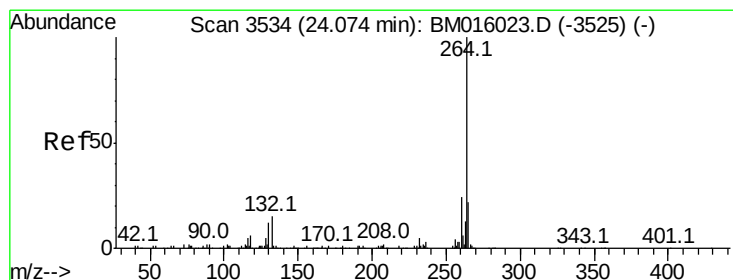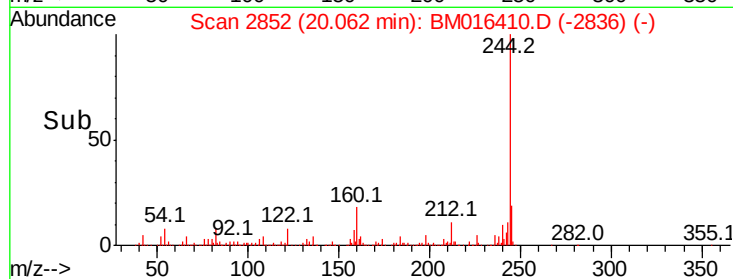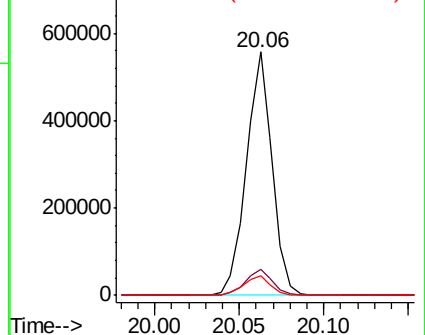

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.94 min Scan# 3511
 Delta R.T. -0.01 min
 Lab File: BM016410.D
 Acq: 16 Aug 2018 10:26

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.5	18.6	27.8
265	24.4	17.3	25.9

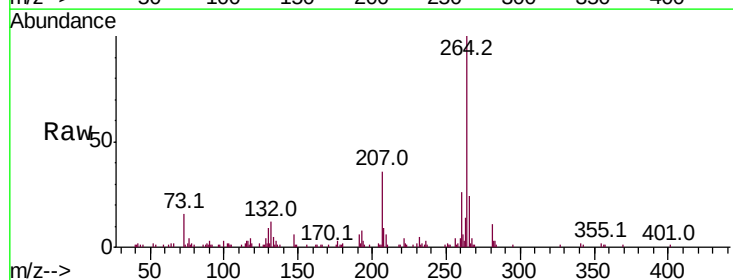

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

