

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081518\
 Data File : BM016410.D
 Acq On : 16 Aug 2018 10:26
 Operator : SJ/JU
 Sample : J4445-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DSN-001A-081018

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.169	315	320	329	rBV	22158	35459	1.62%	0.401%
2	5.640	395	400	415	rBV	229985	363685	16.66%	4.113%
3	7.281	674	679	694	rBB	113797	199822	9.16%	2.260%
4	7.634	733	739	752	rBV	539725	863085	39.54%	9.760%
5	8.104	815	819	826	rBV	98271	159234	7.30%	1.801%
6	8.428	867	874	884	rBV	543486	851973	39.03%	9.634%
7	9.293	1015	1021	1040	rBV	357499	621987	28.50%	7.034%
8	10.922	1292	1298	1307	rBV	104910	175442	8.04%	1.984%
9	13.363	1706	1713	1721	rBV	920914	1257493	57.61%	14.220%
10	14.745	1941	1948	1955	rBB3	130344	192777	8.83%	2.180%
11	16.233	2195	2201	2217	rBB	806711	1086145	49.76%	12.282%
12	17.480	2408	2413	2419	rBV	163529	223244	10.23%	2.524%
13	20.062	2847	2852	2857	rBV	1991723	2182610	100.00%	24.681%
14	21.286	3055	3060	3064	rBV7	12479	27628	1.27%	0.312%
15	21.615	3111	3116	3122	rBV	243181	315685	14.46%	3.570%
16	23.939	3506	3511	3519	rBV	153399	286838	13.14%	3.244%


Sum of corrected areas: 8843107

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081518\
Data File : BM016410.D
Acq On : 16 Aug 2018 10:26
Operator : SJ/JU
Sample : J4445-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DSN-001A-081018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

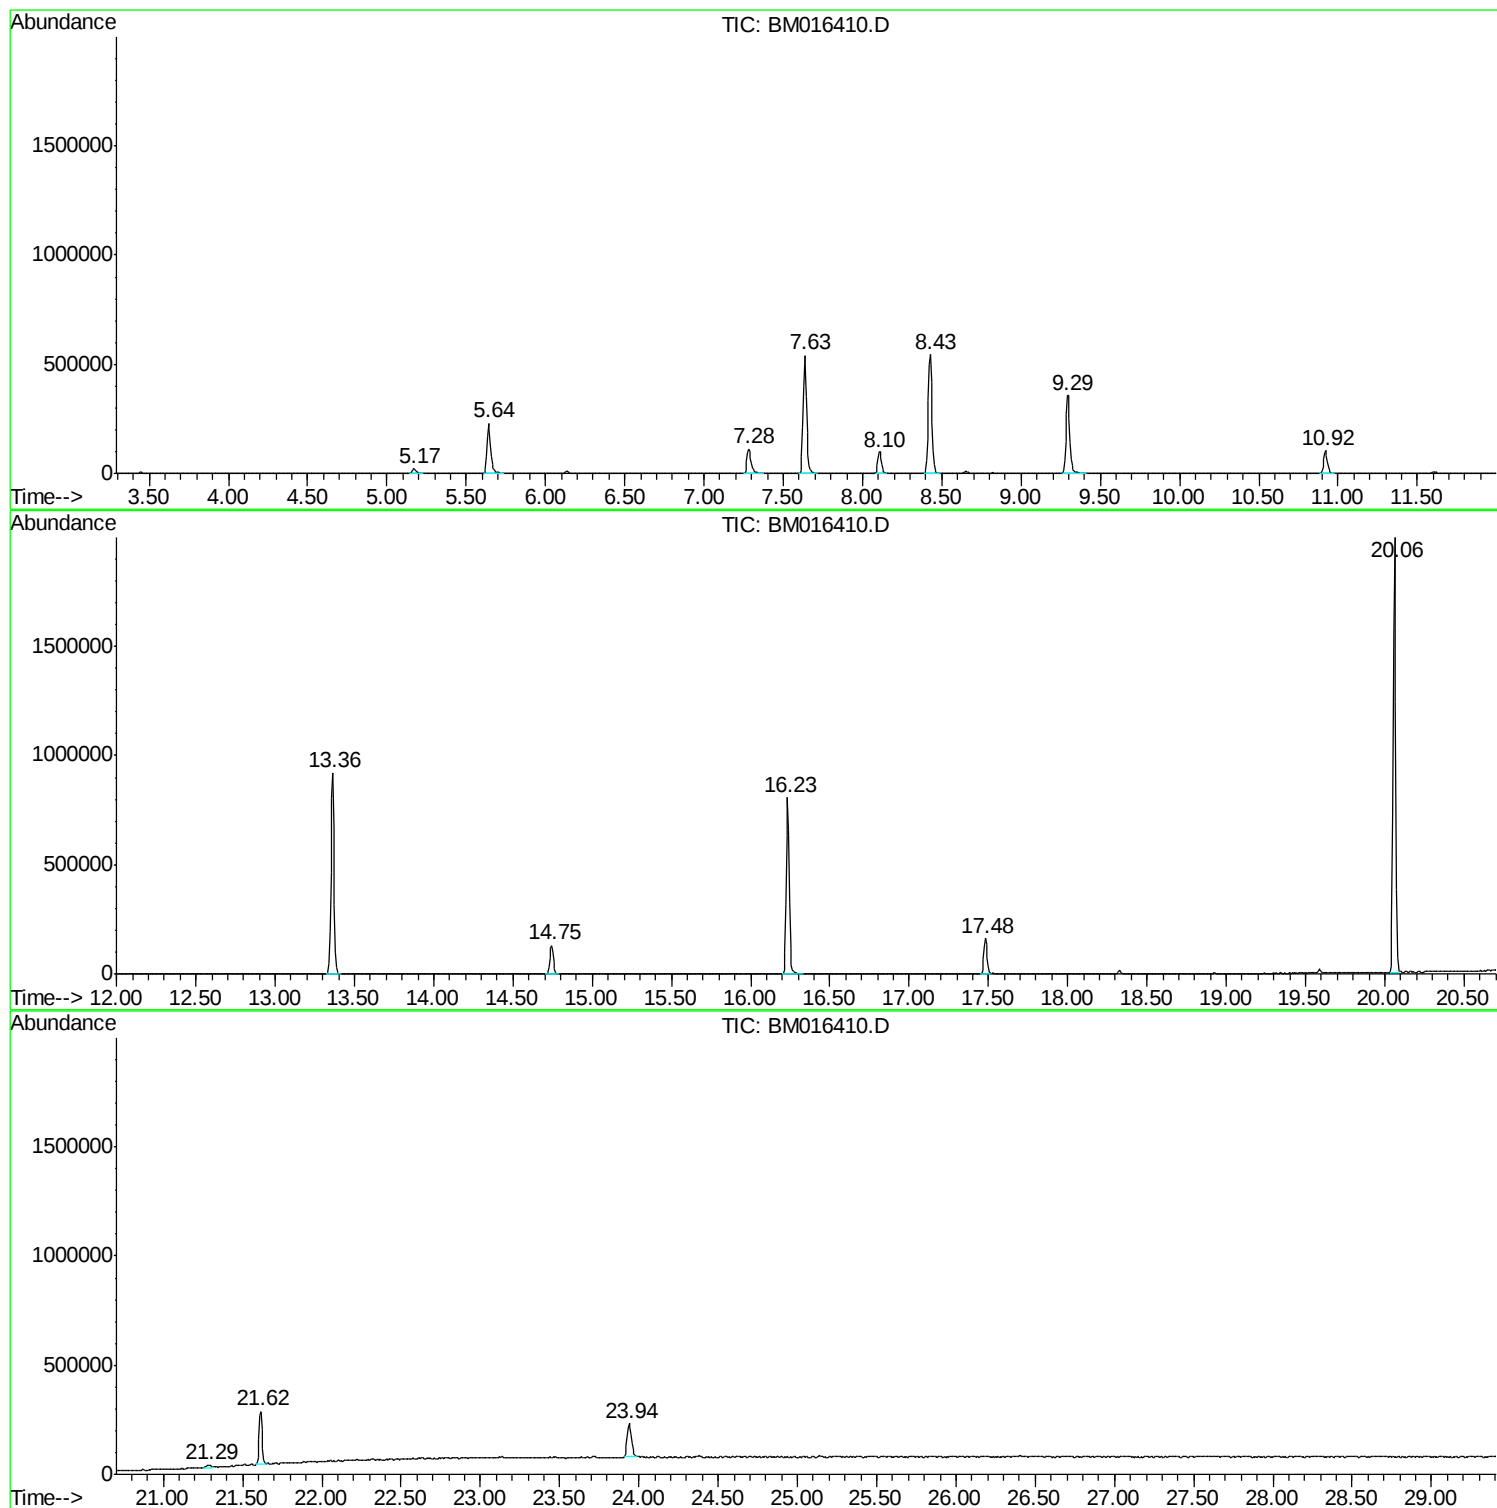

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081518\
Data File : BM016410.D
Acq On : 16 Aug 2018 10:26
Operator : SJ/JU
Sample : J4445-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DSN-001A-081018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081518\
Data File : BM016410.D
Acq On : 16 Aug 2018 10:26
Operator : SJ/JU
Sample : J4445-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DSN-001A-081018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
