


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081518\
 Data File : BM016373.D
 Acq On : 15 Aug 2018 10:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 15 11:23:48 2018

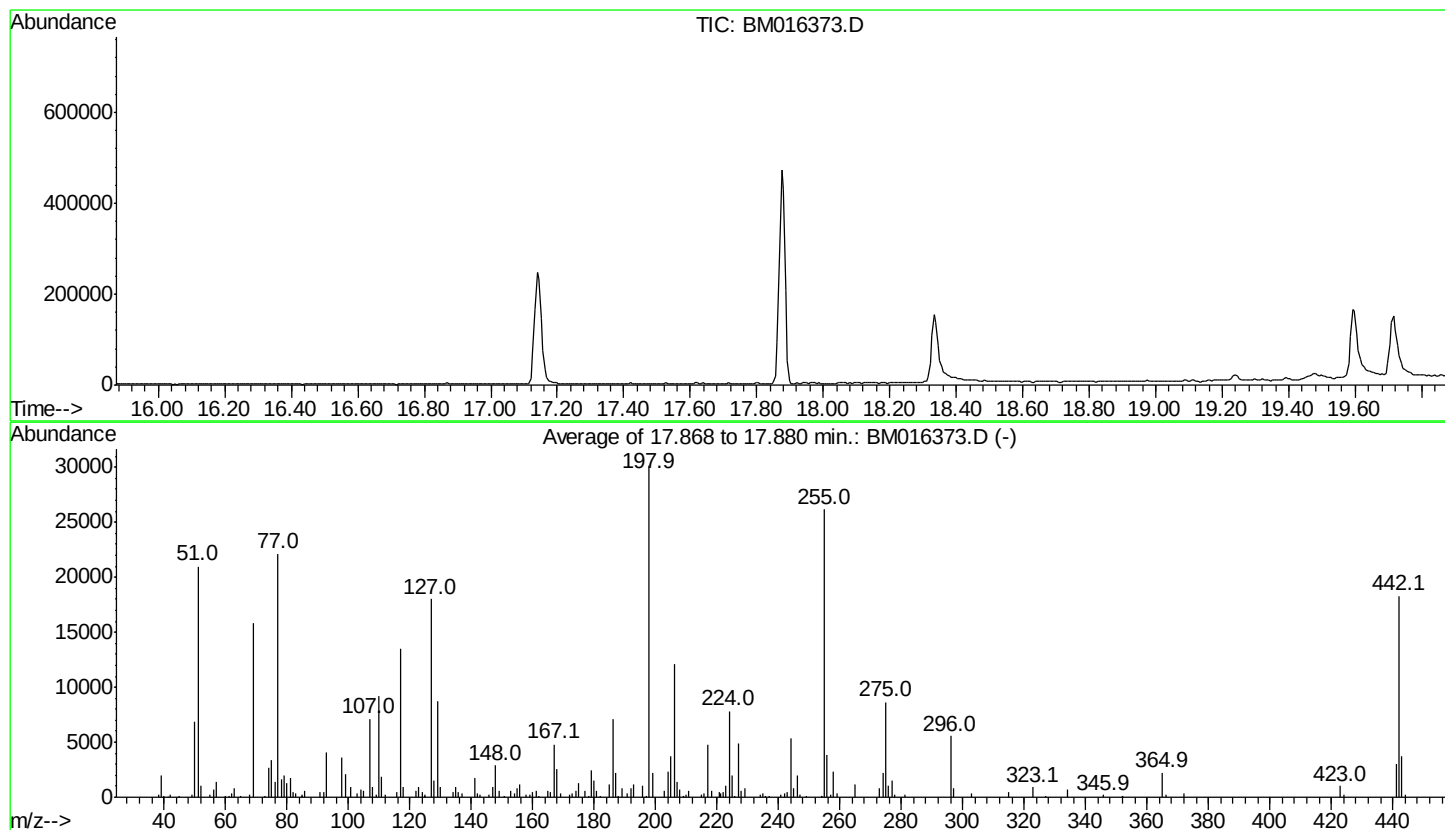

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.6	21000	PASS
68	69	0.00	2	1.7	266	PASS
69	198	0.00	100	52.5	15835	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.8	18025	PASS
197	198	0.00	2	0.4	131	PASS
198	198	100	100	100.0	30154	PASS
199	198	5	9	7.5	2264	PASS
275	198	10	60	28.8	8671	PASS
365	198	1	100	7.4	2244	PASS
441	198	0.01	100	9.9	2995	PASS
442	198	50	100	60.8	18322	PASS
443	442	15	24	20.4	3740	PASS