


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
Data File : BM022148.D
Acq On : 15 Aug 2019 17:56
Operator : HP/JU
Sample : K4242-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual Integrations
APPROVED

mohammad
8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:24:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 13:53:23 2019
Response via : Initial Calibration

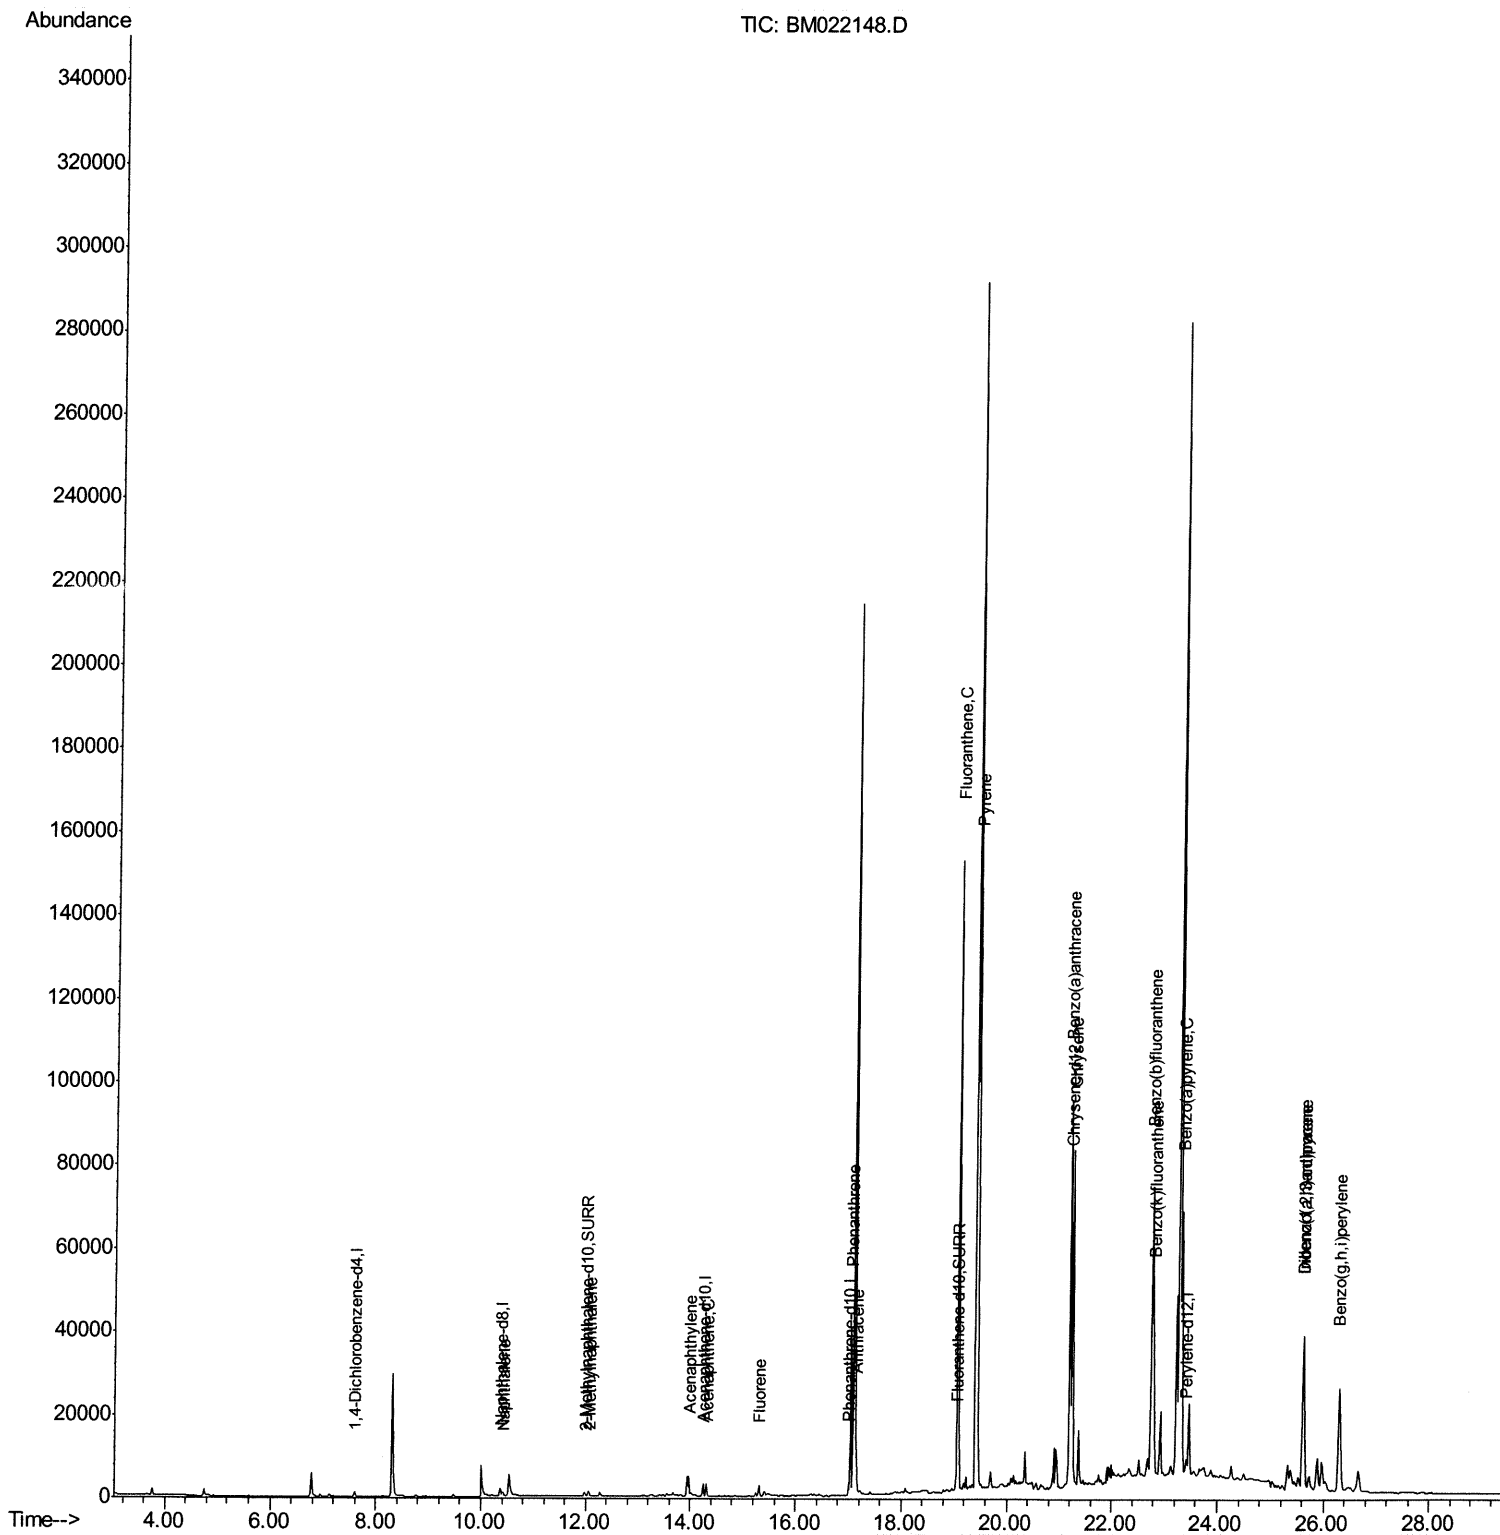


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
Data File : BM022148.D
Acq On : 15 Aug 2019 17:56
Operator : HP/JU
Sample : K4242-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual Integrations
APPROVED

mohammad
8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:12:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 13:53:23 2019
Response via : Initial Calibration

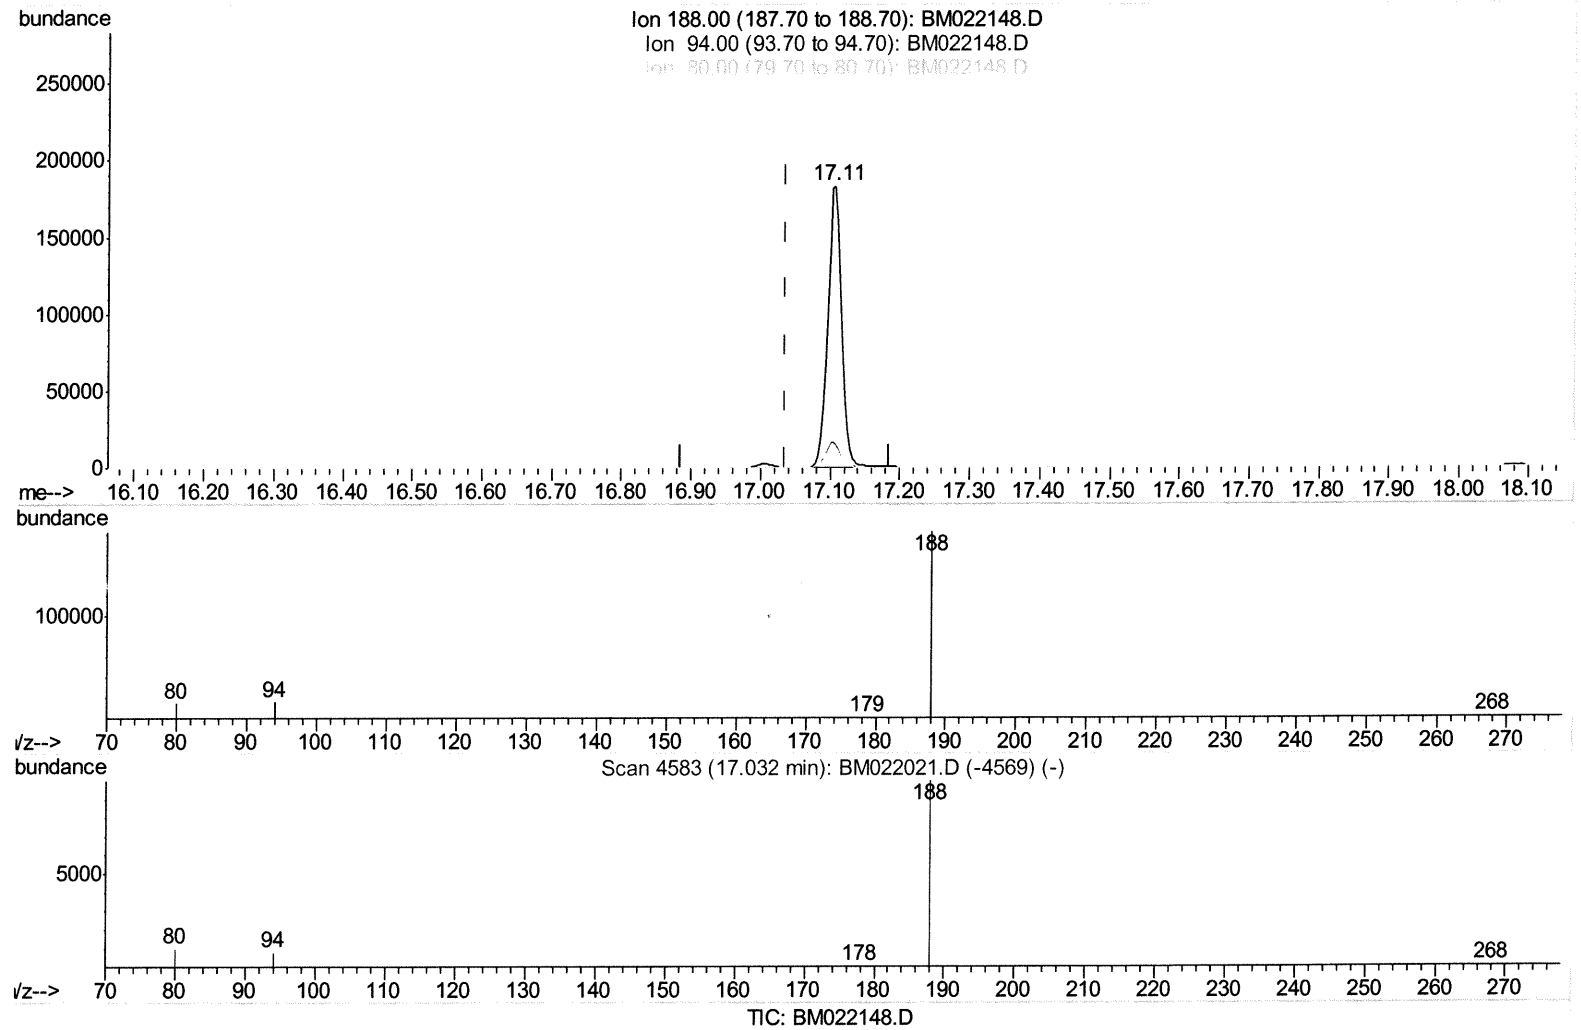

(10) Phenanthrene-d10 (I)

17.107min (+0.071) 0.40ng/ul

response 252092

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	8.68
80.00	11.40	8.24#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:12:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

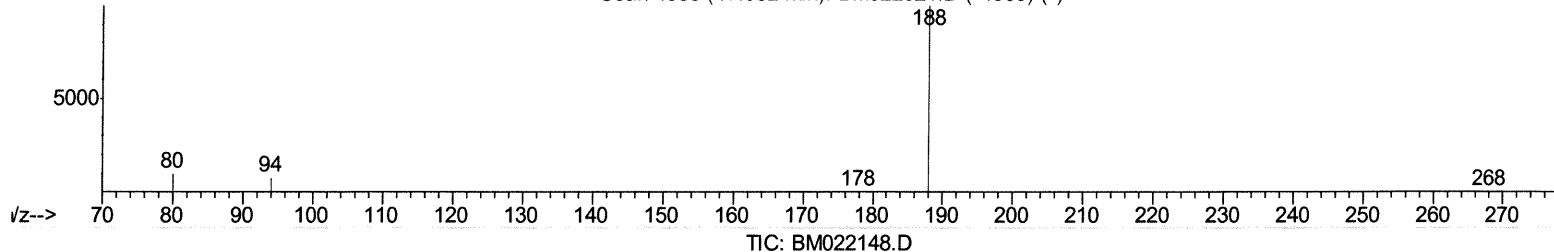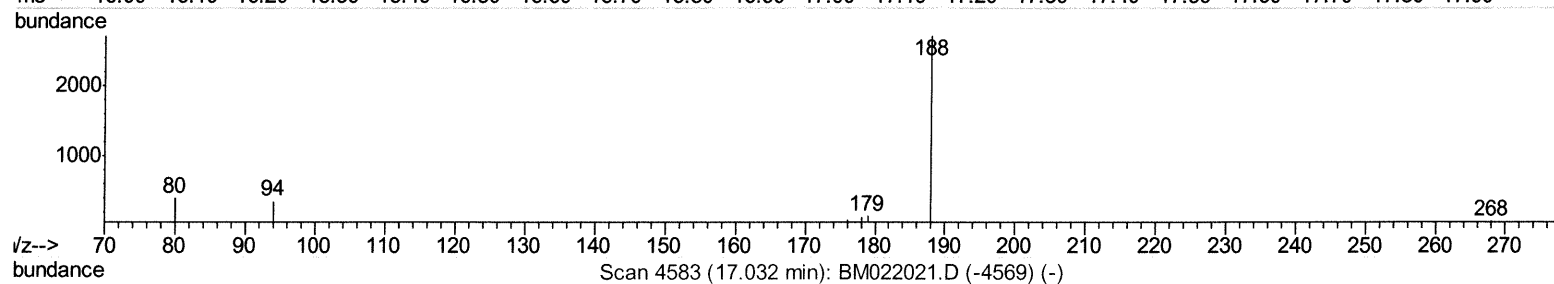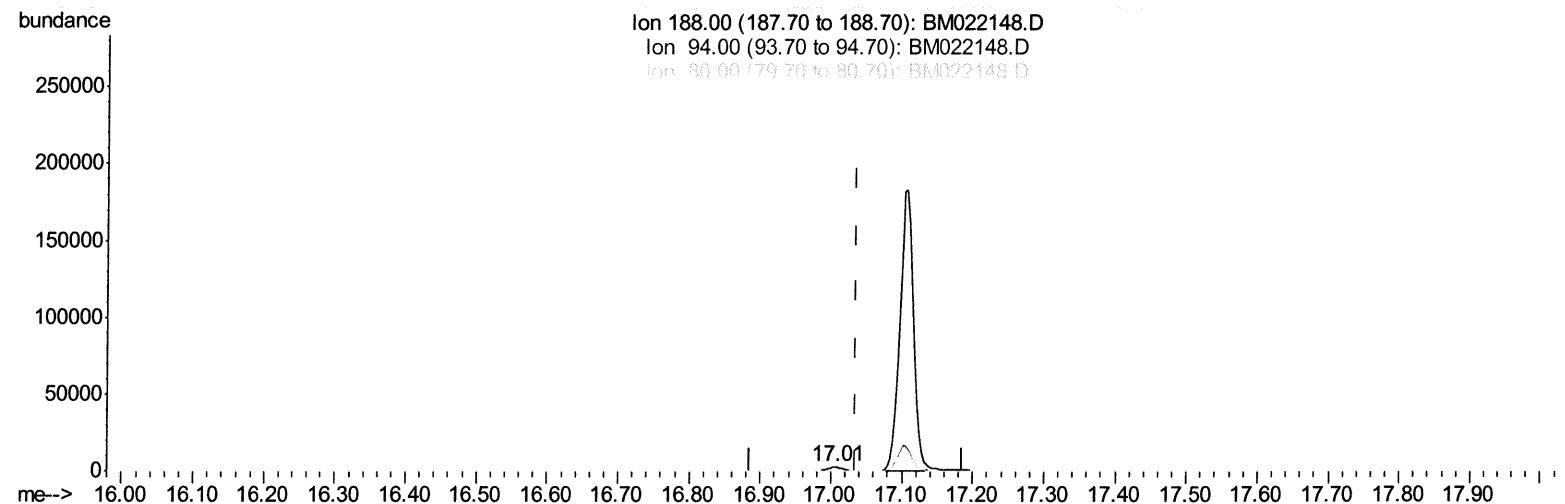

(10) Phenanthrene-d10 (I)

17.006min (-0.030) 0.40ng/ul m

JU
 08/20/19

response 3811

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.84#
80.00	11.40	14.46#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

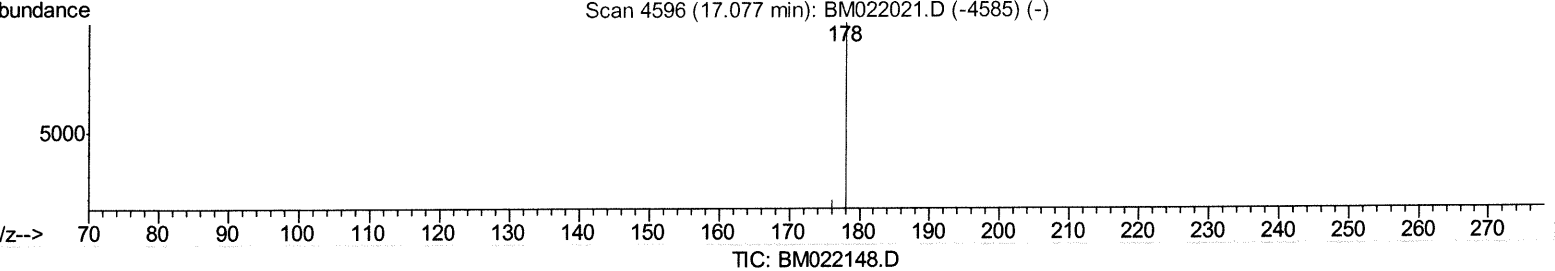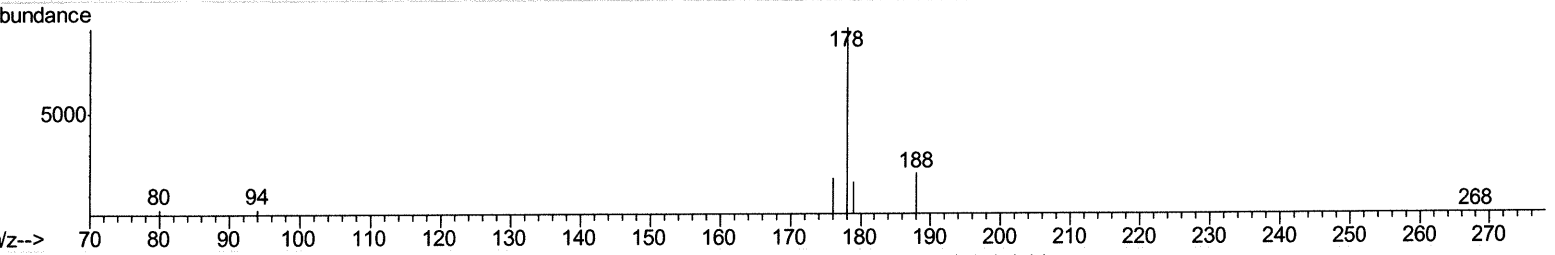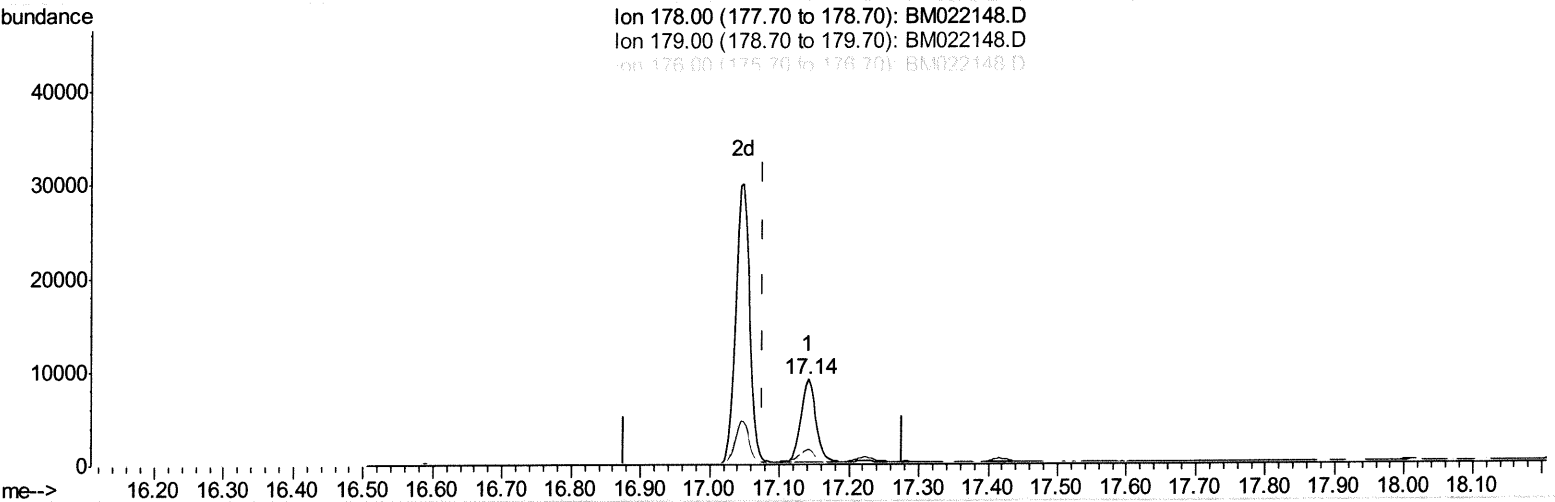

(12) Phenanthrene

17.142min (+0.064) 1.18ng/ul

response 13116

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	17.42
176.00	21.00	19.70
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

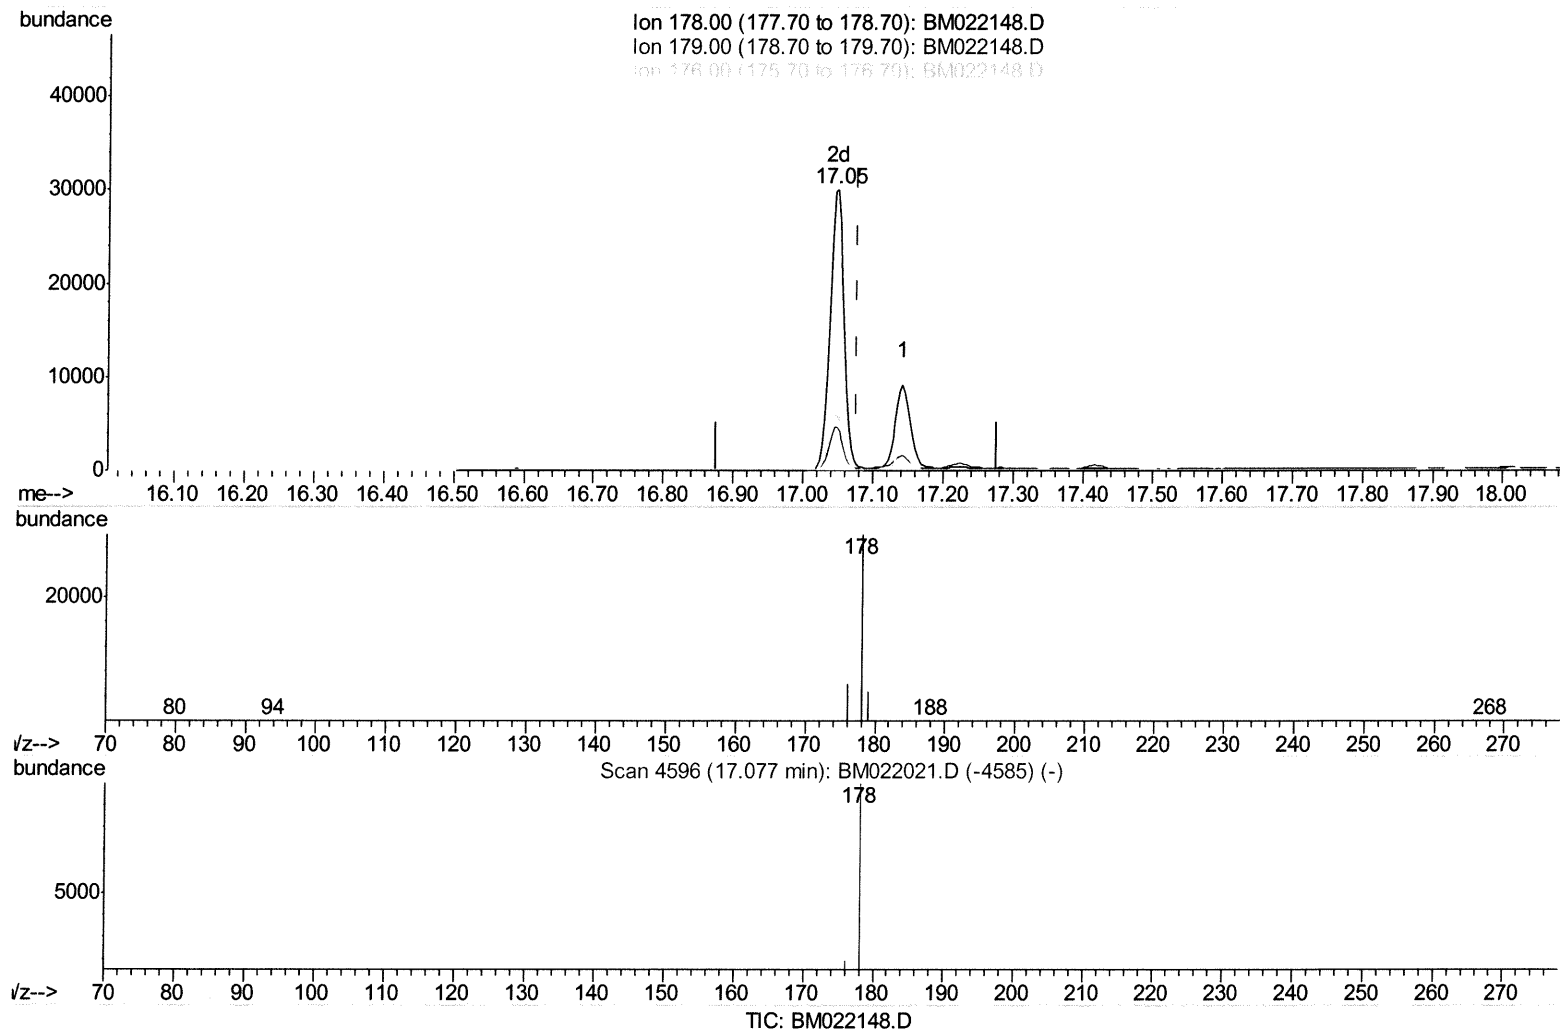

(12) Phenanthrene

17.048min (-0.029) 3.82ng/ul m

JU
 08/20/19

response 42331

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	15.65
176.00	21.00	19.80
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

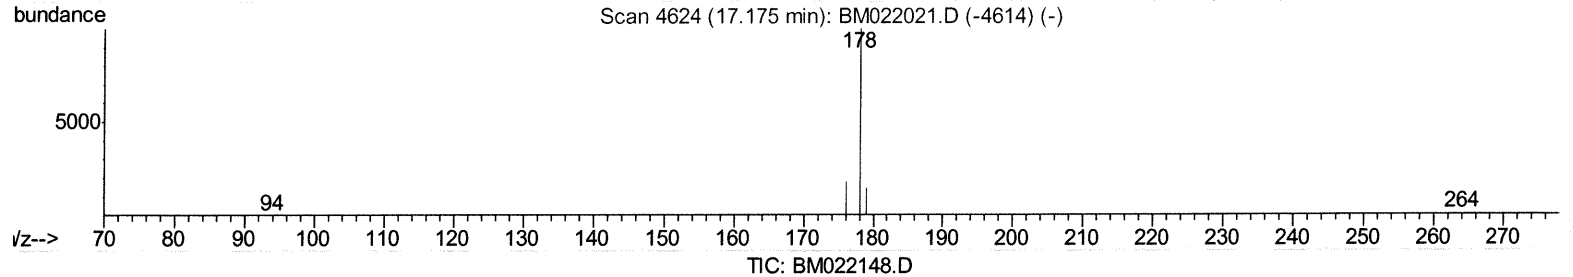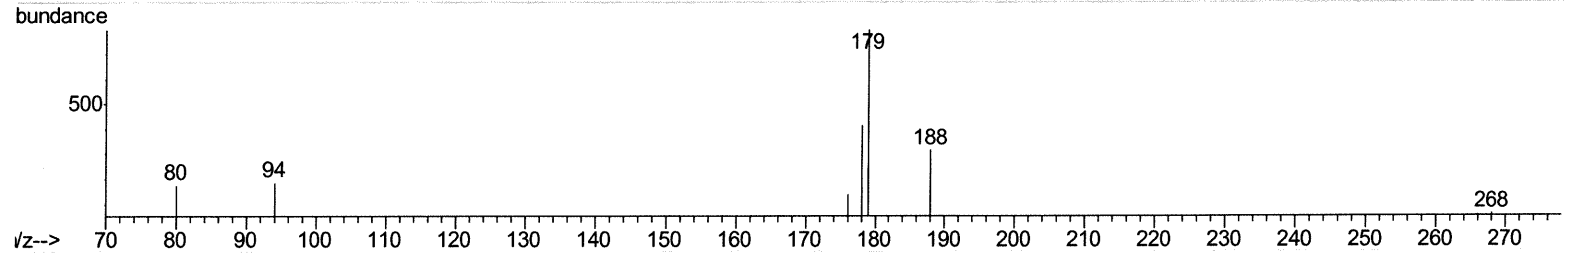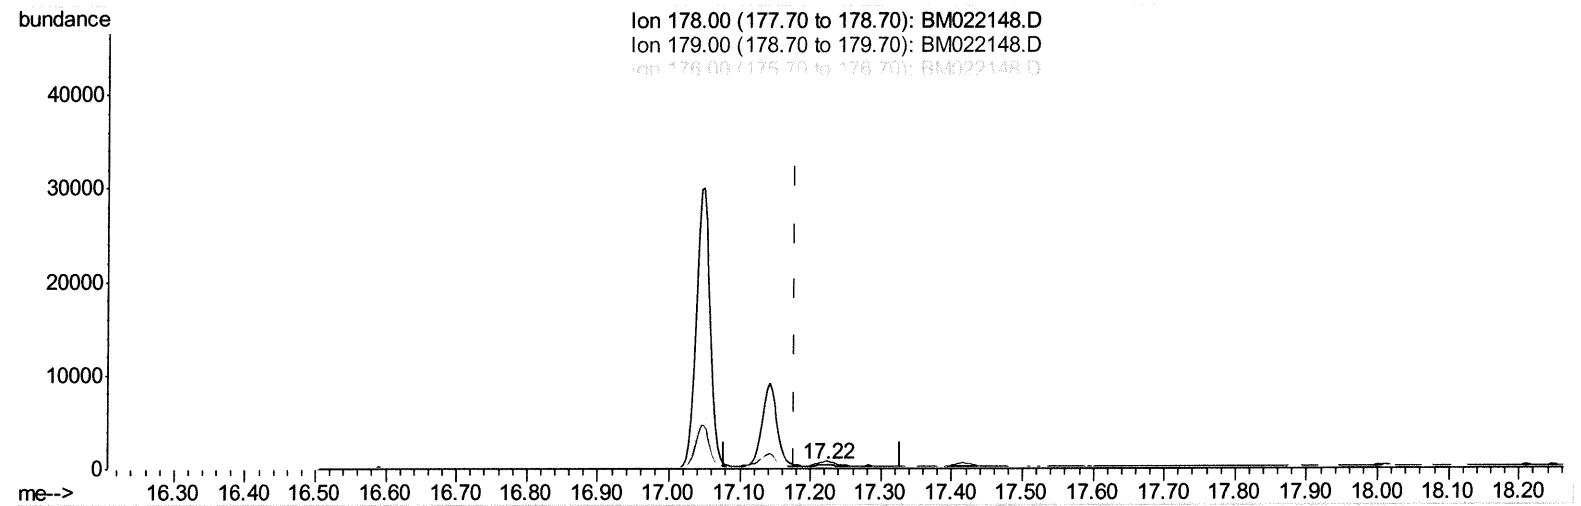

(13) Anthracene

17.221min (+0.043) 0.04ng/ul

response 370

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	193.20#
176.00	20.80	34.22#
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6


Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

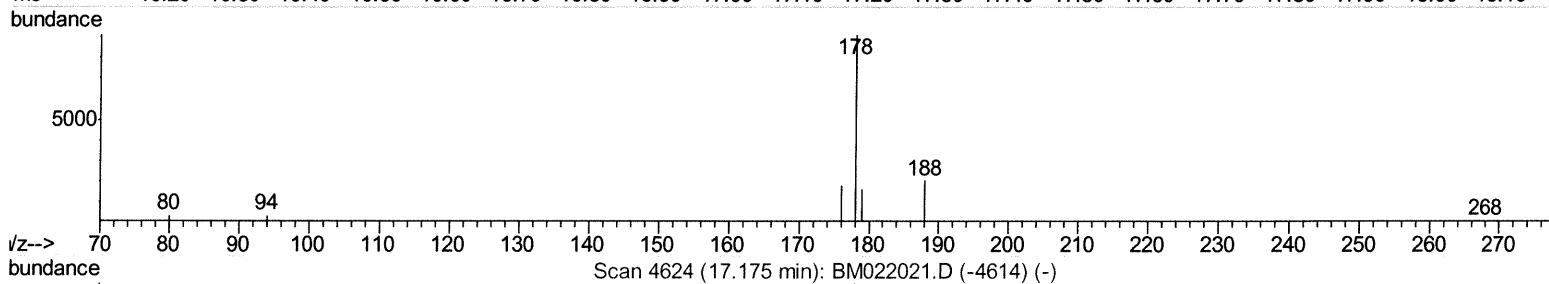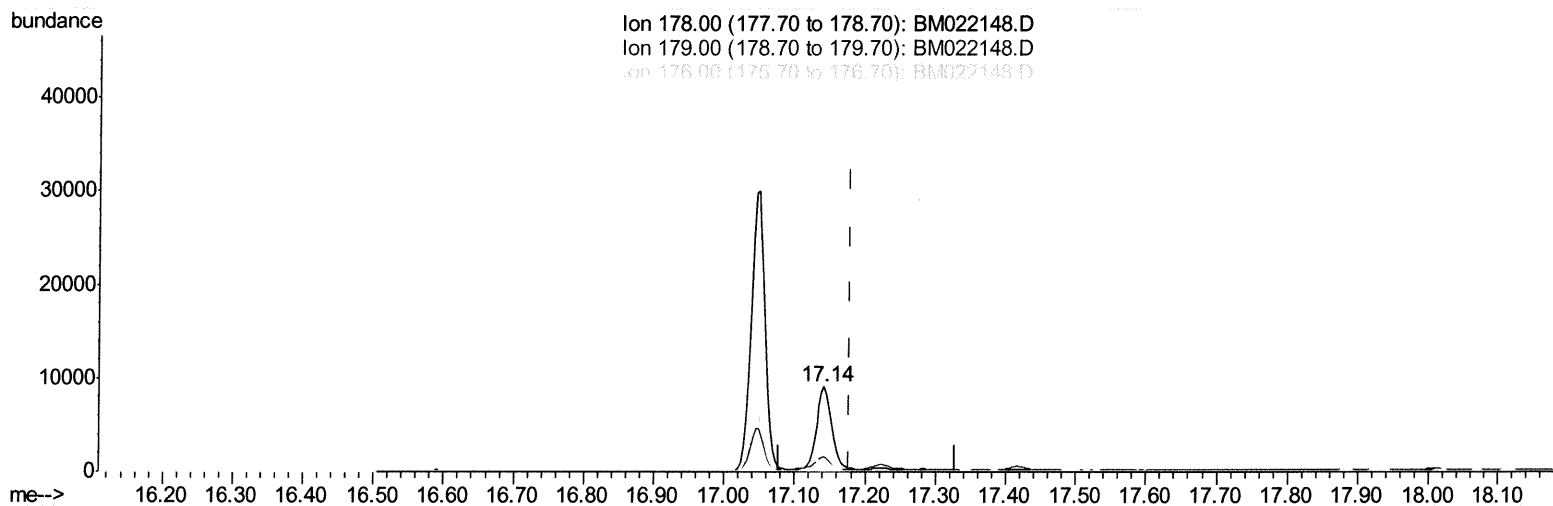

Scan 4624 (17.175 min): BM022021.D (-4614) (-)

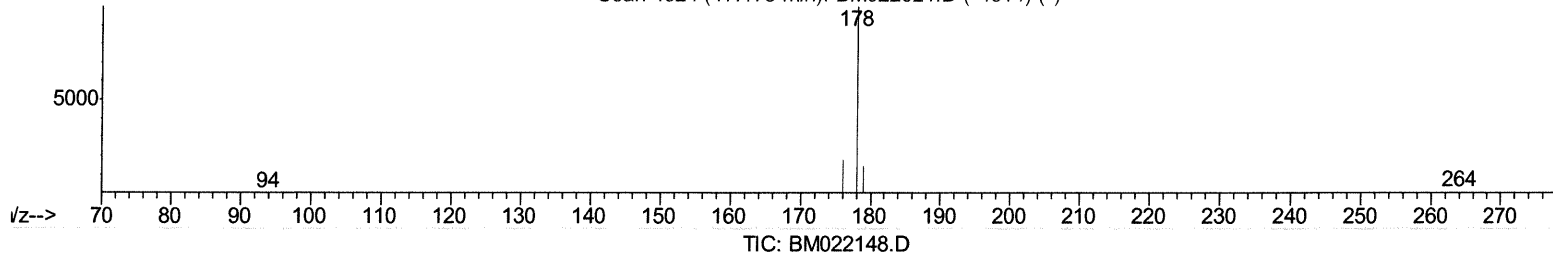

(13) Anthracene

17.142min (-0.036) 1.50ng/ul m

JU
 08/20/19

response 14224

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	17.42
176.00	20.80	19.70
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

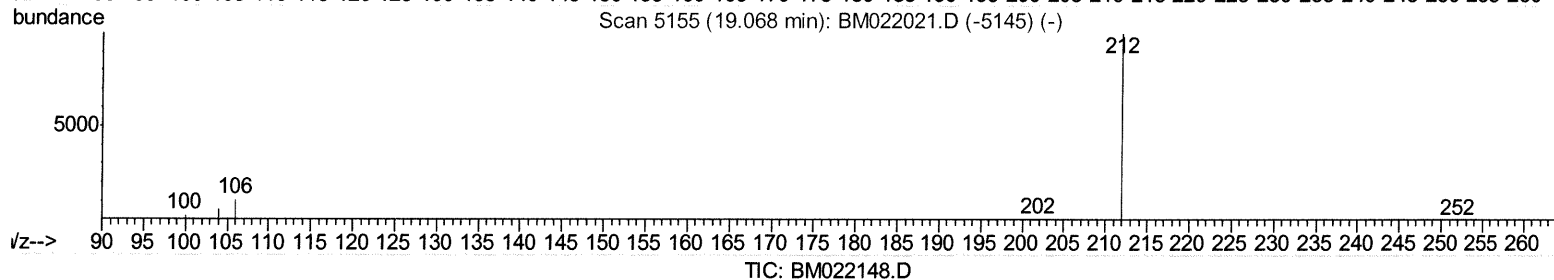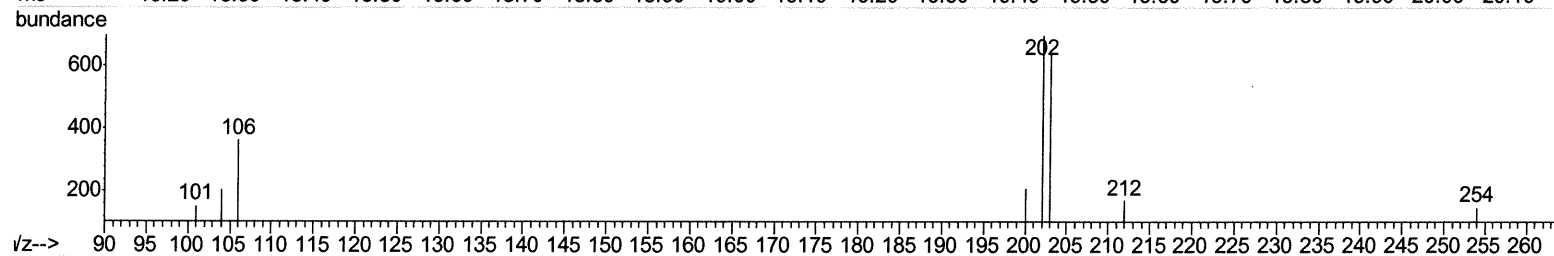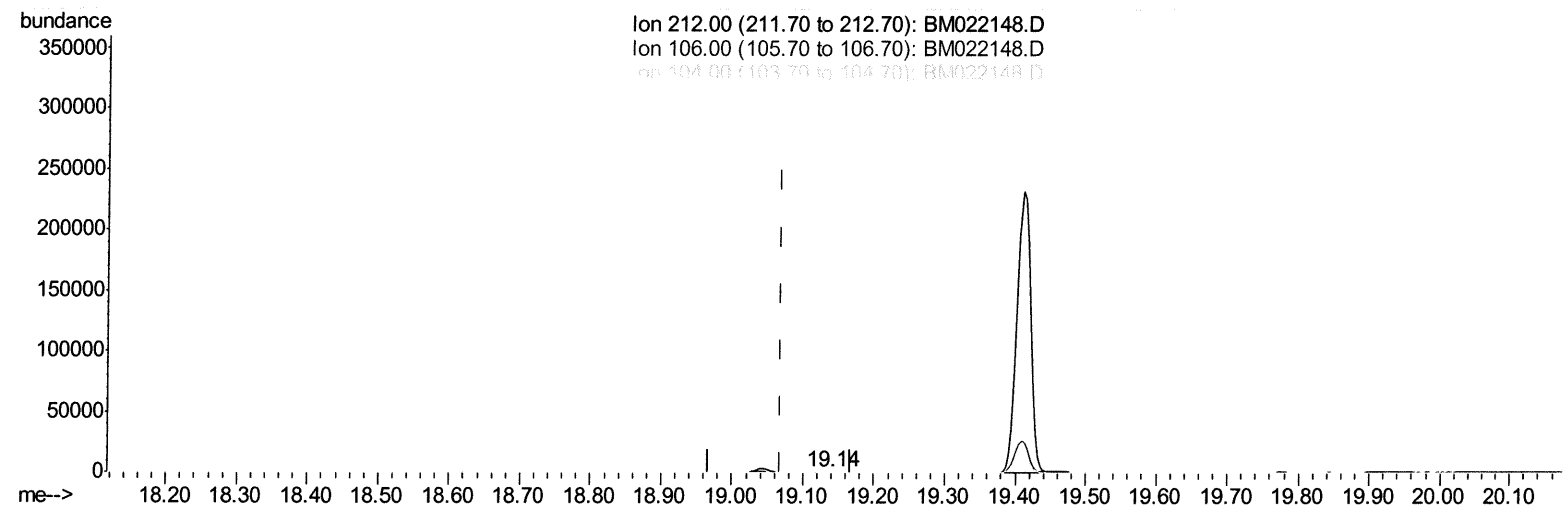

(14) Fluoranthene-d10 (SURR)

19.138min (+0.070) 0.01ng/ul

response 89

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	32.58#
104.00	6.00	40.45#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

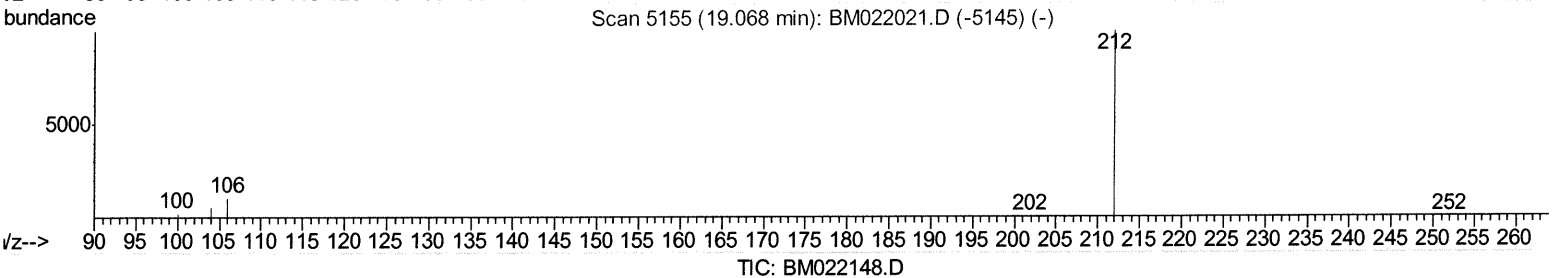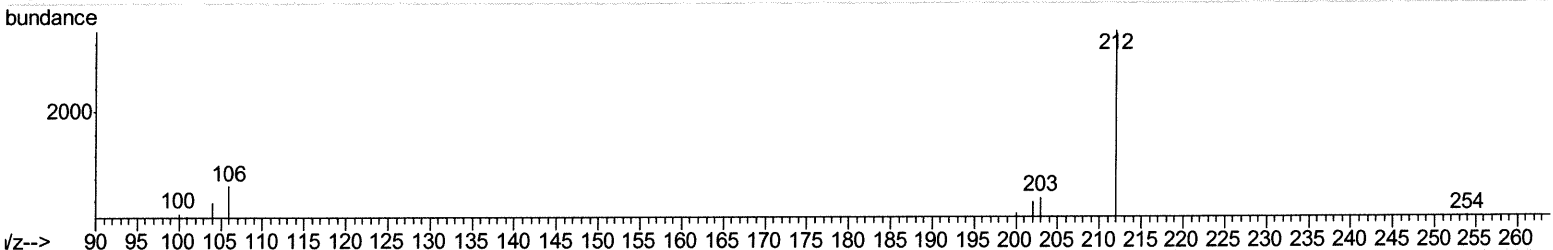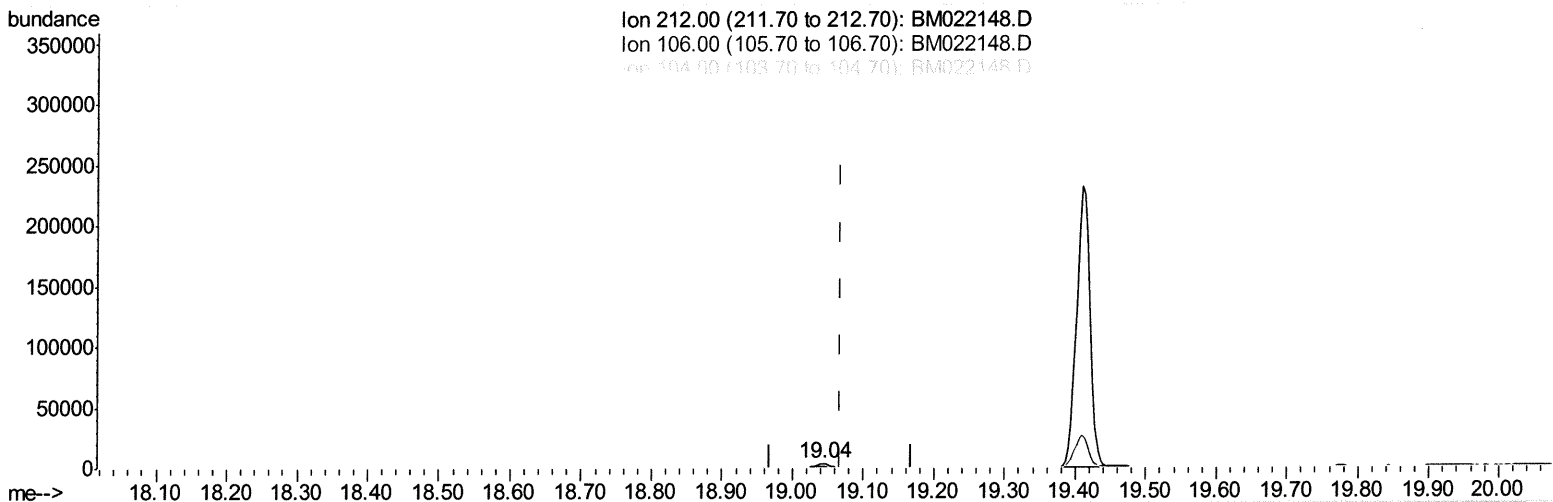

(14) Fluoranthene-d10 (SURR)

19.043min (-0.025) 0.36ng/ul m

JU
08/20/19

response 4586

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.63#
104.00	6.00	0.78#
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

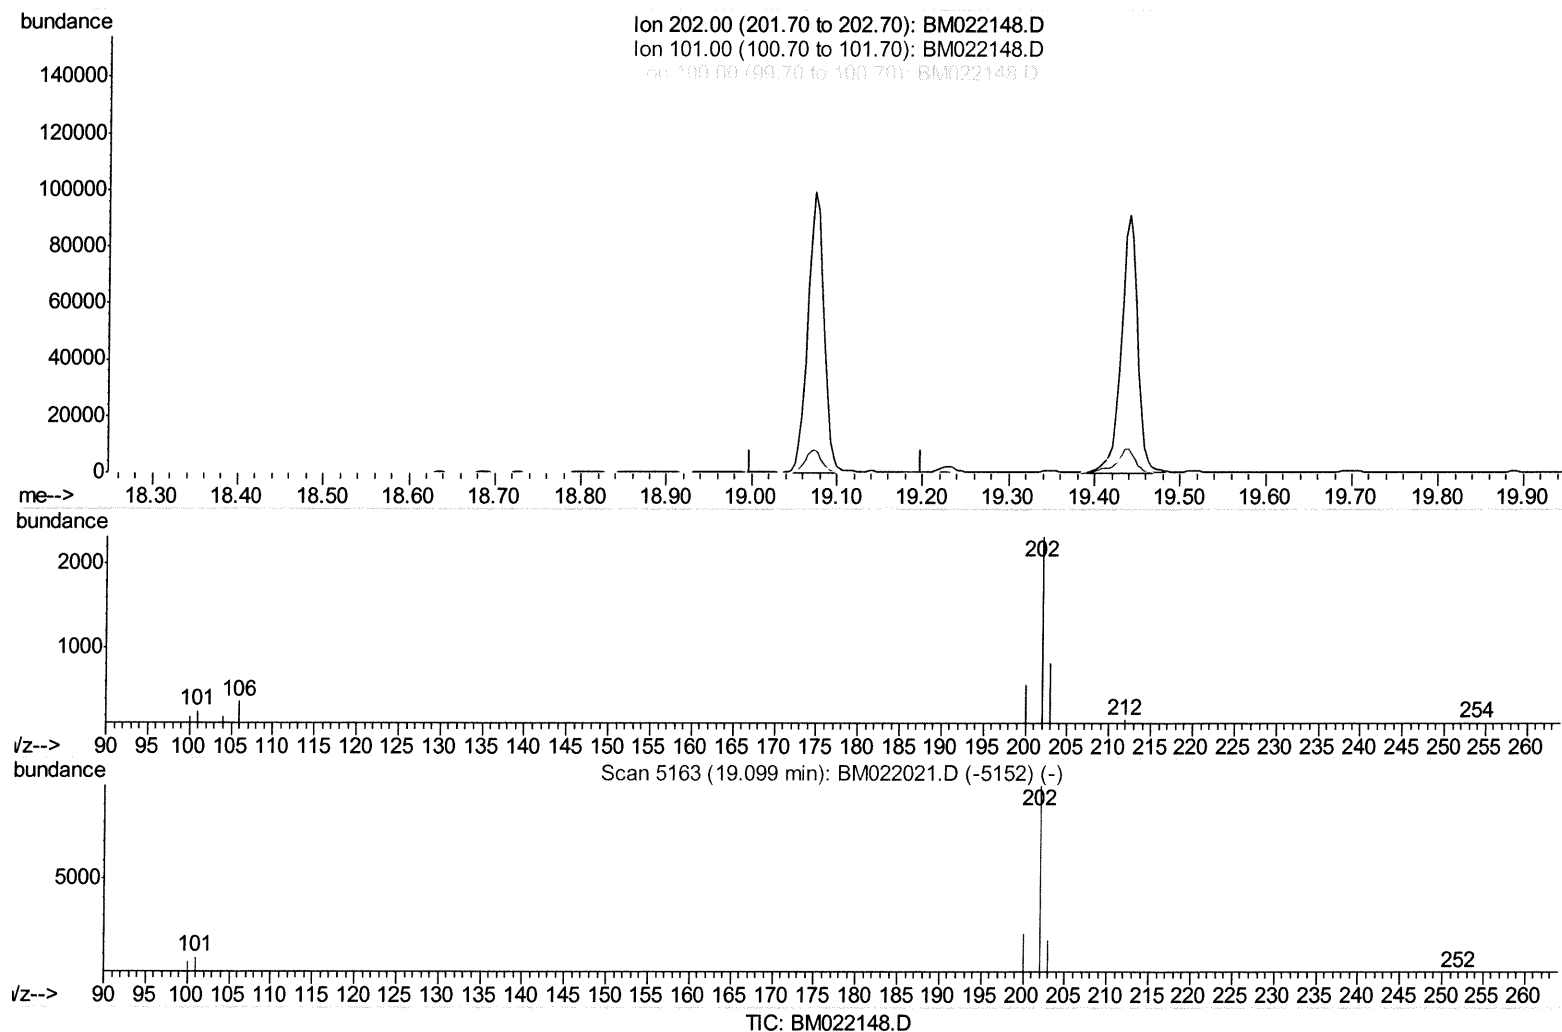

(15) Fluoranthene (C)

19.098min (-19.098) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.20	0.00
100.00	8.10	0.00
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

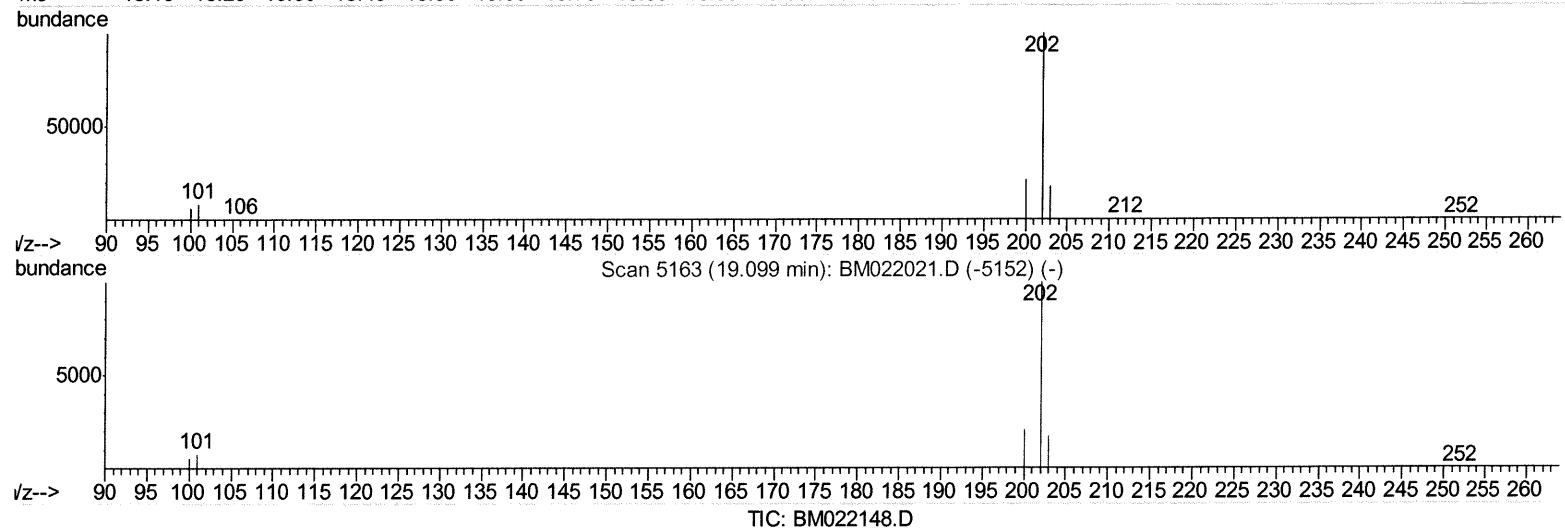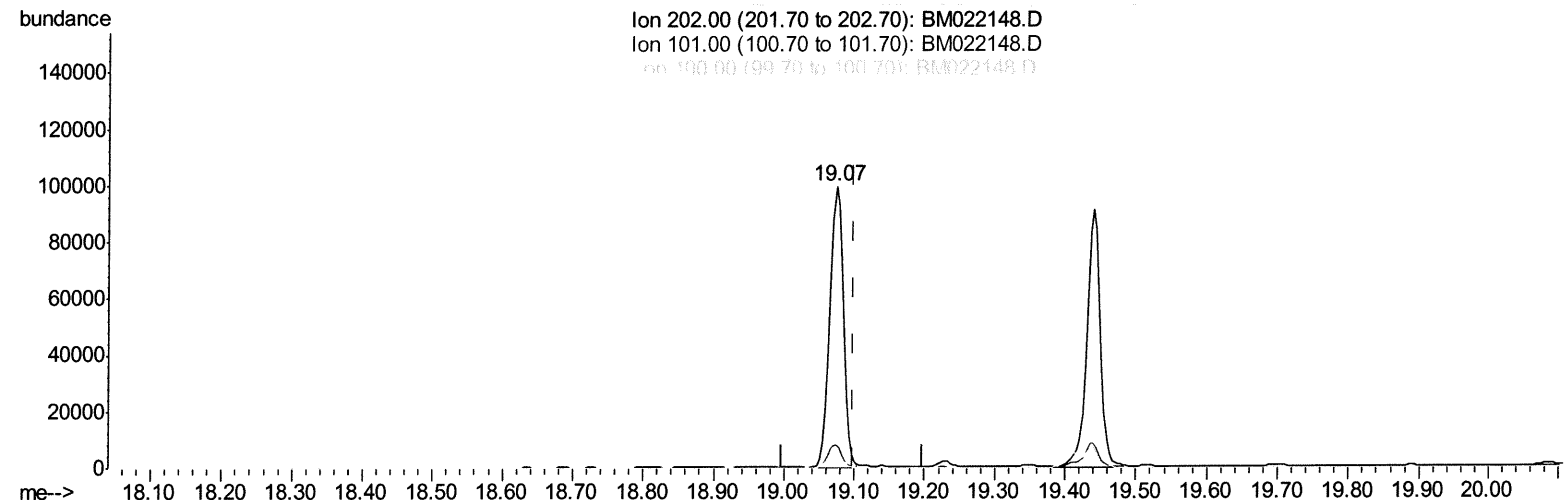

(15) Fluoranthene (C)

19.074min (-0.025) 8.85ng/ul m

JU
08/20/19

response 131427

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	8.33
100.00	8.10	6.52
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
Data File : BM022148.D
Acq On : 15 Aug 2019 17:56
Operator : HP/JU
Sample : K4242-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual Integrations
APPROVED

mohammad
8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 13:53:23 2019
Response via : Initial Calibration

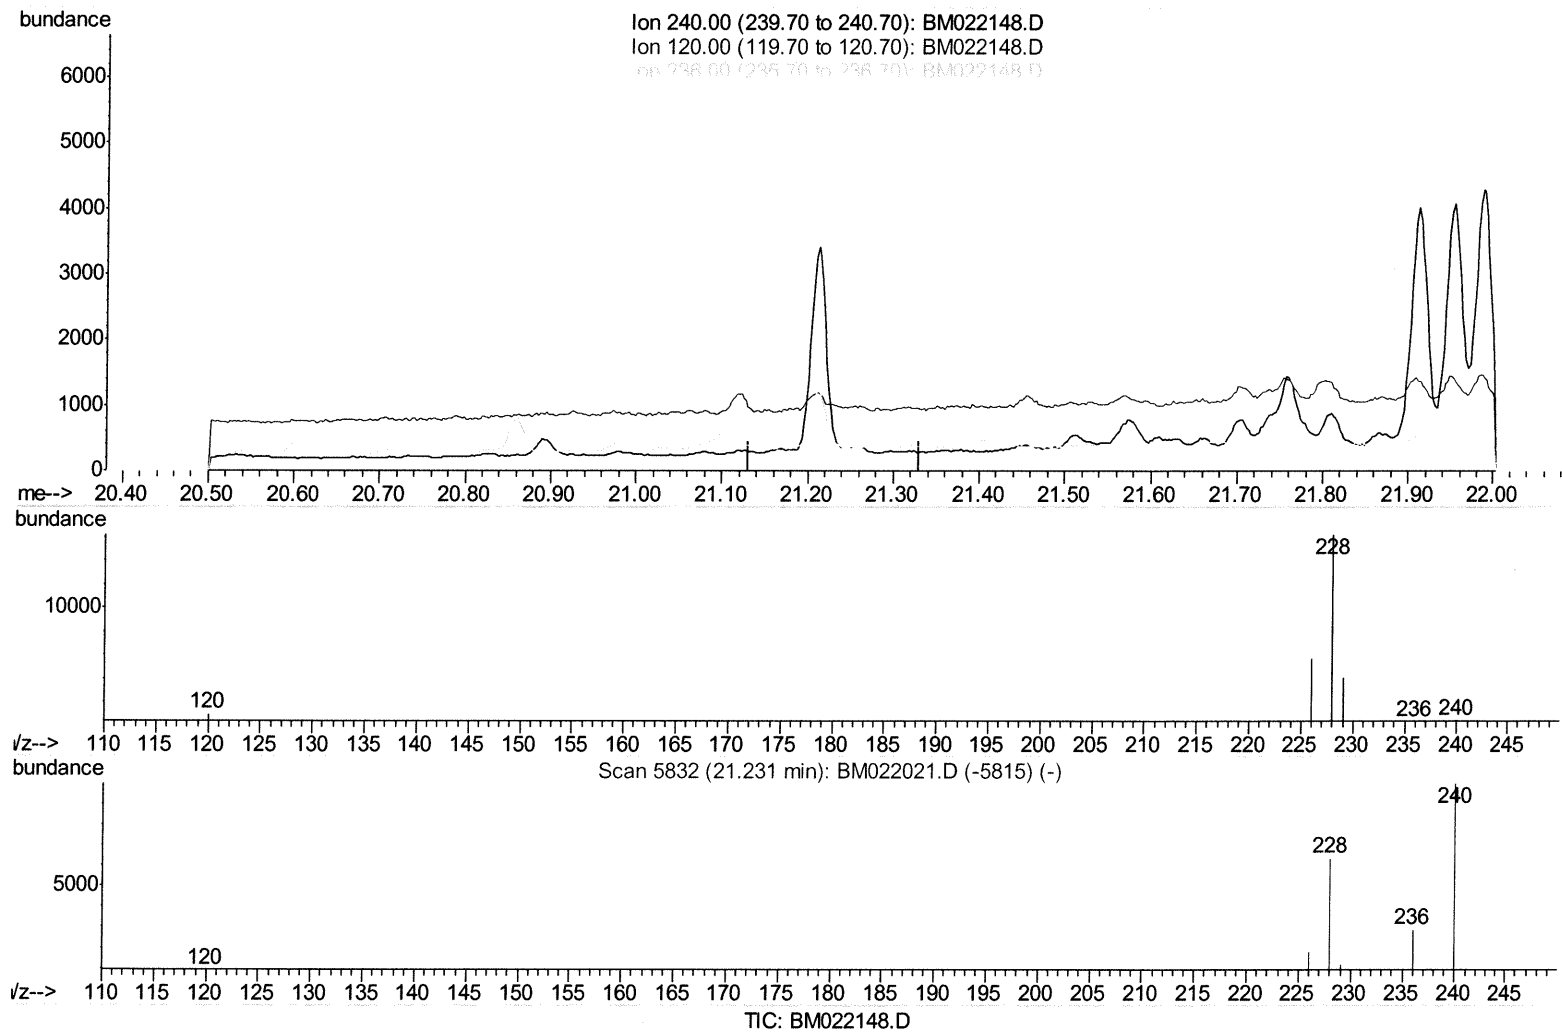

(16) Chrysene-d12 (I)

21.231min (-21.231) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:17:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

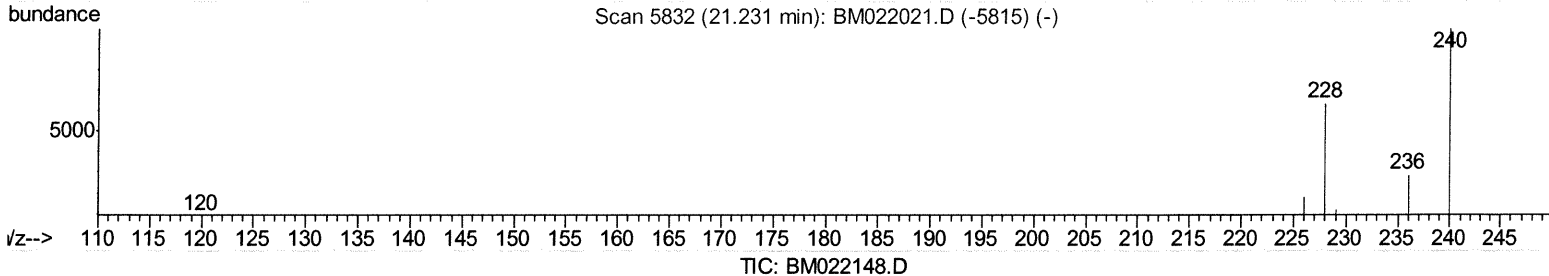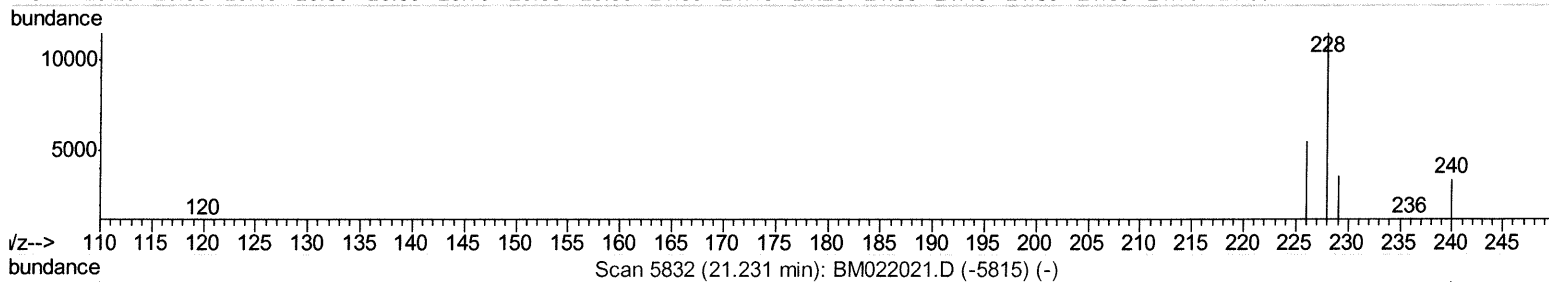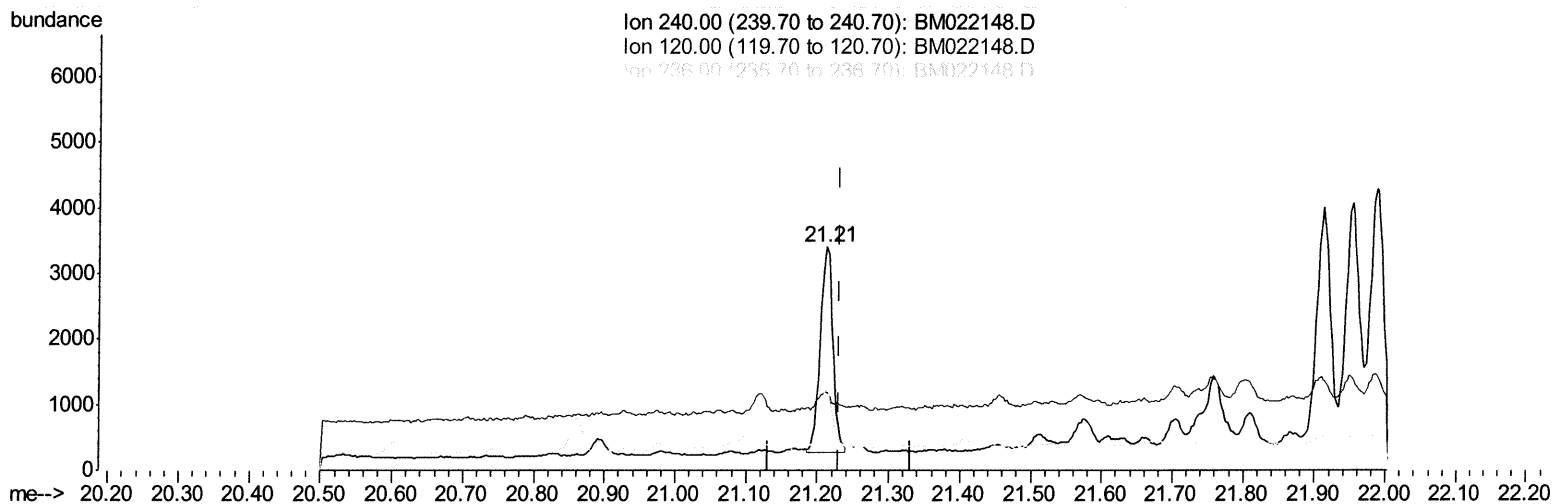

(16) Chrysene-d12 (I)

21.212min (-0.019) 0.40ng/ul m

JU
 08/20/19

response 3889

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	35.02#
236.00	32.30	36.34
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:20:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

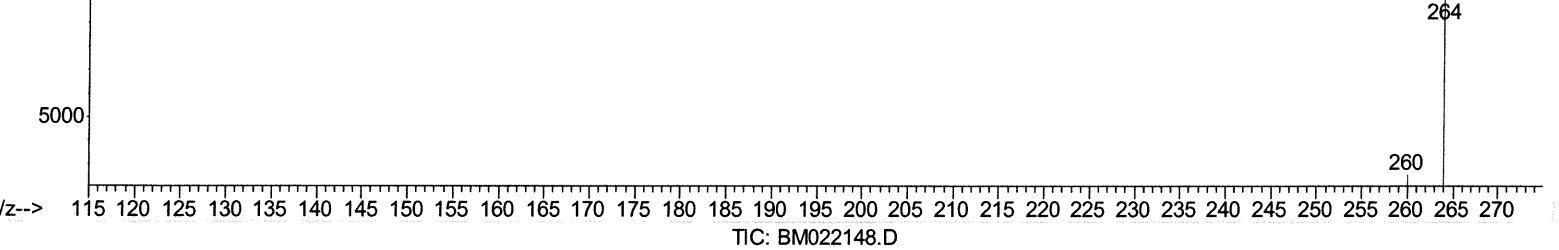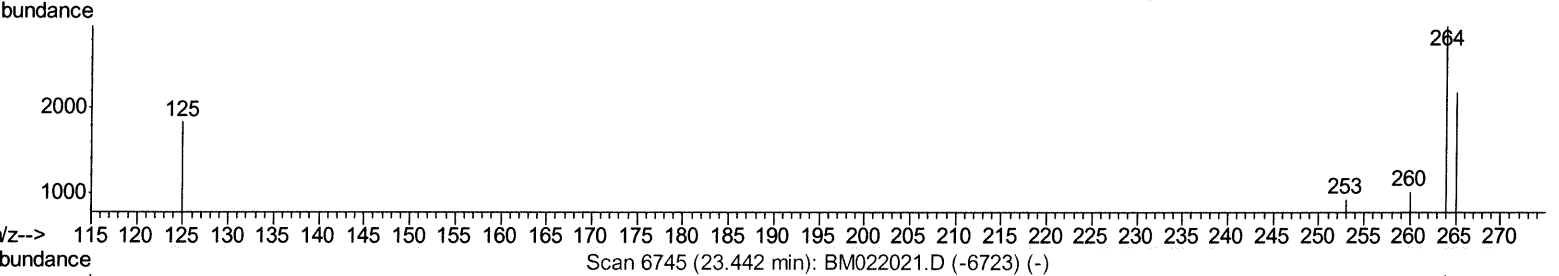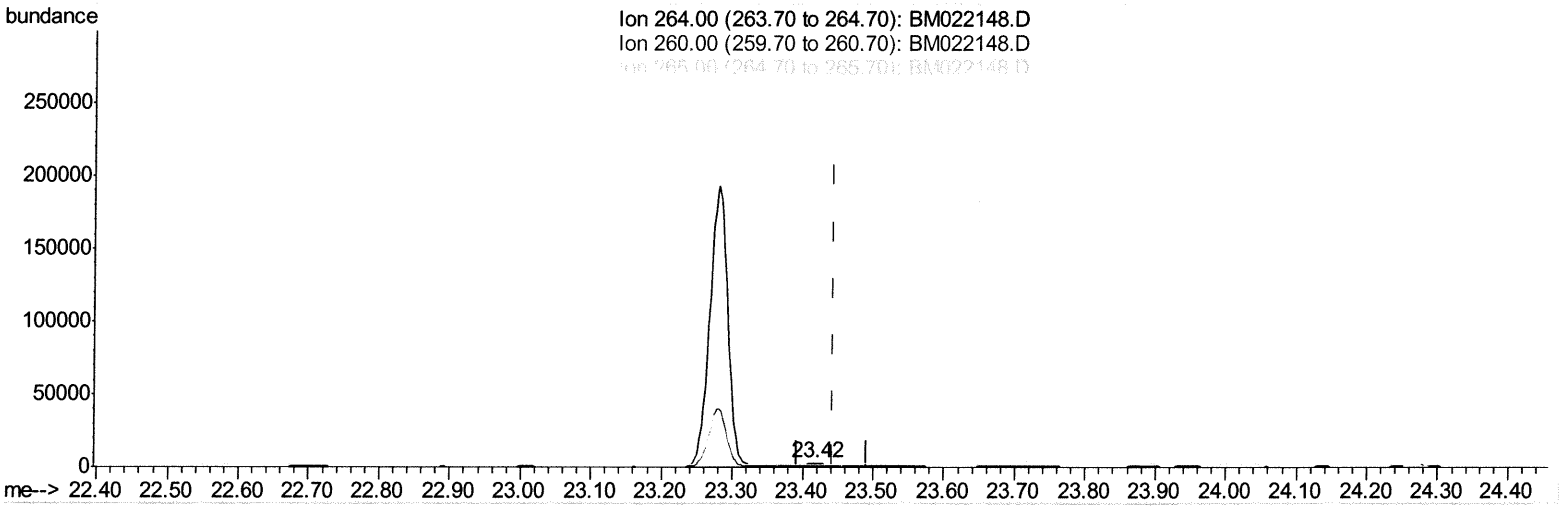

(20) Perylene-d12 (I)

23.419min (-0.024) 0.40ng/ul

response 4054

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	34.23#
265.00	117.00	73.85#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:20:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

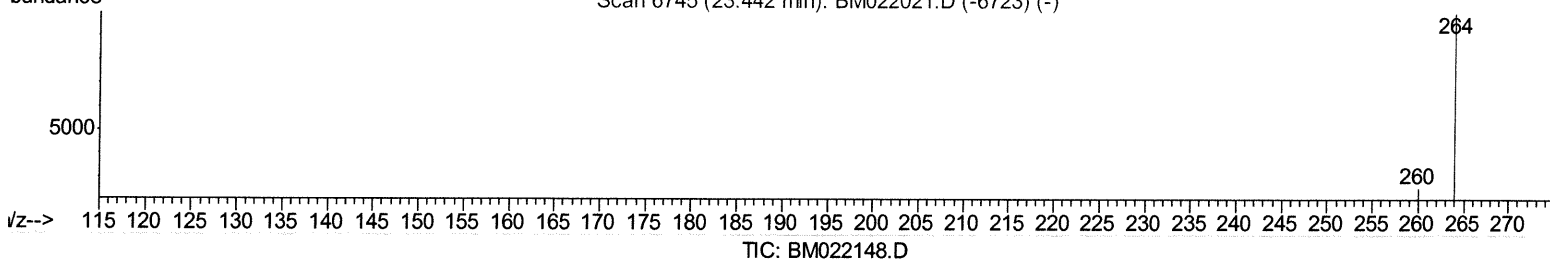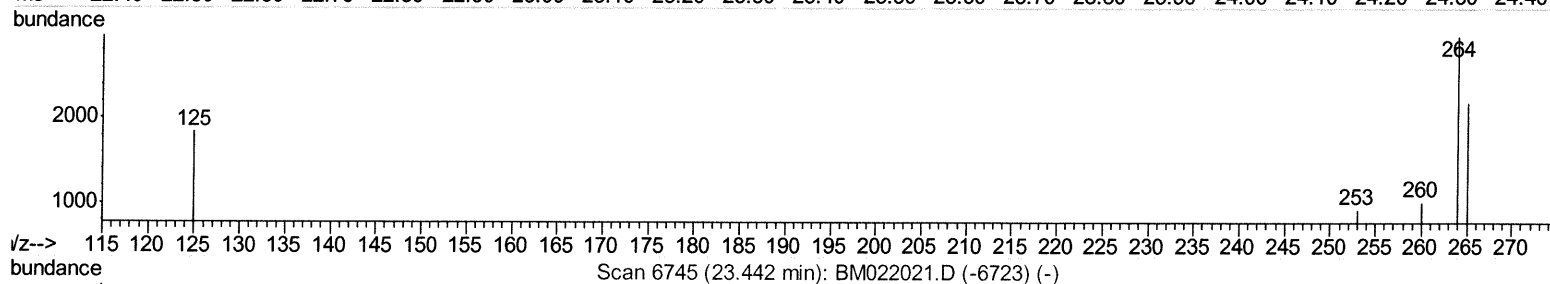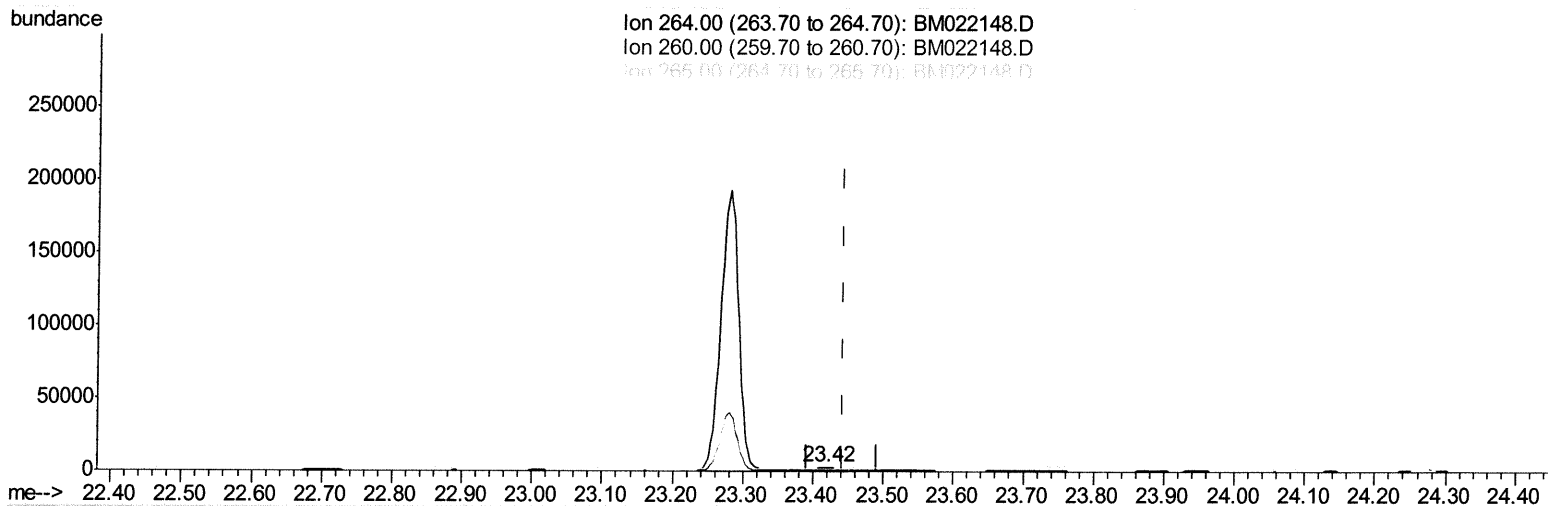

(20) Perylene-d12 (I)

23.419min (-0.024) 0.40ng/ul m

JU
 08/20/19

response 4161

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	34.23#
265.00	117.00	73.85#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:21:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

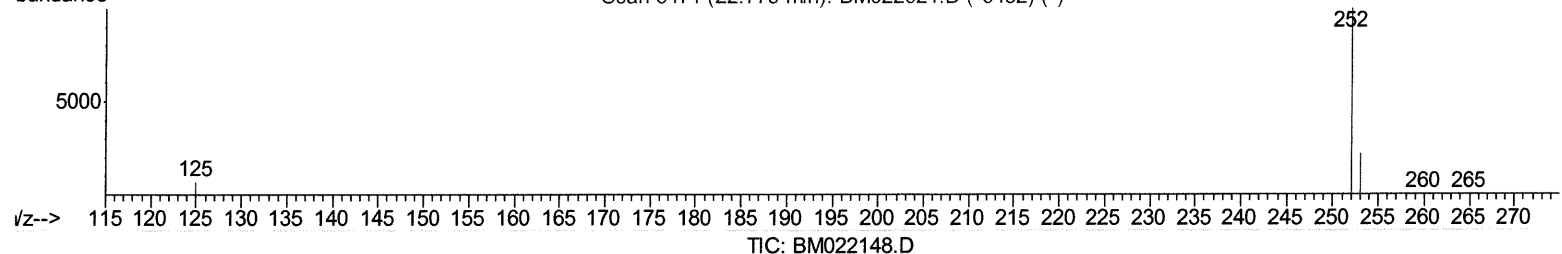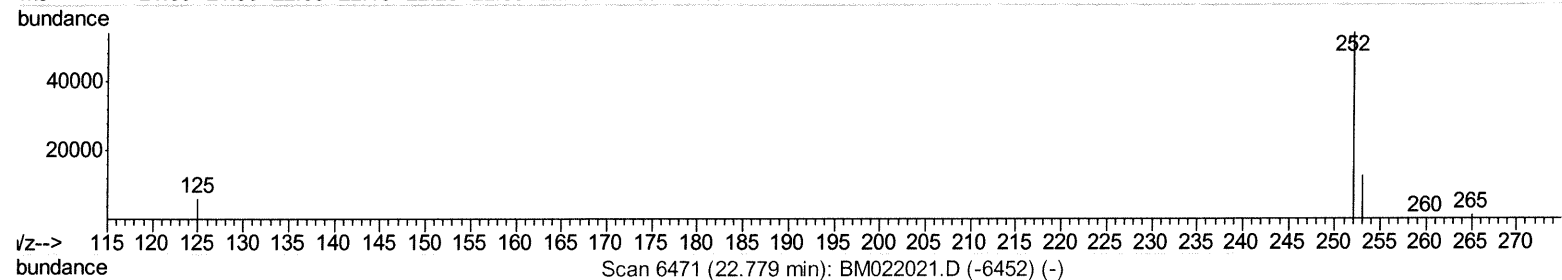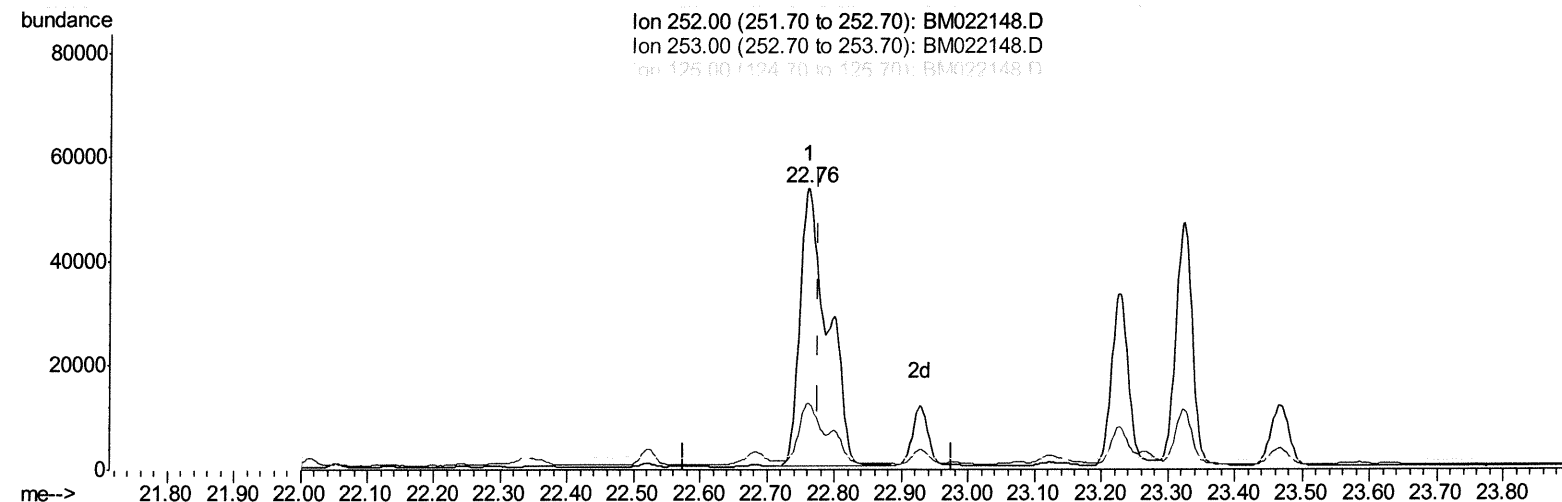

(21) Benzo(b)fluoranthene

22.760min (-0.017) 10.94ng/ul

response 153448

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.87
125.00	15.50	11.44
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:21:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

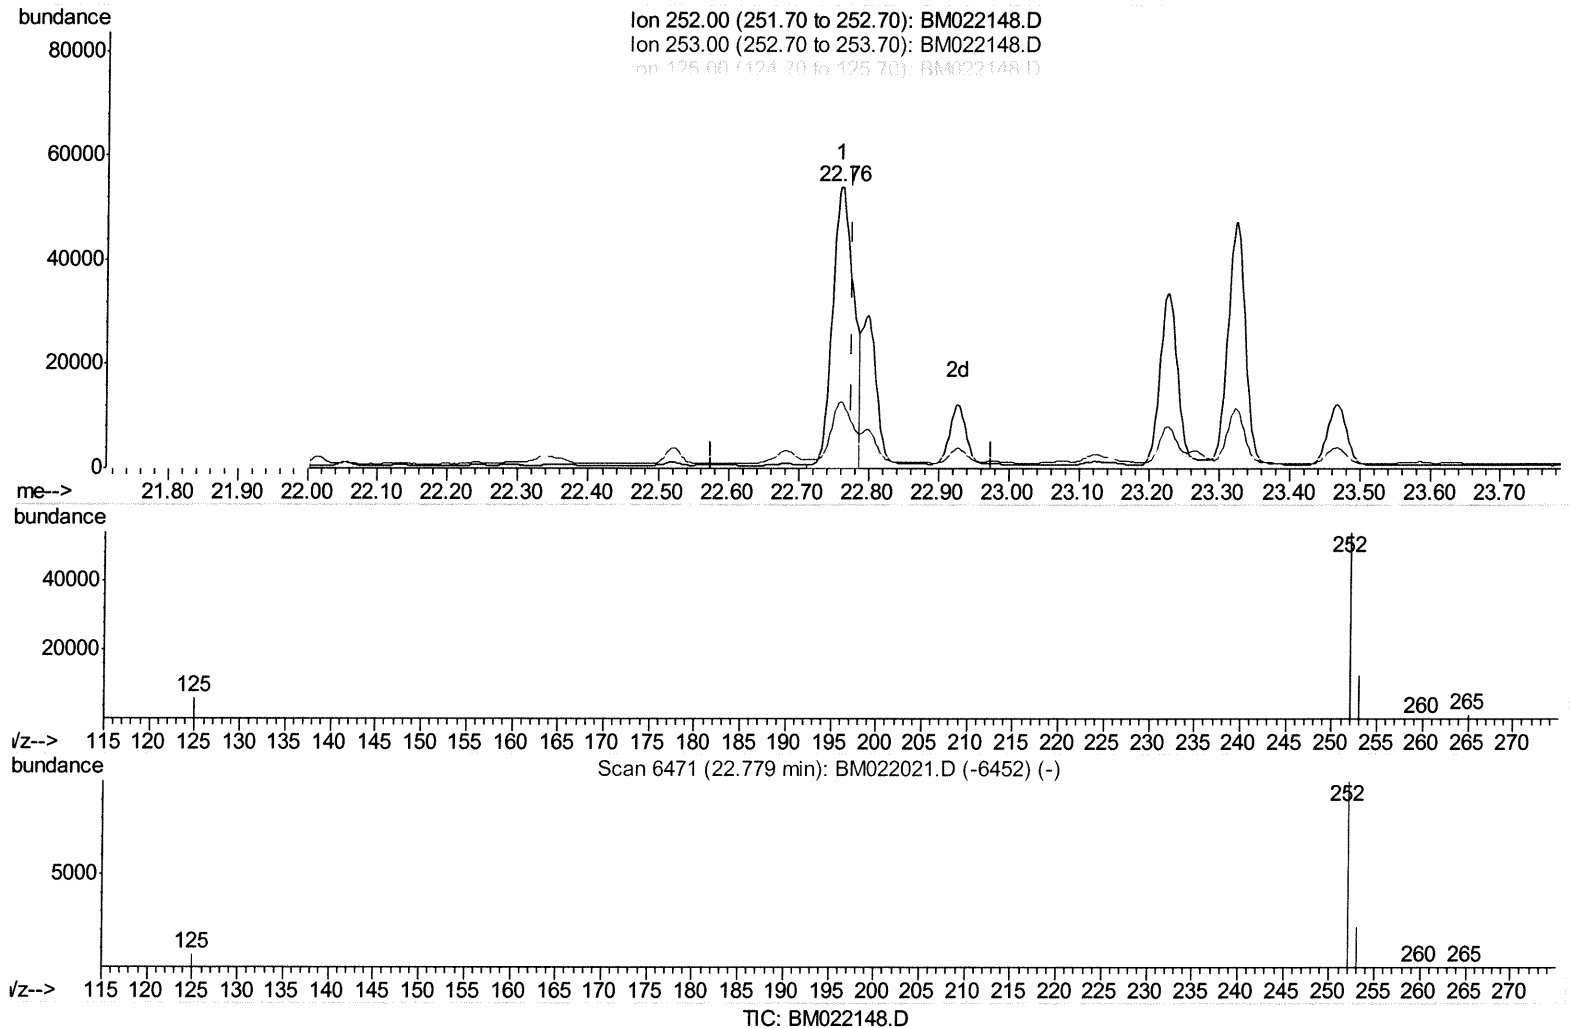

(21) Benzo(b)fluoranthene

22.760min (-0.017) 8.05ng/ul m

JU 8/20/19

response 113014

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.87
125.00	15.50	11.44
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:21:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

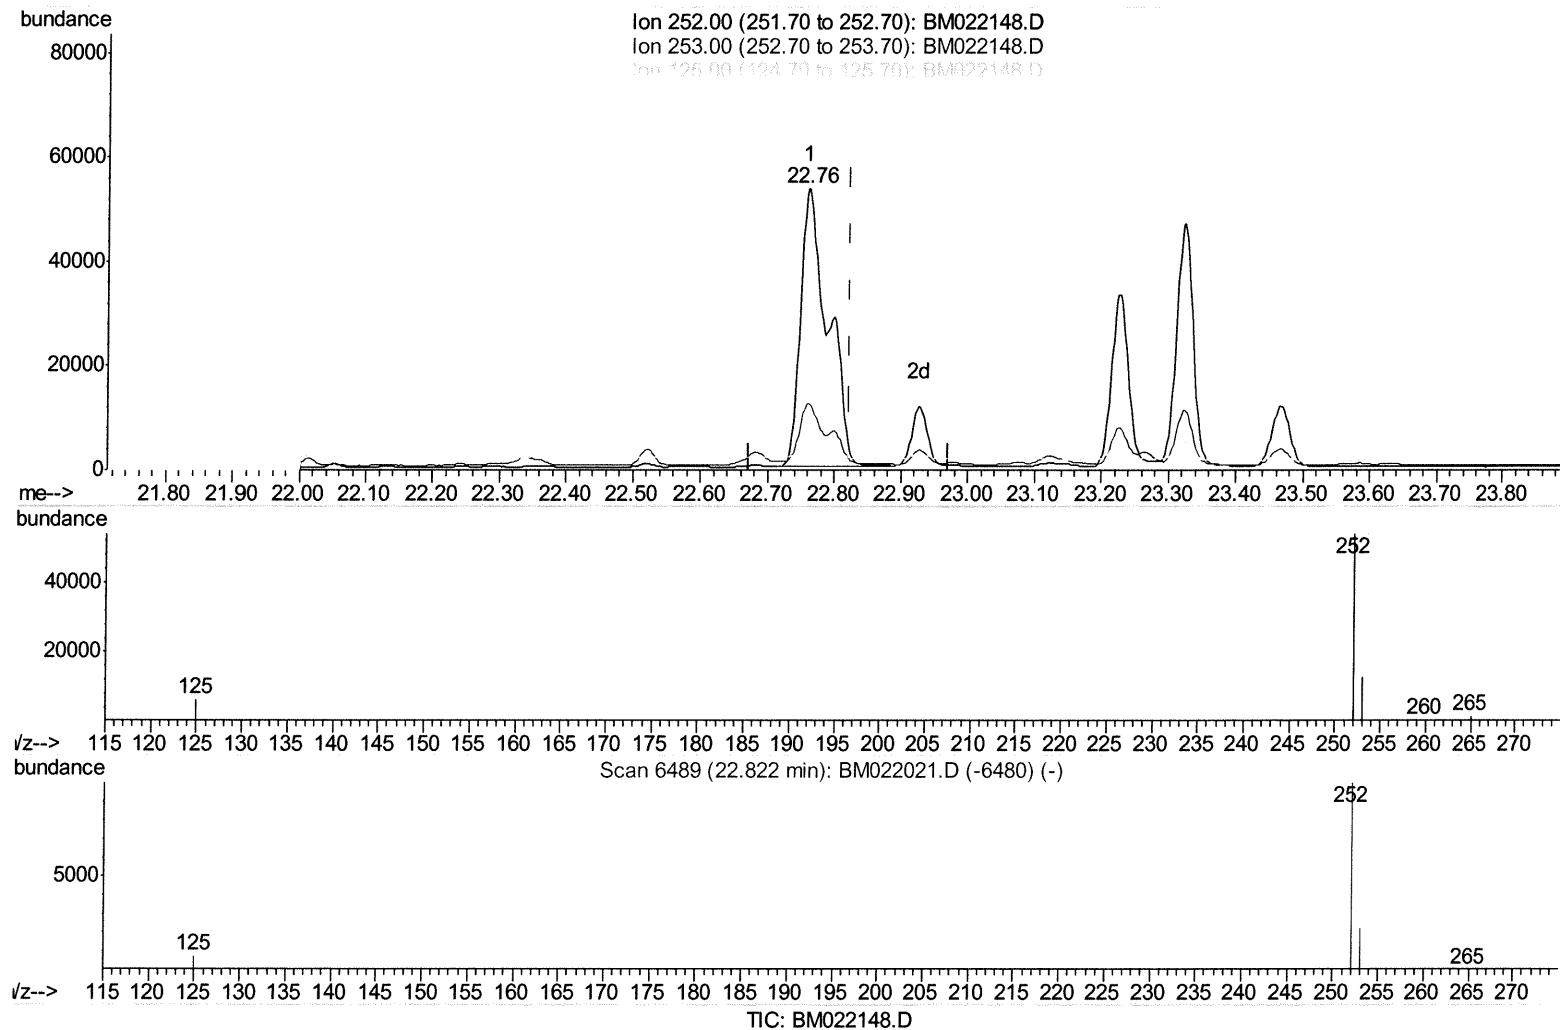

(22) Benzo(k)fluoranthene

22.760min (-0.063) 9.66ng/ul

response 153448

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.87#
125.00	15.20	11.44#
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Quant Time: Aug 16 14:21:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

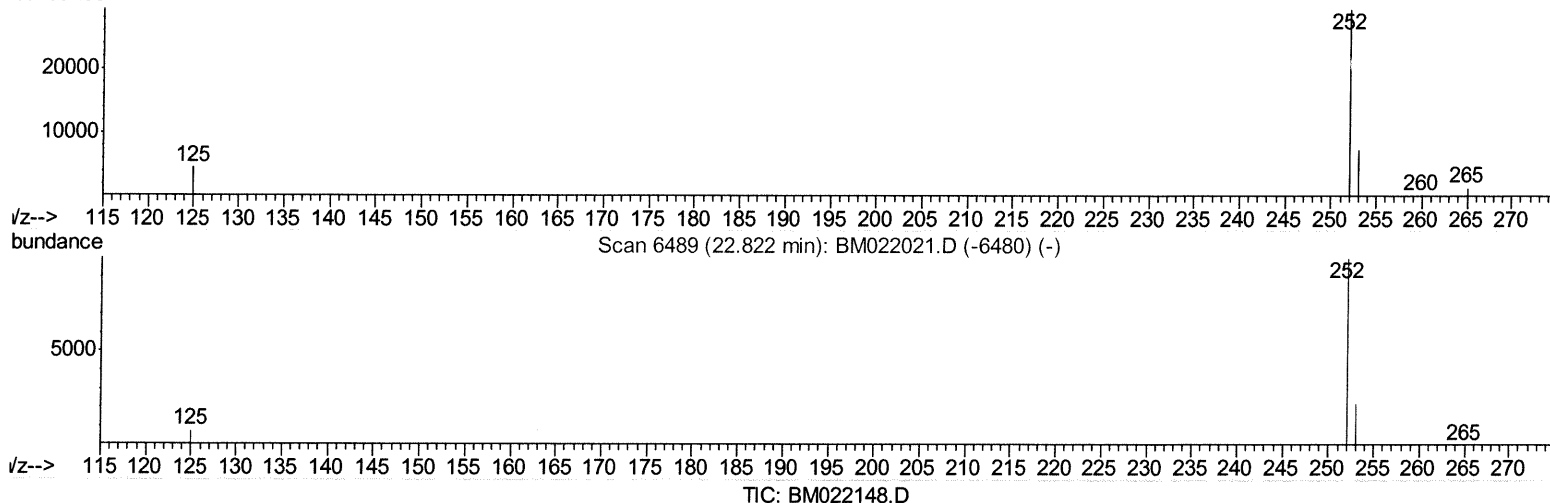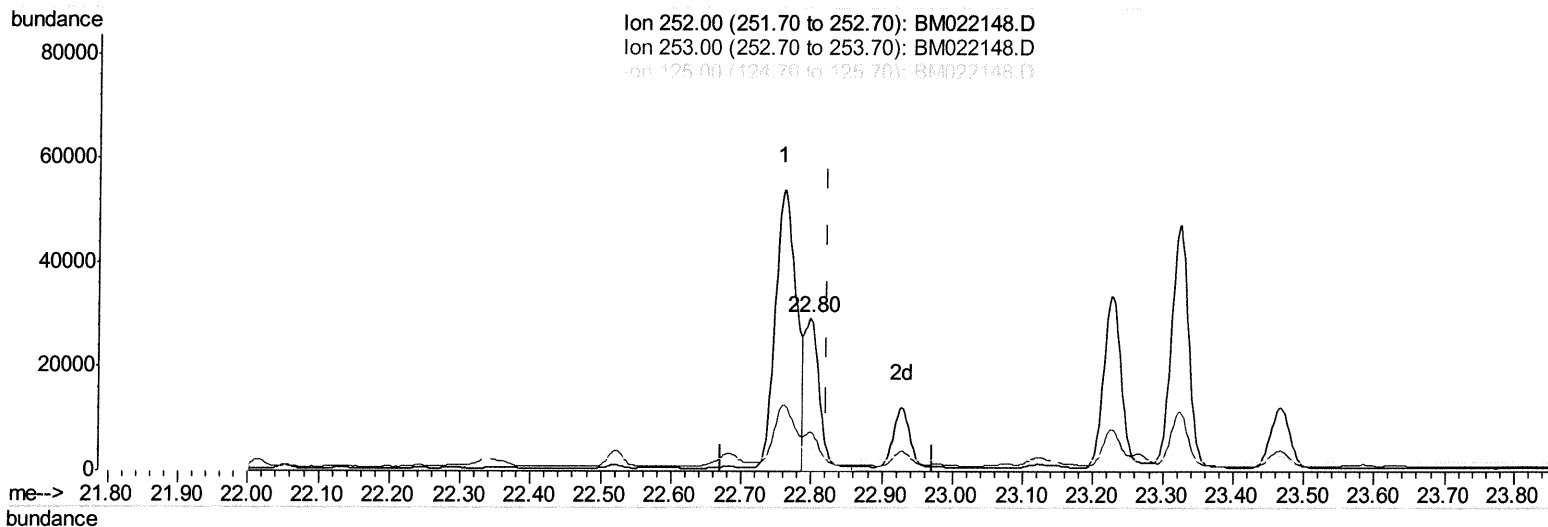

(22) Benzo(k)fluoranthene

22.798min (-0.024) 2.88ng/ul m

JU
 08/20/19

response 45698

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.51#
125.00	15.20	15.54
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081519\
 Data File : BM022148.D
 Acq On : 15 Aug 2019 17:56
 Operator : HP/JU
 Sample : K4242-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 16 14:24:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

mohammad
 8/19/2019 10:45:35 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	619	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.37	136	2625	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.25	164	1516	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.01	188	3811m?	0.40	ng/ul	-0.03
16) Chrysene-d12	21.21	240	3889m?	0.40	ng/ul	-0.02
20) Perylene-d12	23.42	264	4161m?	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.98	152	1447	0.33	ng/ul	-0.02
14) Fluoranthene-d10	19.04	212	4586m?	0.36	ng/ul	-0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.42	128	1028	0.139	ng/ul#	92
5) 2-Methylnaphthalene	12.06	142	945	0.191	ng/ul	96
7) Acenaphthylene	13.97	152	6338	0.896	ng/ul#	82
8) Acenaphthene	14.31	153	1857	0.321	ng/ul	96
9) Fluorene	15.31	166	1981	0.308	ng/ul	99
12) Phenanthrene	17.05	178	42331m?	3.817	ng/ul	
13) Anthracene	17.14	178	14224m?	1.504	ng/ul	
15) Fluoranthene	19.07	202	131427m?	8.848	ng/ul	
17) Pyrene	19.44	202	122411	7.660	ng/ul	98
18) Benzo(a)anthracene	21.20	228	78615	5.651	ng/ul	99
19) Chrysene	21.25	228	77636	4.340	ng/ul	98
21) Benzo(b)fluoranthene	22.76	252	113014m?	8.054	ng/ul	
22) Benzo(k)fluoranthene	22.80	252	45698m?	2.878	ng/ul	
23) Benzo(a)pyrene	23.32	252	80826	5.664	ng/ul#	78
24) Indeno(1,2,3-cd)pyrene	25.62	276	60112	3.528	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.63	278	15148	1.100	ng/ul#	94
26) Benzo(g,h,i)perylene	26.30	276	53851	3.511	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 08/20/19