


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081519\
Data File : BM022146.D
Acq On : 15 Aug 2019 16:43
Operator : HP/JU
Sample : DFTPP04
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP04

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 19 04:47:53 2019

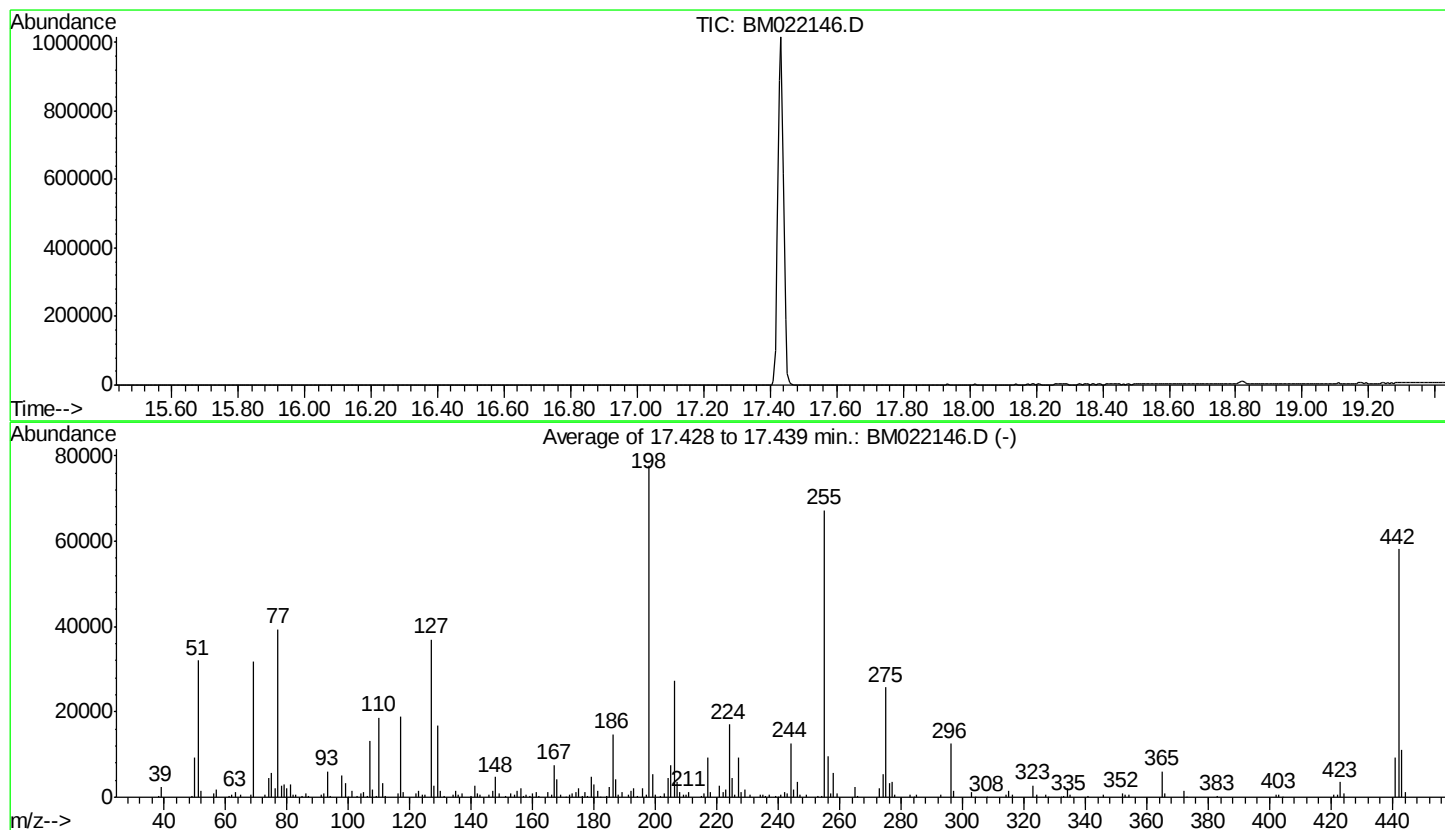

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	32005	PASS
68	69	0.00	2	1.9	606	PASS
69	198	0.00	100	41.1	31885	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	36938	PASS
197	198	0.00	2	0.7	524	PASS
198	198	100	100	100.0	77664	PASS
199	198	5	9	6.9	5358	PASS
275	198	10	60	33.1	25709	PASS
365	198	1	100	7.8	6081	PASS
441	198	0.01	100	11.9	9279	PASS
442	198	50	100	74.8	58112	PASS
443	442	15	24	19.1	11087	PASS

m/z	Abundance
38.00	610.0
39.00	2999.0
44.00	363.0
49.00	438.0
50.00	10779.0
51.00	39336.0
52.00	1807.0
55.90	1034.0
57.00	2243.0
61.00	516.0
62.00	692.0
63.00	1348.0
65.00	656.0
68.00	698.0
69.00	38168.0
72.90	667.0
74.00	4933.0
75.00	6759.0
76.00	2541.0
77.00	46160.0
78.00	3403.0
79.00	3722.0
80.00	2598.0
81.00	3305.0
82.00	889.0
82.90	724.0
84.90	495.0
85.90	1116.0
86.90	606.0
90.90	692.0
92.00	893.0
93.00	7128.0
94.00	366.0
98.00	6080.0
99.00	4040.0
101.00	1839.0
102.90	497.0
104.00	1342.0
105.00	1443.0
106.00	352.0
107.00	14368.0
108.00	2144.0
109.00	369.0
110.00	22136.0
111.00	3843.0
112.00	425.0
115.90	1062.0
117.00	21304.0
118.00	1587.0
122.00	991.0
123.00	1576.0
123.90	934.0
124.90	702.0
127.00	41608.0
128.00	3108.0
129.00	19528.0
130.00	1474.0
131.00	421.0
133.90	687.0
135.00	1643.0
135.90	643.0
137.00	1050.0
139.90	378.0
141.00	3049.0
141.90	900.0
142.90	606.0
145.90	595.0
147.00	1803.0
148.00	5370.0
149.00	1021.0
150.90	322.0
152.90	894.0
154.00	905.0
155.00	1786.0
156.00	2545.0
157.00	318.0
158.00	641.0
158.90	435.0
159.90	876.0
161.00	1304.0
161.90	470.0
165.00	1215.0
166.00	760.0
167.00	8003.0
168.00	4662.0
168.90	684.0
171.90	527.0
172.90	791.0
173.90	1186.0
175.00	2591.0
175.90	474.0
177.00	1267.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

177.90	508.0
178.90	5161.0
180.00	3247.0
181.00	1521.0
182.00	324.0
183.90	436.0
184.90	2668.0
186.00	15516.0
187.00	4436.0
188.00	614.0
188.90	1253.0
190.90	756.0
191.90	1558.0
193.00	1958.0
194.00	359.0
195.90	2149.0
197.00	617.0
197.90	82960.0
198.90	6169.0
200.00	524.0
201.60	320.0
202.90	1047.0
204.00	4830.0
205.00	7784.0
206.00	28064.0
207.00	4245.0
208.00	1232.0
209.00	563.0
210.00	597.0
211.00	1255.0
214.90	428.0
215.90	855.0
217.00	9654.0
217.90	1194.0
221.00	2696.0
221.90	988.0
223.00	2100.0
224.00	17152.0
225.00	4622.0
226.00	671.0
227.00	9639.0
228.00	1310.0
228.90	1856.0
231.00	543.0
233.90	529.0
234.90	720.0
235.90	472.0
237.00	830.0
238.90	386.0
241.00	372.0
242.00	1147.0
243.00	1005.0
244.00	12943.0
245.00	1636.0
246.00	3502.0
246.90	620.0
249.00	472.0
253.00	367.0
254.10	402.0
255.00	68120.0
256.00	9473.0
256.90	1000.0
258.00	5782.0
258.90	785.0
264.90	2383.0
265.90	344.0
273.00	2004.0
274.00	4943.0
275.00	25320.0
276.00	3364.0
276.90	3664.0
277.90	712.0
282.90	515.0
284.00	379.0
284.90	561.0
293.00	733.0
296.00	12111.0
297.00	1620.0
303.00	1259.0
314.00	395.0
314.90	1267.0
316.10	553.0
323.00	2340.0
324.00	399.0
326.90	594.0
334.00	1723.0
334.90	497.0
340.90	325.0
346.00	689.0
352.00	944.0
353.00	524.0
354.00	682.0
365.00	5100.0
365.90	780.0
372.00	1184.0
382.90	364.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

m/z	Abundance
38.00	500.0
39.00	3026.0
43.90	414.0
49.00	379.0
50.00	11261.0
51.00	37152.0
52.00	1969.0
56.00	1130.0
57.00	2159.0
61.00	448.0
61.90	574.0
63.00	1712.0
64.90	647.0
67.90	795.0
69.00	37560.0
73.00	612.0
74.00	5221.0
75.00	6851.0
76.00	2581.0
77.00	46264.0
78.00	3282.0
79.00	3298.0
80.00	2702.0
81.00	3736.0
81.90	828.0
83.00	610.0
85.00	467.0
86.00	1024.0
86.90	537.0
91.00	696.0
91.90	1041.0
93.00	7398.0
93.90	415.0
98.00	5699.0
99.00	3990.0
100.00	345.0
101.00	1737.0
102.90	493.0
104.00	1109.0
105.00	1408.0
106.00	417.0
107.00	16123.0
107.90	2103.0
108.90	386.0
110.00	21680.0
111.00	3702.0
112.00	464.0
116.00	846.0
117.00	22984.0
118.00	1279.0
122.00	1230.0
123.00	1568.0
123.90	748.0
124.90	606.0
127.00	42992.0
128.00	3333.0
129.00	19808.0
130.00	1901.0
131.00	323.0
133.90	726.0
135.00	1520.0
136.00	659.0
137.10	1144.0
140.00	334.0
140.90	3777.0
142.00	1001.0
142.90	802.0
145.90	606.0
147.00	1718.0
148.00	5510.0
148.90	811.0
151.00	371.0
153.00	961.0
153.90	648.0
155.00	1935.0
156.00	2696.0
157.00	377.0
157.90	478.0
158.90	434.0
160.00	1144.0
161.00	1531.0
162.00	386.0
164.90	1328.0
166.00	963.0
167.00	9273.0
168.00	4652.0
168.90	617.0
170.80	331.0
171.90	674.0
173.00	1091.0
174.00	1344.0
175.00	2556.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

175.90	557.0
176.90	1524.0
177.90	531.0
179.00	5700.0
179.90	3354.0
181.00	1662.0
184.00	493.0
185.00	2763.0
186.00	18136.0
187.00	5308.0
188.00	653.0
188.90	1330.0
191.00	735.0
191.90	1983.0
193.00	2361.0
194.00	537.0
195.90	2619.0
197.00	571.0
197.90	94728.0
198.90	6230.0
199.90	706.0
201.40	303.0
203.00	1000.0
204.00	5251.0
205.00	9498.0
206.00	33528.0
207.00	4877.0
208.00	1687.0
209.00	586.0
209.90	744.0
210.90	1618.0
215.00	468.0
215.90	913.0
216.90	11070.0
217.90	1394.0
220.90	3101.0
221.80	1366.0
222.90	2259.0
224.00	21256.0
225.00	5375.0
225.90	517.0
227.00	11285.0
227.90	1596.0
228.90	2263.0
231.00	706.0
234.00	813.0
234.90	670.0
235.90	499.0
236.90	795.0
238.90	425.0
240.00	316.0
241.00	694.0
241.90	1275.0
243.00	1360.0
244.00	14905.0
245.00	2093.0
246.00	4619.0
246.90	734.0
249.00	542.0
253.00	417.0
254.00	526.0
255.00	82008.0
256.00	11256.0
256.90	1049.0
258.00	7356.0
258.90	1181.0
265.00	2962.0
266.00	402.0
272.90	2479.0
274.00	6959.0
275.00	31160.0
276.00	4178.0
276.90	4332.0
277.90	765.0
283.00	599.0
285.00	681.0
293.00	942.0
296.00	15109.0
297.00	2030.0
303.00	1451.0
303.90	349.0
308.00	300.0
314.00	674.0
315.00	1798.0
316.00	793.0
323.00	3531.0
324.00	875.0
326.90	980.0
328.00	386.0
331.90	323.0
333.00	362.0
334.00	2676.0
335.00	719.0
341.00	453.0
345.90	911.0
352.00	1094.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

352.90	629.0
354.00	980.0
365.00	7622.0
365.90	1047.0
372.00	1684.0
372.90	357.0
383.00	373.0
402.00	600.0
403.00	730.0
420.90	723.0
422.00	661.0
423.00	4340.0
424.00	1122.0
441.00	11205.0
442.00	71920.0
443.00	14009.0
444.00	1378.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

401.90	403.0
402.90	614.0
420.90	513.0
421.90	551.0
423.00	3061.0
424.10	758.0
441.00	7566.0
442.00	46608.0
443.00	9504.0
444.00	810.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

m/z	Abundance
39.00	1389.0
43.90	482.0
50.00	5640.0
51.00	19528.0
52.00	1036.0
55.90	638.0
57.00	1168.0
61.90	425.0
63.00	822.0
65.10	379.0
68.10	326.0
69.00	19928.0
73.00	505.0
74.00	3043.0
75.00	3473.0
76.00	1412.0
77.00	25552.0
78.00	1744.0
79.00	1844.0
80.00	1336.0
81.00	2207.0
81.90	492.0
83.00	375.0
85.00	375.0
86.00	582.0
90.90	339.0
92.00	498.0
93.00	3770.0
98.00	3387.0
99.00	2141.0
100.90	1091.0
103.00	369.0
104.00	639.0
105.00	784.0
107.00	8782.0
108.00	1272.0
110.00	11967.0
111.00	1954.0
112.00	316.0
115.90	519.0
117.00	12001.0
117.90	652.0
122.00	772.0
122.90	993.0
123.90	319.0
125.00	441.0
127.00	26216.0
128.00	2050.0
129.00	11328.0
129.90	922.0
133.90	355.0
134.90	1077.0
135.80	476.0
136.90	595.0
141.00	1638.0
142.00	548.0
142.80	354.0
145.90	307.0
147.00	1243.0
147.90	3392.0
148.90	572.0
152.90	737.0
154.00	552.0
155.00	1117.0
156.00	1358.0
158.00	301.0
158.90	430.0
160.00	575.0
161.00	747.0
164.90	937.0
165.90	544.0
167.00	5386.0
168.00	3006.0
168.80	314.0
171.90	315.0
172.90	512.0
174.00	932.0
175.00	1541.0
176.00	346.0
176.90	712.0
178.00	310.0
178.90	3361.0
180.00	2199.0
181.00	1056.0
185.00	1485.0
186.00	10633.0
187.00	3053.0
188.00	342.0
188.90	902.0
190.90	471.0
191.90	1206.0
193.00	1567.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

193.90	309.0
195.90	1724.0
197.00	386.0
197.90	55304.0
198.90	3676.0
199.90	438.0
202.90	684.0
204.00	3300.0
205.00	5672.0
206.00	20192.0
207.00	3312.0
208.00	1069.0
208.90	455.0
210.00	315.0
211.00	811.0
215.00	324.0
215.90	779.0
216.90	7270.0
217.90	968.0
221.00	2106.0
221.90	846.0
222.90	1325.0
224.00	12700.0
225.00	3234.0
225.90	362.0
227.00	6600.0
228.00	867.0
229.00	1318.0
230.90	558.0
233.90	464.0
234.90	399.0
236.00	375.0
236.90	590.0
240.90	401.0
242.00	857.0
243.00	800.0
244.00	10115.0
245.00	1271.0
246.00	2703.0
246.90	536.0
249.00	391.0
252.90	377.0
253.90	361.0
255.00	51376.0
256.00	7824.0
257.00	667.0
258.00	4068.0
258.90	726.0
264.90	1818.0
272.90	1648.0
274.00	4426.0
275.00	20648.0
276.00	2793.0
276.90	3056.0
277.90	412.0
282.90	319.0
284.90	392.0
293.00	494.0
296.00	10284.0
297.00	1285.0
303.00	1131.0
314.00	374.0
314.90	1165.0
316.00	580.0
323.00	2331.0
323.90	389.0
326.90	590.0
333.00	300.0
334.00	1567.0
335.00	367.0
340.90	323.0
346.00	665.0
351.90	725.0
352.90	445.0
354.00	592.0
365.00	5523.0
366.00	896.0
372.00	1392.0
382.90	320.0
402.00	566.0
402.90	678.0
404.00	304.0
421.00	547.0
422.00	354.0
423.00	3182.0
424.00	651.0
441.00	9066.0
442.00	55808.0
443.00	9748.0
444.00	1088.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04

Scan 2449 (17.392 min): BM022146.D
DFTPP04

m/z	Abundance
43.90	591.0
206.90	583.0

Instrument :
BNA_M
ClientSampleId :
DFTPP04