
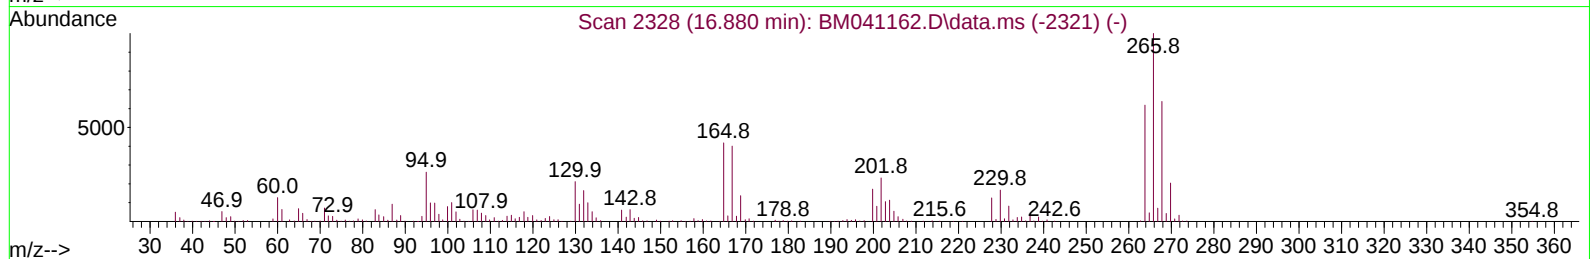
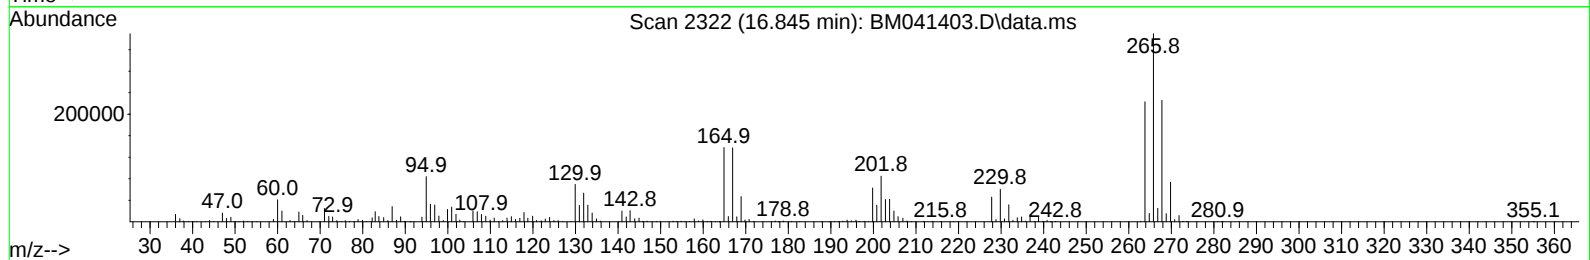


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081523\
Data File : BM041403.D
Acq On : 15 Aug 2023 12:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 02:04:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 17:51:06 2023
Response via : Initial Calibration

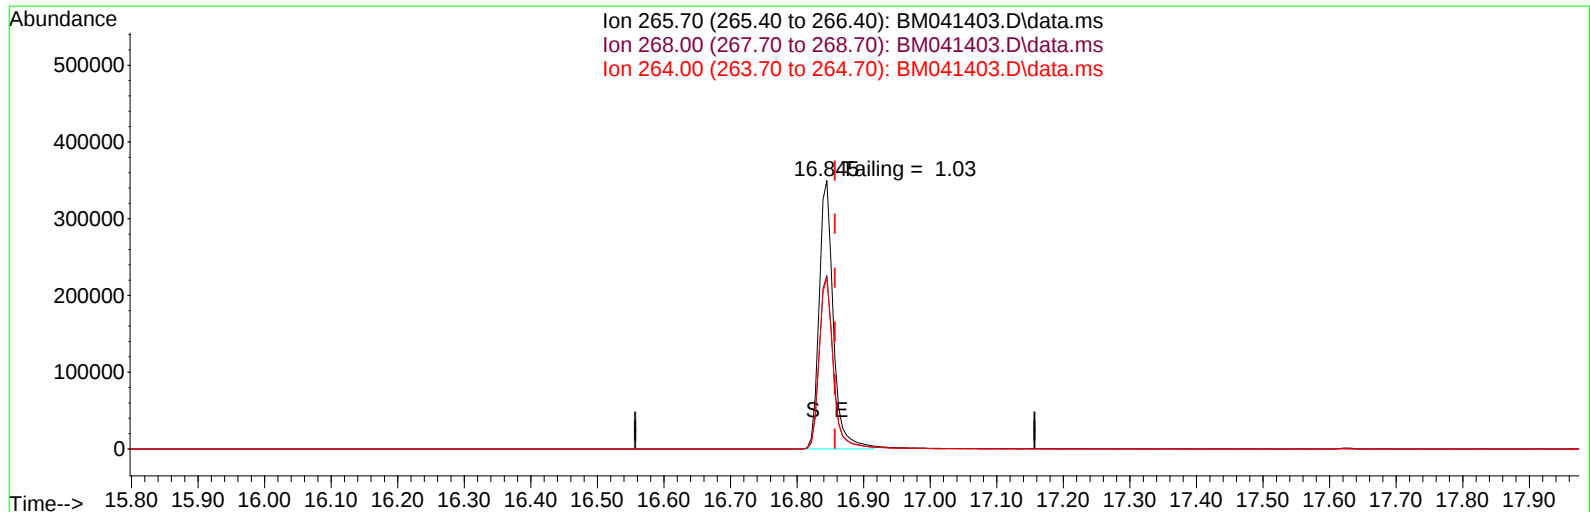

TIC: BM041403.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.012) 0.00 ng

response 523278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.61
264.00	61.80	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081523\
 Data File : BM041403.D
 Acq On : 15 Aug 2023 12:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 02:04:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 17:51:06 2023
 Response via : Initial Calibration

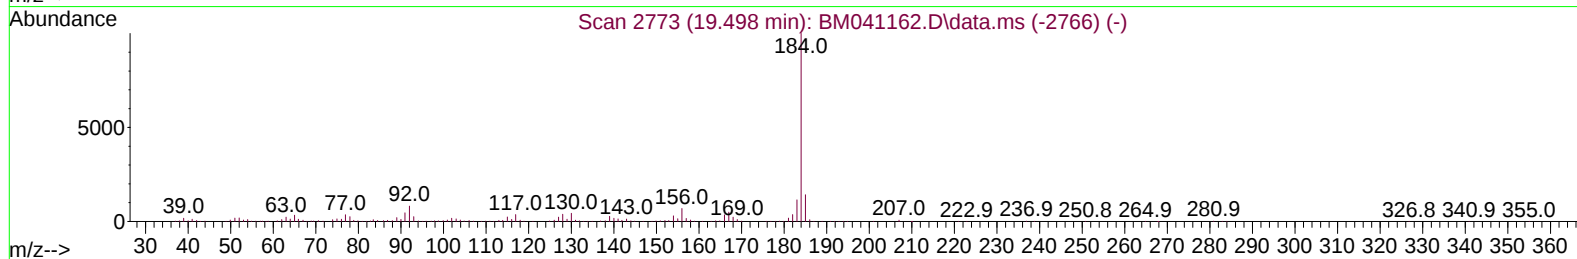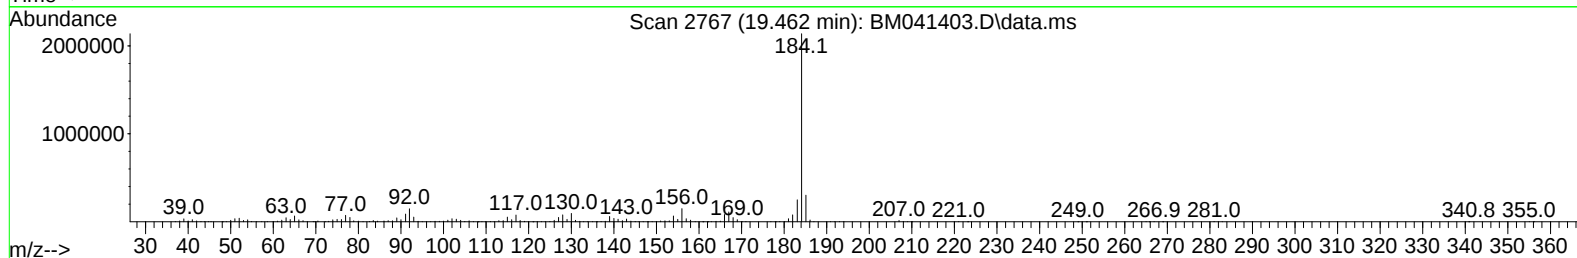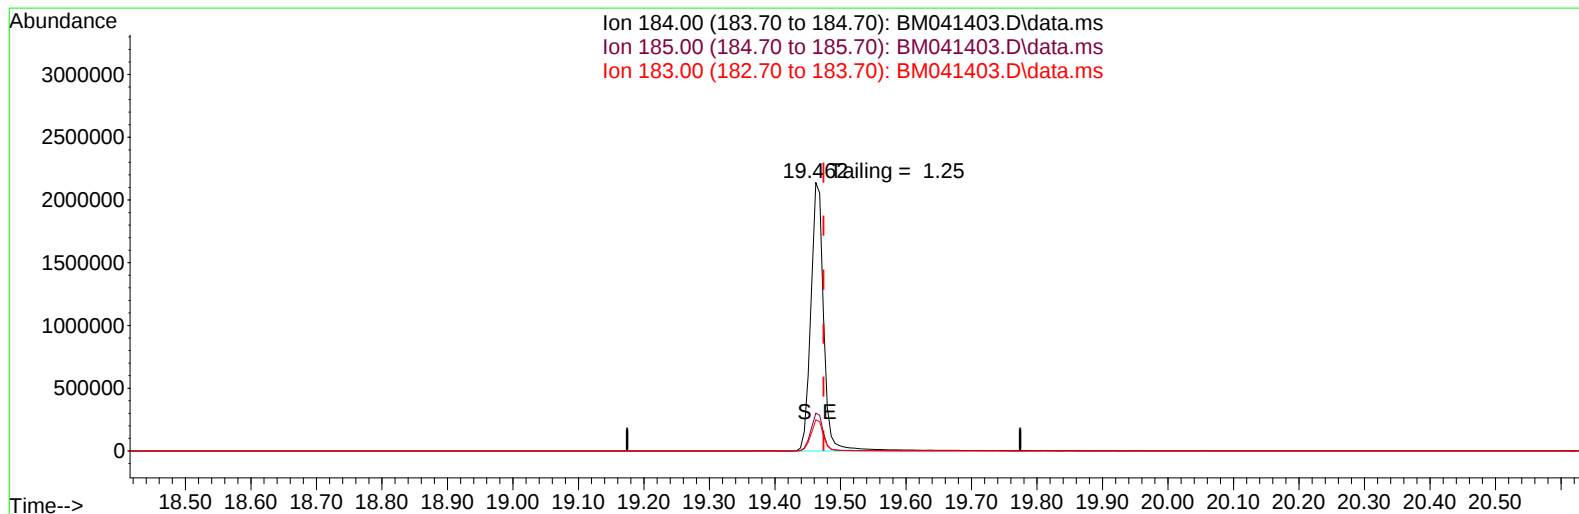

TIC: BM041403.D\data.ms

(77) Benzidine**19.462min (-0.012) 269402.37 ng****response 2922853**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.13
183.00	11.50	11.60
0.00	0.00	0.00