


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081523\
Data File : BM041403.D
Acq On : 15 Aug 2023 12:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 11 17:51:06 2023

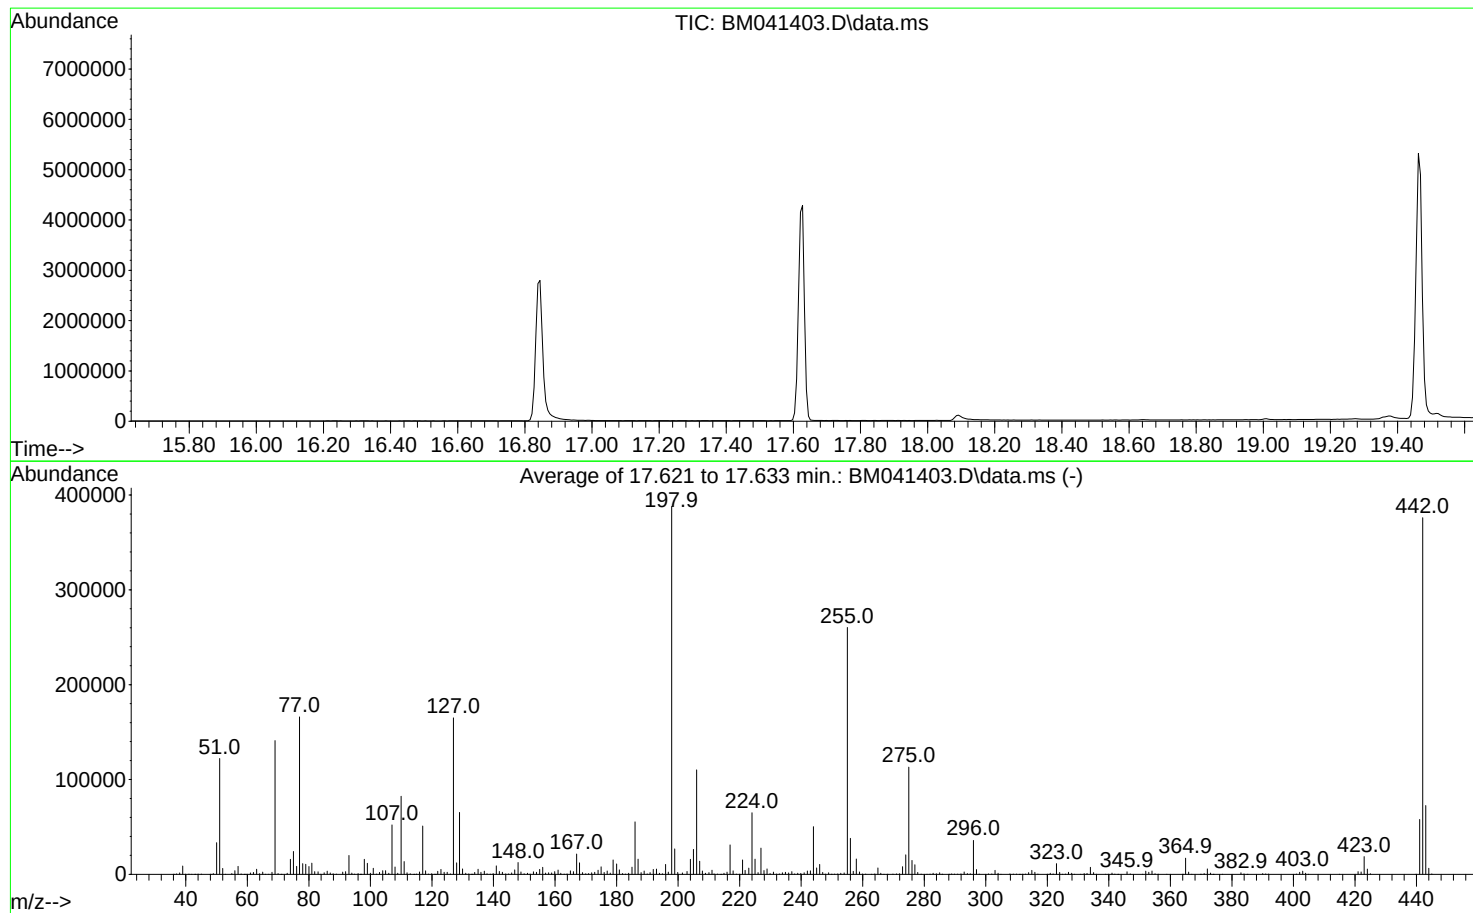




Spectrum Information: Average of 17.621 to 17.633 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	31.5	122139	PASS
68	69	0.00	2	1.5	2158	PASS
69	198	0.00	100	36.4	141021	PASS
70	69	0.00	2	0.6	785	PASS
127	198	10	80	42.5	165037	PASS
197	198	0.00	2	0.6	2381	PASS
198	198	100	100	100.0	387883	PASS
199	198	5	9	6.9	26812	PASS
275	198	10	60	29.2	113104	PASS
365	198	1	100	4.4	17010	PASS
441	198	0.01	100	14.9	57891	PASS
442	442	50	100	100.0	376000	PASS
443	442	15	24	19.3	72523	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081523\
 Data File : BM041403.D
 Acq On : 15 Aug 2023 12:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 16 02:04:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 17:51:06 2023
 Response via : Initial Calibration

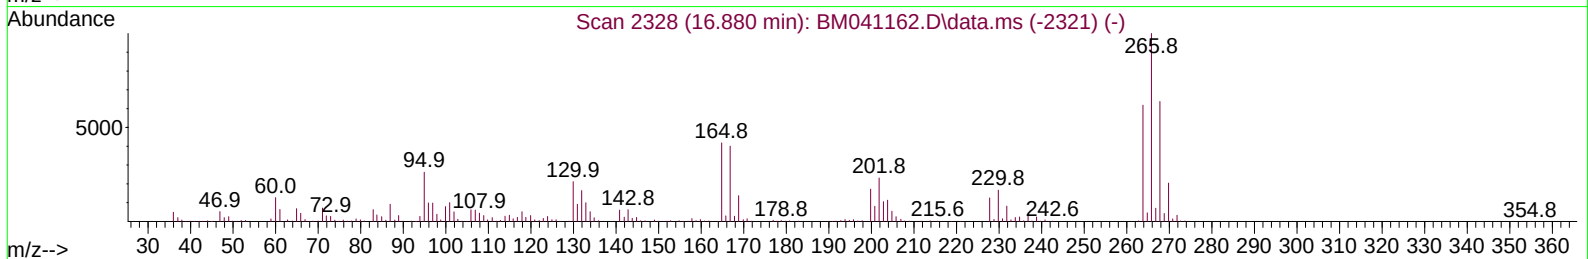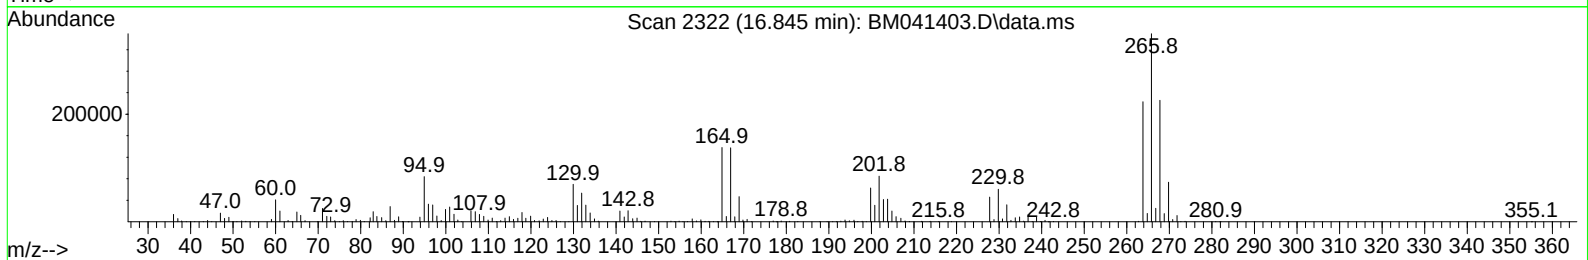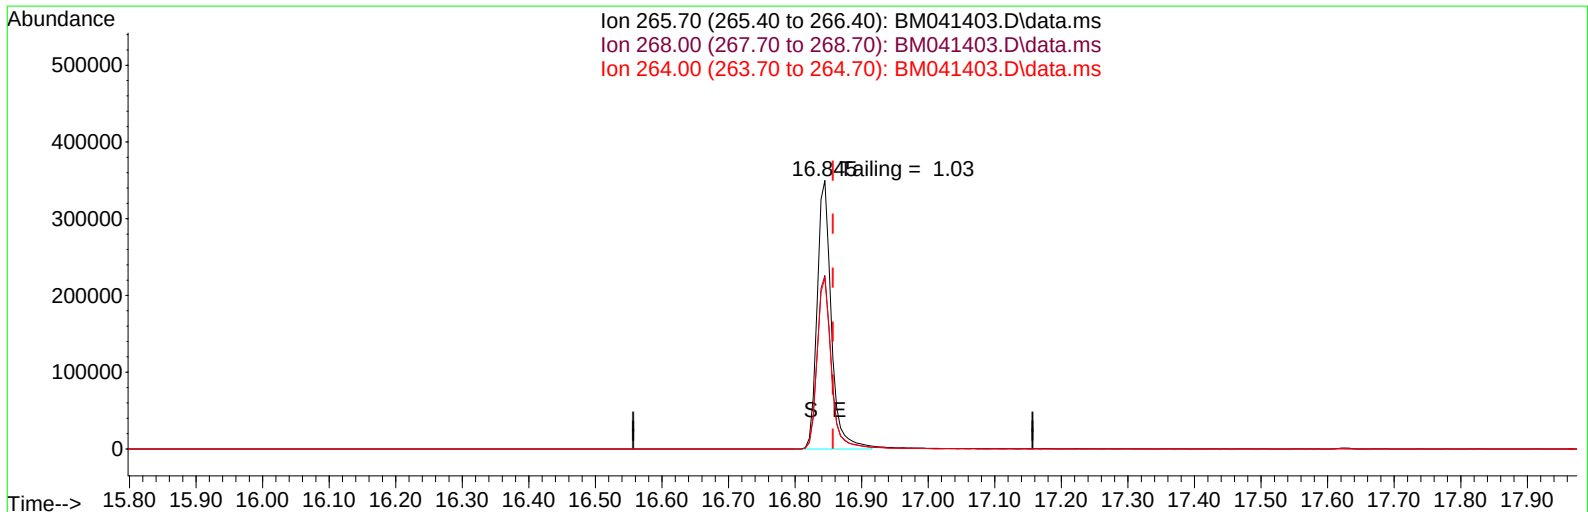

TIC: BM041403.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.012) 0.00 ng




response 523278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.61
264.00	61.80	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081523\
 Data File : BM041403.D
 Acq On : 15 Aug 2023 12:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 16 02:04:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 17:51:06 2023
 Response via : Initial Calibration

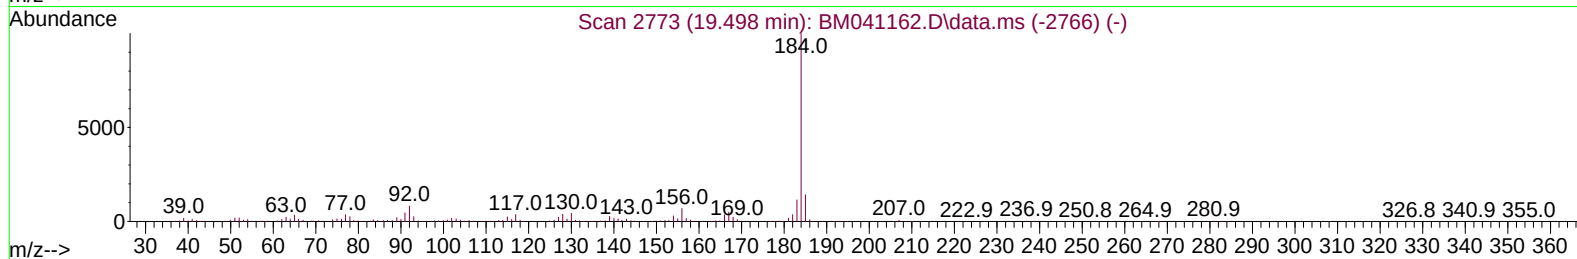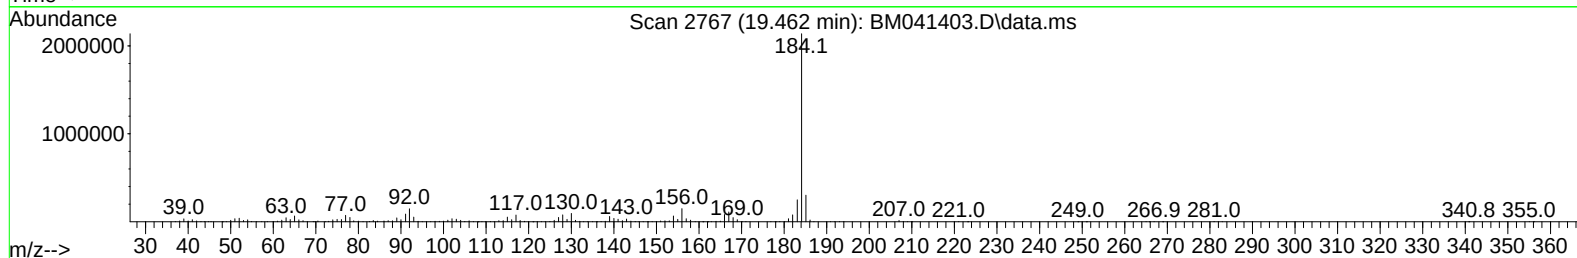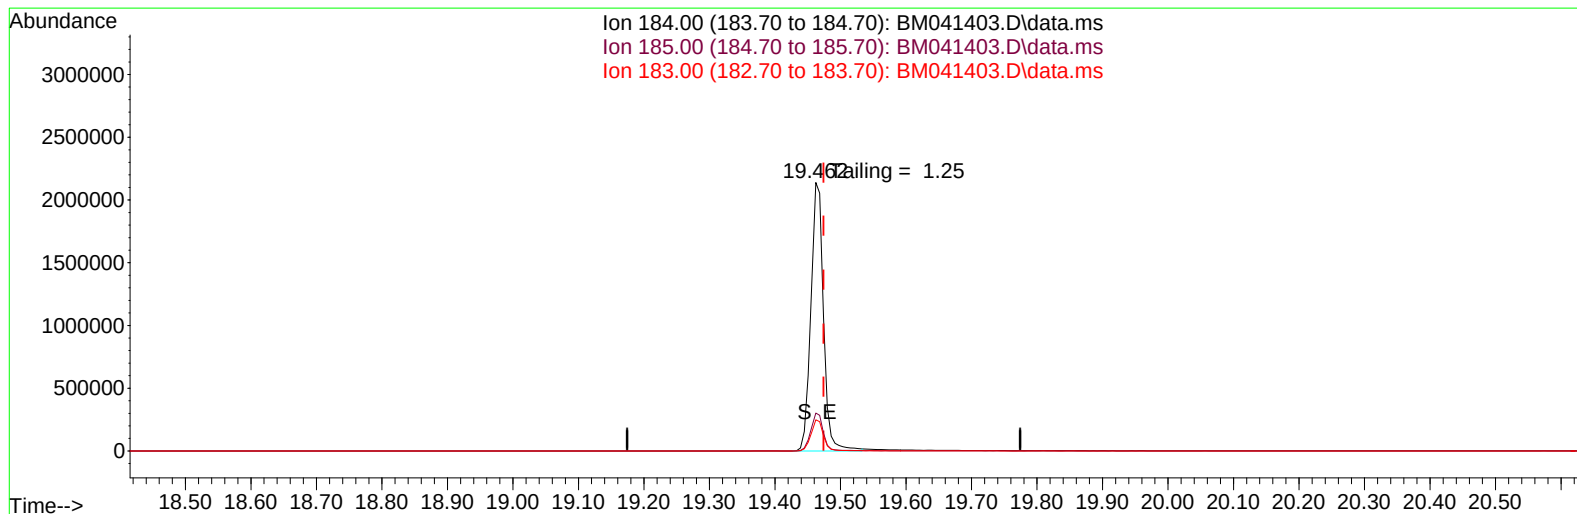

TIC: BM041403.D\data.ms

(77) Benzidine

19.462min (-0.012) 269402.37 ng

response 2922853

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.13
183.00	11.50	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2023	BNA_M	<u>BM041403.D</u>
Compound Name	Response	Retention Time
DDT	1591710	20.686
DDD	22274	20.292
DDE	1922	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24196	1615906	1.50

Instrument :
BNA_M
ClientSampleId :
DFTPP