

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041427.D
Acq On : 16 Aug 2023 17:08
Operator : MA/JU
Sample : PB154844BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154844BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.346	360	367	387	rBV	3685140	5356849	43.62%	10.415%
2	6.951	631	640	657	rBV	3333694	5267071	42.89%	10.240%
3	7.763	770	778	787	rBV	625853	974022	7.93%	1.894%
4	8.945	970	979	996	rBV	1925372	3292667	26.81%	6.402%
5	10.569	1247	1255	1276	rBV	718548	1310554	10.67%	2.548%
6	13.045	1669	1676	1699	rBV	5350203	7746550	63.08%	15.061%
7	14.427	1905	1911	1927	rVB	1174352	1762818	14.35%	3.427%
8	15.927	2160	2166	2187	rBV	4510895	6527656	53.15%	12.691%
9	17.186	2374	2380	2395	rBV	1448513	2135631	17.39%	4.152%
10	19.827	2823	2829	2839	rBV	10464759	12281043	100.00%	23.877%
11	21.392	3090	3095	3107	rBV	1793459	2411403	19.64%	4.688%
12	23.750	3490	3496	3510	rVB	1158807	2369384	19.29%	4.607%




Sum of corrected areas: 51435648

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041427.D
Acq On : 16 Aug 2023 17:08
Operator : MA/JU
Sample : PB154844BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154844BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

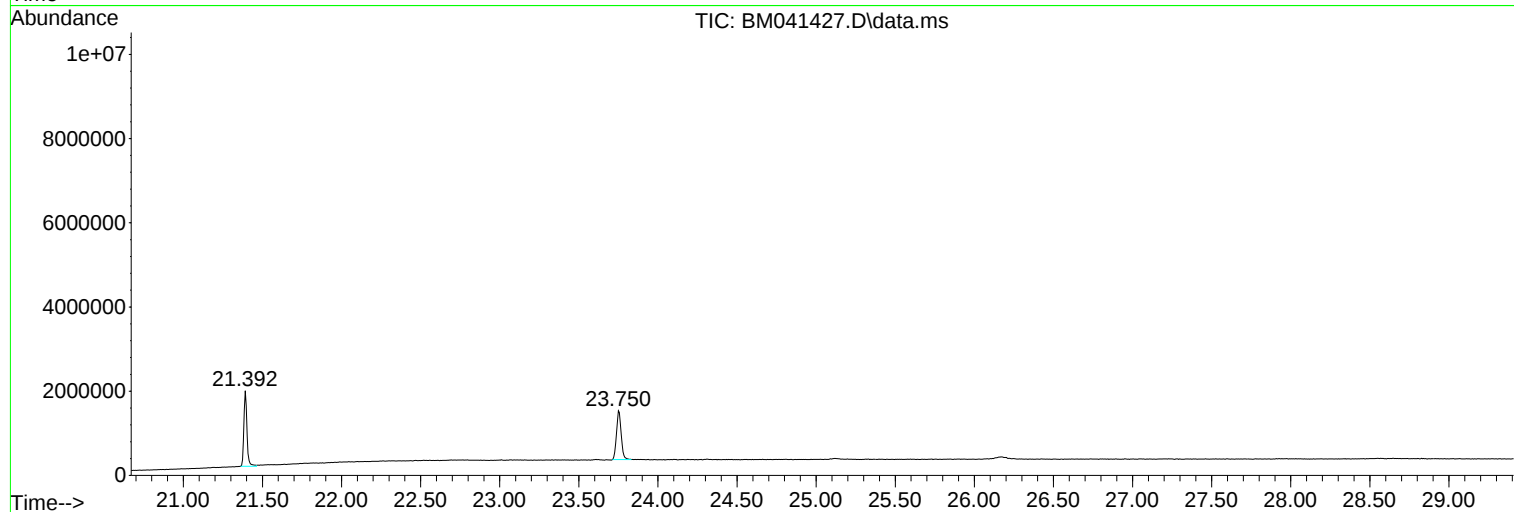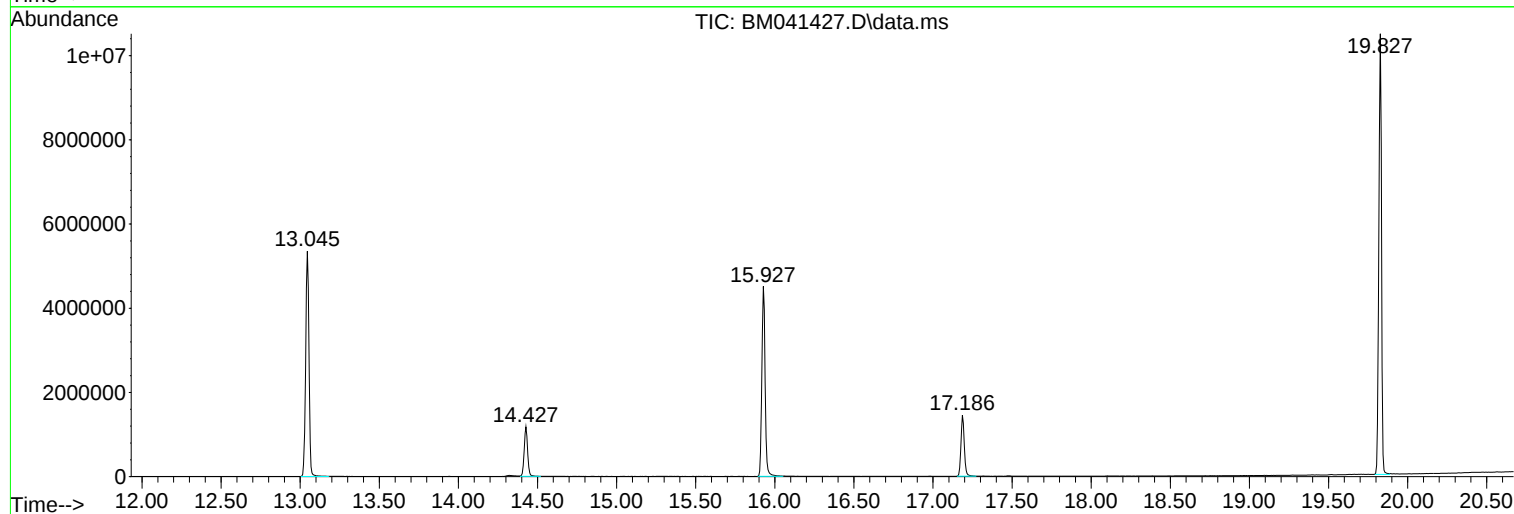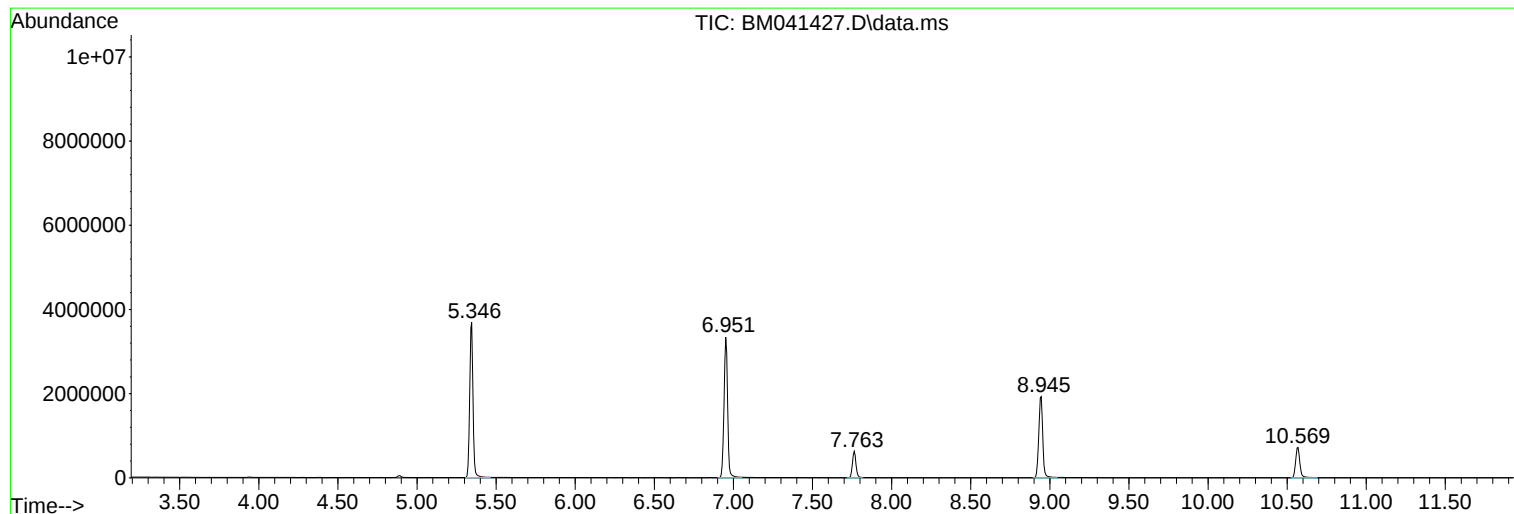

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041427.D
Acq On : 16 Aug 2023 17:08
Operator : MA/JU
Sample : PB154844BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154844BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041427.D
Acq On : 16 Aug 2023 17:08
Operator : MA/JU
Sample : PB154844BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154844BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------