


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041416.D
Acq On : 16 Aug 2023 07:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 17 02:13:45 2023

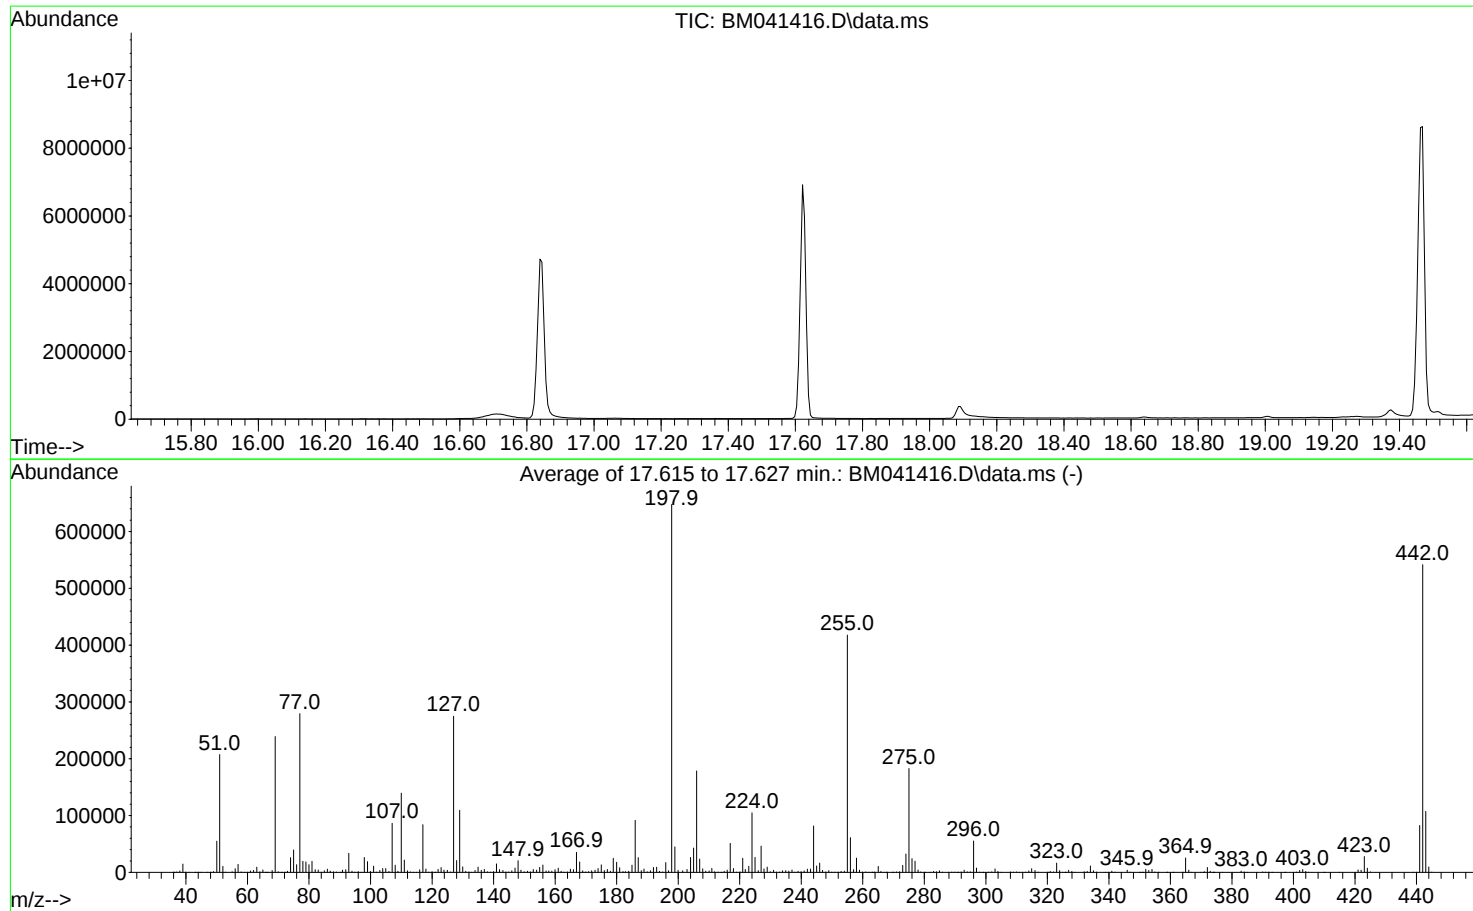




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	207392	PASS
68	69	0.00	2	1.4	3463	PASS
69	198	0.00	100	36.9	239192	PASS
70	69	0.00	2	0.5	1267	PASS
127	198	10	80	42.4	274880	PASS
197	198	0.00	2	0.5	2938	PASS
198	198	100	100	100.0	647573	PASS
199	198	5	9	6.9	44789	PASS
275	198	10	60	28.2	182821	PASS
365	198	1	100	3.9	25392	PASS
441	198	0.01	100	12.8	82621	PASS
442	442	50	100	100.0	541675	PASS
443	442	15	24	19.8	107355	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041416.D
Acq On : 16 Aug 2023 07:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 02:20:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

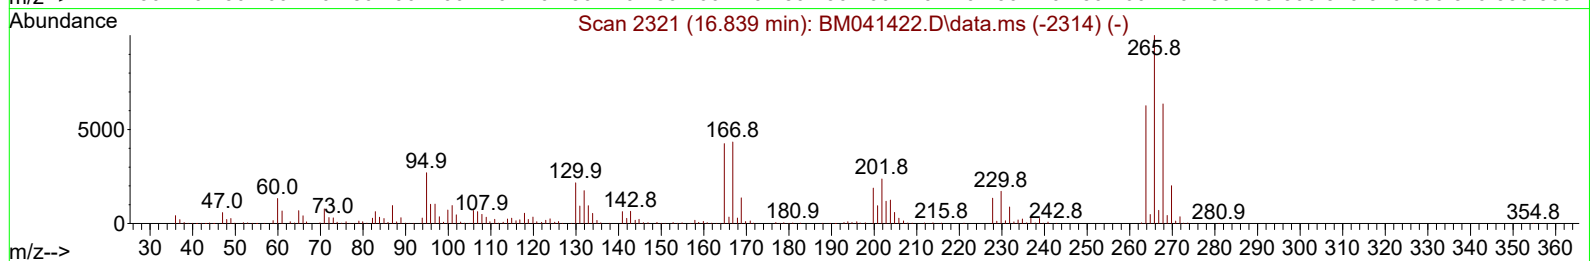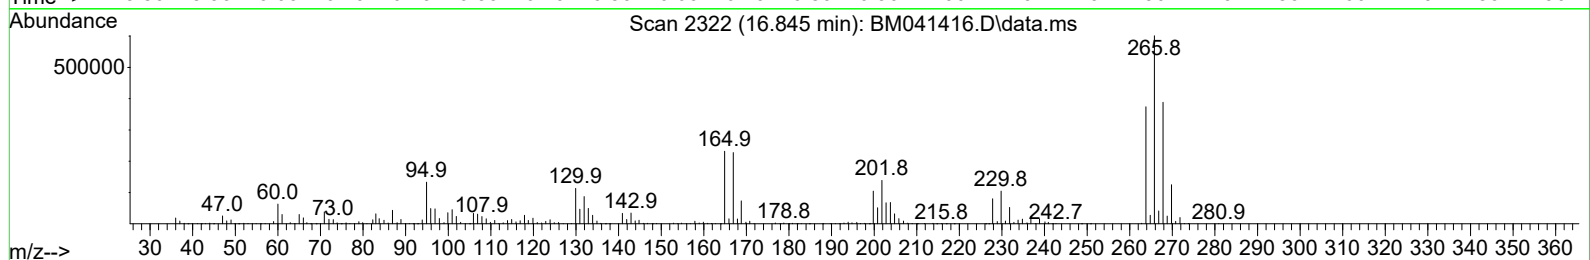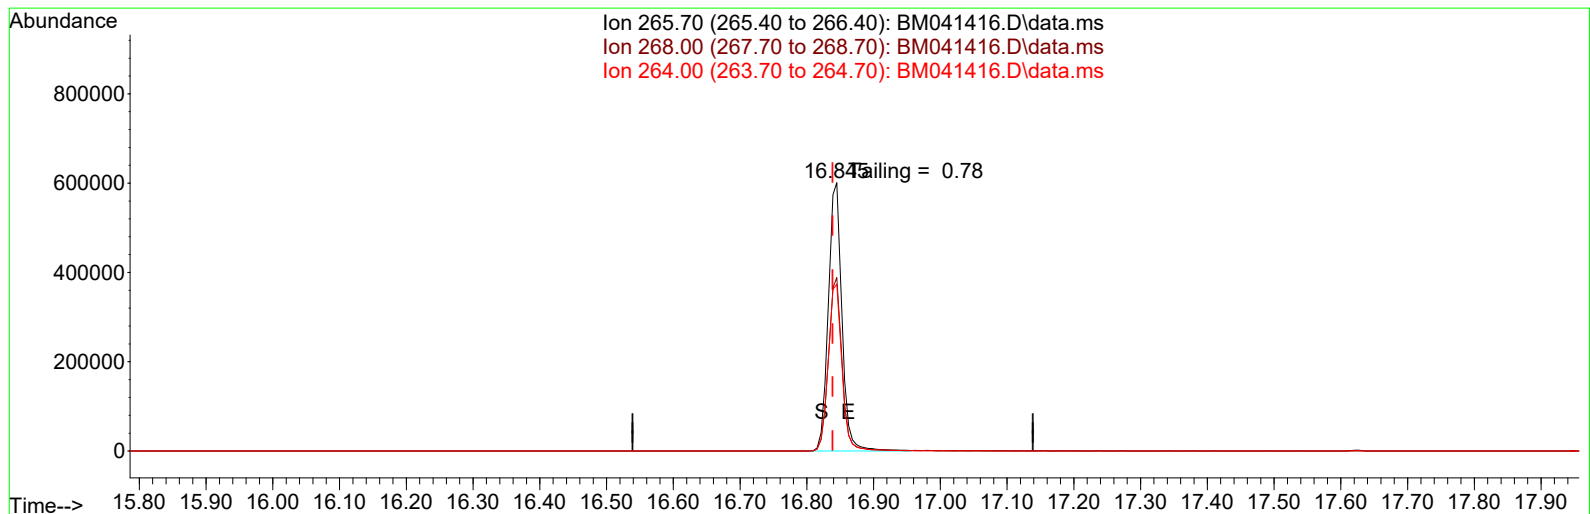

TIC: BM041416.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.006) 0.00 ng




response 854700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.62
264.00	62.70	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081623\
Data File : BM041416.D
Acq On : 16 Aug 2023 07:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 02:20:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

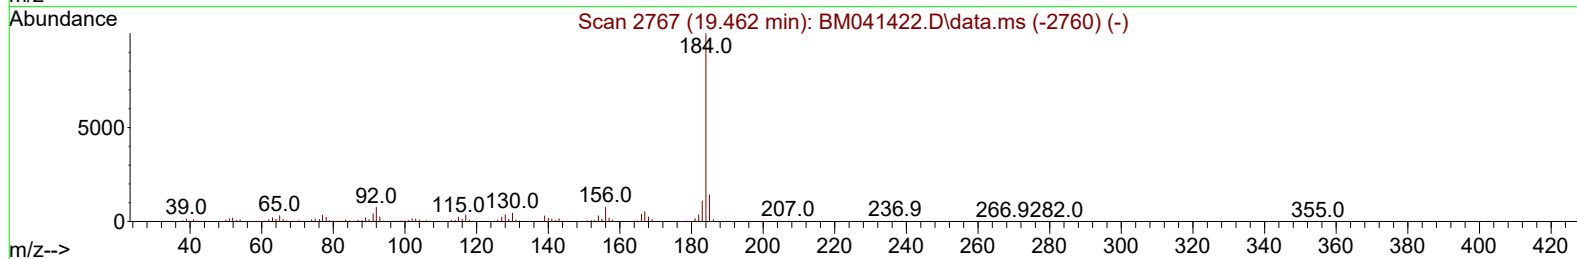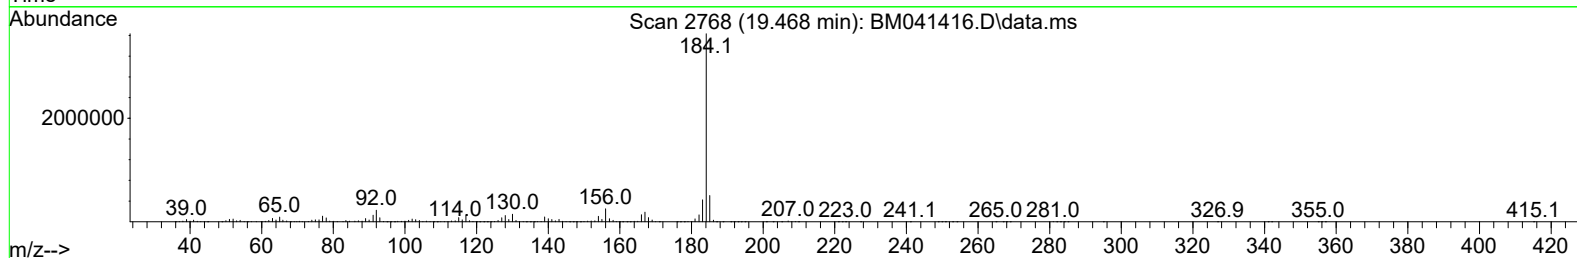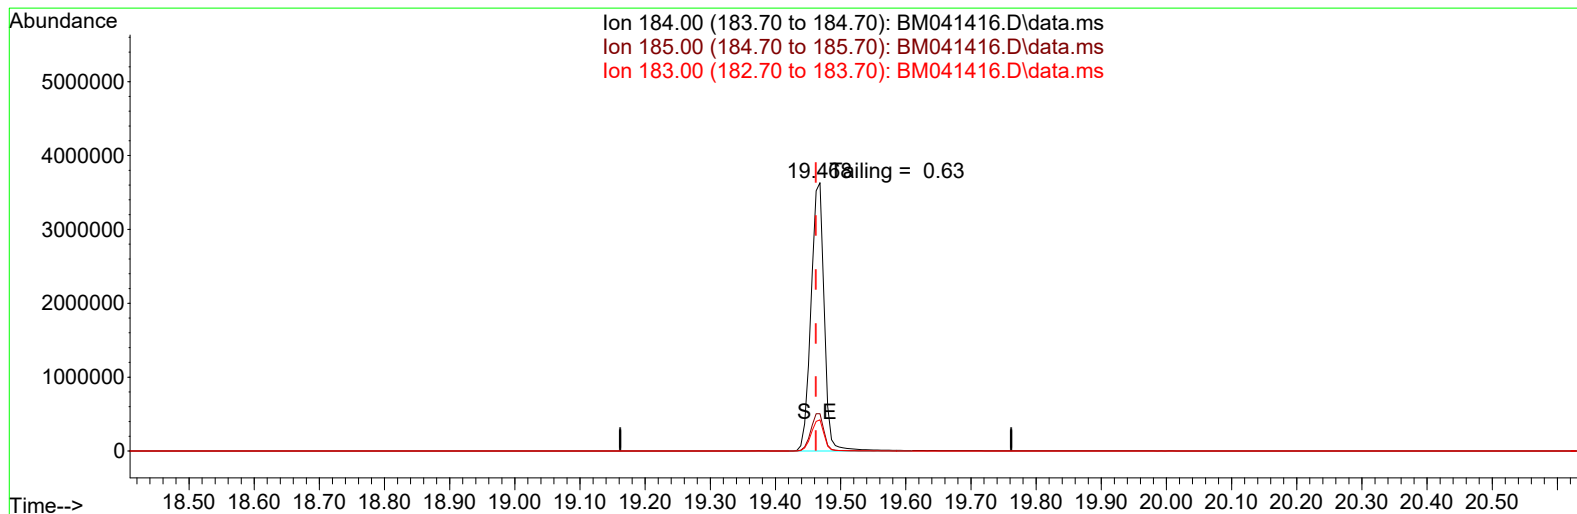

TIC: BM041416.D\data.ms

(77) Benzidine

19.468min (+ 0.006) 449789.27 ng

response 5129945

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.93
183.00	11.00	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2023	BNA_M	<u>BM041416.D</u>
Compound Name	Response	Retention Time
DDT	2628680	20.686
DDD	40226	20.286
DDE	1828	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42054	2670734	1.57

Instrument :
BNA_M
ClientSampleId :
DFTPP