
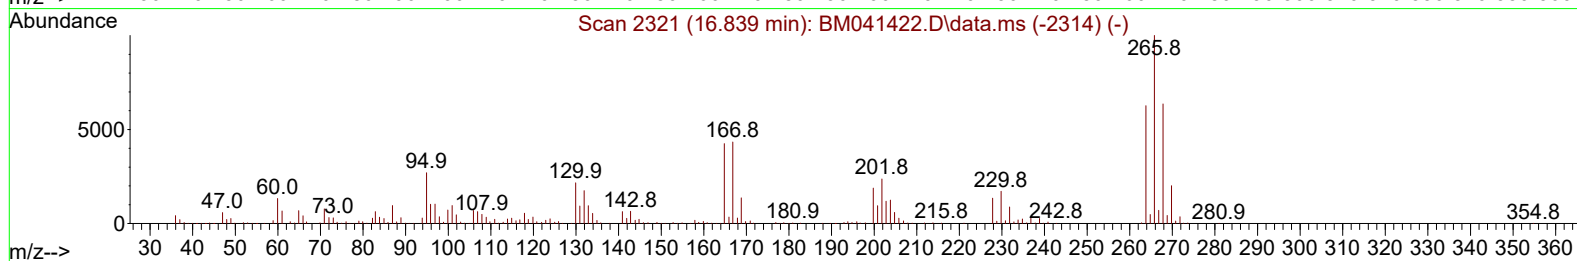
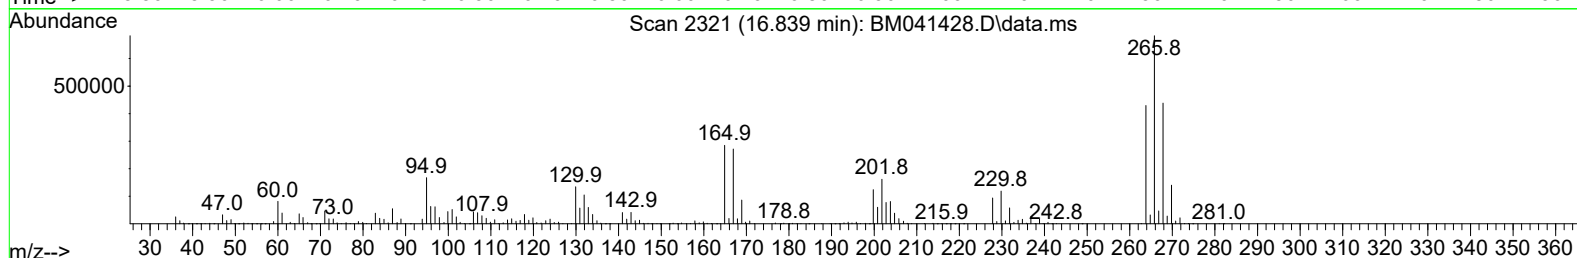


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041428.D
Acq On : 17 Aug 2023 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 09:29:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

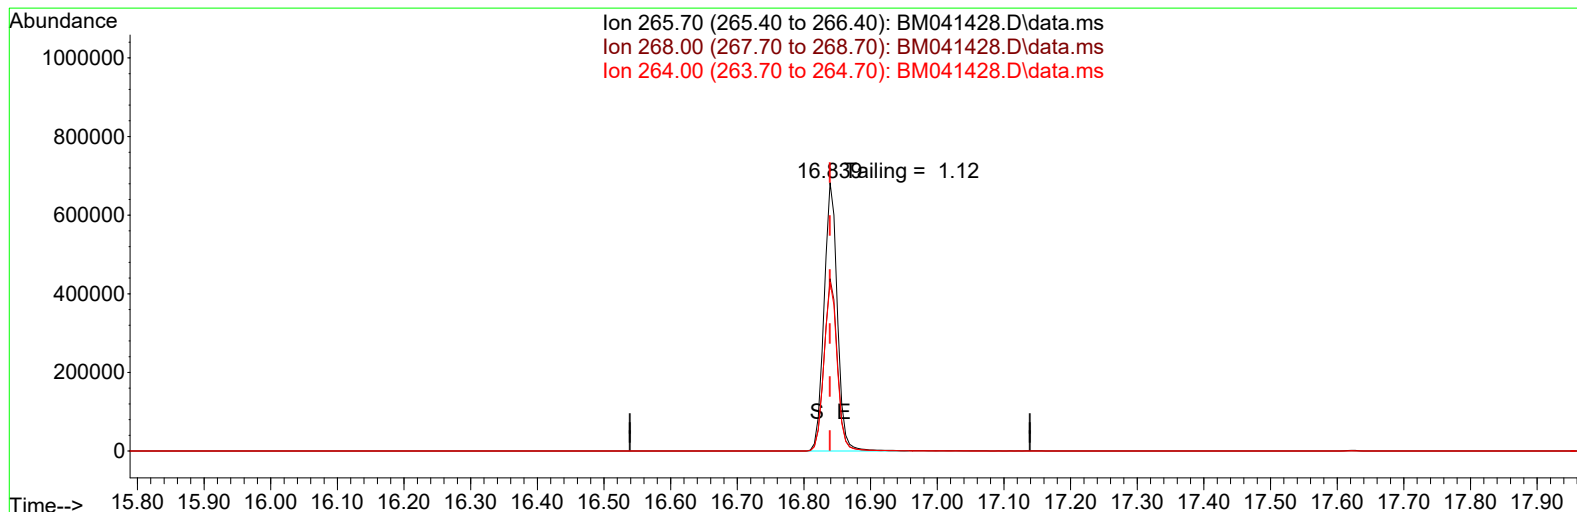

TIC: BM041428.D\data.ms

(70) Pentachlorophenol (C)




16.839min (+ 0.000) 1387986.77 ng

response 948077

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.15
264.00	62.70	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041428.D
Acq On : 17 Aug 2023 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 09:29:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

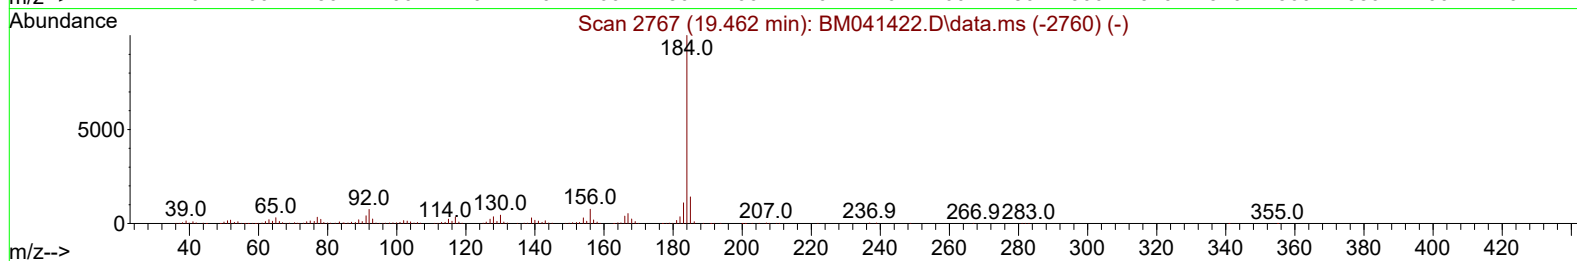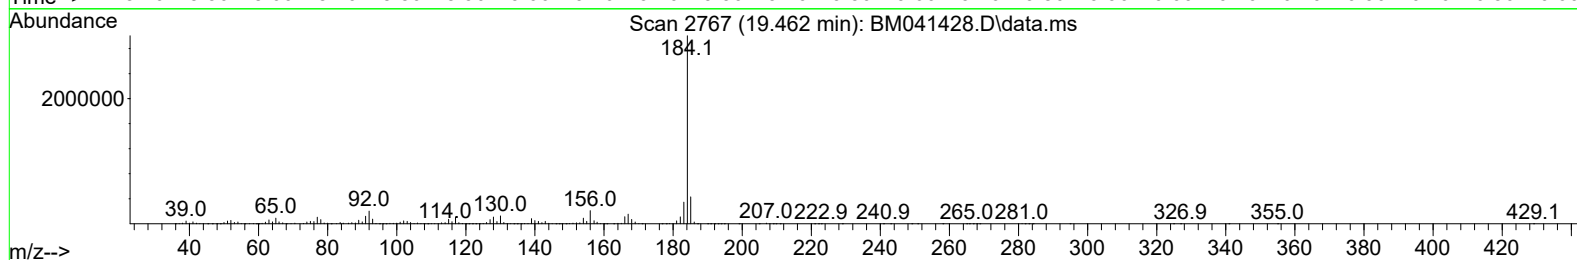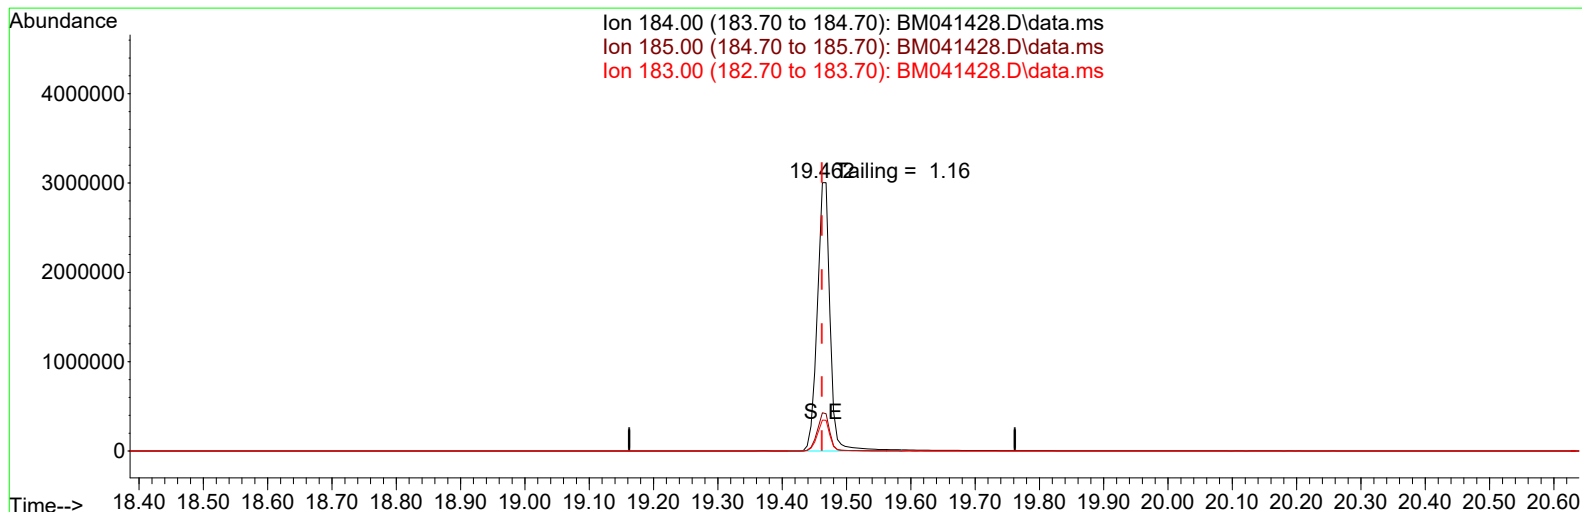

TIC: BM041428.D\data.ms

(77) Benzidine**19.462min (+ 0.000) 53070.60 ng****response 4181615**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.27
183.00	11.00	11.53
0.00	0.00	0.00