
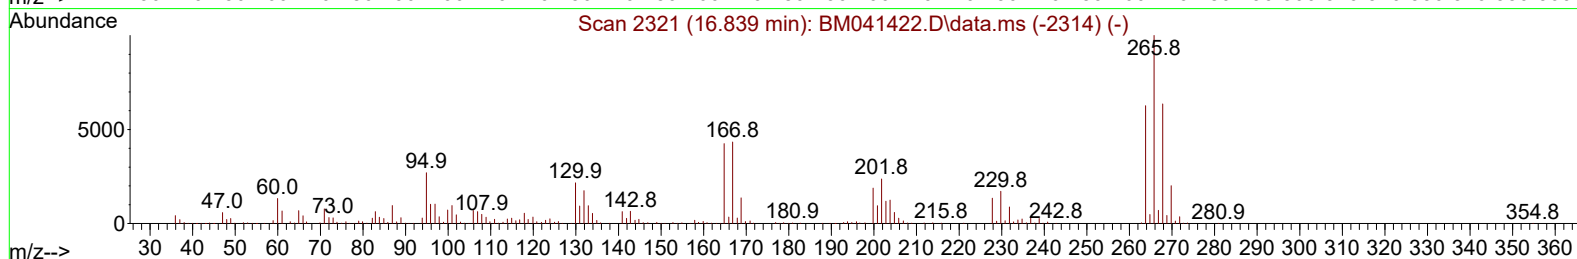
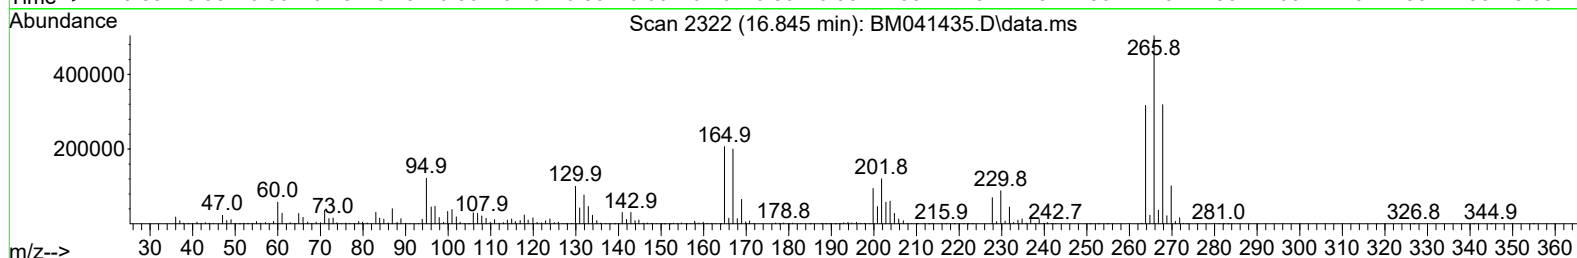


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
 Data File : BM041435.D
 Acq On : 17 Aug 2023 14:11
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 18:30:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 02:13:45 2023
 Response via : Initial Calibration

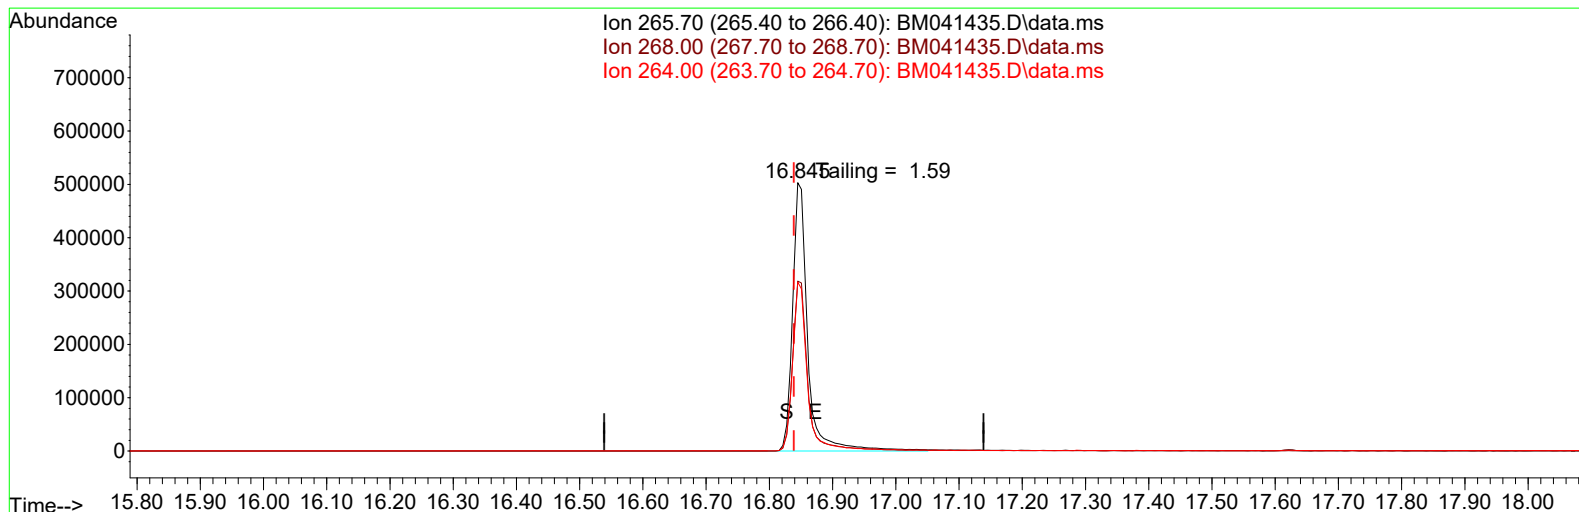

TIC: BM041435.D\data.ms

(70) Pentachlorophenol (C)




16.845min (+ 0.006) 0.00 ng

response 842005

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.34
264.00	62.70	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041435.D
Acq On : 17 Aug 2023 14:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 18:30:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

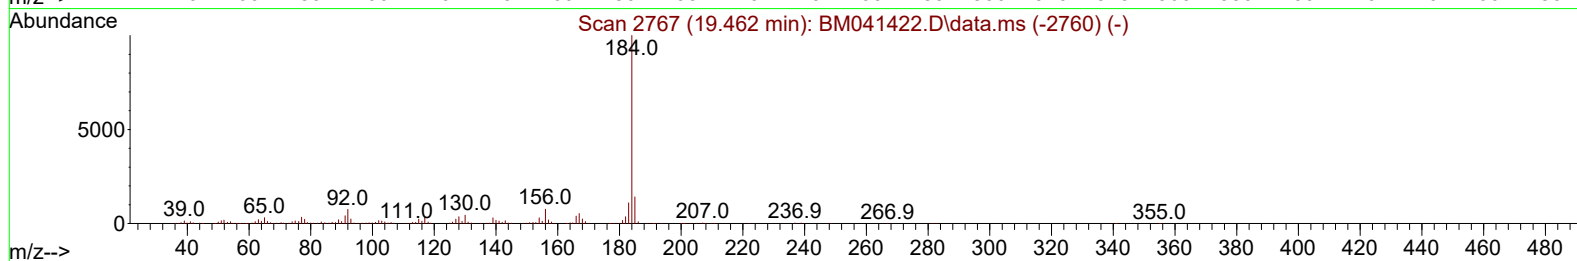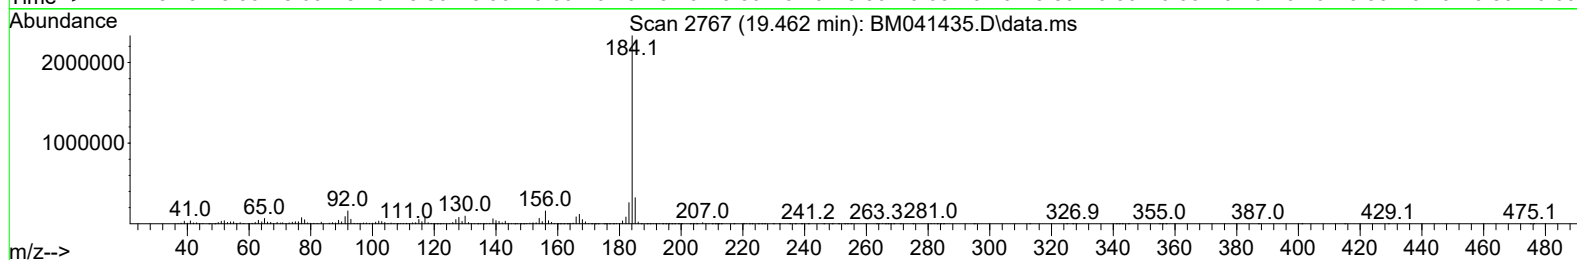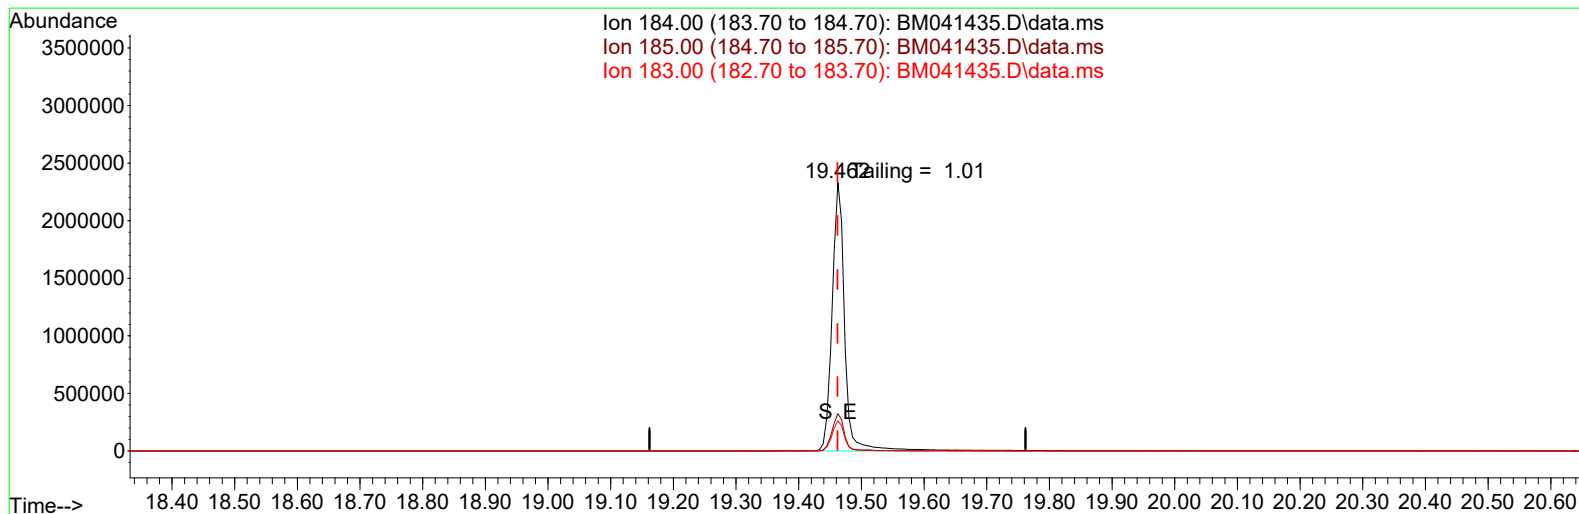

TIC: BM041435.D\data.ms

(77) Benzidine**19.462min (+ 0.000) 353067.39 ng****response 3253825**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.89
183.00	11.00	11.26
0.00	0.00	0.00