

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041432.D
Acq On : 17 Aug 2023 11:43
Operator : MA/JU
Sample : PB154837BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154837BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.881	282	288	303	rBV	1363137	1843084	19.66%	4.737%
2	5.340	360	366	383	rBV	2205097	3115512	33.23%	8.008%
3	6.945	632	639	664	rBV	1916458	3141274	33.51%	8.074%
4	7.763	771	778	792	rBV	575113	901294	9.61%	2.317%
5	8.939	969	978	1004	rBV	1787697	2971185	31.69%	7.637%
6	10.563	1246	1254	1271	rBV	641697	1172716	12.51%	3.014%
7	13.045	1669	1676	1693	rBV	4492500	6603193	70.44%	16.972%
8	14.427	1904	1911	1926	rBV	972375	1496539	15.96%	3.846%
9	15.927	2160	2166	2188	rBV	2135428	3265016	34.83%	8.392%
10	17.186	2374	2380	2401	rBV	1157627	1756406	18.74%	4.514%
11	19.827	2823	2829	2843	rBV	7835918	9374748	100.00%	24.095%
12	21.391	3090	3095	3107	rBV	1264760	1768025	18.86%	4.544%
13	23.750	3490	3496	3513	rVB	690629	1497969	15.98%	3.850%




Sum of corrected areas: 38906961

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041432.D
Acq On : 17 Aug 2023 11:43
Operator : MA/JU
Sample : PB154837BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154837BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

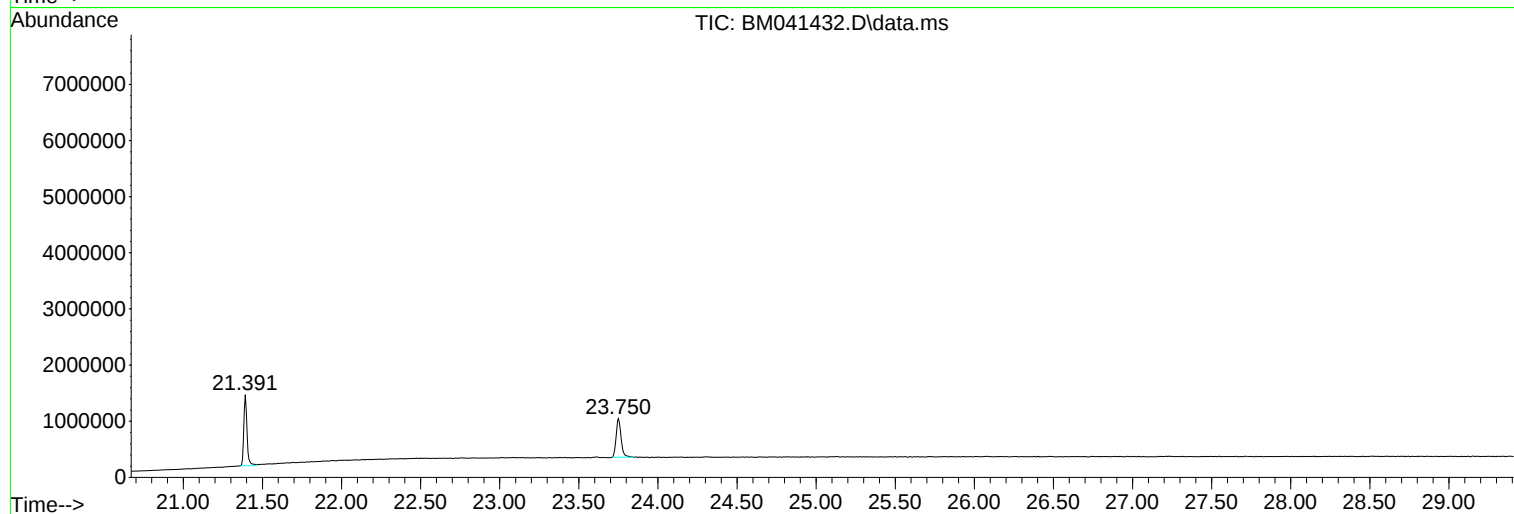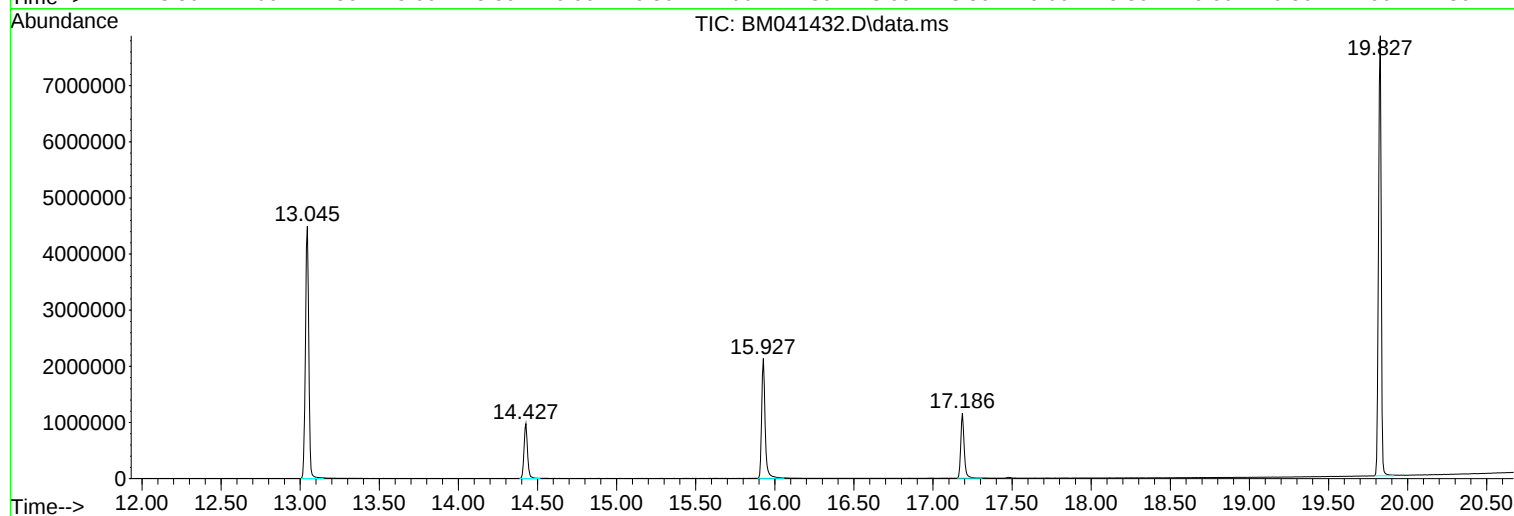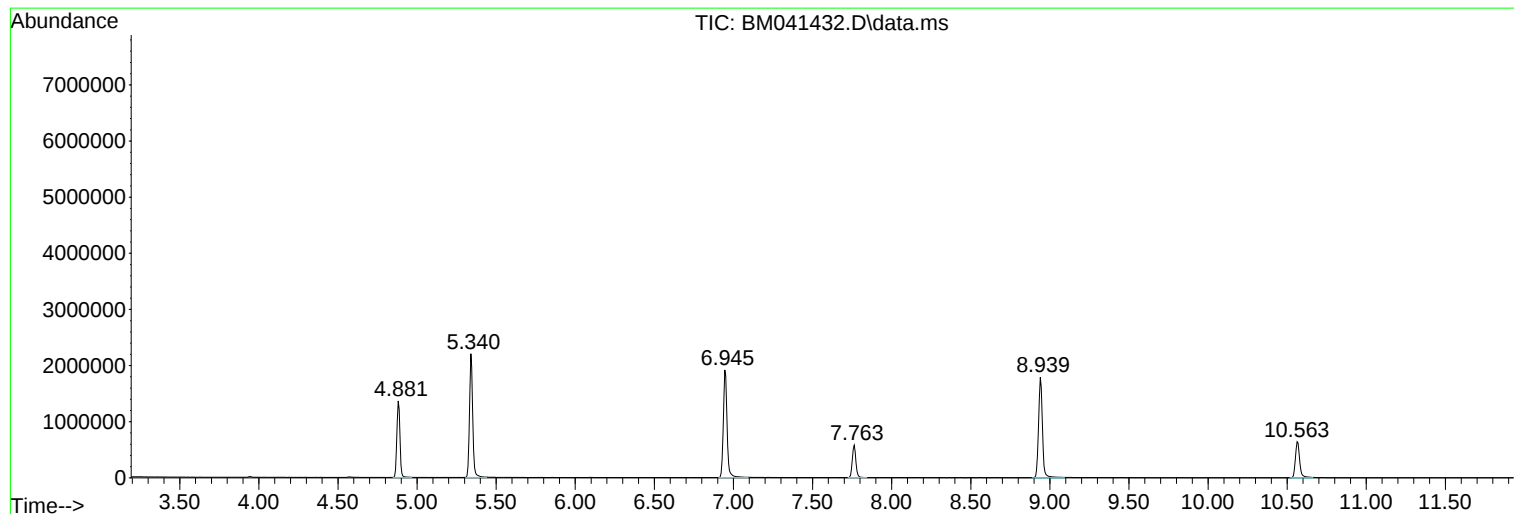

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041432.D
Acq On : 17 Aug 2023 11:43
Operator : MA/JU
Sample : PB154837BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB154837BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.881	40.90 ng	1843080	1,4-Dichlorobenzene-d4			7.763
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

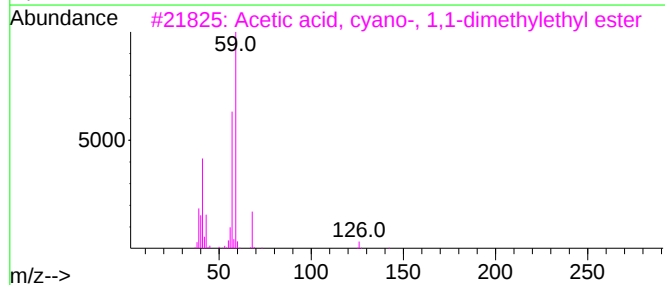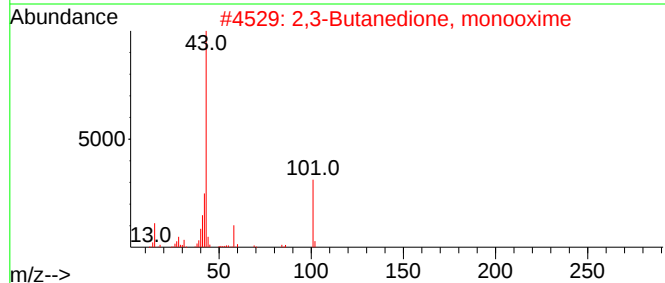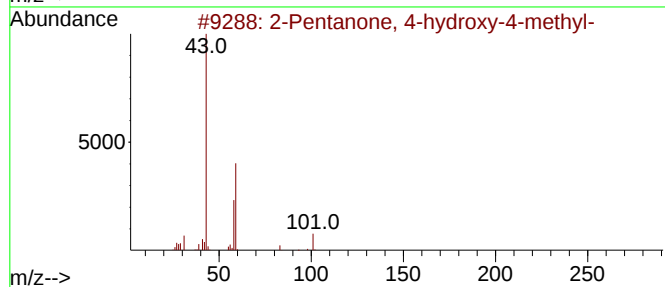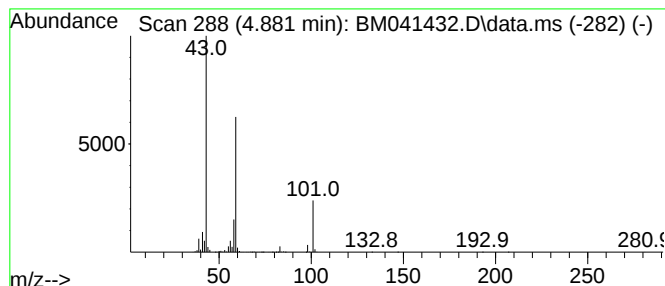

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041432.D
Acq On : 17 Aug 2023 11:43
Operator : MA/JU
Sample : PB154837BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154837BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.881	40.9	ng	1843080	1	7.763	901294	20.0