


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041428.D
Acq On : 17 Aug 2023 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 17 02:13:45 2023

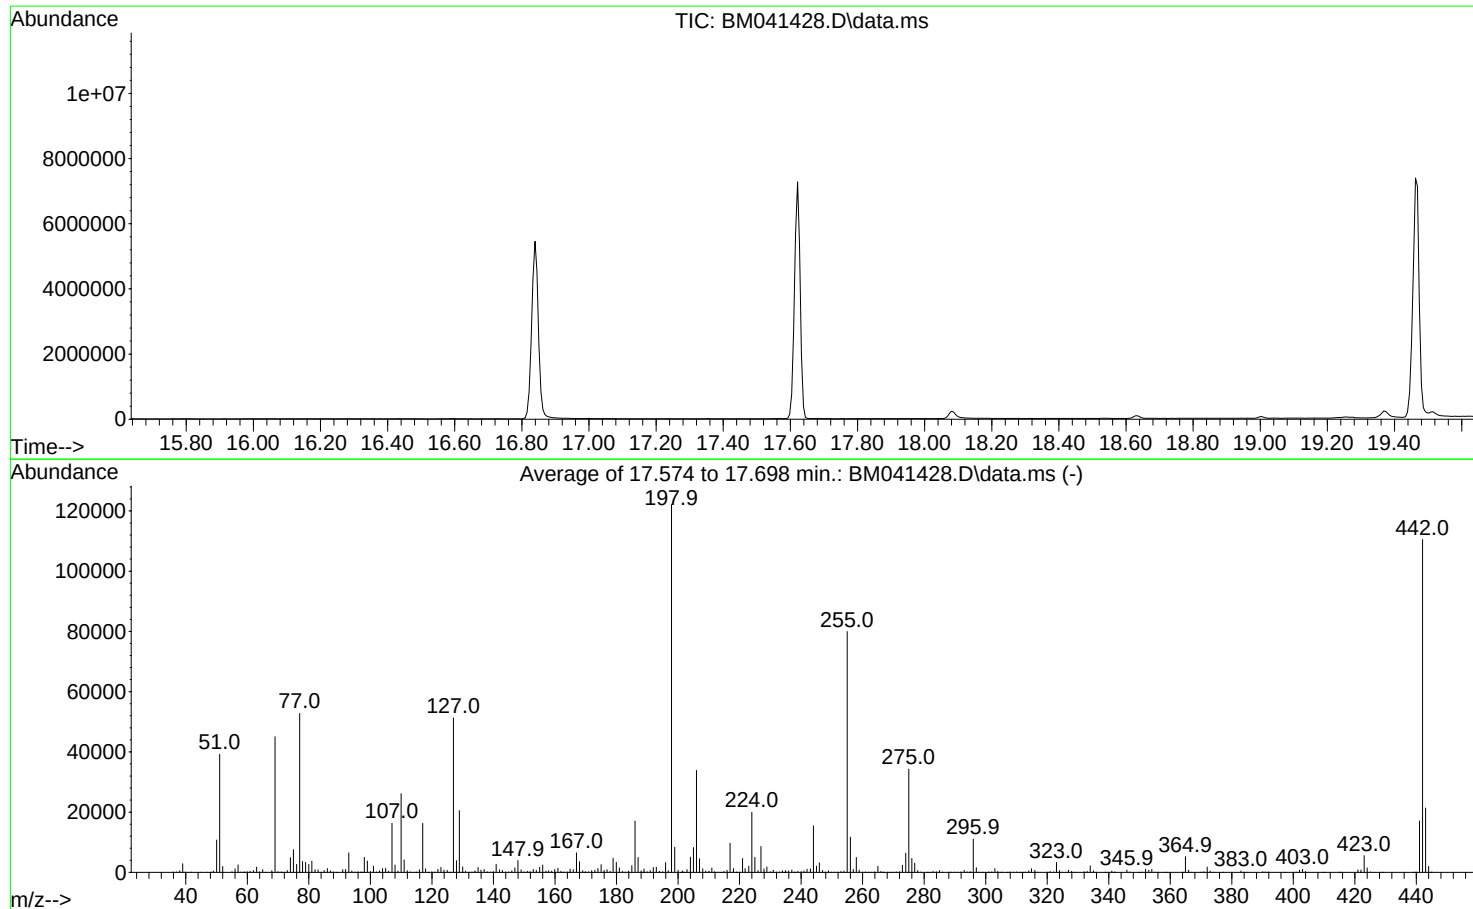




Spectrum Information: Average of 17.574 to 17.698 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	32.1	39230	PASS
68	69	0.00	2	1.2	561	PASS
69	198	0.00	100	36.9	45072	PASS
70	69	0.00	2	0.6	269	PASS
127	198	10	80	42.0	51294	PASS
197	198	0.00	2	0.4	545	PASS
198	198	100	100	100.0	122141	PASS
199	198	5	9	6.8	8340	PASS
275	198	10	60	28.1	34295	PASS
365	198	1	100	4.3	5201	PASS
441	198	0.01	100	13.9	17035	PASS
442	442	50	100	100.0	110492	PASS
443	442	15	24	19.3	21372	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041428.D
Acq On : 17 Aug 2023 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 09:29:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

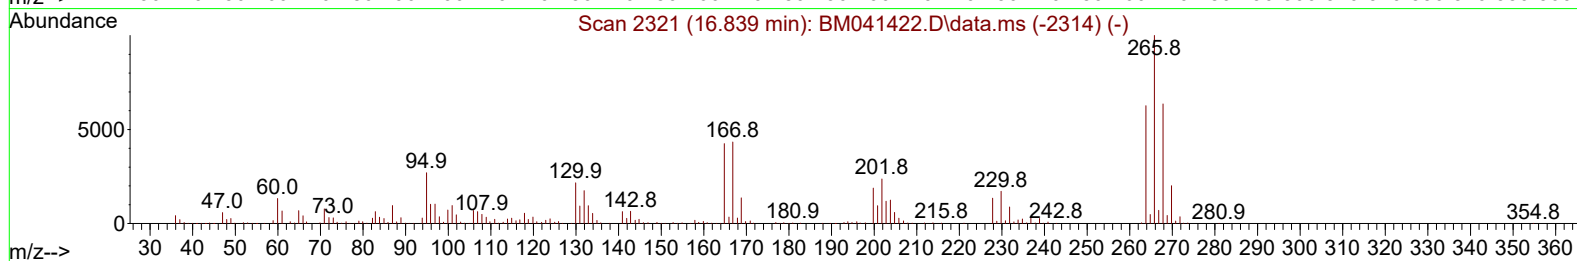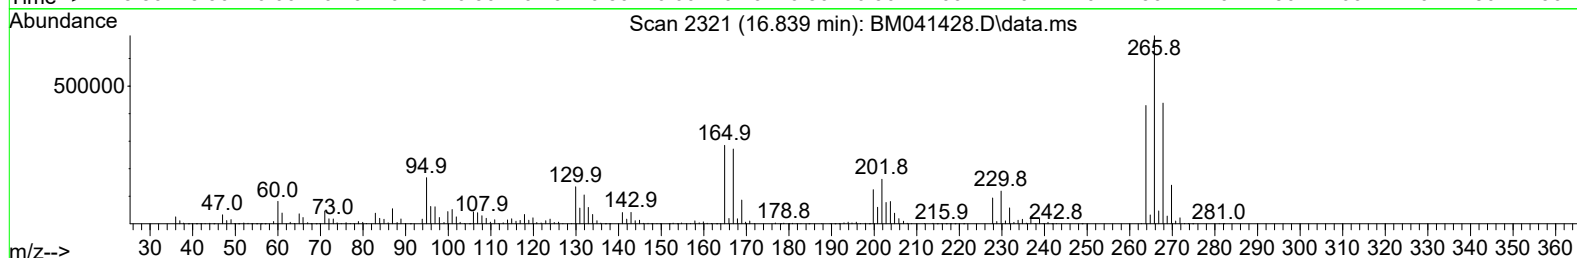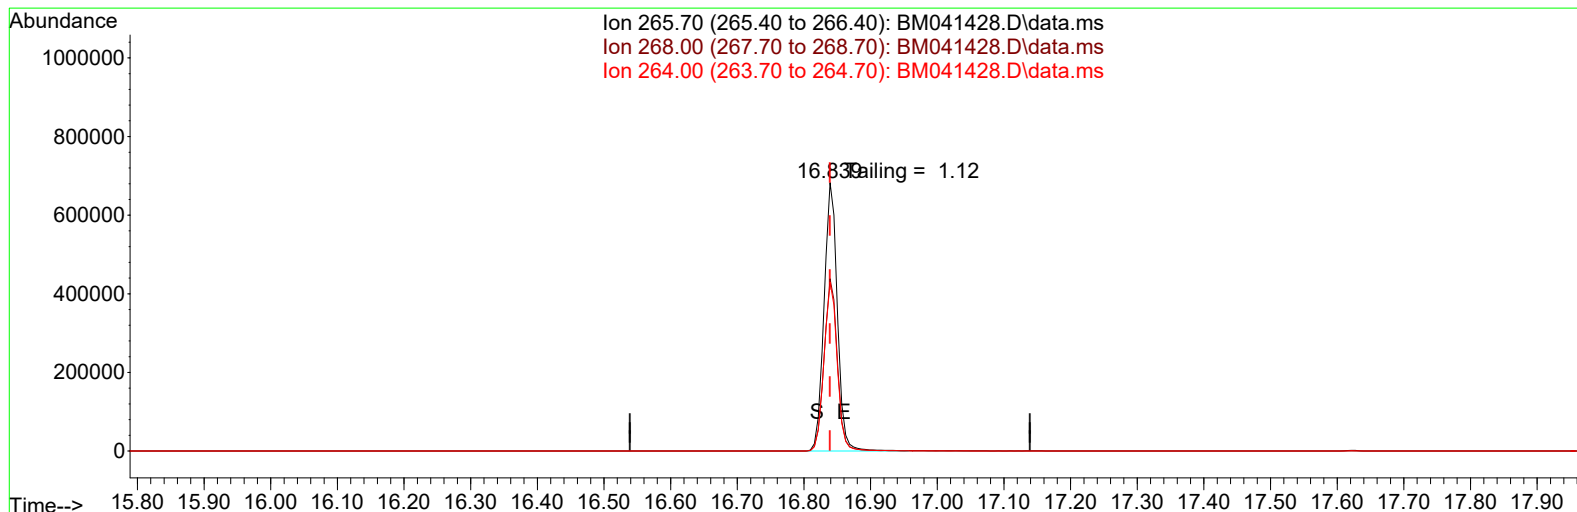

TIC: BM041428.D\data.ms

(70) Pentachlorophenol (C)

16.839min (+ 0.000) 1387986.77 ng




response 948077

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.15
264.00	62.70	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041428.D
Acq On : 17 Aug 2023 08:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 09:29:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

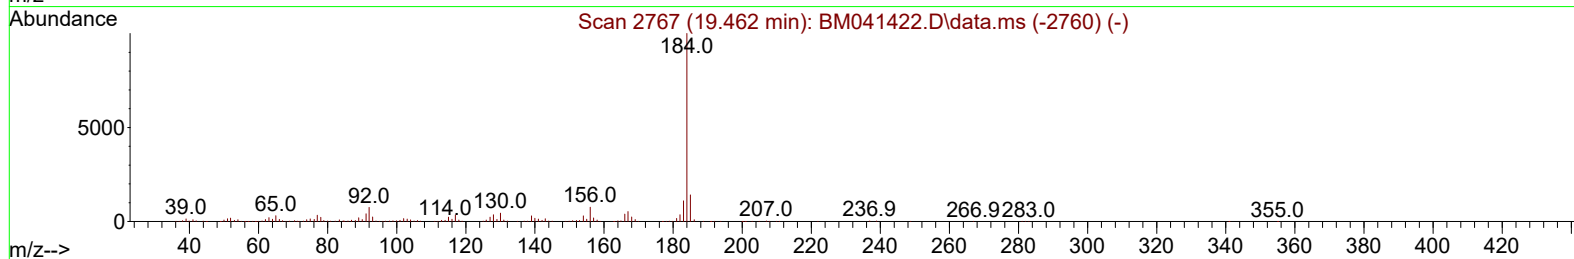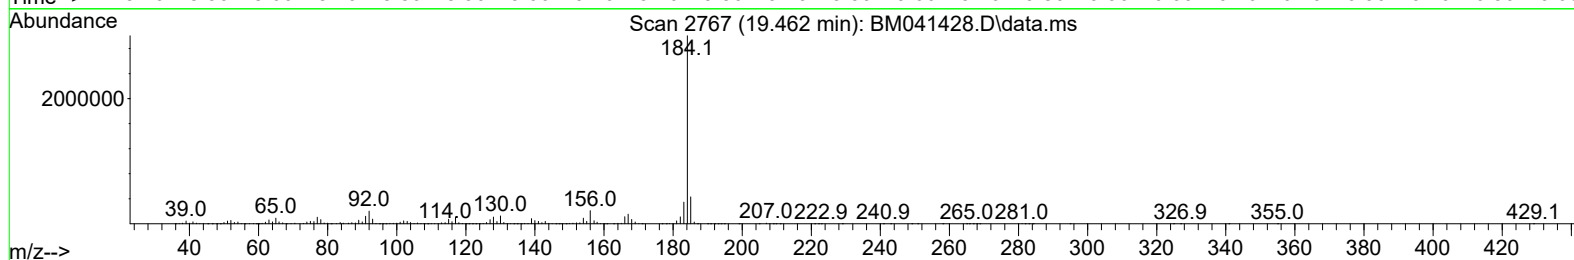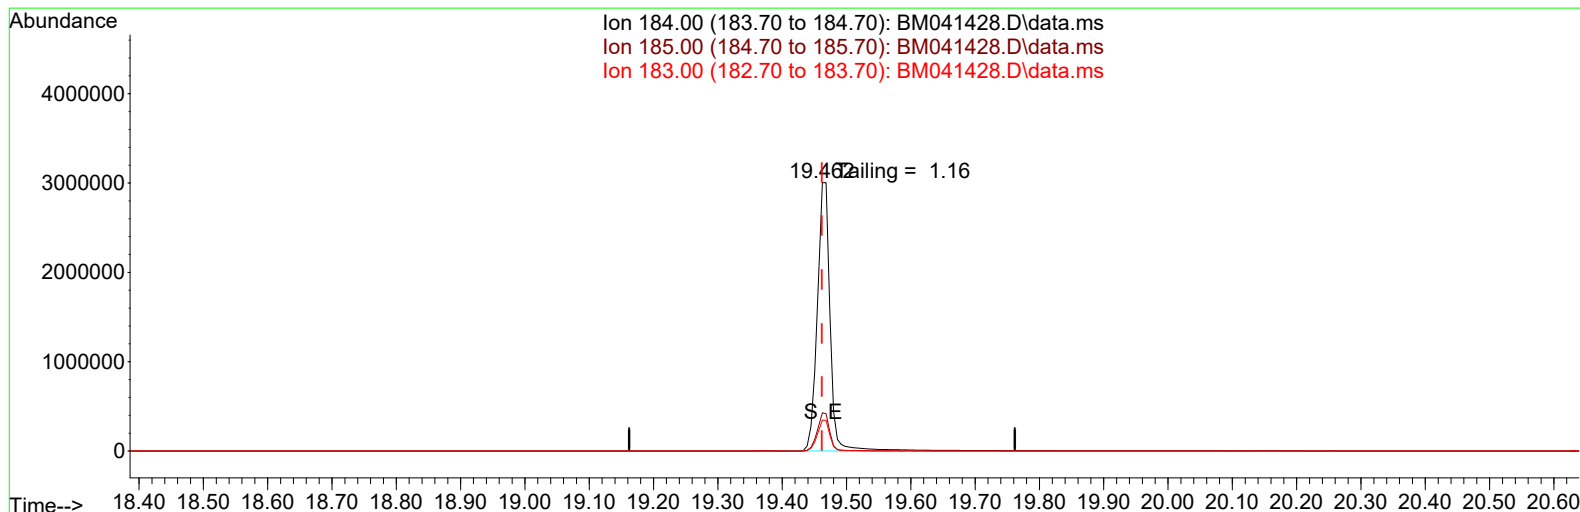

TIC: BM041428.D\data.ms

(77) Benzidine

19.462min (+ 0.000) 53070.60 ng

response 4181615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.27
183.00	11.00	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2023	BNA_M	<u>BM041428.D</u>
Compound Name	Response	Retention Time
DDT	2614149	20.686
DDD	28060	20.286
DDE	1009	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29069	2643218	1.10

Instrument :
BNA_M
ClientSampleId :
DFTPP