
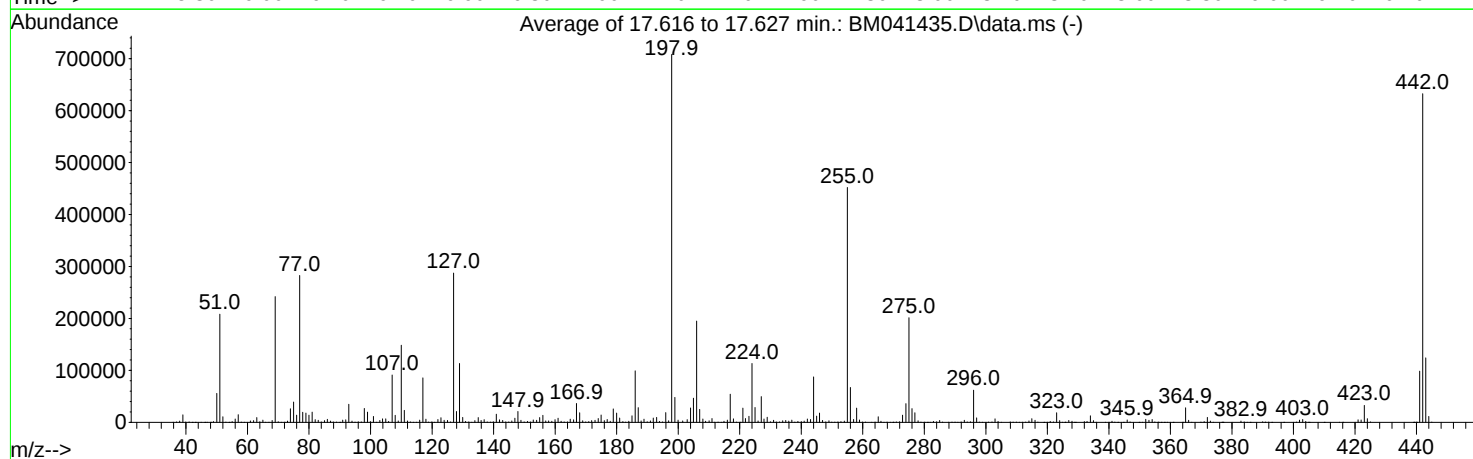


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
 Data File : BM041435.D
 Acq On : 17 Aug 2023 14:11
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 17 02:13:45 2023

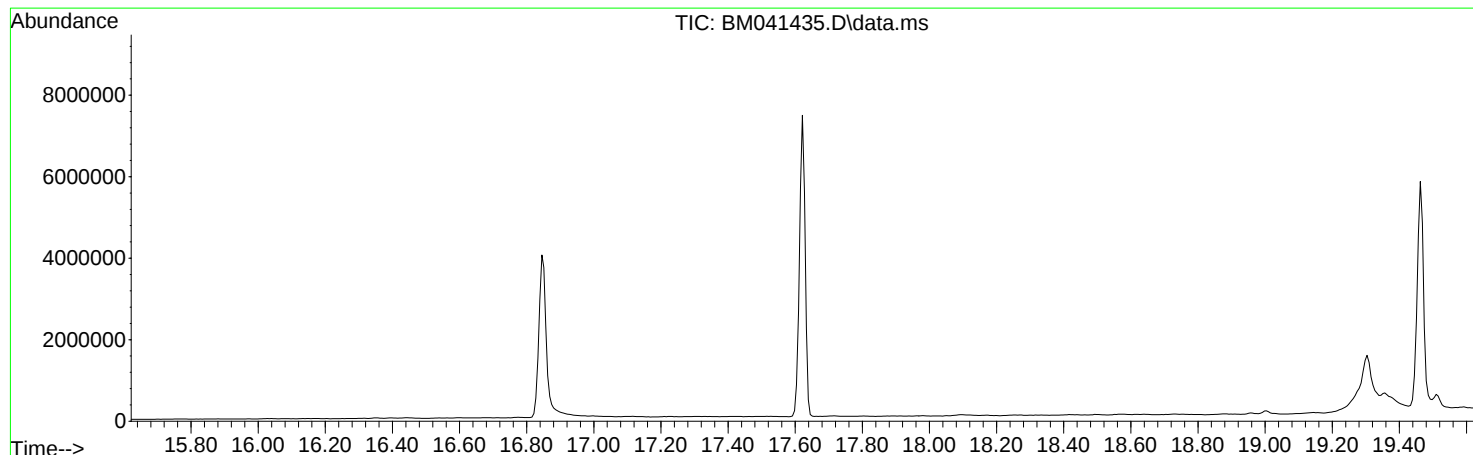




Spectrum Information: Average of 17.616 to 17.627 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	208339	PASS
68	69	0.00	2	1.5	3637	PASS
69	198	0.00	100	34.2	242145	PASS
70	69	0.00	2	0.5	1213	PASS
127	198	10	80	40.6	287200	PASS
197	198	0.00	2	0.5	3223	PASS
198	198	100	100	100.0	707968	PASS
199	198	5	9	6.8	48009	PASS
275	198	10	60	28.4	201365	PASS
365	198	1	100	4.0	28059	PASS
441	198	0.01	100	13.9	98659	PASS
442	442	50	100	100.0	632491	PASS
443	442	15	24	19.6	124029	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
 Data File : BM041435.D
 Acq On : 17 Aug 2023 14:11
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 17 18:30:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 02:13:45 2023
 Response via : Initial Calibration

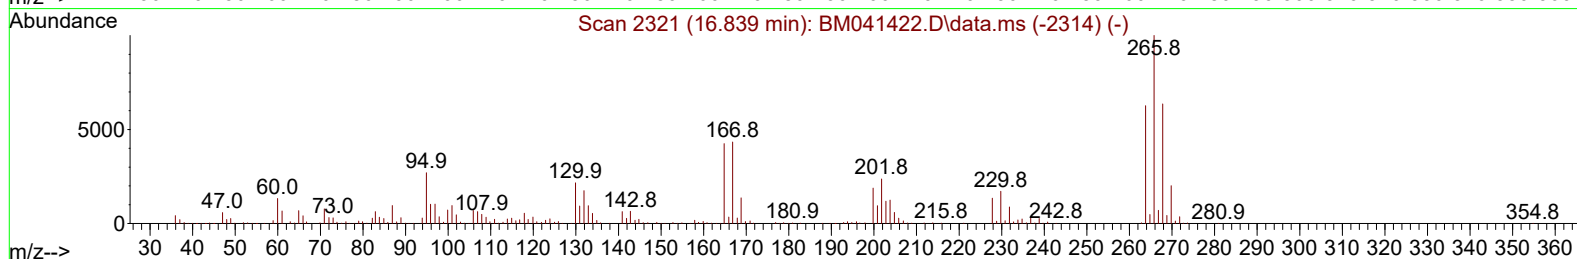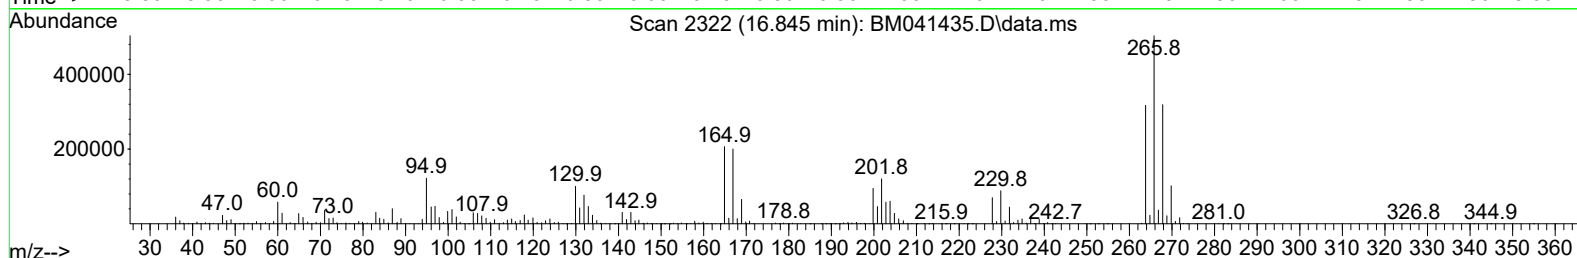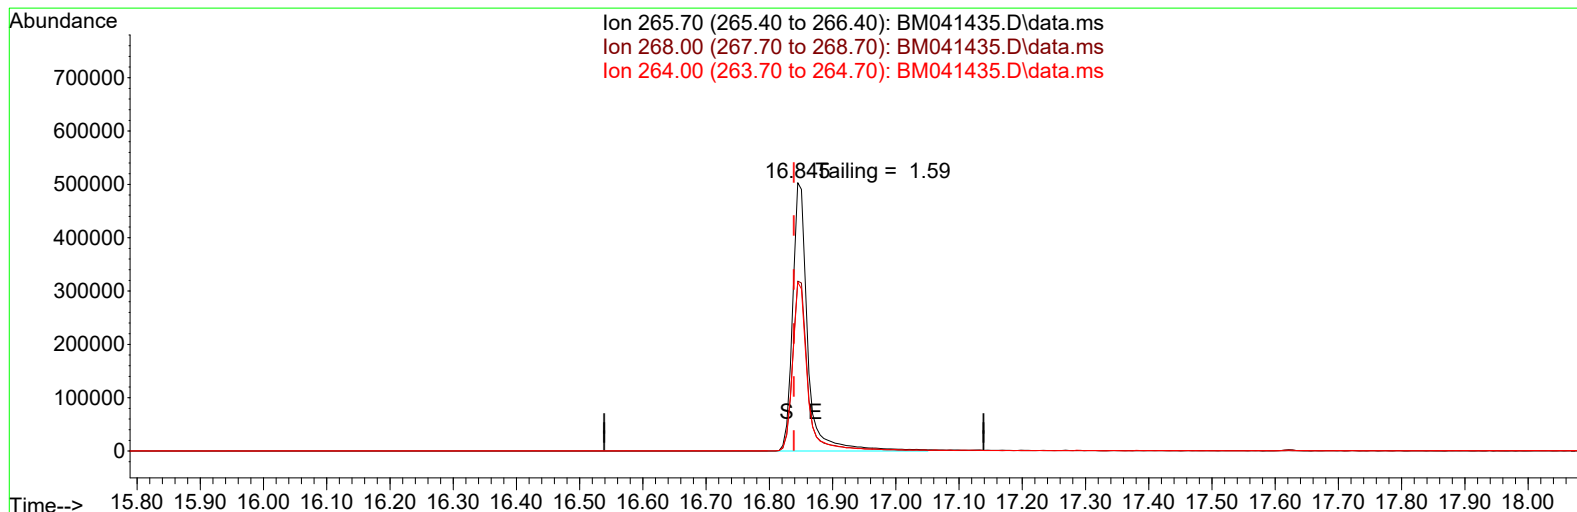

TIC: BM041435.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.006) 0.00 ng




response 842005

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.34
264.00	62.70	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081723\
Data File : BM041435.D
Acq On : 17 Aug 2023 14:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 18:30:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 02:13:45 2023
Response via : Initial Calibration

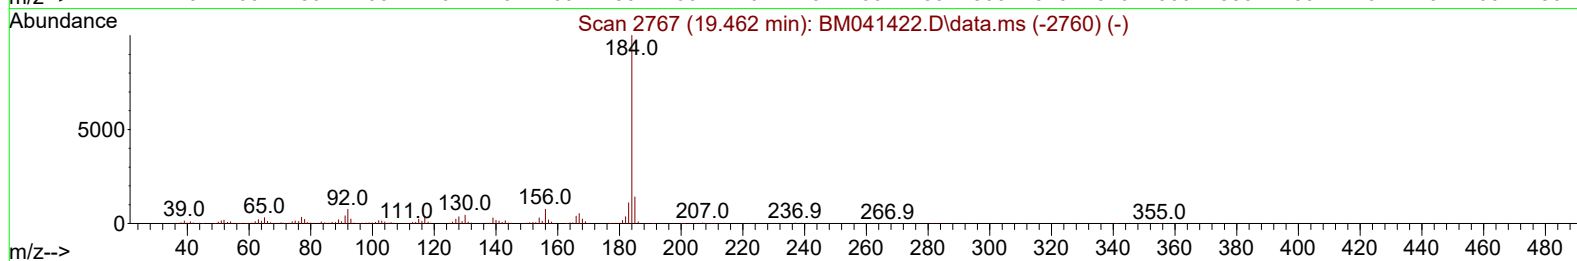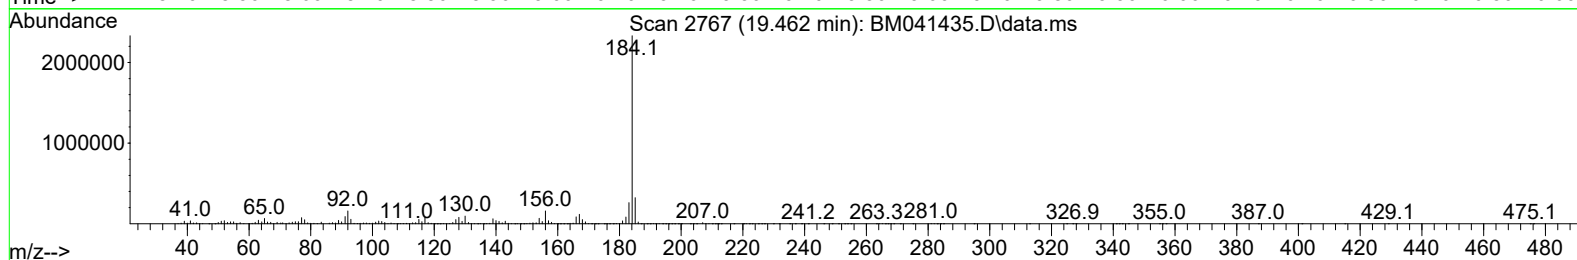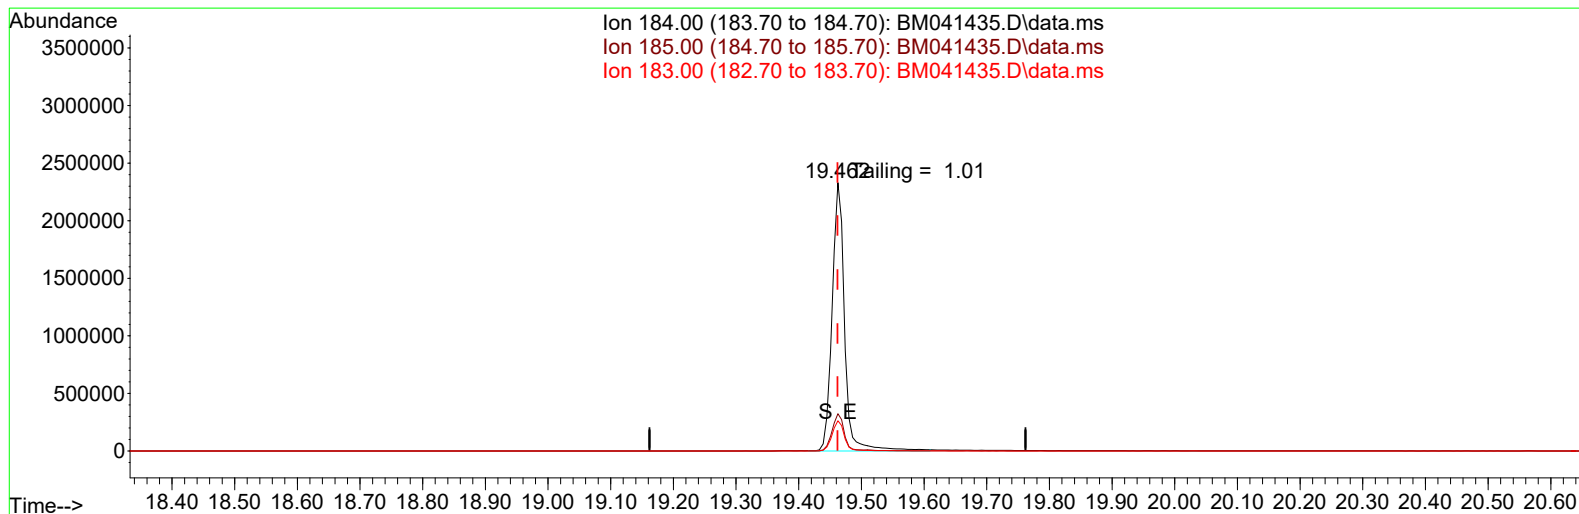

TIC: BM041435.D\data.ms

(77) Benzidine

19.462min (+ 0.000) 353067.39 ng

response 3253825

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.89
183.00	11.00	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2023	BNA_M	<u>BM041435.D</u>
Compound Name	Response	Retention Time
DDT	2104257	20.68
DDD	100825	20.245
DDE	4867	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
105692	2209949	4.78

Instrument :
BNA_M
ClientSampleId :
DFTPP