
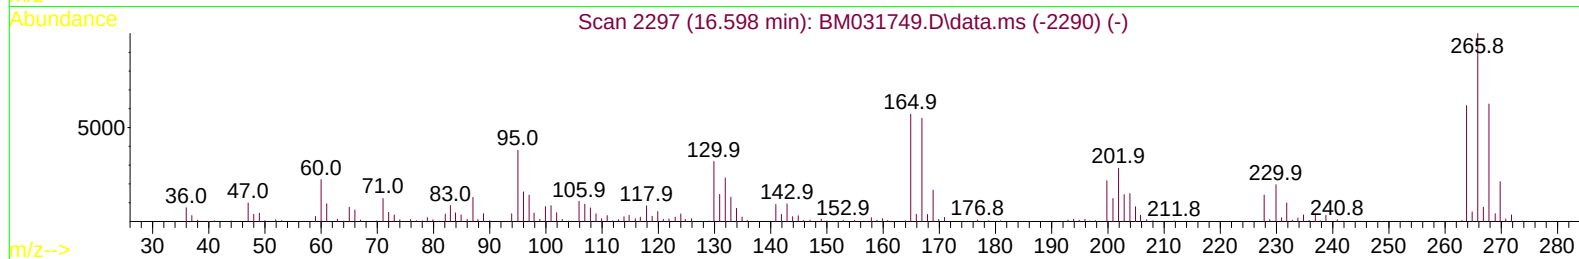
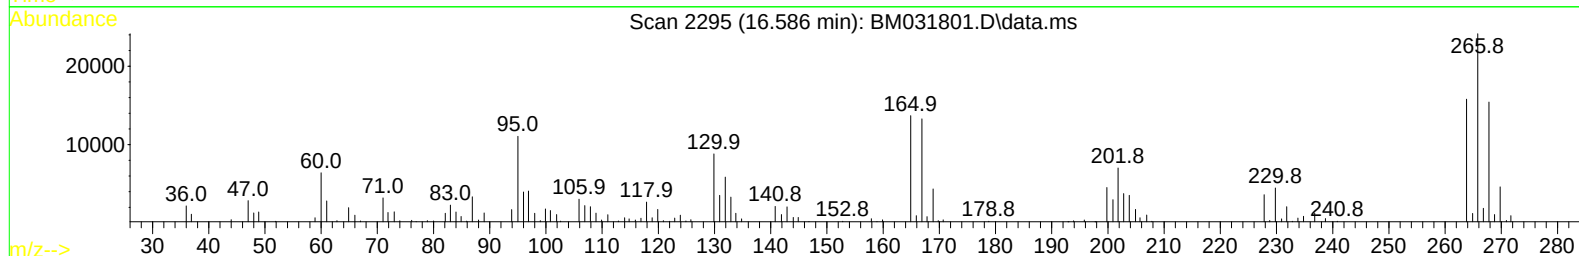


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081821\
Data File : BM031801.D
Acq On : 18 Aug 2021 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 14:09:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

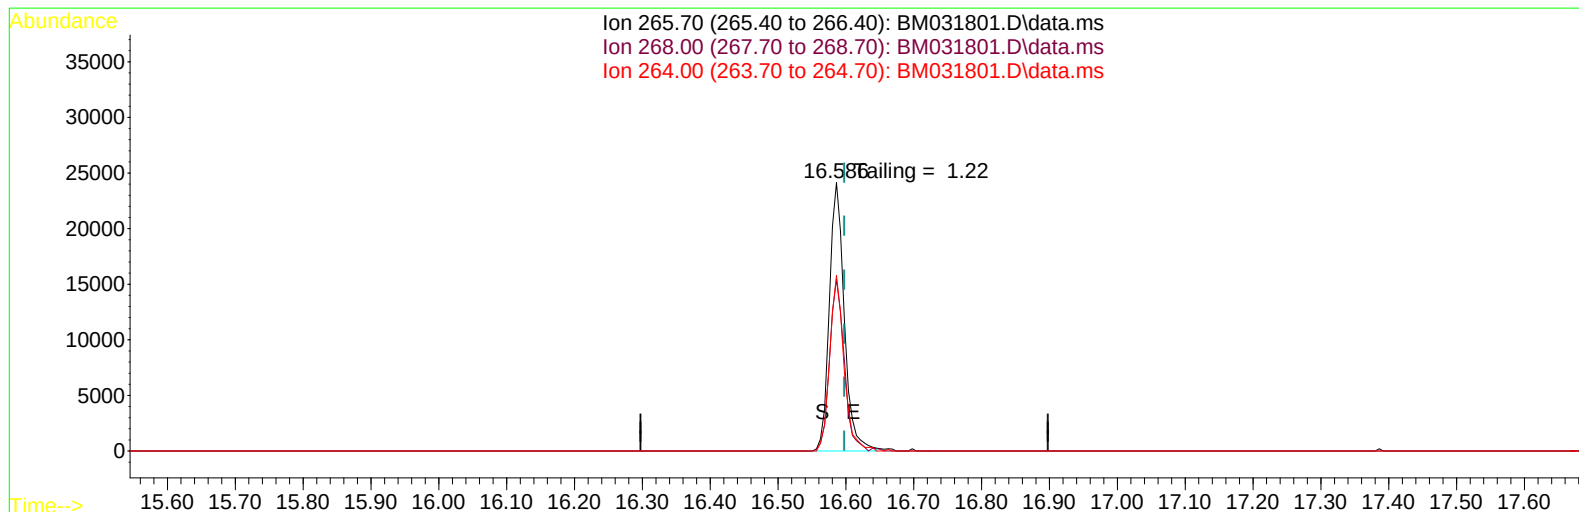

TIC: BM031801.D\data.ms

(70) Pentachlorophenol (C)




16.586min (-0.012) 0.00 ng

response 37182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.94
264.00	64.90	65.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081821\
 Data File : BM031801.D
 Acq On : 18 Aug 2021 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 14:09:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

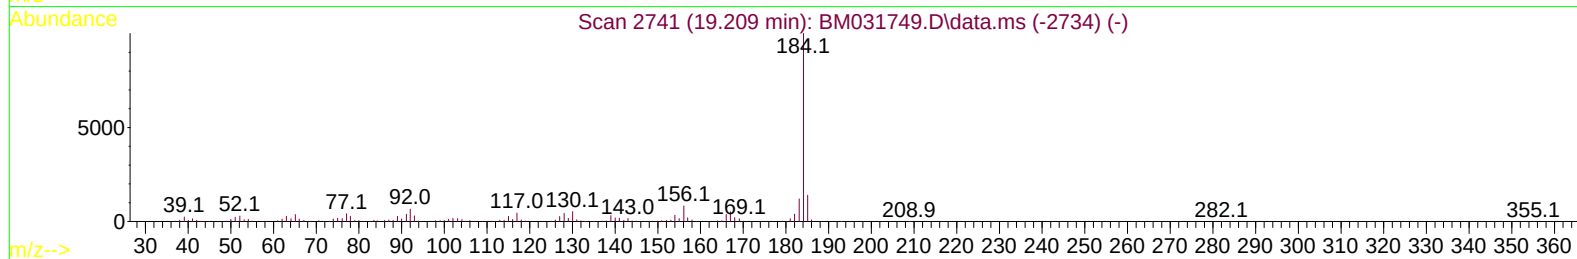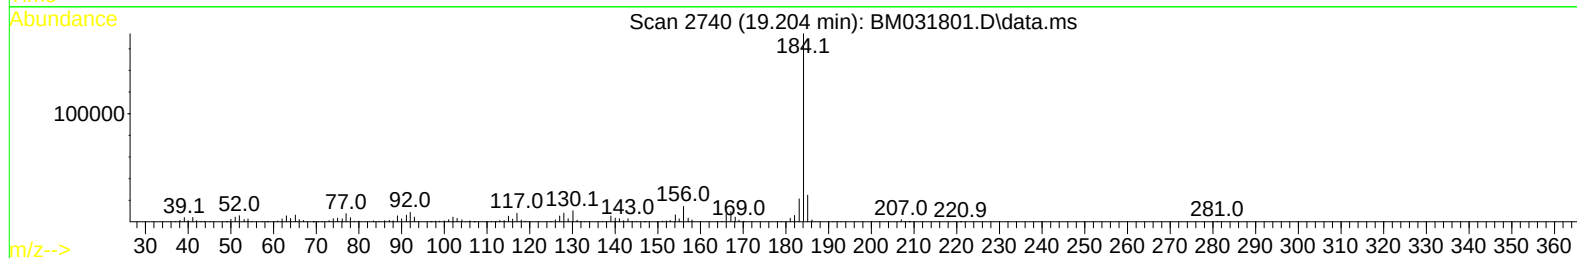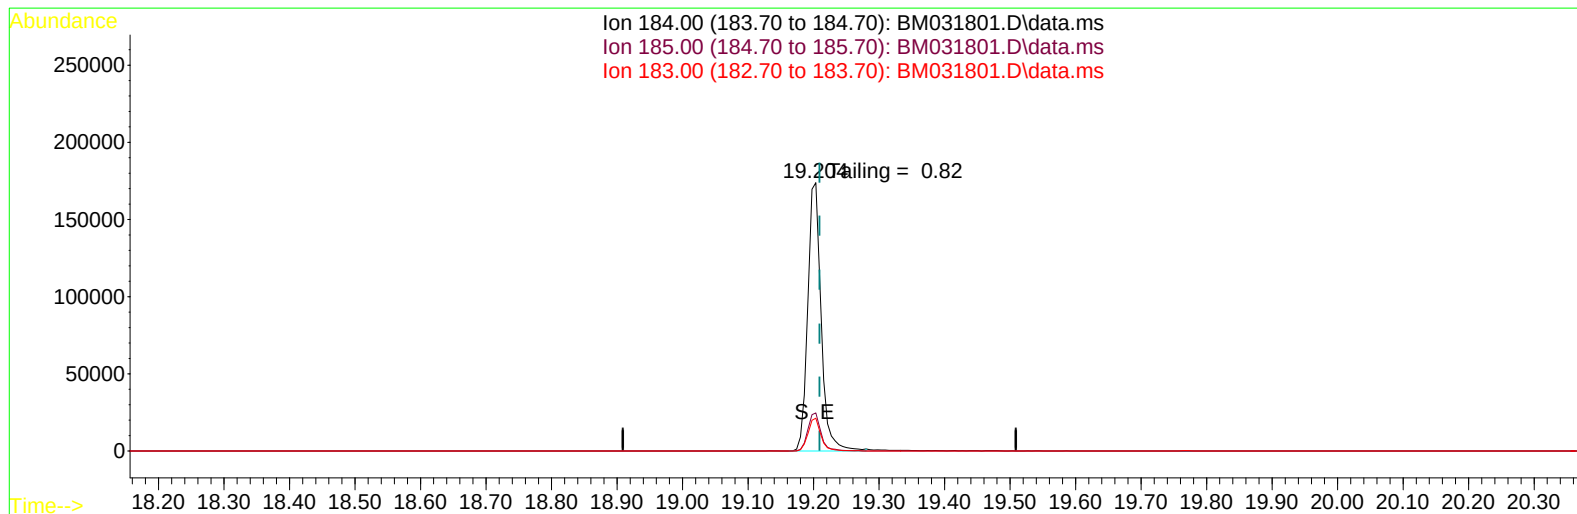

TIC: BM031801.D\data.ms

(77) Benzidine

19.204min (-0.006) 0.00 ng

response 248580

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.19
183.00	12.30	12.23
0.00	0.00	0.00