


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081821\
 Data File : BM031801.D
 Acq On : 18 Aug 2021 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 14:13:35 2021

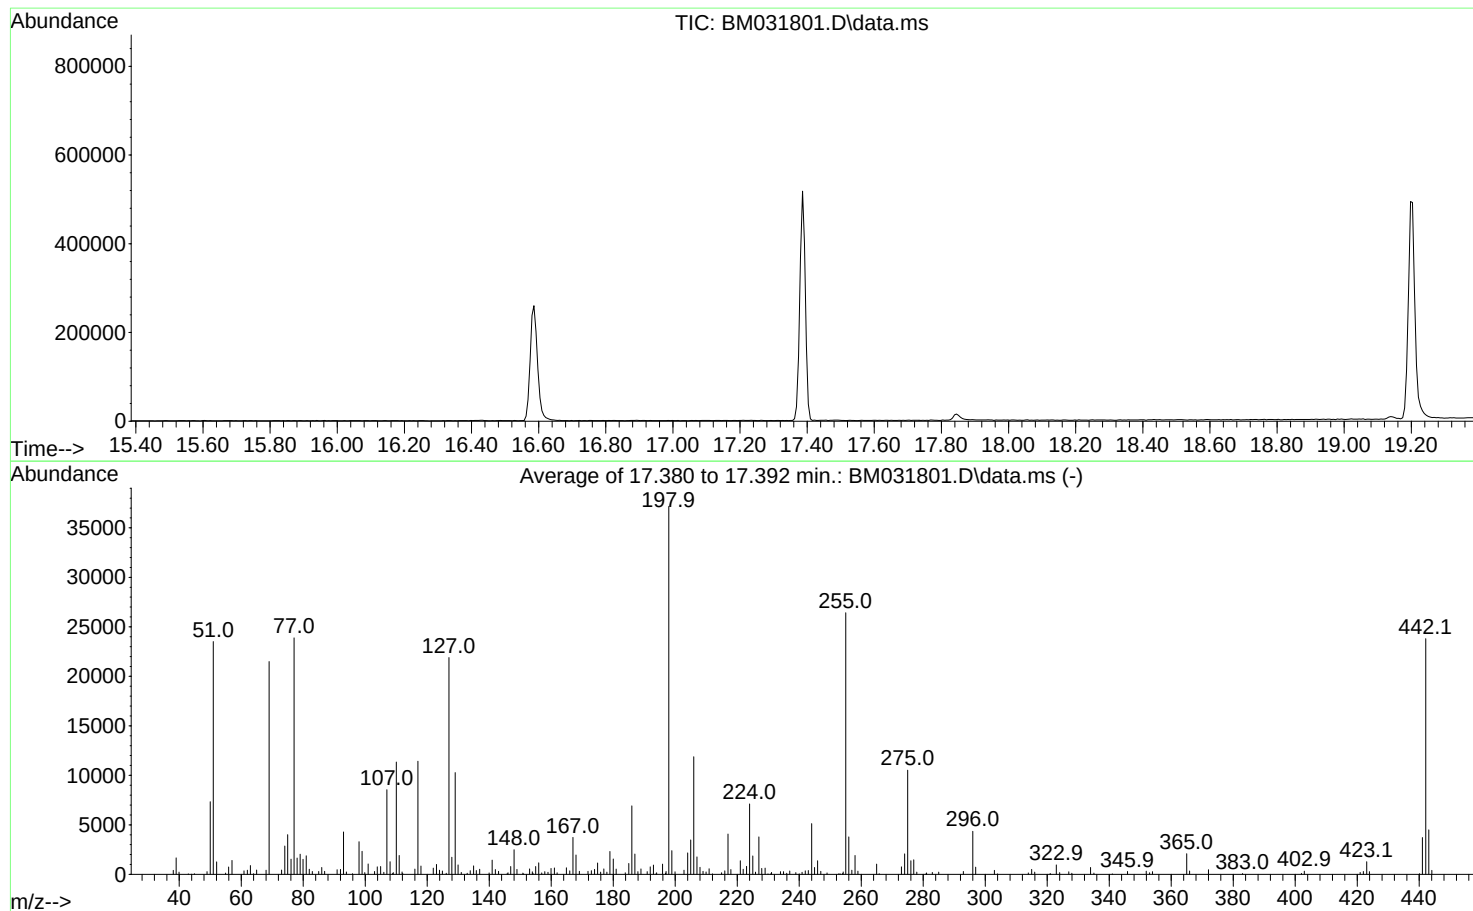




AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2424

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.3	23520	PASS
68	69	0.00	2	2.0	421	PASS
69	198	0.00	100	57.9	21496	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.9	21893	PASS
197	198	0.00	2	0.8	291	PASS
198	198	100	100	100.0	37155	PASS
199	198	5	9	6.4	2393	PASS
275	198	10	60	28.3	10522	PASS
365	198	1	100	5.6	2079	PASS
441	198	0.01	100	10.0	3714	PASS
442	442	50	100	100.0	23810	PASS
443	442	15	24	18.8	4488	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081821\
 Data File : BM031801.D
 Acq On : 18 Aug 2021 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 18 14:09:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

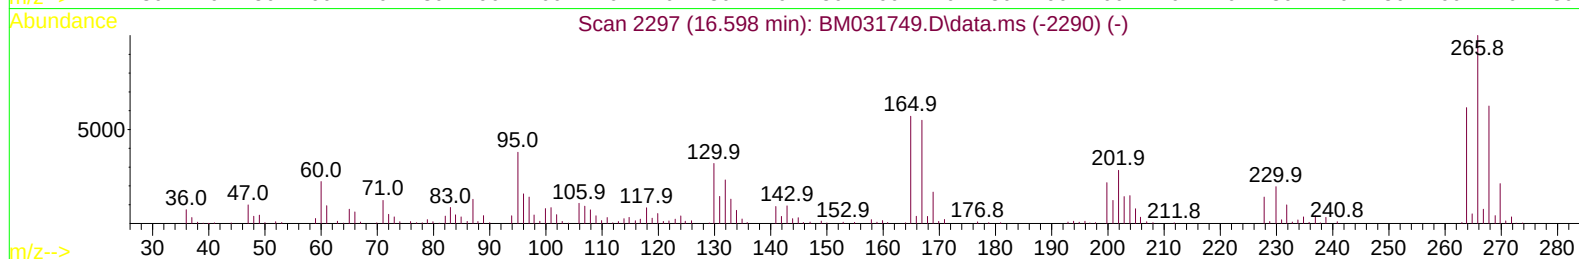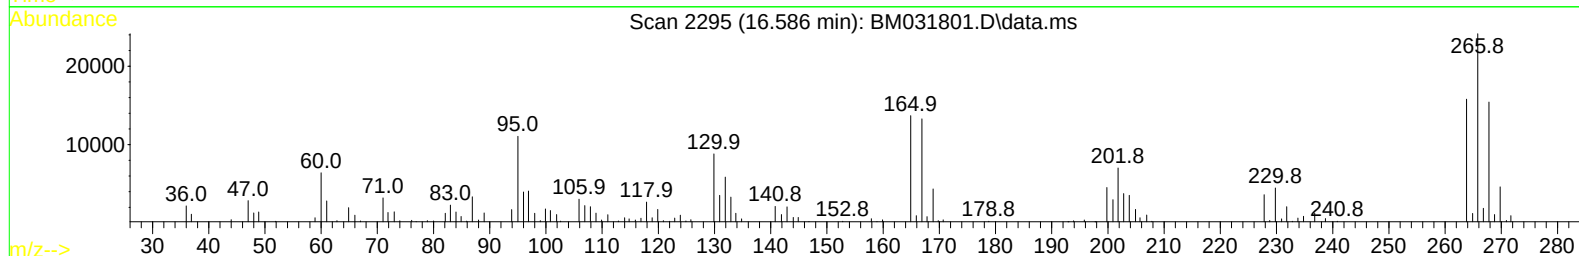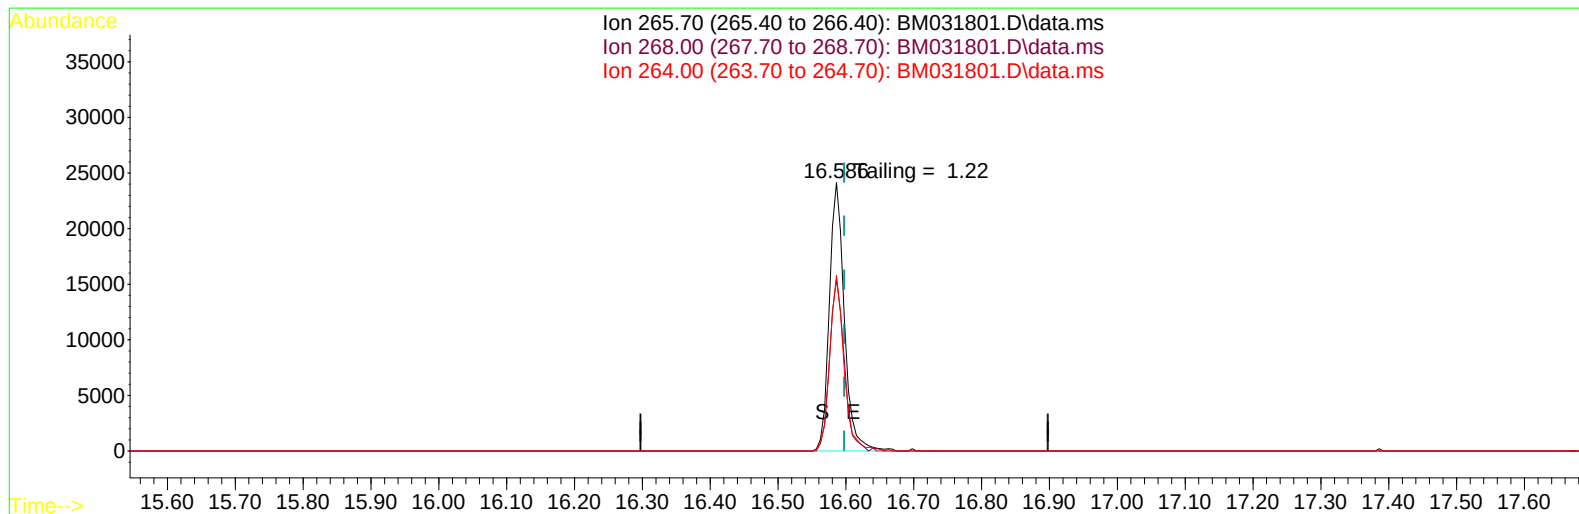

TIC: BM031801.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.012) 0.00 ng




response 37182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.94
264.00	64.90	65.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081821\
Data File : BM031801.D
Acq On : 18 Aug 2021 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 18 14:09:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

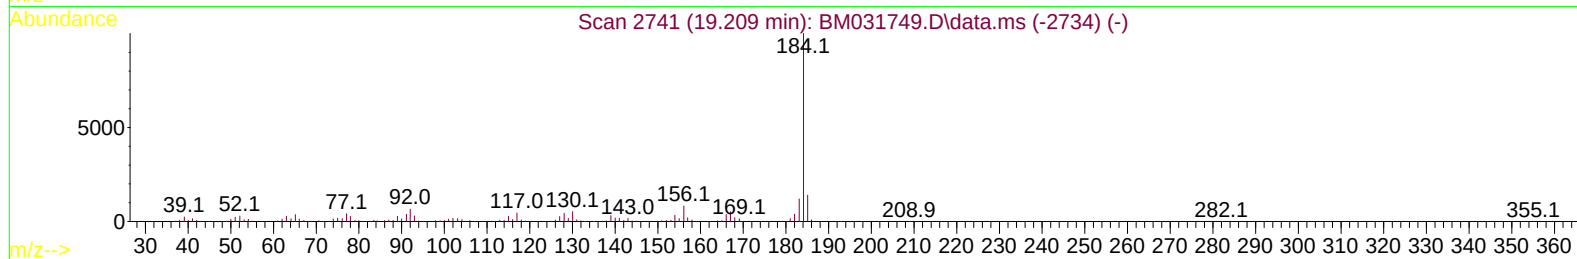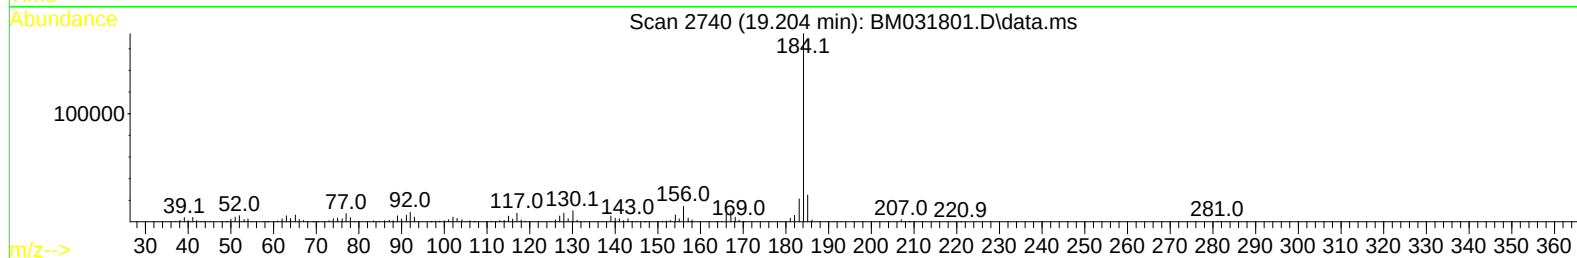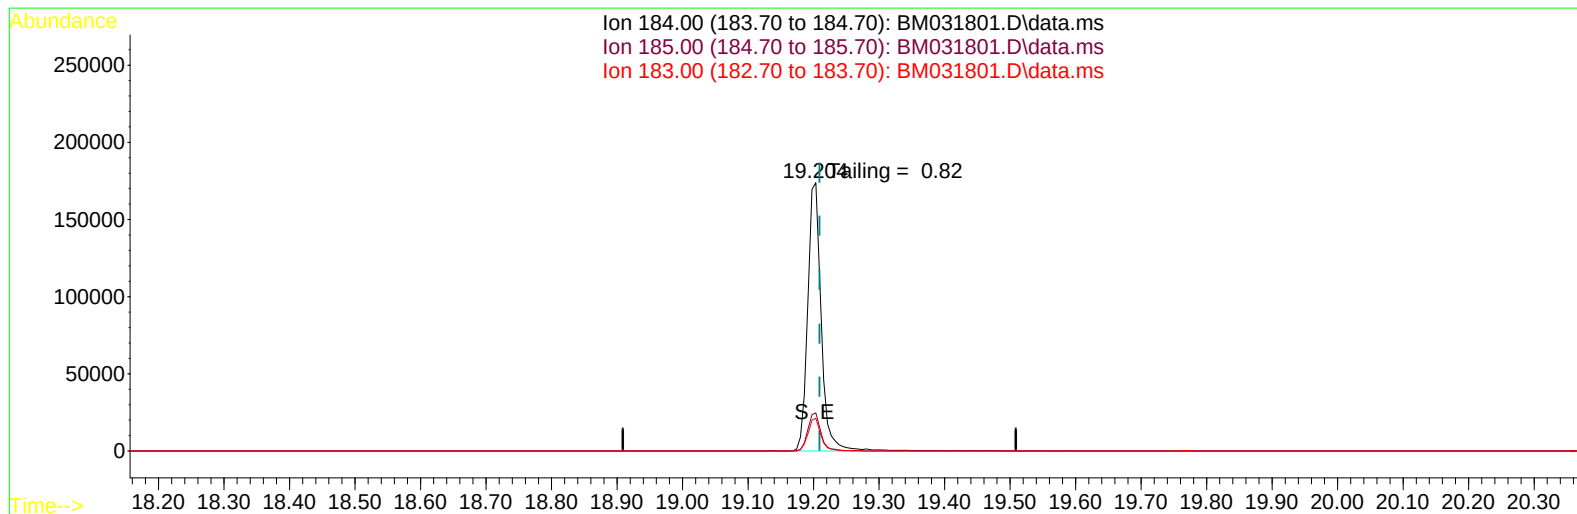

TIC: BM031801.D\data.ms

(77) Benzidine

19.204min (-0.006) 0.00 ng

response 248580

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.19
183.00	12.30	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/18/2021	BNA_M	<u>BM031801.D</u>
Compound Name	Response	Retention Time
DDT	142168	20.43
DDD	5961	19.99
DDE	612	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6573	148741	4.42