
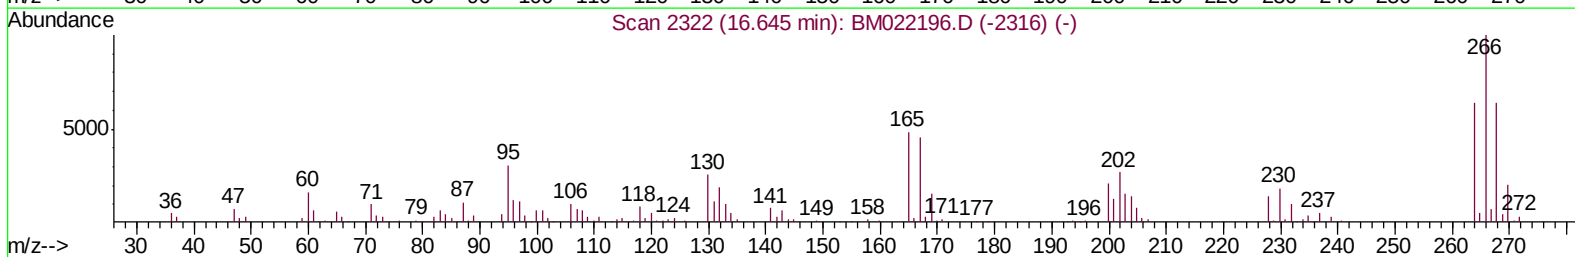
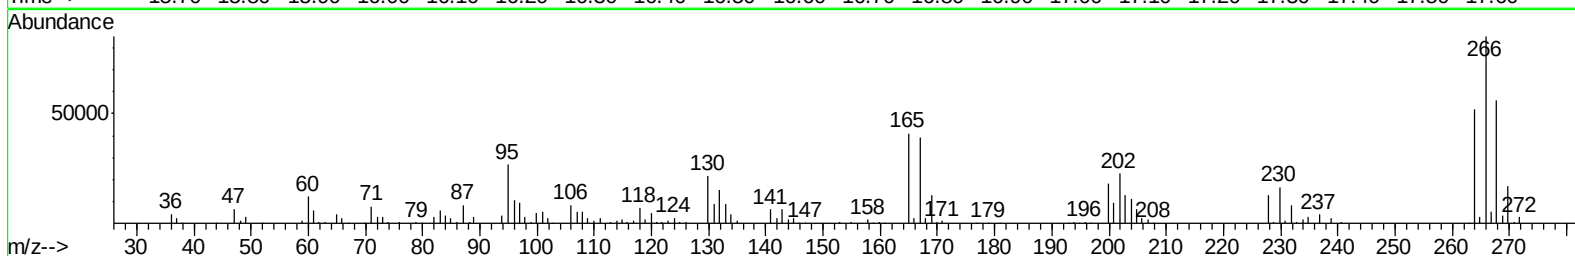


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082019\
Data File : BM022193.D
Acq On : 19 Aug 2019 17:13
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 11:26:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 02:18:05 2019
Response via : Initial Calibration

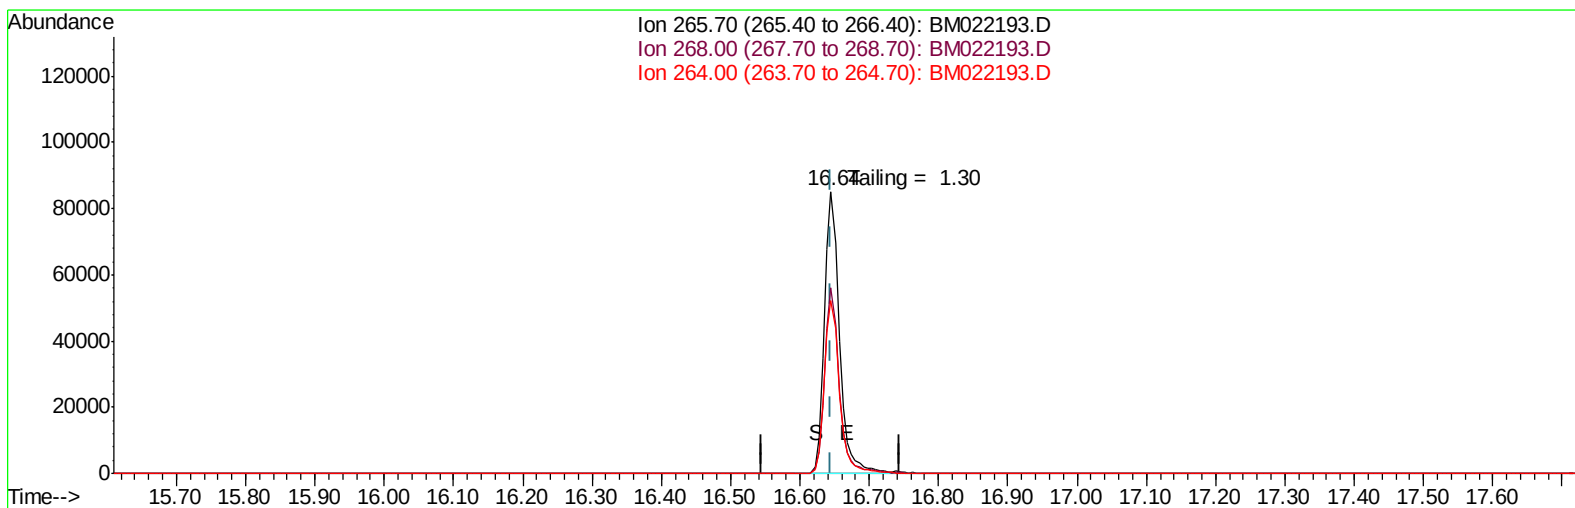

TIC: BM022193.D

(70) Pentachlorophenol (C)




16.645min (+0.000) 0.00ng

response 126878

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	65.93
264.00	62.40	61.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082019\
Data File : BM022193.D
Acq On : 19 Aug 2019 17:13
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 11:26:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 02:18:05 2019
Response via : Initial Calibration

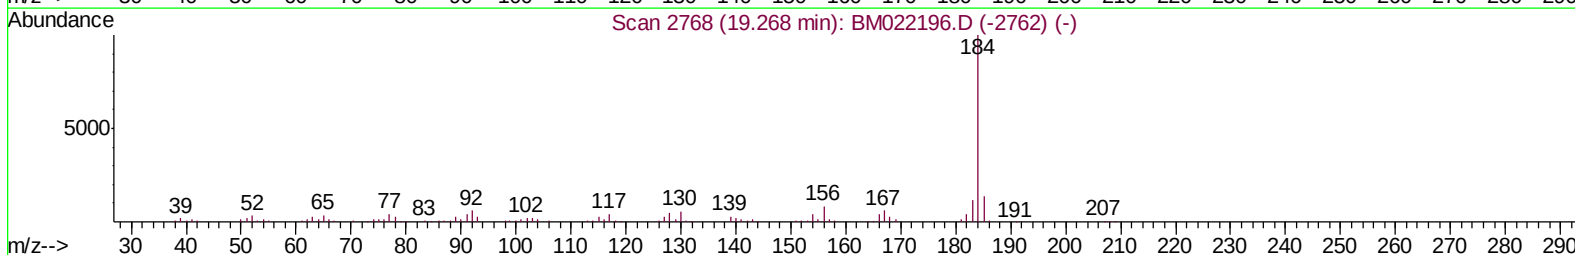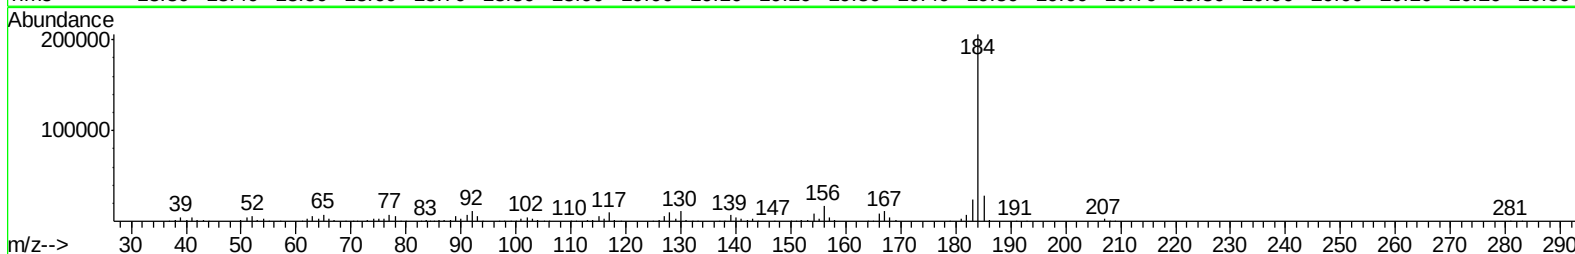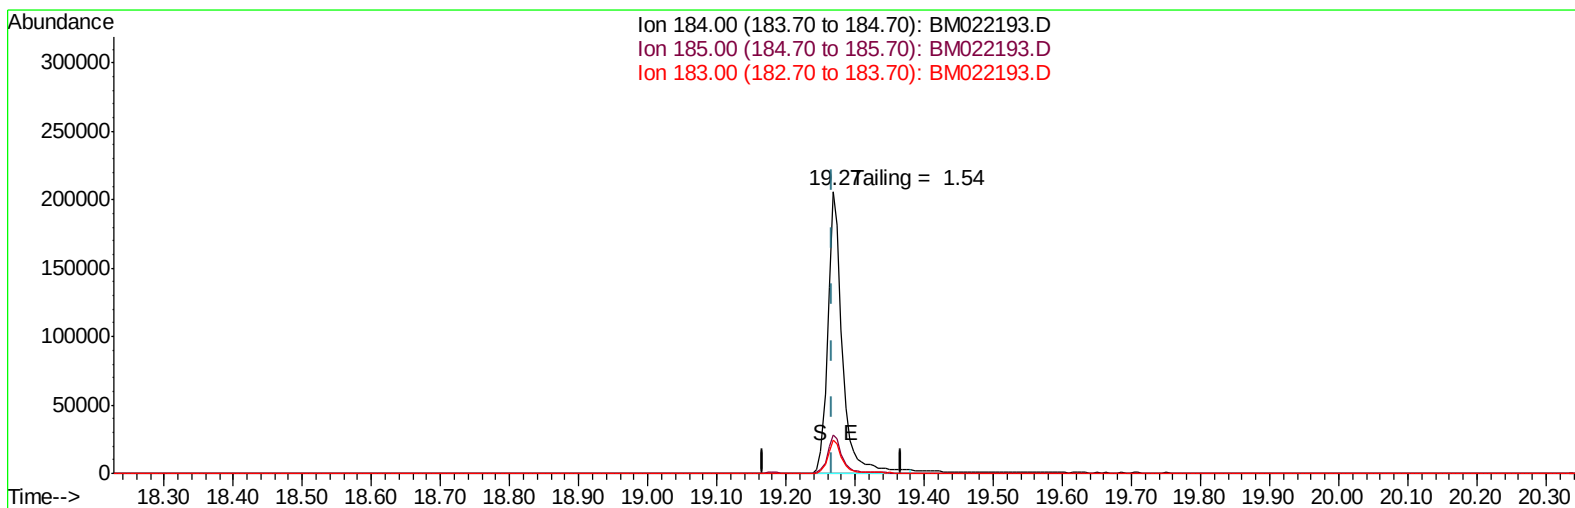

TIC: BM022193.D

(77) Benzidine

19.268min (+0.000) 0.00ng

response 297376

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.56
183.00	12.00	11.99
0.00	0.00	0.00