
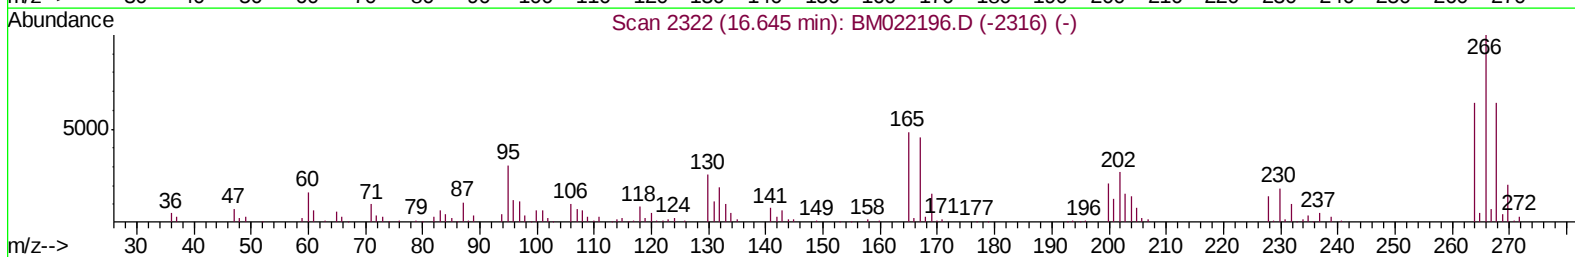
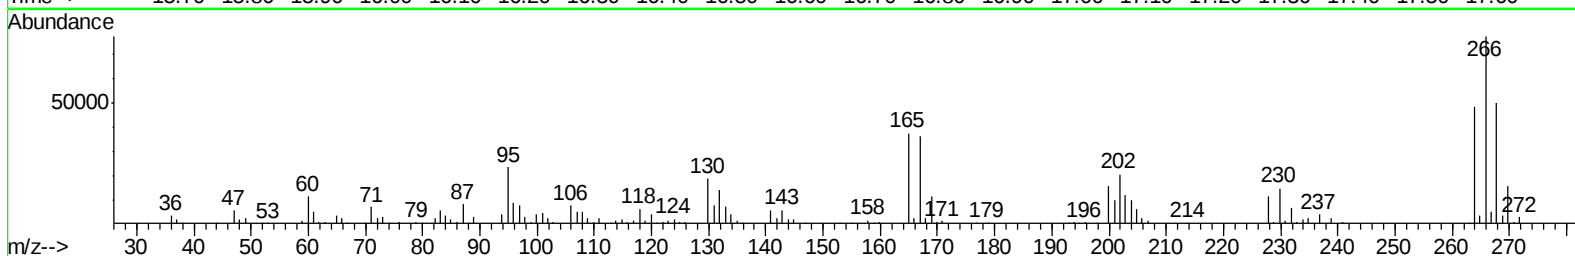


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082019\
 Data File : BM022202.D
 Acq On : 20 Aug 2019 08:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 11:29:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 20 02:18:05 2019
 Response via : Initial Calibration

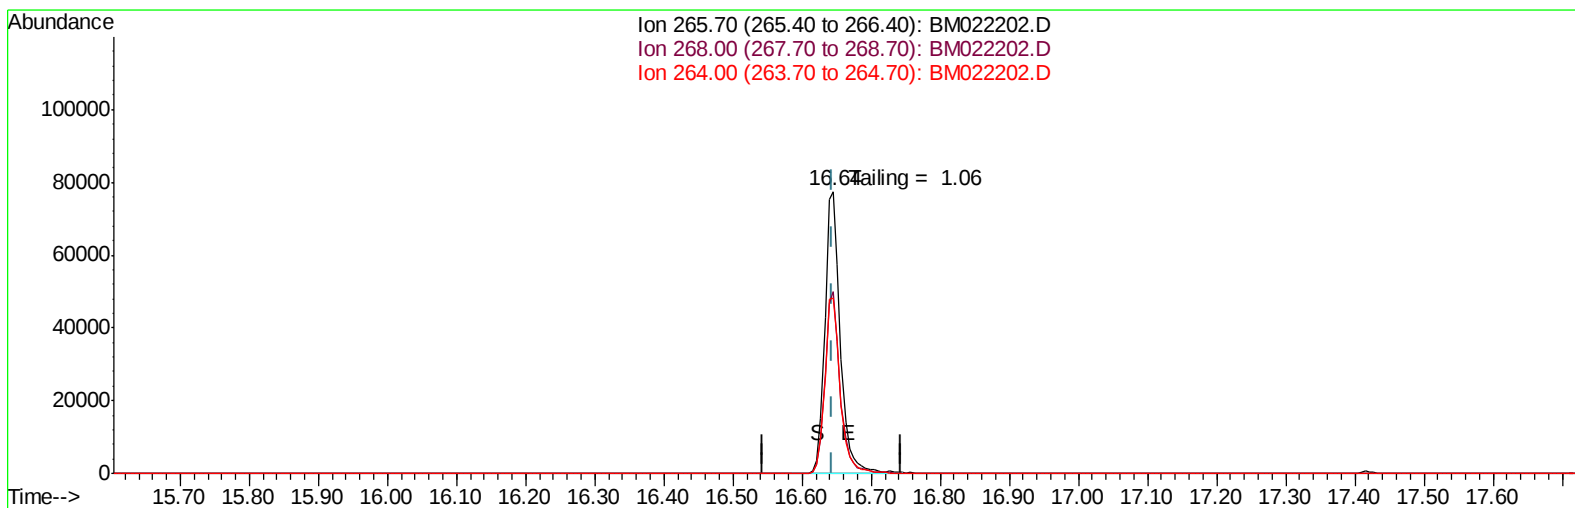

TIC: BM022202.D

(70) Pentachlorophenol (C)




16.645min (+0.000) 0.00ng

response 119456

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	64.37
264.00	62.40	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082019\
Data File : BM022202.D
Acq On : 20 Aug 2019 08:15
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 11:29:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 02:18:05 2019
Response via : Initial Calibration

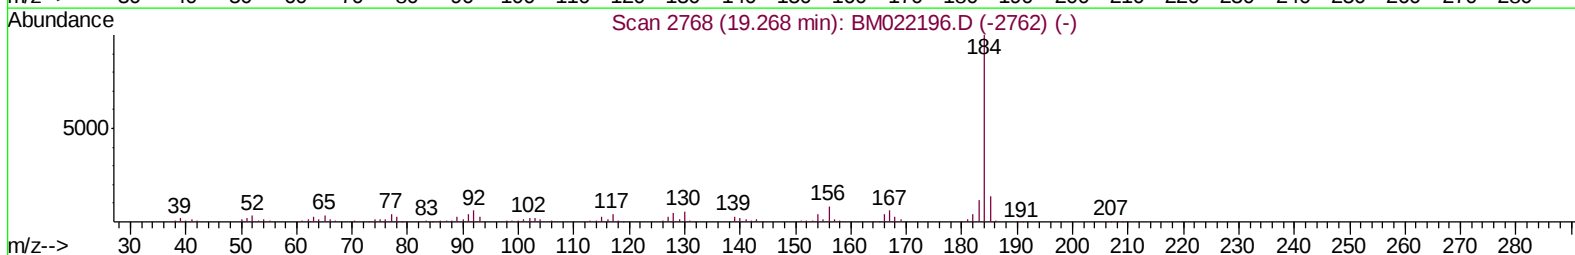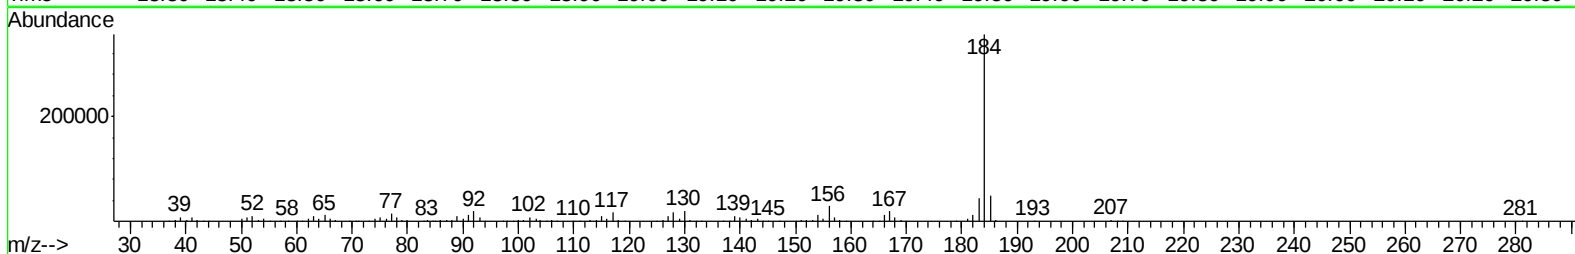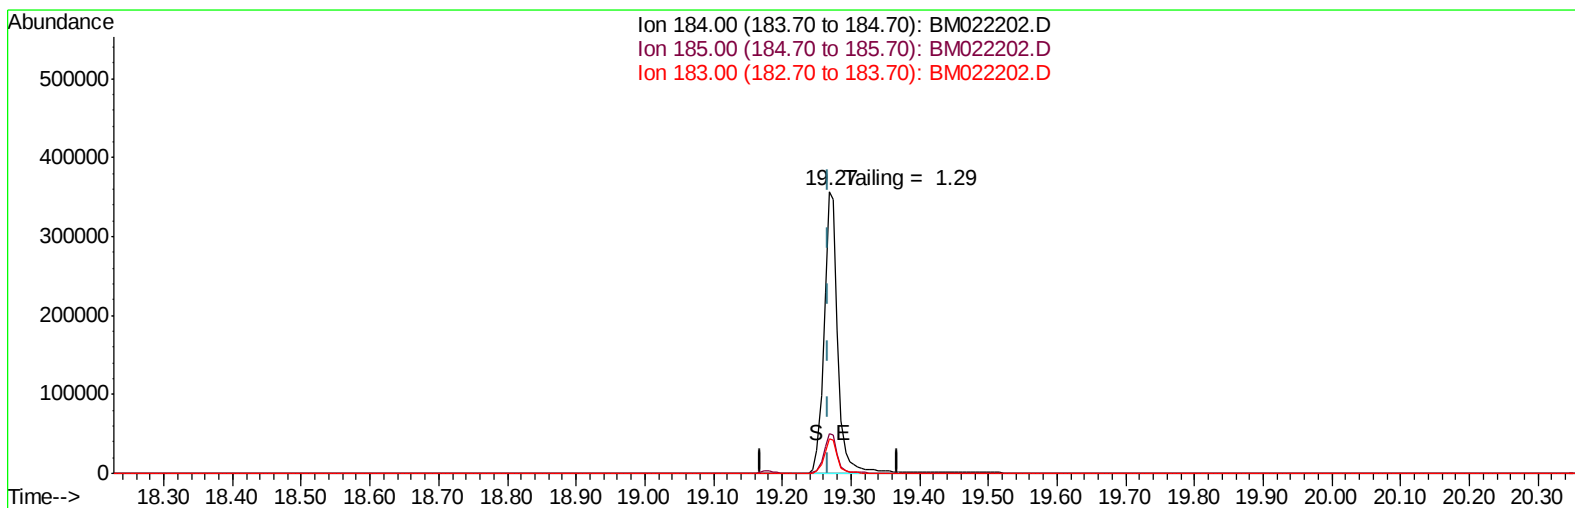

TIC: BM022202.D

(77) Benzidine

19.268min (+0.000) 8226.72ng

response 497283

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.11
183.00	12.00	12.08
0.00	0.00	0.00