


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082019\
 Data File : BM022193.D
 Acq On : 19 Aug 2019 17:13
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 02:18:05 2019

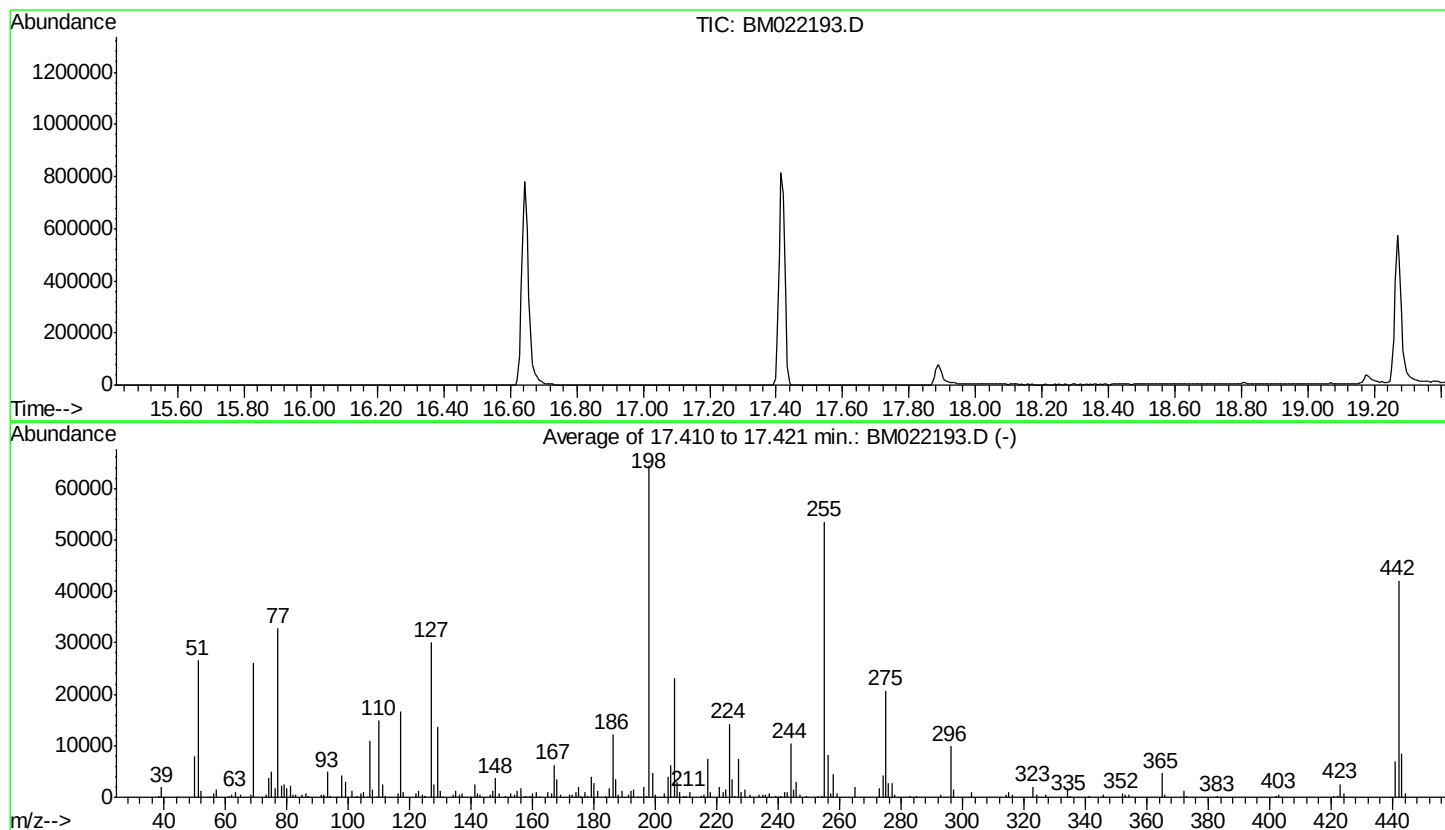

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	26565	PASS
68	69	0.00	2	2.0	522	PASS
69	198	0.00	100	40.6	26109	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	30069	PASS
197	198	0.00	2	0.5	348	PASS
198	198	100	100	100.0	64381	PASS
199	198	5	9	7.3	4681	PASS
275	198	10	60	32.1	20686	PASS
365	198	1	100	7.3	4693	PASS
441	198	0.01	100	10.9	7003	PASS
442	198	50	100	65.3	42056	PASS
443	442	15	24	19.9	8367	PASS