


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082019\
 Data File : BM022202.D
 Acq On : 20 Aug 2019 08:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 02:18:05 2019

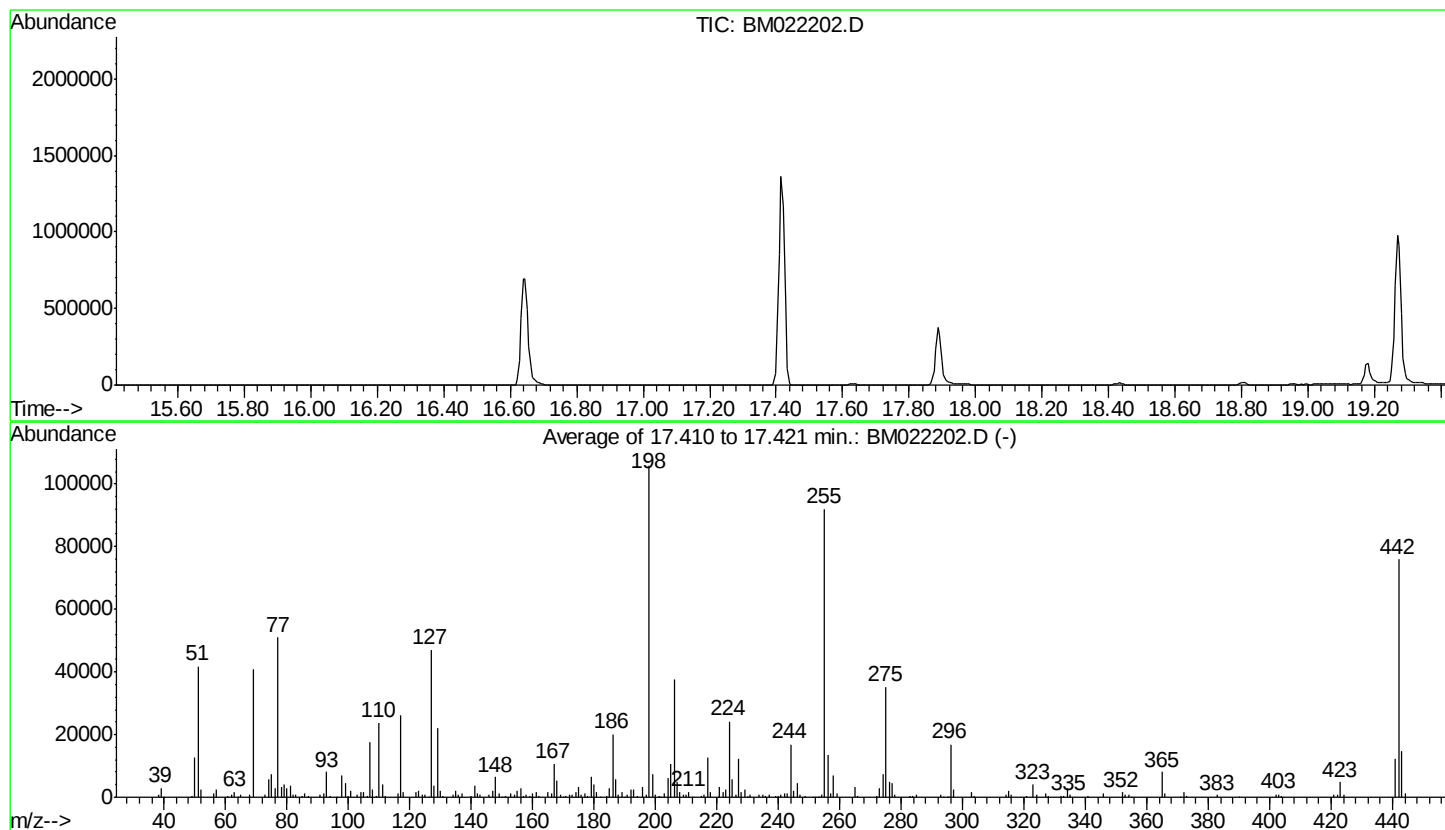

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	41781	PASS
68	69	0.00	2	1.9	792	PASS
69	198	0.00	100	38.5	40776	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	47002	PASS
197	198	0.00	2	0.6	677	PASS
198	198	100	100	100.0	105848	PASS
199	198	5	9	6.8	7225	PASS
275	198	10	60	33.3	35218	PASS
365	198	1	100	7.7	8110	PASS
441	198	0.01	100	11.7	12369	PASS
442	198	50	100	71.6	75818	PASS
443	442	15	24	19.3	14598	PASS