

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
 Data File : BM016511.D
 Acq On : 22 Aug 2018 09:11
 Operator : SJ/JU
 Sample : J4275-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 22 11:32:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 21 16:31:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	163886	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	506557	20.00	ng	0.00
38) Acenaphthene-d10	14.66	164	404406	20.00	ng	-0.01
63) Phenanthrene-d10	17.40	188	1436927	20.00	ng	0.00
75) Chrysene-d12	21.54	240	2016597	20.00	ng	0.00
86) Perylene-d12	23.83	264	2002988	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	1189608	142.24	ng	0.00
7) Phenol-d6	7.20	99	1284540	116.07	ng	0.00
23) Nitrobenzene-d5	9.20	82	1323887	119.33	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	2943895	260.41	ng	0.00
44) 2-Fluorobiphenyl	13.28	172	5403431	128.43	ng	0.00
78) Terphenyl-d14	19.99	244	12839267	134.76	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.34	79	28895	2.812	ng	Qvalue # 1
31) Naphthalene	10.88	128	181409	7.517	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016511.D
Acq On : 22 Aug 2018 09:11
Operator : SJ/JU
Sample : J4275-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 22 11:32:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

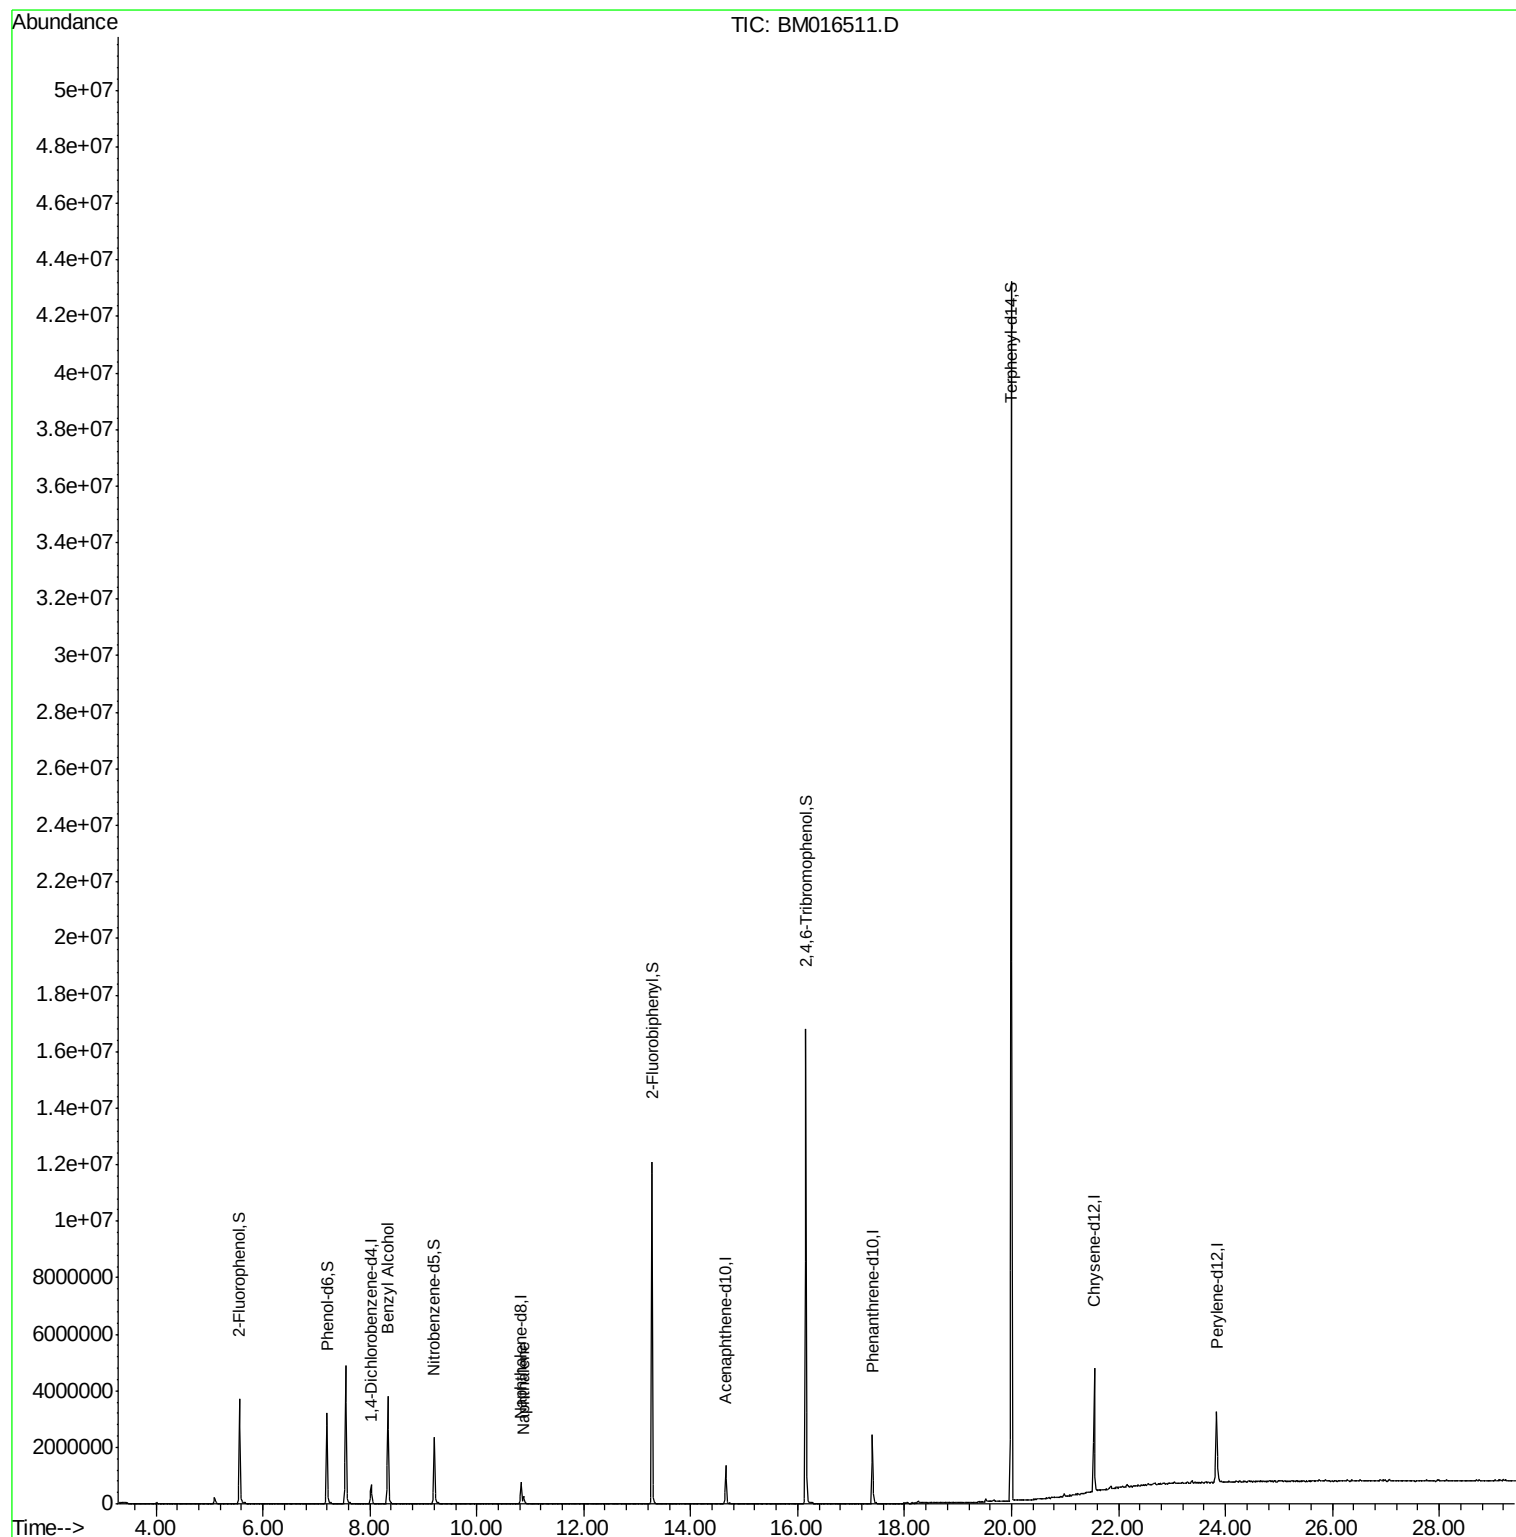




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.02 min Scan# 805
Delta R.T. -0.00 min
Lab File: BM016511.D
Acq: 22 Aug 2018 09:11

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.2	119.5	179.3
115	56.2	43.0	64.4






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

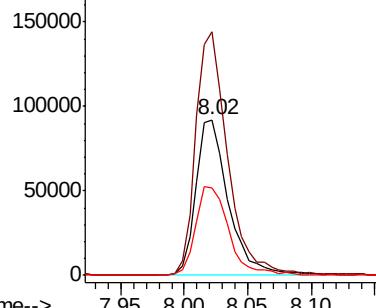

#5

2-Fluorophenol
Concen: Below ng
RT: 5.56 min Scan# 387
Delta R.T. 0.01 min
Lab File: BM016511.D
Acq: 22 Aug 2018 09:11

Tgt Ion	Ratio	Lower	Upper
112	100		
64	51.7	38.6	57.8
63	40.4	19.3	28.9






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

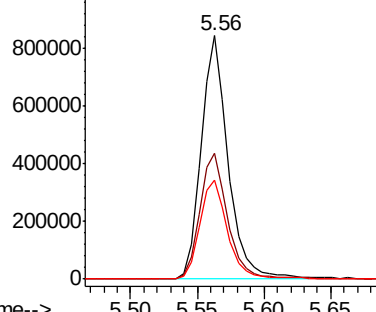



#7

Phenol-d6

Concen: N.D. ng

RT: 7.20 min Scan# 665

Delta R.T. -0.00 min

Lab File: BM016511.D

Acq: 22 Aug 2018 09:11

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 1284540

Ion Ratio Lower Upper

99 100

42 20.9 11.0 16.4#




71 64.3 23.4 35.2#



Abundance Ion 99.00 (98.70 to 99.70): BM016511.D (-648) (-)

Ion 42.00 (41.70 to 42.70): BM016511.D (-648) (-)

Ion 71.00 (70.70 to 71.70): BM016511.D (-648) (-)

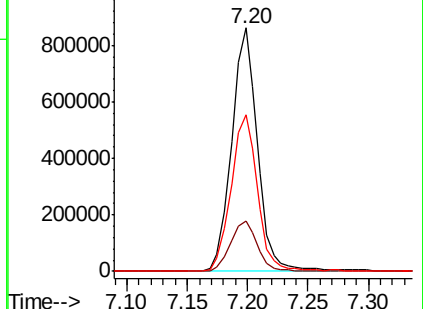

#15

Benzyl Alcohol

Concen: 2.812 ng

RT: 8.34 min Scan# 859

Delta R.T. 0.06 min

Lab File: BM016511.D

Acq: 22 Aug 2018 09:11


Tgt Ion: 79 Resp: 28895

Ion Ratio Lower Upper

79 100

108 109.5 65.0 97.4#



77 229.6 53.0 79.6#




Abundance Ion 79.00 (78.70 to 79.70): BM016511.D (-832) (-)

Ion 108.00 (107.70 to 108.70): BM016511.D (-832) (-)

Ion 77.00 (76.70 to 77.70): BM016511.D (-832) (-)



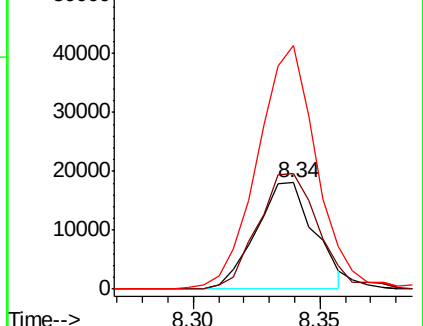



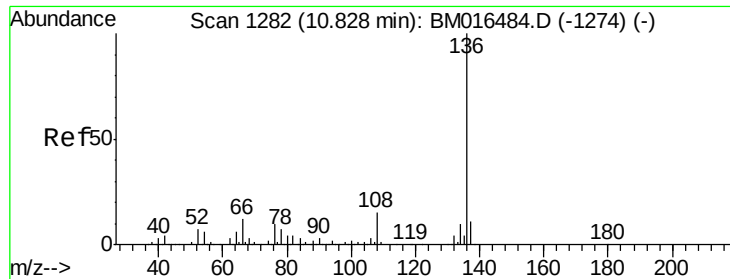

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.83 min Scan# 1282
Delta R.T. -0.00 min
Lab File: BM016511.D
Acq: 22 Aug 2018 09:11




Instrument :
BNA_M
ClientSampleId :


Tot Ion:136	Resp:	506557
Ion	Ratio	Lower Upper
136	100	
137	11.4	8.7 13.1
54	7.5	4.6 6.8#
68	3.2	3.7 5.5#

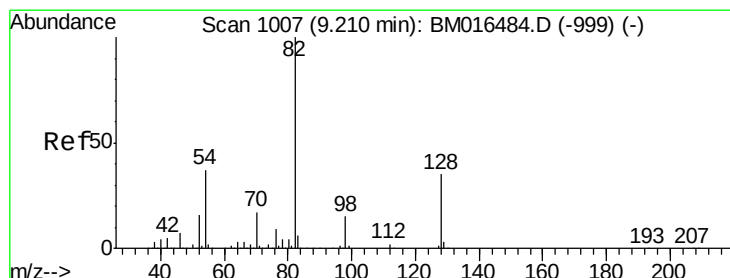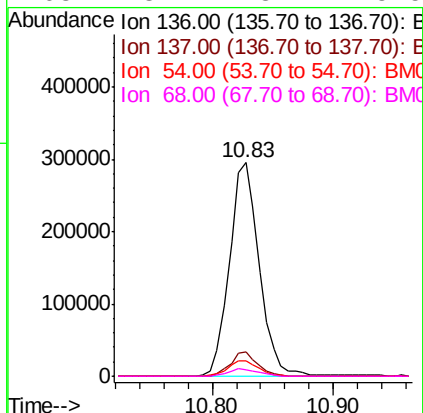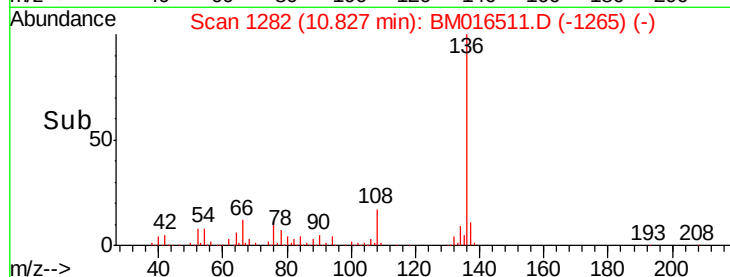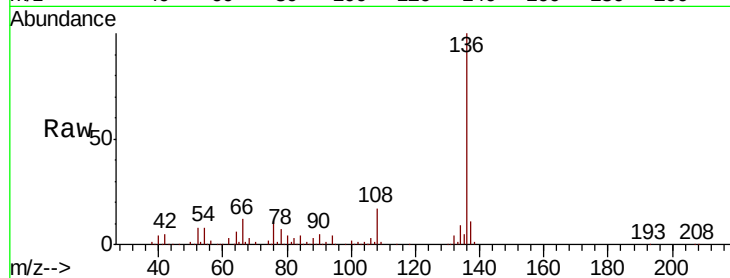

#23
Nitrobenzene-d5
Concen: Below ng
RT: 9.20 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BM016511.D
Acq: 22 Aug 2018 09:11

Tgt Ion: 82	Resp:	1323887
Ion	Ratio	Lower Upper
82	100	
128	34.2	32.8 49.2
54	39.0	40.6 60.8#

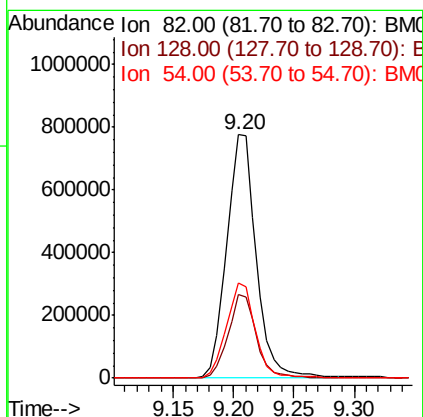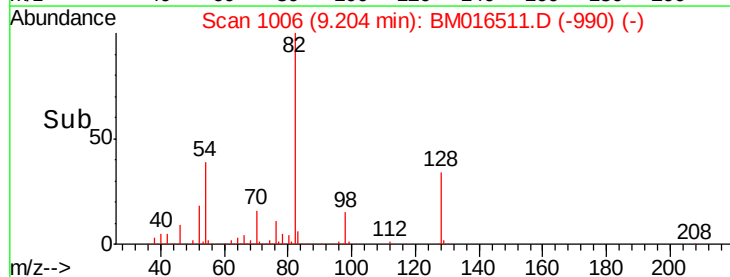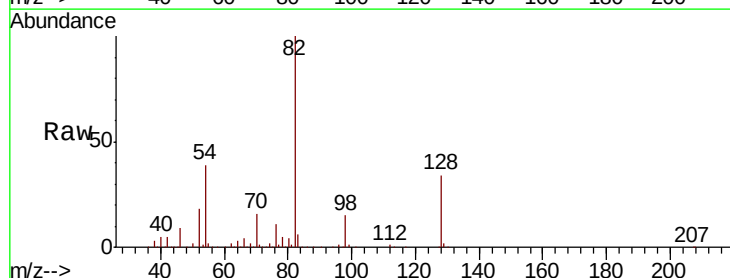

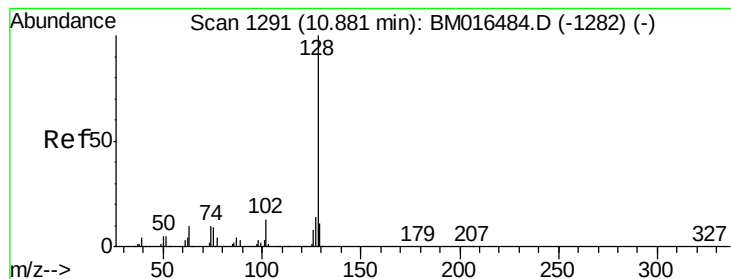

#31

Naphthalene

Concen: 7.517 ng

RT: 10.88 min Scan# 1291

Delta R.T. -0.00 min

Lab File: BM016511.D

Acq: 22 Aug 2018 09:11

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 181409

Ion Ratio Lower Upper

128 100

129 12.3 8.9 13.3

127 14.0 10.4 15.6



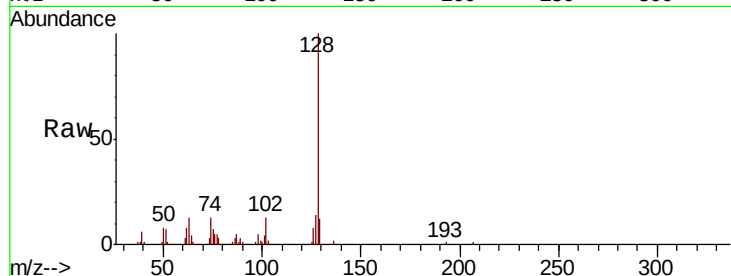


Abundance

Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

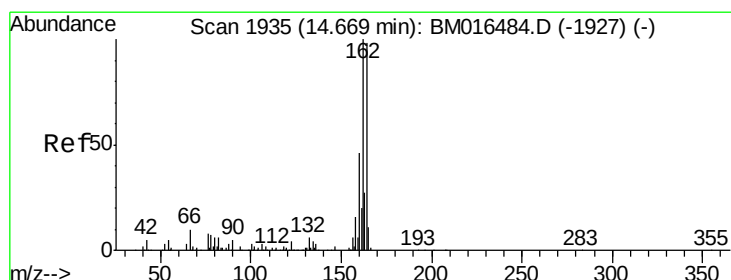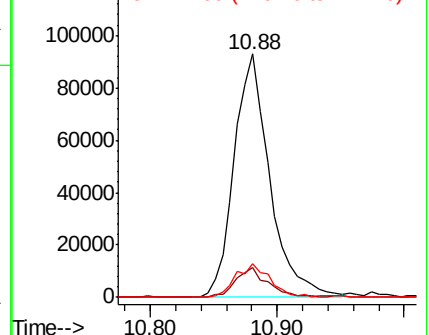

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1933

Delta R.T. -0.01 min

Lab File: BM016511.D

Acq: 22 Aug 2018 09:11


Tgt Ion:164 Resp: 404406

Ion Ratio Lower Upper

164 100

162 103.2 82.4 123.6

160 45.4 35.8 53.6






Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



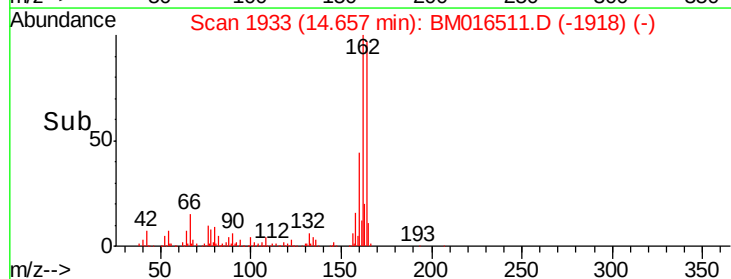
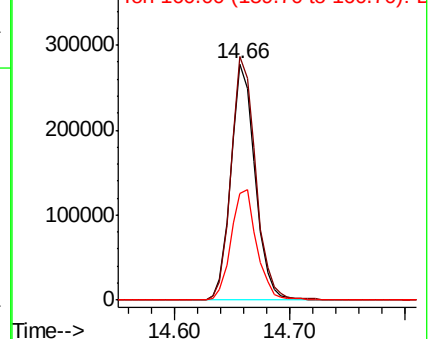




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.16 min Scan# 2188
 Delta R.T. 0.00 min
 Lab File: BM016511.D
 Acq: 22 Aug 2018 09:11




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:330 Resp: 2943895
 Ion Ratio Lower Upper
 330 100
 332 96.9 0.0 0.0#
 141 29.7 0.0 0.0#

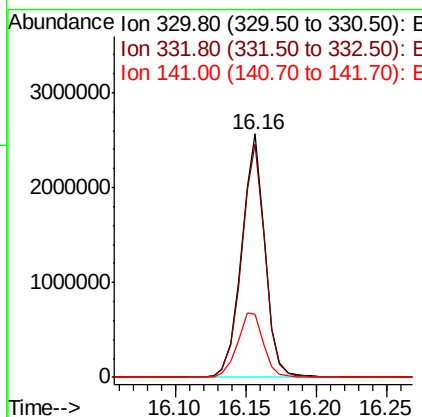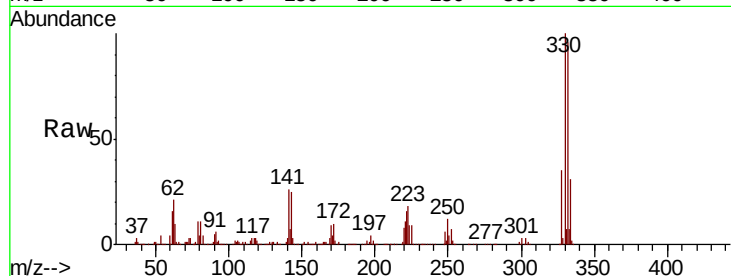

#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.28 min Scan# 1699
 Delta R.T. -0.00 min
 Lab File: BM016511.D
 Acq: 22 Aug 2018 09:11

Tgt Ion:172 Resp: 5403431
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.5 42.7
 170 23.1 18.8 28.2

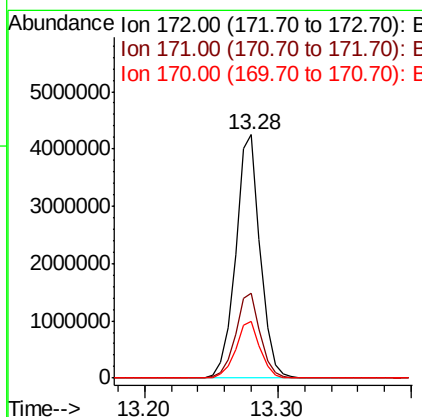



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2400

Delta R.T. -0.00 min

Lab File: BM016511.D

Acq: 22 Aug 2018 09:11

Instrument :

BNA_M

ClientSampled :


Tot Ion:188 Resp: 1436927

Ion Ratio Lower Upper

188 100

94 2.3 8.7 13.1#




80 3.2 9.3 13.9#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

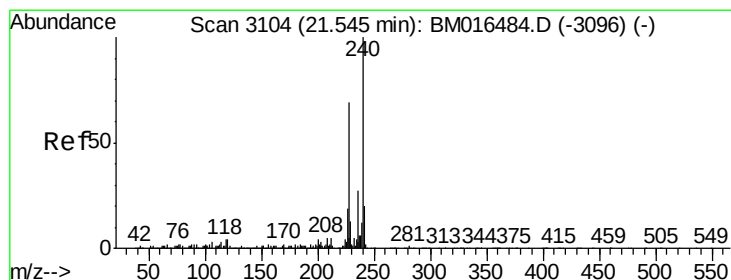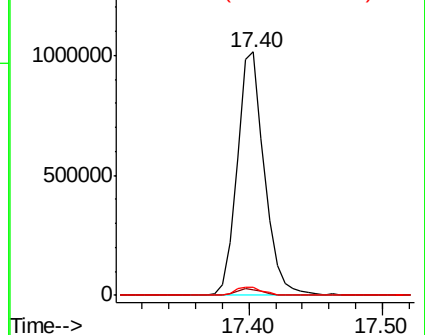

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.54 min Scan# 3104

Delta R.T. -0.00 min

Lab File: BM016511.D

Acq: 22 Aug 2018 09:11


Tgt Ion:240 Resp: 2016597

Ion Ratio Lower Upper

240 100

120 2.4 8.2 12.2#



236 25.8 20.0 30.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



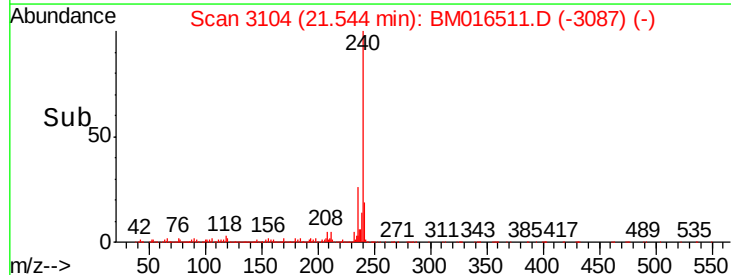
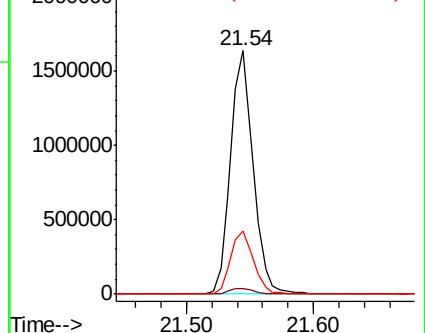


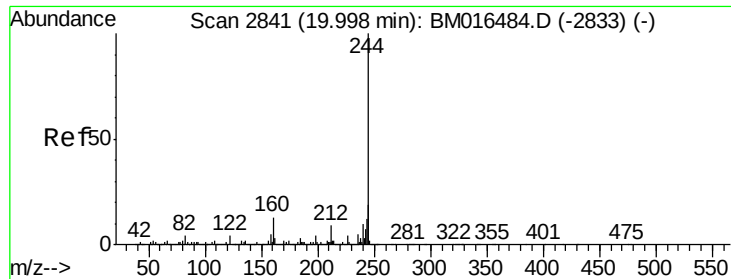

#78
 Terphenyl-d14
 Concen: Below na
 RT: 19.99 min Scan# 2840
 Delta R.T. -0.01 min
 Lab File: BM016511.D
 Acq: 22 Aug 2018 09:11

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:244 Resp:12839267
 Ion Ratio Lower Upper
 244 100
 212 15.7 4.9 7.3#
 122 6.9 6.2 9.4

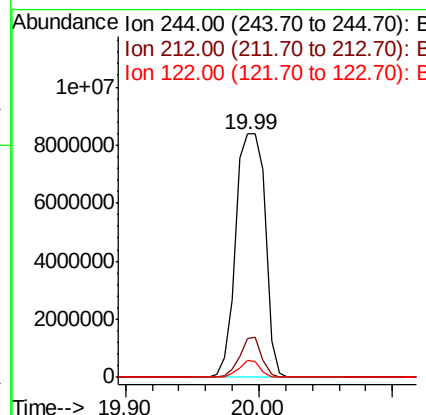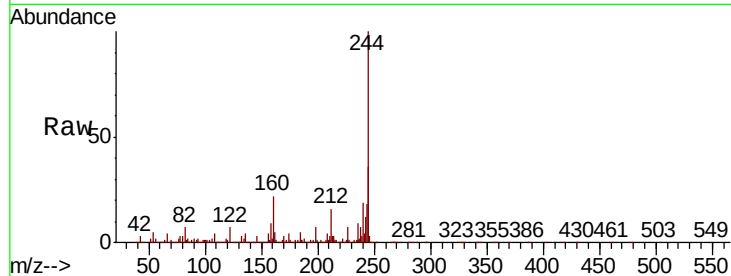

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.83 min Scan# 3493
 Delta R.T. -0.01 min
 Lab File: BM016511.D
 Acq: 22 Aug 2018 09:11

Tgt Ion:264 Resp: 2002988
 Ion Ratio Lower Upper
 264 100
 260 24.7 18.6 27.8
 265 21.5 17.3 25.9

