
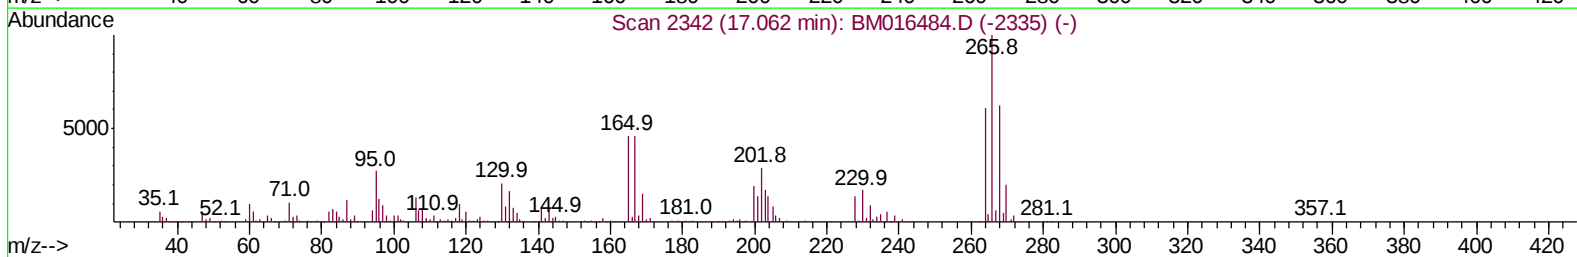
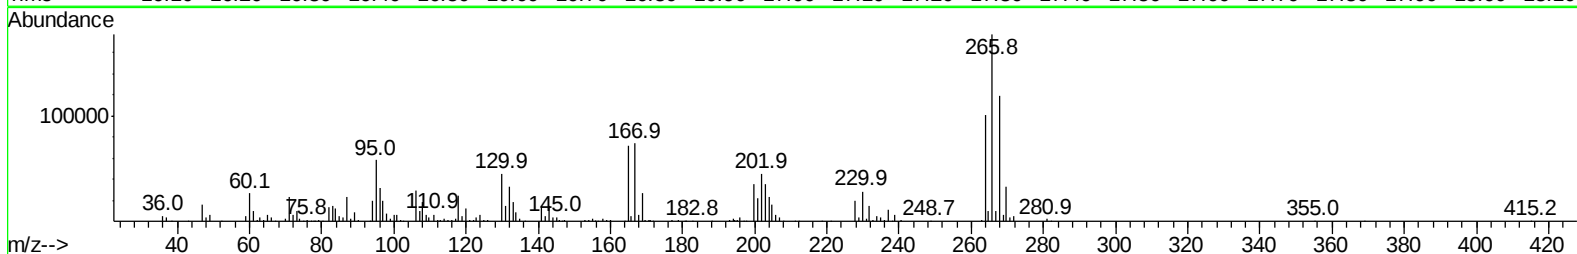


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016479.D
Acq On : 21 Aug 2018 10:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:49:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

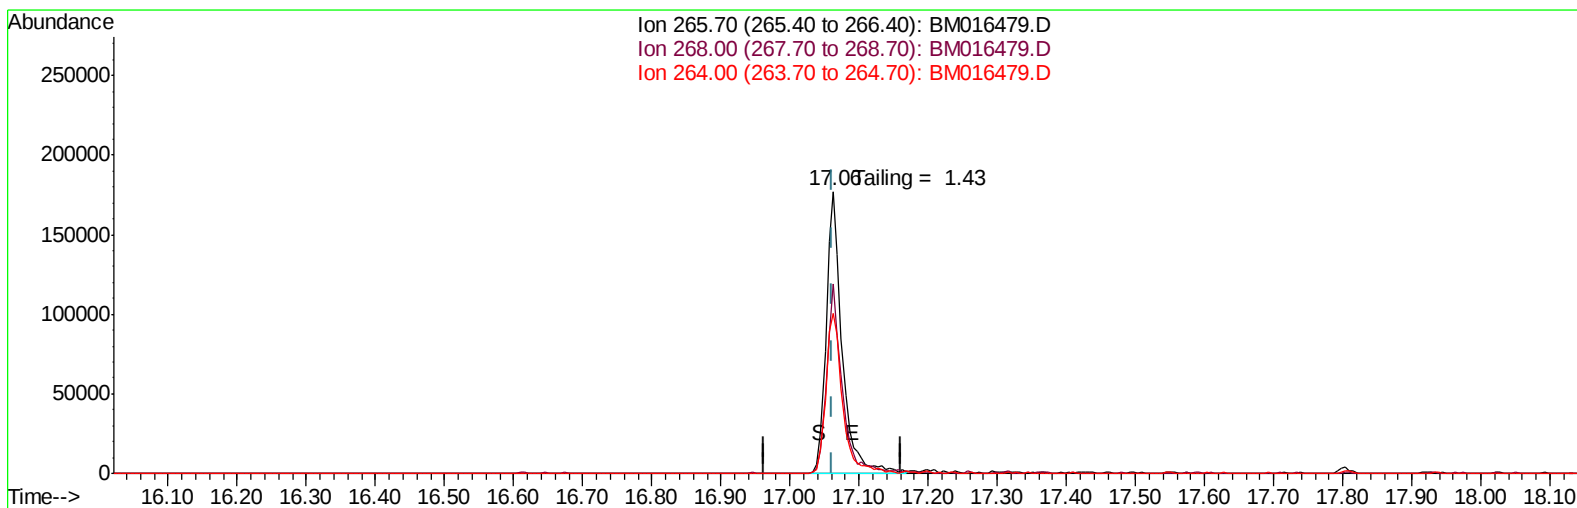

TIC: BM016479.D

(69) Pentachlorophenol (C)




17.062min (-0.000) 0.00ng

response 280611

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.26
264.00	61.20	56.83
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016479.D
Acq On : 21 Aug 2018 10:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:49:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

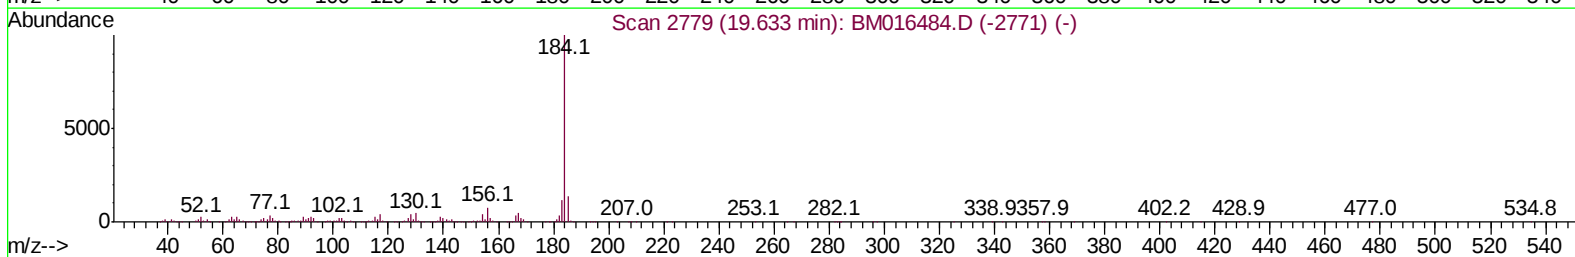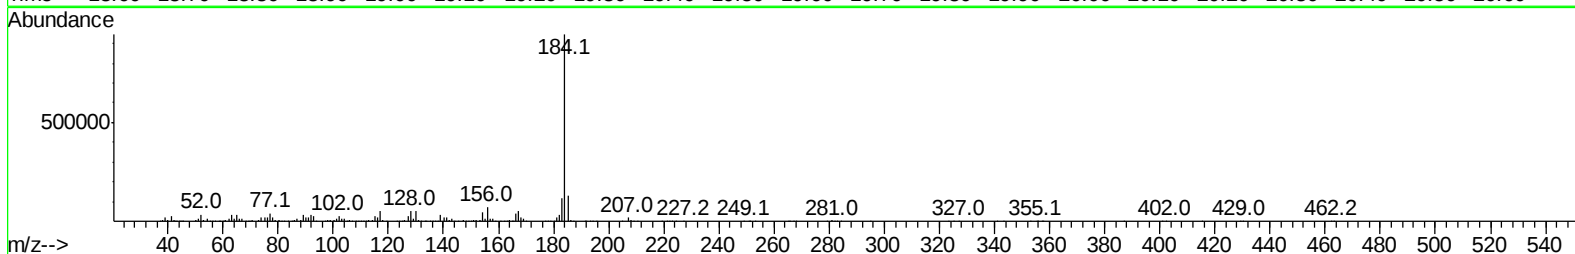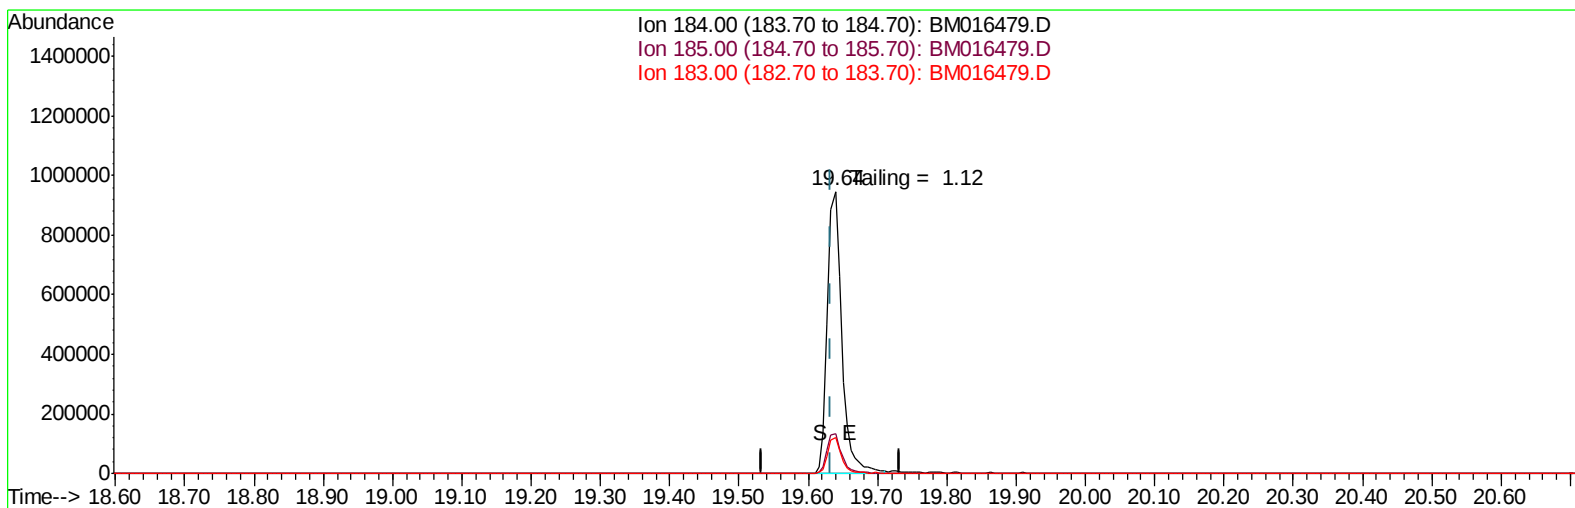

TIC: BM016479.D

(76) Benzidine

19.639min (+0.006) 499721.29ng

response 1364645

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.95
183.00	11.10	12.56
0.00	0.00	0.00