
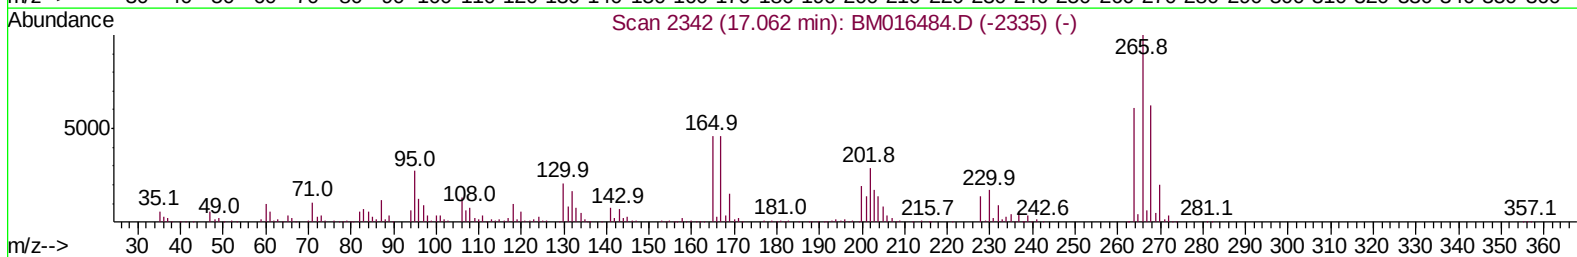
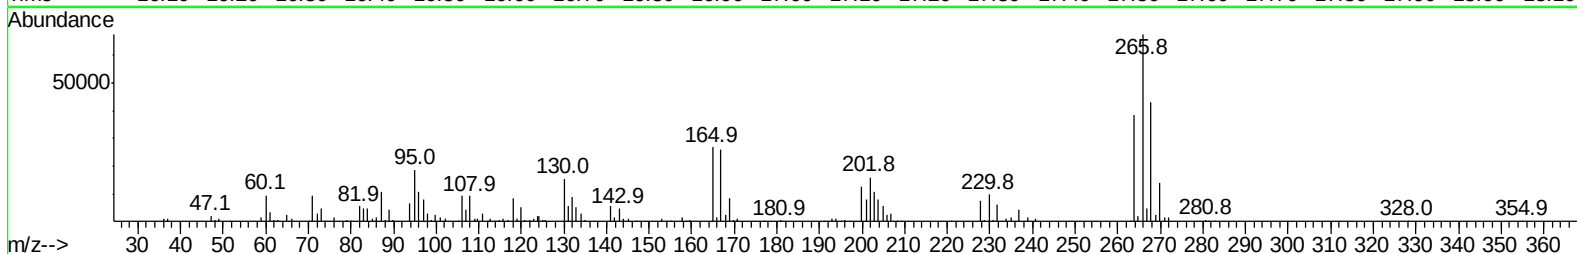


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016489.D
Acq On : 21 Aug 2018 18:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:51:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

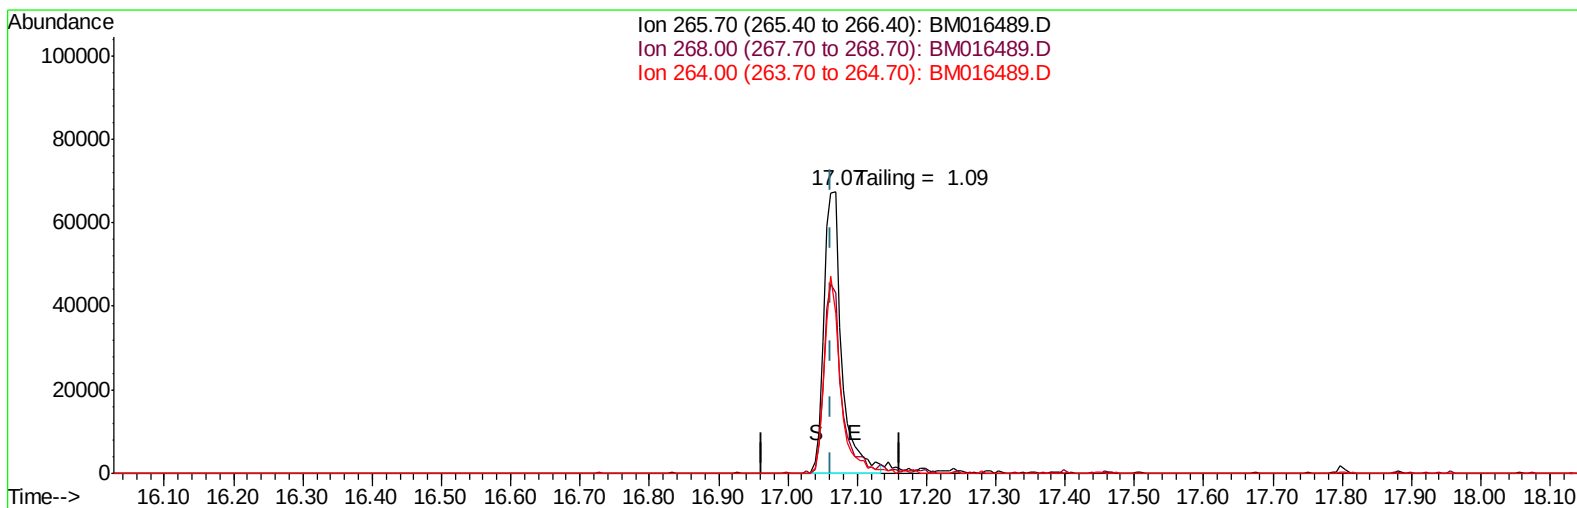

TIC: BM016489.D

(69) Pentachlorophenol (C)




17.068min (+0.006) 0.00ng m

response 119978

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.21
264.00	61.20	56.76
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016489.D
Acq On : 21 Aug 2018 18:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:51:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

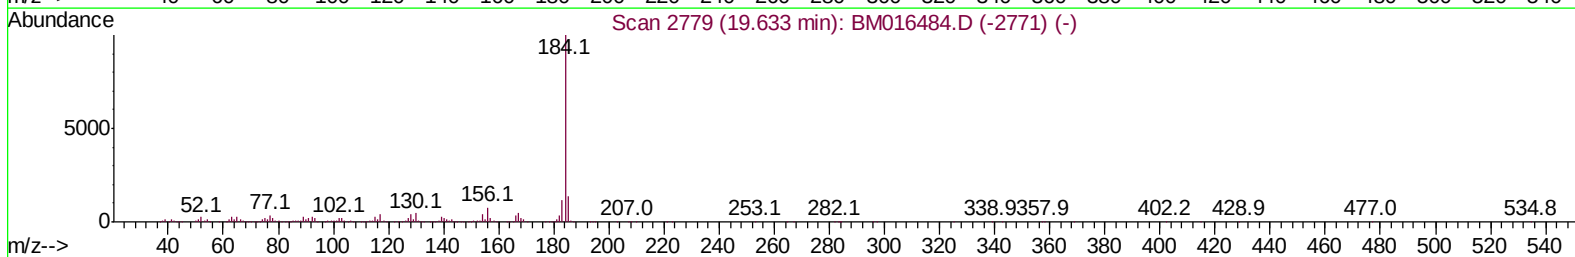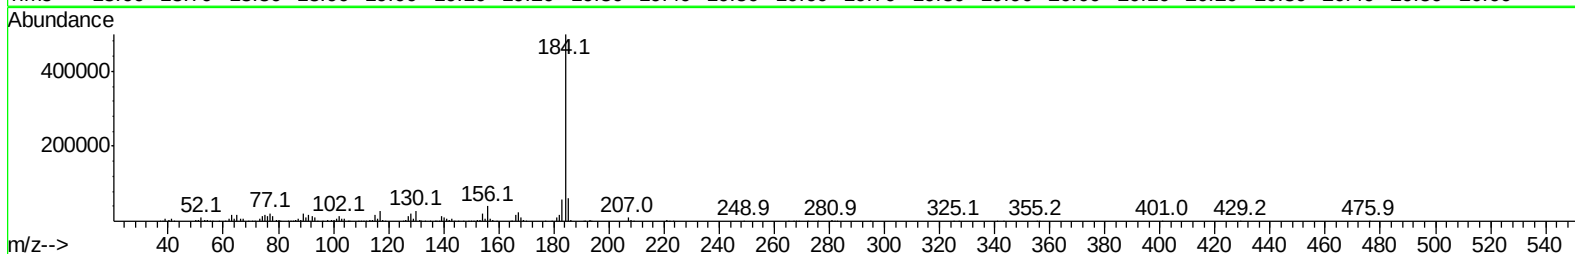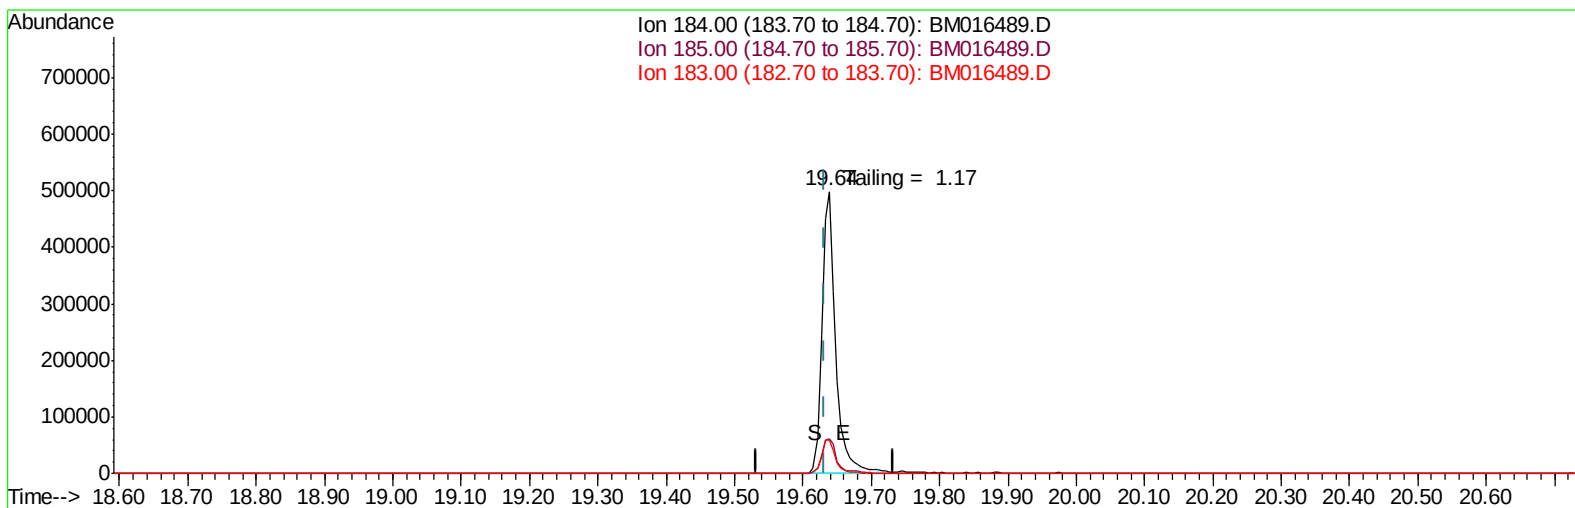

TIC: BM016489.D

(76) Benzidine

19.639min (+0.006) 281983.96ng

response 704971

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	12.46
183.00	11.10	12.04
0.00	0.00	0.00