
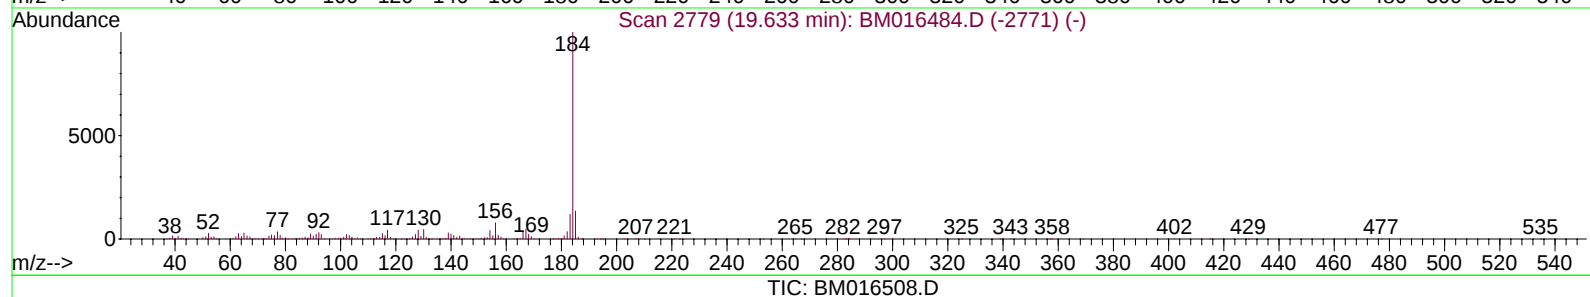
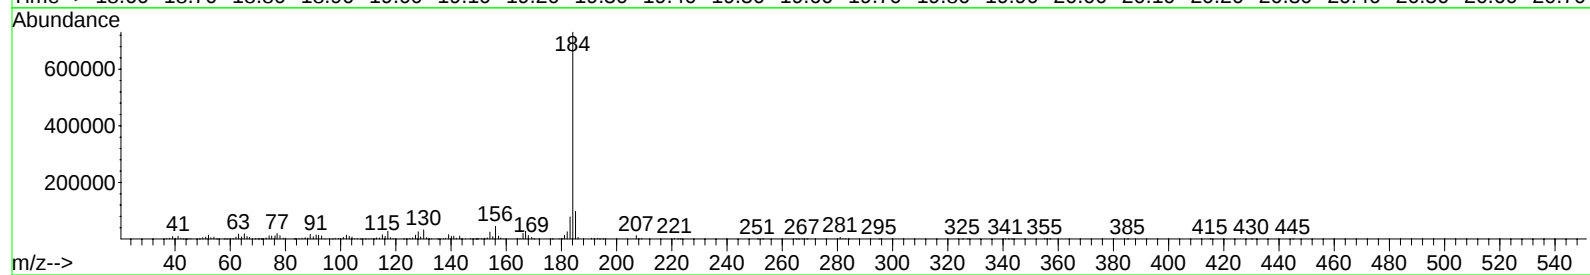


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082118\
Data File : BM016508.D
Acq On : 22 Aug 2018 07:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 14:43:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

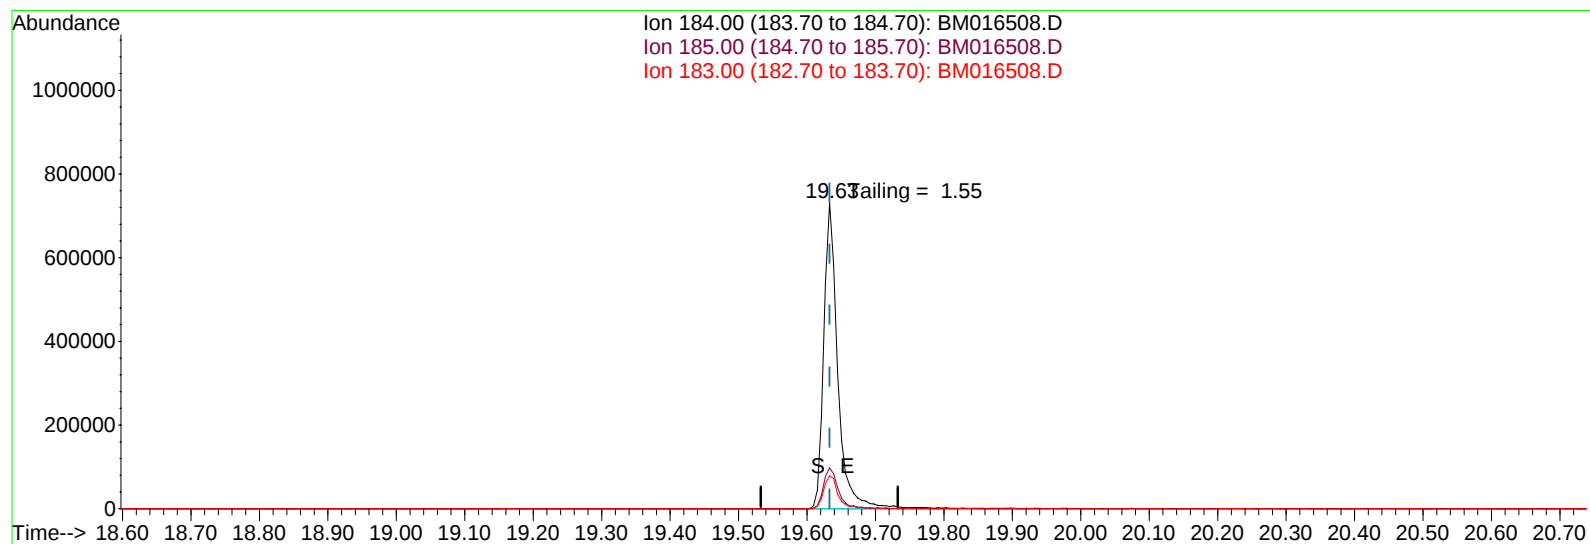

(76) Benzidine




19.633min (-0.000) 406463.42ng

response 1031808

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.34
183.00	11.10	10.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082118\
Data File : BM016508.D
Acq On : 22 Aug 2018 07:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 14:43:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

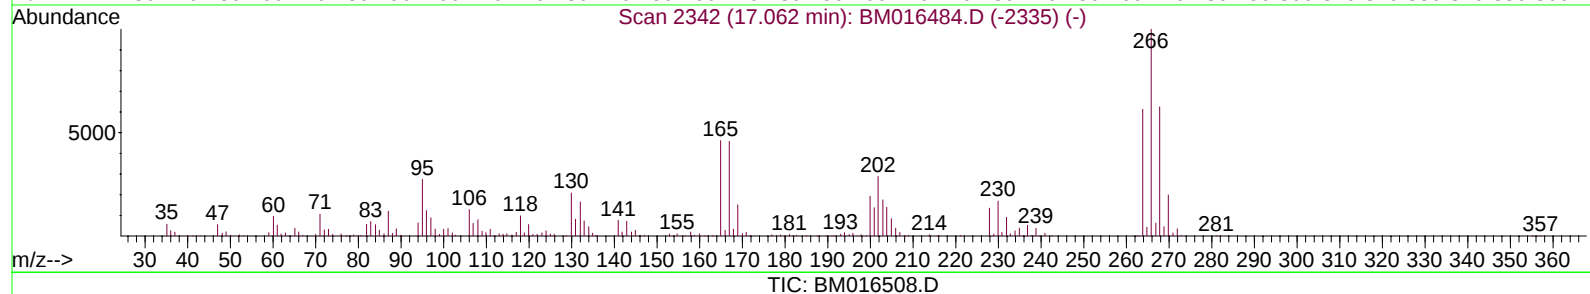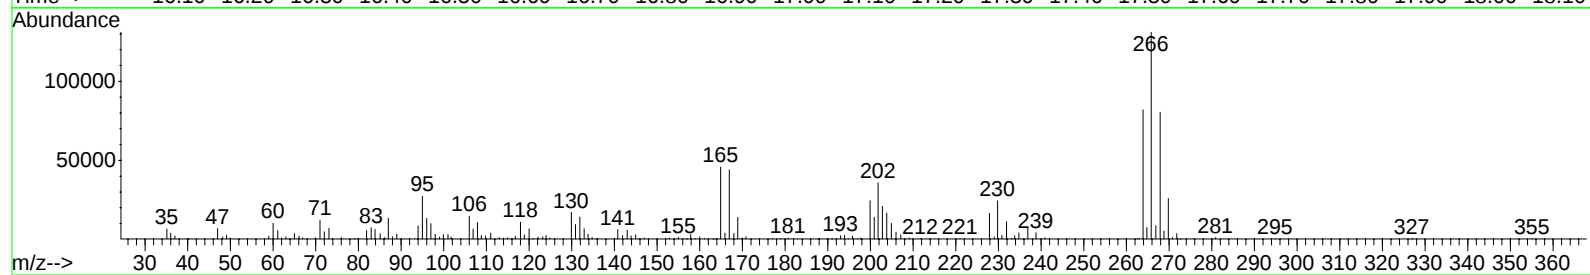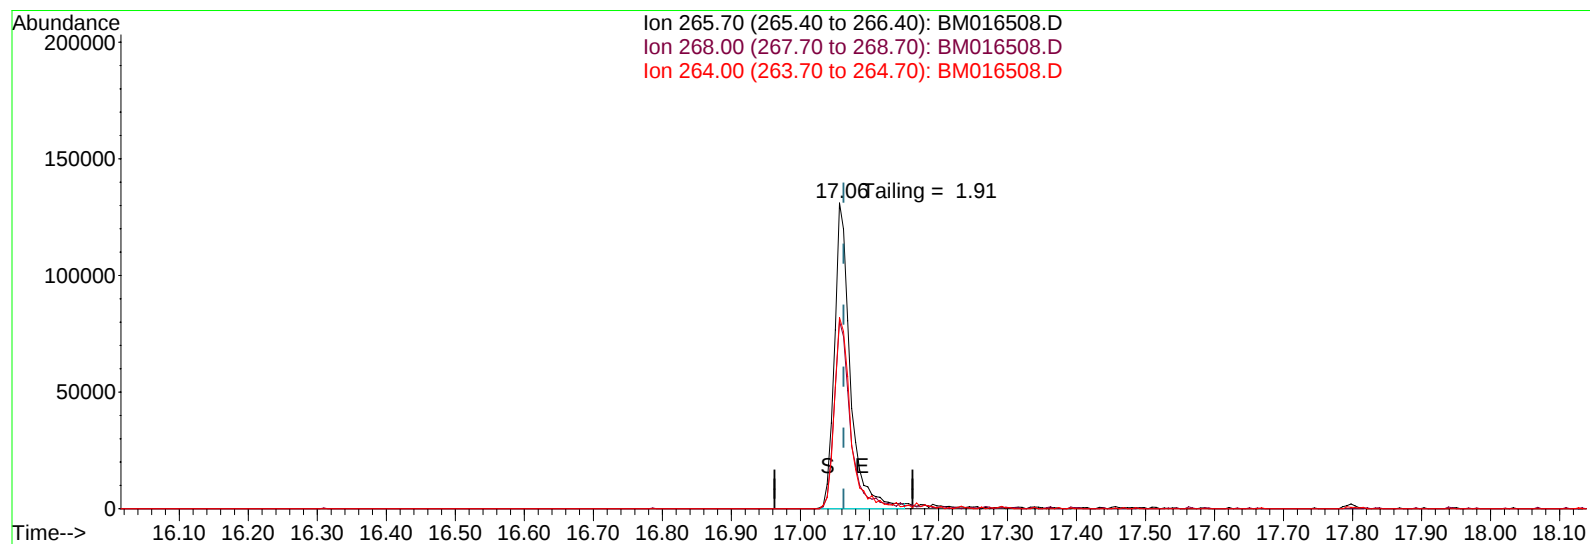

(69) Pentachlorophenol (C)

17.057min (-0.006) 0.00ng

response 208597

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.37
264.00	61.20	62.56
0.00	0.00	0.00